



USER MANUAL



SV 971A POCKET-SIZE SOUND LEVEL METER & ANALYSER

Warsaw, 2024-05-28

Rev. 1.03

Copyright © 2024 SVANTEK.

All rights reserved.



Note: On account of continuous product improvement SVANTEK reserves the right to make changes to product specifications without notice. To download the most up to date user's manual please visit our website at www.svantek.com.

This user's manual presents the firmware revision named 1.09.x.

The succeeding software revisions (marked with the higher numbers) can change the view of some displays presented in the text of the manual.



WEEE Note: Do not throw the device away with the unsorted municipal waste at the end of its life. Instead, hand it in at an official collection point for recycling. By doing this you will help to preserve the environment.

The software described in this manual is furnished under a license agreement and may be used only in accordance with the terms of that agreement.

Copyright Notice

Copyright © 2024 Svantek Sp. z o.o.

All rights reserved.

Reproduction without permission is prohibited.

Trademarks

Trademarks or registered marks in this manual belong to their respective manufacturers.

Microsoft, Windows, Excel and Word are registered trademarks of Microsoft Corporation.

The *Bluetooth*® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc.

Disclaimer

Information in this document is subject to change without notice and does not represent a commitment on the part of Svantek.

Svantek provides this document “as is”, without warranty of any kind, either expressed or implied, including, but not limited to, its particular purpose. Svantek reserves the right to make improvements and/or changes to this manual, or to the products and/or the programs described in this manual, at any time.

Information provided in this manual is intended to be accurate and reliable. However, Svantek assumes no responsibility for its use, or for any infringements on the rights of third parties that may result from its use.

This product might include unintentional technical or typographical errors. Changes are periodically made to the information herein to correct such errors, and these changes are incorporated into new editions of the publication.

Technical Support Contact Information:

web: www.svantek.com/contact

CONTENTS

INDEX	9
1 INTRODUCTION	12
1.1 SV 971A AS SOUND LEVEL METER & ANALYSER.....	12
1.2 GENERAL FEATURES OF SV 971A.....	13
1.3 ACCESSORIES INCLUDED.....	13
1.4 ACCESSORIES AVAILABLE	14
1.5 FIRMWARE AND SOFTWARE OPTIONS AVAILABLE.....	14
2 GENERAL INFORMATION	15
2.1 MEASUREMENT CONFIGURATIONS.....	15
2.2 SOUND MEASUREMENTS IN SPECIAL CONDITIONS.....	16
2.3 INPUT AND OUTPUT SOCKETS OF THE INSTRUMENT.....	16
2.4 INSTRUMENT POWER	17
2.5 CONTROL PANEL	18
2.6 WORKING WITH THE INSTRUMENT	19
2.6.1 <i>Measurement mode</i>	19
2.6.2 <i>Configuration mode</i>	20
2.7 DEFAULT SETTINGS	23
2.8 DESCRIPTION OF ICONS.....	24
2.9 OVERLOAD AND UNDERRANGE DETECTION	25
2.10 SAVING DATA	26
2.11 DOWNLOADING AND UPLOADING FILES.....	27
2.12 ACTIVATING OPTIONAL FUNCTIONS	27
3 MEASUREMENT FUNCTIONS AND CALIBRATION – FUNCTION	29
3.1 ACTIVATING MEASUREMENT FUNCTIONS – MEASUREMENT FUNCTION	29
3.2 CALIBRATION OF THE INSTRUMENT – CALIBRATION	29
3.2.1 <i>Calibration – By Measurement</i>	30
3.2.2 <i>Last calibration record – Last Calibration</i>	31
3.2.3 <i>History of calibrations – Calibration History</i>	32
3.2.4 <i>Erasing calibration records – Clear History</i>	32
3.2.5 <i>Post measurement calibration – Post Calibration</i>	32
3.2.6 <i>Automatic calibration – Auto Calibration</i>	32
4 CONFIGURING MEASUREMENT PARAMETERS – MEASUREMENT	34
4.1 SETTING GENERAL MEASUREMENT PARAMETERS – GENERAL SETTINGS	34
4.2 SETTING THE MEASUREMENT TRIGGER – MEASUREMENT TRIGGER	36
4.3 SETTING PARAMETERS FOR PROFILES – PROFILES	38
4.4 SETTING ALARM THRESHOLDS FOR DOSE METER – ALARM	39
4.5 CONFIGURING DATA LOGGING – LOGGING	39

4.5.1	<i>Setting general logging parameters – Logger Setup</i>	40
4.5.2	<i>Selecting results for logging – Logger Results</i>	41
4.5.3	<i>Logger trigger settings – Logger Trigger</i>	42
4.5.4	<i>Configuring signal recording – Wave Recording</i>	43
4.6	SELECTING MEASUREMENT RANGE – RANGE.....	46
4.7	SELECTING MICROPHONE COMPENSATION – COMPENSATION FILTER.....	46
4.8	SETTING STATISTICAL LEVELS – STATISTICAL LEVELS.....	47
4.9	PROGRAMMING INSTRUMENT’S INTERNAL TIMER – TIMER	47
4.9.1	<i>Example of timer execution</i>	48
5	CONFIGURING DATA VIEWING – DISPLAY	49
5.1	ENABLING VIEWS – DISPLAY MODES.....	49
5.1.1	<i>One Result view</i>	49
5.1.2	<i>Three profiles view</i>	50
5.1.3	<i>Logger view</i>	51
5.1.4	<i>Statistics view</i>	52
5.1.5	<i>Running SPL view</i>	52
5.1.6	<i>File information view</i>	52
5.2	ADJUSTING PLOT SCALE – DISPLAY SCALE.....	53
5.3	SELECTING MEASUREMENT RESULTS TO BE DISPLAYED – MEASUREMENT RESULTS.....	53
5.4	SELECTING LOGGER RESULTS TO BE DISPLAYED – LOGGER RESULTS.....	54
5.5	CONFIGURING POWER SAVER – SCREEN SETUP.....	54
6	MANAGING FILES – FILE	55
6.1	MANAGING FILES – FILE MANAGER	56
6.1.1	<i>Assigning the directory for saving data files – Working Directory</i>	56
6.1.1	<i>Opening file/directory – Open</i>	57
6.1.2	<i>Renaming file/directory – Rename</i>	57
6.1.3	<i>Viewing information about file/directory – Info</i>	57
6.1.4	<i>Deleting file/directory – Delete</i>	58
6.1.5	<i>Erasing memory – Erase Disk</i>	58
6.2	MANAGING SETUP FILES – SETUP MANAGER	58
7	CONFIGURING INSTRUMENT – INSTRUMENT	59
7.1	CHOOSING USER INTERFACE MODE – USER INTERFACE.....	59
7.2	CHECKING POWER – BATTERY.....	59
7.3	PROGRAMMING KEYBOARD FUNCTIONS – KEYBOARD	60
7.4	AUTOMATIC POWER OFF – POWER OFF.....	60
7.5	CONFIGURING THE USB INTERFACE – USB.....	61
7.6	SETTING INTERFACE PARAMETERS – COMMUNICATION PORTS	61
7.1	CHECKING THE RS232 STATUS – RS232 STATUS	61

7.2	SELF-VIBRATION MARKER – SELF VIBRATION.....	61
7.3	PROGRAMMING THE INTERNAL REAL TIME CLOCK – RTC.....	62
7.4	CHECKING INSTRUMENT PROPERTIES – UNIT LABEL.....	62
8	AUXILIARY SETTINGS – AUXILIARY SETUP	63
8.1	SELECTING THE INTERFACE LANGUAGE – LANGUAGE.....	63
8.2	RESTORING FACTORY SETTINGS – FACTORY SETTINGS	63
8.3	VOICE COMMENTS – COMMENTS.....	64
8.4	DISPLAYING LEQ & LAV RESULTS – LEQ & LAV	64
8.5	ACTIVATING WARNINGS – WARNINGS.....	64
9	PRINTING REPORTS – REPORT	66
9.1	PRINTING MEASUREMENT RESULTS – PRINT.....	66
9.2	SELECTING PRINT OPTIONS – OPTIONS.....	67
9.3	SELECTING RESULTS FOR THE REPORT – RESULTS.....	68
9.4	SELECTING STATISTICS FOR THE REPORT – STATISTICS.....	68
9.5	SELECTING SPECTRA FOR THE REPORT – SPECTRUM	68
9.6	PRINTER SETTINGS – PRINTER	68
10	1/1 AND 1/3 OCTAVE ANALYSER.....	69
10.1	SELECTING 1/1 OCTAVE OR 1/3 OCTAVE FUNCTION.....	69
10.2	1/1 OCTAVE OR 1/3 OCTAVE ANALYSER CONFIGURATION.....	69
10.2.1	<i>General settings for 1/1 and 1/3 octave analysis – General Settings</i>	<i>69</i>
10.2.2	<i>Selecting measurement range for 1/1 and 1/3 octave analysis – Range</i>	<i>69</i>
10.2.3	<i>Logging of the 1/1 and 1/3 octave spectra – Logging.....</i>	<i>70</i>
10.2.4	<i>Setting parameters of the 1/1 and 1/3 octave analysis – Spectrum</i>	<i>70</i>
10.3	CONFIGURING 1/1 AND 1/3 OCTAVE SPECTRA VIEWS.....	71
10.3.1	<i>Presentation of the 1/1 and 1/3 octave spectra.....</i>	<i>71</i>
10.3.2	<i>Adjusting the spectrum plot scale – Display Scale.....</i>	<i>72</i>
10.3.3	<i>Selecting spectra to view – Spectrum View.....</i>	<i>72</i>
11	SOUND EXPOSURE METER – DOSIMETER.....	74
11.1	SELECTING THE DOSIMETER FUNCTION	74
11.2	SETTING GENERAL PARAMETERS – GENERAL SETTINGS.....	74
11.3	SETTING PROFILE PARAMETERS – PROFILE X.....	74
11.4	CHECKING THE MEASUREMENT RANGE – RANGE.....	75
11.5	SETTING THE EXPOSURE TIME – EXPOSURE TIME	75
11.6	SETTING ALARM THRESHOLDS FOR DOSE METER RESULTS – ALARM.....	75
11.7	DISPLAYING DOSIMETER RESULTS	76
11.7.1	<i>Displaying of Leq & Lav results – Leq & Lav</i>	<i>76</i>
12	REVERBERATION TIME MEASUREMENTS – RT60.....	77
12.1	SELECTING THE RT60 FUNCTION	77

12.2	SETTING RT60 PARAMETERS – RT60 SETTINGS	77
12.3	STARTING RT60 MEASUREMENTS.....	79
12.4	VIEWING RT60 RESULTS.....	80
12.5	AVERAGING RT60 RESULTS	80
13	STI CALCULATIONS – STIPA	82
13.1	STI METHOD BACKGROUND	82
13.2	SELECTING THE STIPA FUNCTION	82
13.3	STIPA MEASUREMENT AND CALCULATION PROCESS	83
13.3.1	<i>Measured results</i>	83
13.3.2	<i>Project structure</i>	85
13.3.3	<i>Results averaging</i>	85
13.3.4	<i>STIPA settings</i>	86
13.3.5	<i>Considering ambient noise distortion</i>	88
13.3.6	<i>STIPA measurements</i>	88
13.4	DOWNLOADING FILES AND PROCESSING DATA	91
13.4.1	<i>Measurement with Building Acoustics application</i>	91
13.4.2	<i>Direct measurement with the instrument (without Building Acoustics application)</i>	92
13.4.3	<i>Presentation of STIPA results</i>	94
13.4.4	<i>Changing background noise values</i>	95
13.4.5	<i>Generating reports</i>	95
14	PC SOFTWARE AND SMARTPHONE APPLICATIONS	96
15	MAINTENANCE	97
15.1	REPLACING BATTERIES	97
15.2	EXTRACTING AND INSERTING THE MEMORY CARD.....	97
15.3	REPLACING THE MICROPHONE AND MICROPHONE PREAMPLIFIER.....	97
15.4	RESETTING THE INSTRUMENT	98
15.5	UPGRADING THE FIRMWARE	98
15.6	PRESERVATION OF INTERNAL BATTERIES	99
15.7	TRANSPORTATION AND STORAGE	99
15.8	CLEANING	99
15.9	TROUBLESHOOTING	99
16	GLOSSARY	100
16.1	MODES AND MEASUREMENT FUNCTIONS	100
16.2	CALIBRATION	101
16.3	MEASURED RESULTS	102
16.4	MEASUREMENT PARAMETERS	106
16.5	DISPLAY PARAMETERS	119
16.6	INSTRUMENT PARAMETERS.....	122

16.7	AUXILIARY PARAMETERS	124
16.8	REPORT	125
APPENDIX A. REMOTE CONTROL		127
A.1	INPUT/OUTPUT TRANSMISSION TYPES	127
A.2	FUNCTION #1 – GENERAL CONTROL FUNCTIONS	127
A.3	FUNCTION #2 – MEASUREMENT RESULTS READ-OUT IN THE SLM MODE	129
A.4	FUNCTION #3 – MEASUREMENT RESULTS READ-OUT IN 1/1 AND 1/3 OCTAVE MODES.....	132
A.5	FUNCTION #4 – SETUP FILE READ-OUT	133
A.6	FUNCTION #5 – STATISTICAL ANALYSIS RESULTS READ-OUT.....	134
A.7	FUNCTION #7 – SPECIAL CONTROL FUNCTIONS	135
A.8	FUNCTION #9 – SETUP FILE WRITE-IN	135
A.1	FUNCTION #D – DATA FILES ACCESS	136
A.2	FUNCTION #S – DIRECT SETUP ACCESS	137
A.3	CONTROL SETTING CODES	138
APPENDIX B. DATA FILE STRUCTURES.....		165
B.1	GENERAL STRUCTURE OF THE SV 971A FILES.....	165
B.2	STRUCTURE OF THE FILE CONTAINING RESULTS FROM LOGGER'S FILE	187
	<i>B.2.1. The contents of the files in the logger.....</i>	<i>188</i>
	B.2.1.1. Record with the results	188
	B.2.1.2. Record with the state of the markers	189
	B.2.1.3. Record with the breaks in the results registration	189
	B.2.1.4. Record with the breaks account PAUSE in the results registration.....	189
	B.2.1.5. Record with the wave file name	189
	B.2.1.6. Record with Summary Results	190
	B.2.1.8. Record with name of the comment file	190
	B.2.1.9. Record with GPS data.....	191
B.3	STRUCTURE OF THE SETUP FILE	192
B.4	DATE AND TIME	192
APPENDIX C. TECHNICAL SPECIFICATIONS		193
C.1	SPECIFICATION OF SV 971A AS SOUND LEVEL METER (SLM).....	193
	<i>C.1.1 Specification of SV 971A as SLM in the standard configuration</i>	<i>193</i>
	<i>C.1.2 Effect of the SA 22 windscreen.....</i>	<i>213</i>
	<i>C.1.3 Effect of the SA 271A outdoor microphone kit.....</i>	<i>225</i>
	<i>C.1.4 Effect of Vibration</i>	<i>225</i>
C.2	SPECIFICATION OF SV 971A AS 1/1 OCTAVE AND 1/3 OCTAVE ANALYSER.....	227
	<i>C.2.1 Specification of SV 971A as 1/1 and 1/3 octave analyser in the standard configuration</i>	<i>227</i>
	<i>C.2.2 1/1 and 1/3 octave filters characteristics.....</i>	<i>230</i>
C.3	FREQUENCY CHARACTERISTICS OF THE IMPLEMENTED DIGITAL FILTERS.....	239
C.4	MISCELLANEOUS SPECIFICATION OF SV 971A.....	241

C.5	USING THE SA 271A OUTDOOR MICROPHONE KIT	246
C.6	DECLARATION OF CONFORMITY	269
APPENDIX D.	DEFINITIONS AND FORMULAE OF MEASURED VALUES	270
D.1	BASIC TERMS AND DEFINITIONS	270
D.2	DEFINITIONS AND FORMULAS OF THE SLM RESULT.....	271
D.3	DEFINITIONS AND FORMULAS OF THE ADDITIONAL DOSIMETER FUNCTION RESULTS.....	274
D.4	STATISTICAL LEVELS – LN DEFINITION.....	275
APPENDIX E. REVERBERATION TIME CALCULATIONS.....		277
E.1	INTRODUCTION	277
E.2	DEFINITIONS AND CALCULATION OF THE RT 60 REVERBERATION TIME	278
E.3	DESCRIPTION OF THE DECAY CURVE RECORDING IN DIFFERENT MEASUREMENT METHODS.....	280
APPENDIX F. SA 271A OUTDOOR MICROPHONE KIT ASDOSIMETERBLY GUIDE		283
F.1	PART SET.....	283
F.2	ASSEMBLY OF SA 271A	285
F.3	IMPORTANT NOTES	291

INDEX

1

1/1-octave · 29, 69
1/3-octave · 29, 69

3

3 Profiles view · 50

A

Accessories · 13
Advanced interface · 59
Airport compensation · 47
Alarm · 39, 75
Auto calibration · 32
Automatic file saving · 26
Automatic pauses · 74
Autoscale · 53, 72
Auxiliary settings · 63
Averaged spectrum · 72

B

Battery · 59
Bluetooth · 61

C

Calibration · 29
Calibration by measurement · 30
Calibration drift · 30
Calibration factor · 30
Calibration history · 31, 32
Calibration level · 30
Calibration result · 30
Compensation filter · 46
Complex parameter · 22
Configuration mode · 20
Control keys · 18
Criterion level · 75

D

Day time limits · 35
Decay · 77
Decay method · 79
Default settings · 23

Deleting files · 58
Detector · 75
Display colour · 54
Display mode · 19, 49, 71
Display scale · 53, 72
Display settings · 49
Dosimeter · 29, 74
Dosimeter results · 76

E

Environment compensation · 47
Erasing disk · 58
Exchange rate · 75
Exponential integration · 36
Exposure time · 75

F

Factory settings · 23, 63
File info view · 52
File information · 57
File manager · 26, 56
File name · 78
Files · 55
Filter · 38, 70, 74
Filter Peak · 38, 74
Firmware options · 14
Firmware upgrade · 98
Format wave · 43
Function · 29

G

General settings · 34, 69, 74
Gradient · 45
Gradient threshold · 38
Gradient trigger · 37, 44
Grid · 72

H

Help information · 23

I

Icons · 24
Impulse · 77
Impulse method · 79
Impulse response method · 77

Inactive parameters · 23
Information screen · 23
Input/output · 15, 16
Instantaneous spectrum · 72
Instrument settings · 59
Integration period · 35, 39, 69
Integration period trigger · 44
Interrupted noise method · 77

K

Key lock · 60
Keyboard · 18, 60

L

Language · 63
Last calibration · 31, 32
Leq & Lav display · 64, 76
LEQ integration · 36
Level · 79
Level meter · 29
Level trigger · 37, 42, 44
Linear integration · 36
List of parameters · 22
Logger · 26, 40
Logger name · 41
Logger results · 41, 54, 70
Logger setup · 40
Logger split · 40
Logger step · 40, 70
Logger trigger · 42
Logger view · 51
Logging · 39, 70
Low range · 46

M

Main menu · 21
Manual trigger · 45
Matrix of parameters · 22
Max spectrum · 72
Measurement function · 29, 69, 74, 77, 82
Measurement mode · 19
Measurement settings · 34
Measurement trigger · 36
Measurement view · 19
Memory · 25, 26
Menu position · 21
Min spectrum · 72

N

Noise margin · 78
Normal range · 46

O

One result view · 49
Optional functions · 27

P

Post-calibration · 32
Post-trigger · 42
Power Off · 60
Power saver · 54
Powering · 17
Pre-trigger · 42, 46
Print options · 67
Print results · 66
Printed results · 68
Printed spectrum · 68
Printed statistics · 68
Printer settings · 68
Profiles · 38, 74
PTC threshold level · 75

R

Range · 46, 69, 75
Recording time · 46, 78
Renaming files · 57
Repetition cycles · 35, 39, 69
Report · 66
Resetting · 98
Results presentation · 19
Results view · 49, 71
RMS detector · 38
Rolling Leq · 36
RT averaging · 78
RT frequency range · 78
RT method · 78
RT octave · 78
RT step · 78
RT60 averaging · 80
RT60 settings · 77
RTC · 62
Running LEQ · 29, 77
Running SPL · 19
Running SPL view · 52

S

Screen dim · 54
Screen setup · 54
SD card · 25, 26, 97
Self vibration · 61
Setup manager · 27, 58
Shift key mode · 60
Simple interface · 59
SLM/Dosimeter results · 53
Slope trigger · 36, 43
Sound analyser · 12
Sound level meter · 12

Spectrum · 71
Spectrum settings · 70
Spectrum view · 71
Speech intelligibility · 82
Start delay · 34
Start measurements · 20
Start synchronisation · 35
Start/Stop interface · 59
Statistics view · 52
STI · 82
STIPA · 82
Summary results · 39, 41, 70

T

Text editor · 22
Threshold level · 42, 75
Timer · 47
Total value · 69
Trigger · 42
Trigger source · 38, 42, 45
Trigger step · 45

Troubleshooting · 99
Turn on · 19

U

ULT threshold level · 75
Unit label · 62
USB · 61
User interface · 21, 59

V

Viewed spectra · 72
Voice comments · 64

W

Warnings · 64
Wave recording · 43
Working directory · 56

1 INTRODUCTION

SV 971A is an extremely small Class 1 IEC 61672-1:2013 Sound Level Meter (SLM) with the optional real time 1/1 & 1/3 octave analyser and Sound Exposure Meter (Dosimeter) conforming to international standards ISO 9612 and OSHA (IEC 61252; ANSI S1.25).

The new user interface of this instrument makes measurement configuration as easy as possible. This all makes SV 971A an ideal choice for industrial hygiene noise measurements, short period environmental noise measurements, acoustics consultancy surveys, technical engineers dealing with noise issues and general acoustics noise measurements.

The instrument enables huge time history logging capability providing broad band results and spectra with adjustable double (long and short) logging steps. Audio recording on user selectable trigger conditions complete the logging functionality. Data are stored on a micro-SD memory card and can be easily downloaded to a PC over the USB interface. Optional RS 232 interface can be used for the connection of the instrument with the device that provides this type of connection. Direct printing feature enables quick on-site printing with the use of optional portable printer.

The instrument can be easily calibrated in the field using a sound calibrator. The calibration process can be automatically activated whenever a sound calibrator with the auto run function is installed on the microphone.

SV 971A is supplied with Svantek PC software packages – *Supervisor* for basic data download, visualisation, post-processing and reporting, and *SvanPC++* for advanced data download, visualisation, data post-processing and analysis and reporting.

SV 971A is equipped with a Bluetooth®¹ module and can be remotely controlled via the *Assistant* or *Building Acoustics* smartphone applications.

With a rugged, pocket-sized housing and a low energy, long range Bluetooth® Smart wireless interface, this instrument is an excellent tool for anyone involved in acoustic measurement.



1.1 SV 971A AS SOUND LEVEL METER & ANALYSER

- SLM mode: **Lpeak, Lmax, Lmin, L, Leq, LE, Lden, LEPd, Ltm3, Ltm5, Leq statistics (Ln),** expected Leq value (**EX**), standard Leq deviation (**SD**), measurement time and overload time % (**OVL**) and two rolling Leq (**LR1** and **LR2**) with Class 1 IEC 61672-1:2013 accuracy in the frequency range 5 Hz ÷ 20 kHz
- Dosimeter mode: **Lpeak, Lmax, Lmin, L, Leq, LE, LEPd, Ltm3, Ltm5, Leq statistics (Ln),** expected Leq value (**EX**), standard Leq deviation (**SD**), **Lc-a, DOSE, D_8h, PrDOSE, LAV, SEL8(LAE8), PSEL(PLAE), E, E_8h,** peak counter (**PTC**), peak threshold (**PTP**), upper limit time (**ULT**), **TWA, PrTWA,** measurement time and overload time % (**OVL**) with Class 1 IEC 61672-1:2013 accuracy in the frequency range 5 Hz ÷ 20 kHz

¹ "The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by SVANTEK is under license. Other trademarks and trade names are those of their respective owners.

- Parallel **Impulse**, **Fast** and **Slow** detectors for the measurements with **A**, **B**, **C**, **Z** and **LF** frequency filters
- Two measurement ranges 25 dBA LEQ ÷ 123 dB Peak (**Low**) and 30 dBA LEQ ÷ 140 dB Peak (**High**).
- **1/1 Octave** real-time analysis (option). Eleven 1/1 octave filters with center frequencies from 16.0 Hz to 16 kHz (meeting Class 1 requirements of IEC 61260-1:2014) available simultaneously with three user definable profiles for broadband measurements (SLM and Dosimeter), time history logging and audio recording
- **1/3 Octave** real-time analysis (option). Thirty-five 1/3 octave filters with center frequencies from 8 Hz to 20 kHz (meeting Class 1 requirements of IEC 61260-1:2014) available simultaneously with three user definable profiles for broadband measurements (SLM and Dosimeter), time history logging and audio recording
- **Audio signal** recording (option), trigger and continuous mode, 12 kHz and 24 kHz sampling rate, WAV format
- Reverberation time **RT60** analysis function (option) for 1/1 octave bands or 1/3 octave bands and three total RMS levels (**A**, **C** and **Z** weighted) in accordance with the ISO 3382 standard.
- **STIPA** (speech transmission index for public address systems) measurements of electro-acoustic and acoustic environments effects that affect the speech intelligibility in the room acoustics and/or public address systems.

1.2 GENERAL FEATURES OF SV 971A

- Sound Level Meter in extremely small pocket size body
- Noise measurements meeting Class 1 IEC 61672-1:2013 accuracy
- Two overlapping wide measurement ranges
- 1/1 & 1/3 octave real-time frequency analysis (option)
- Dosimeter function for personal noise monitoring in the workplace (option)
- Audio signal recording (option)
- Reverberation time function (option)
- Speech transmission index function (option)
- Audio records on demand, created before or after measurement, added to a measurement file
- Statistical analysis with up to 10 percentile values
- Time-history with two logging step intervals
- Automated calibration start and save
- Free-field & diffuse-field measurements
- Integration measurement run time programmable up to 24 h
- Wireless connectivity with low energy Long Range Bluetooth® Smart (5.2) interface
- Setup editor available with *Supervisor* or *SvanPC++* software
- Super contrast colour OLED display
- Bluetooth® for remote control by the *Assistant* smartphone applications
- Wide range of temperature operating conditions
- Very handy, light weight and robust pocket size case
- Easy and friendly user interface for quick start and stop

1.3 ACCESSORIES INCLUDED

- | | |
|--------------------|--|
| • ACO 7152 | prepolarised ½" condenser microphone with nominal sensitivity 32 mV/Pa |
| • SV 18A | microphone preamplifier |
| • SC 158 | USB type C to USB type A cable |
| • SA 22 | foam windscreen |
| • batteries | four AAA type |

1.4 ACCESSORIES AVAILABLE

- **SV 36** Class 1 sound calibrator: 94/114 dB @ 1000 Hz
- **SP 75** RS232 interface option with external power supply plug
- **SC 91A** extension cable for the SV 18A preamplifier and SV 971A
- **SA 72** carrying case for SV 971A and accessories (waterproof)
- **SA 80** pocket soft bag
- **SA 271A** outdoor microphone kit
- **SA 270D** desiccator for the SA 271A outdoor microphone kit



Note: SV 971A is compatible only with the SC 91A cable!

1.5 FIRMWARE AND SOFTWARE OPTIONS AVAILABLE

- **SF 971A_P1** Package: SF 971A_1 and SF 971A_3
- **SF 971A_P2** Package: SF 971A_5, SF 971A_20, SvanPC++_BA
- **SF 971A_P3** Package: P1 and P2 packages
- **SF 971A_1** 1/1 octave analysis option
- **SF 971A_3** 1/3 octave analysis option
- **SF 971A_5** Reverberation time analysis (RT60) option including SvanPC++_BA
- **SF 971A_10** Noise dosimetry option
- **SF 971A_15** Audio events recording option
- **SF 971A_20** STIPA option
- **SvanPC++_BA** Building acoustics option for *SvanPC++*
- **SvanPC++_EM** Environmental monitoring module for *SvanPC++* (hardware key, single license)



Note: The firmware and software options listed above can be purchased at any time, as only the entry of a special unlock code is required for their activation.

2 GENERAL INFORMATION

2.1 MEASUREMENT CONFIGURATIONS

The normal mode of operation of the instrument as an SLM is with the microphone attached to the instrument and without the windscreen. Optionally the instrument can be operated with the windscreen attached to the microphone or with the preamplifier and microphone fitted in the outdoor microphone kit and connected with the instrument by the extension cable (see Appendix C for specification).



During sound measurements, to meet the requirements of the Class 1 accuracy, it is recommended to install the instrument on a tripod or in a holder to minimize the possibility of reflection and diffraction of acoustic waves. In particular, the instrument must not be held close to the body of the person performing the measurement. The instrument should be directed so that the microphone diaphragm plane is perpendicular to the direction of the measured sound source (the incidence angle of the sound wave is 0 degree). To control the instrument and readout results, it is recommended to use the *Assistant* smartphone application.

If there are significant differences between the temperature of the instrument and the ambient temperature at the measuring point, it is recommended that the instrument be acclimatised for a sufficient period of time to bring its temperature as close as possible to the ambient temperature.

When taking measurements in the presence of wind, it is necessary to use a windscreen. The windscreen should simply be placed over the microphone with the preamplifier without any significant force.

For measurements according to IEC 61672-1:2013 it is necessary to set the appropriate compensation filter in the **Compensation Filter** menu (see Chapter 4.7).

When measuring in a diffusion field (in small rooms), it is recommended to switch on the diffuse field filter.

Chapter [15.3](#) presents the way the microphone should be attached to the preamplifier and the preamplifier to the instrument.

Before starting measurements, the instrument should be calibrated using the recommended sound calibrator (see Chapter [3.2](#)).



2.2 SOUND MEASUREMENTS IN SPECIAL CONDITIONS

While measuring a low-level acoustic pressure, the instrument should be placed on a tripod and the person measuring should be at least 1 meter from the microphone and do not touch the instrument. To control the instrument and readout results, it is recommended to use the *Assistant* smartphone application!

At locations where the static (ambient) pressure is from 65 kPa up to, but not including, 85 kPa, before the measurement, the device must be calibrated with a Class 1 calibrator (e.g., SV 36).

2.3 INPUT AND OUTPUT SOCKETS OF THE INSTRUMENT

Top cover of the instrument

The measurement **Input** is placed in the centre of the instrument's top cover. The **SV 18A** microphone preamplifier has a specially designed matching plug with a locking screw to secure the preamplifier to the meter body. After plugging in the preamplifier to the measurement input, the screw should be tightened to light resistance only. Do not over tighten this connector. It is not necessary to remove this preamplifier from the top of the instrument unless the meter is in a calibration laboratory as it is always used close coupled to the meter body. The full description of the signals connected to the sockets is given in Appendix C.



Bottom cover of the instrument

In the bottom cover, there is only one socket – **USB** (C type).



The **USB 2.0** interface is the serial interface working with 12 MHz clock in the full speed mode and with 480 MHz in the high-speed mode, which is a default mode of the instrument. The USB-C socket is described in detail in Appendix C.



Note: Switch the power off before connecting the instrument to any other device (e.g. a printer or a Personal Computer) or fitting the microphone capsule.

There is a memory micro-SD card slot under the bottom cover of the instrument and spaces for the 4 x AAA batteries.

You can access the card and batteries by unscrewing the coin slot screw and removing the bottom cover – see Chapter [15.1](#).



Note: The originally supplied Kingston Industrial memory card has been tested by SVANTEK and cards of this type are strongly recommended for use when the original card is going to be replaced.

2.4 INSTRUMENT POWER

SV 971A can be powered from one of the following sources:

- Four AAA standard size batteries fitted internally. In the case of alkaline type, a new fully charged set can operate more than 12 h (6.0 V / 1.6 Ah). Instead of the ordinary alkaline cells, four AAA rechargeable batteries can be used (a separate external charger is required for charging them). In this case, using the best NiMH type, the operation time can be increased up to 16 h (4.8 V / 2.6 Ah)
- **USB** interface – 100 mA HUB.

When the instrument is powered from internal batteries, the “**battery**” icon is displayed on the top line of the display.

The battery status can be checked on the **Battery** screen. It is also continuously indicated on the top line of the display by the number of bars in the “**battery**” icon.

If the voltage of the batteries is too low for reliable measurements, the icon will be red and when you try to switch on the instrument, the message **Low Battery!** Will appear on the display for 2 seconds and the instrument will switch off automatically.

To power the instrument from the USB-C interface, connect its **USB** port to a PC or other USB power source using the SC 158 cable.

When the USB power is connected, the instrument automatically switches from the internal battery power to the USB power. When the USB power is disconnected, the instrument automatically switches to internal battery power.



Note: When the instrument is powered via USB, the internal batteries will discharge slightly. Be aware of this effect and remove the battery if you do not want it to discharge.



Note: Only use high quality USB-C cables, such as SC 158. Many inferior cables do not ensure low resistance of the cable and thus prevent proper operation of the instrument.

When powered from the USB-C source, the “**USB**” or “**plug**” icon is displayed at the top of the display and the **Battery** screen displays the source voltage.



Note: If the “**battery**” icon is red, it is strongly recommended to use the USB-C power as soon as possible to ensure reliable operation. If no suitable external power source is available, the instrument will automatically switch off after a short time!

Prolonging the internal power source of the instrument can be achieved by using the LCD screen **Dim Mode**. You can configure the power saving function (**Dim Mode**) in the **Screen Set.** screen (path: *<Menu> / Display / Screen Set.*).

2.5 CONTROL PANEL

The instrument is controlled in a fully interactive way using the control keys and the configuration menu.

The following control keys are located on the front panel of the instrument:

- **<ESC>**, (**<P/S>**)
- **<Enter>**, (**<Menu>**)
- **▲**, **◀**, **▶**, **▼**
- **<Shift>**
- **<Start/Stop>**

The action given in (...) brackets denotes the second key function which is available after pressing it in conjunction (or in sequence) with the **<Shift>** key.



<Shift> The second function of a key (**<P/S>**, **<Menu>**) can be used when the **<Shift>** key is pressed with **<Enter>**, **<ESC>** or some other keys. This key can be used in two different modes, which can be configured in the **Keyboard** list (path: *<Menu> / Instrument / Keyboard*):

- as on a computer keyboard, when both **<Shift>** and the second key must be pressed simultaneously (**Direct** mode);
- as on a smartphone keyboard, when the first **<Shift>** key should be pressed and released and then the second key pressed (**2nd Function** mode).



Note: Pressing **<Alt>** and **<Start/Stop>** at the same time switches the instrument on or off.

<Start/Stop> This key starts or stops the measurement.

<Enter> This key opens the selected item in the menu and confirms the selected settings. In the Measurement mode, it switches between sub-views. Some additional functions of this key will be described in the following chapters of this manual.

<ESC> This key is used to exit parameter list without saving changes, menu lists or other screens and return to the top screen. It has the opposite effect to the **<ENTER>** key. In Measurement mode, it switches between the views.

◀ / ▶ These keys allow you in particular to:

- change viewed result in Measurement mode,
- select the column in a multi-column parameter list,
- select the parameter value in an active item (e.g., filter **Z**, **A**, **C** etc., **Start Delay** period: **1s**, **2s**, **3s**, ... etc.). In the case of numerical values, it speeds up selecting by pressing and holding,
- control cursor in graph views (Logger, Spectrum etc.),
- select position of a character in the text editor screen.

(◀ / ▶) These **◀ / ▶** keys, used in conjunction with **<Shift>**, allow you in particular to:

- select parameter value in an active item (e.g., filter **Z**, **A**, **C**; integration period: **1s**, **2s**, **3s**, ... etc.),
- move the cursor from the first to the last position on the graph and back again.

▲ / ▼ These keys allow you in particular to:

- select item in the list,

- select character in the text editor screen,
 - change profile in Measurement mode.
- (▲ / ▼) These ▲ / ▼ keys used in conjunction with <Shift> allow you, in particular, to:
- change view in Measurement mode,
 - change relationship between Y-axis and X-axis in the Logger and Spectrum views,
 - program the Real Time Clock (RTC) and delayed run **Timer**.
- (<Menu>) This key (<Shift> + <Enter>) opens the main **Menu** in Configuration mode. Double pressing the <Menu> key opens the list of recently opened configuration screens. This provides quick access to frequently used configuration screens for easy navigation.
- (<P/S>) This key (<Shift> + <ESC>) allows you to pause or break the measurement process temporarily. If there is no current running measurement in progress this key opens the Setup Manager menu.
- <REC> Pressing the ◀ and ▶ keys simultaneous starts the recording of a voice comment (see Chapter 8.3).

2.6 WORKING WITH THE INSTRUMENT

The instrument is controlled by nine keys on the keypad. These keys allow access to all the available functions and change the value of all the available parameters.

The instrument is equipped with a high contrast OLED colour display (96 x 96 pixels), which displays the measurement results and the configuration menu.

The instrument has two operating modes: Measurement mode with result preview and Configuration mode using the Menu functionality.

Switching on the instrument

To switch on the instrument, press the <Shift> and <Start/Stop> keys simultaneously. The instrument will perform the self-test routine on power-up (displaying the manufacturer's logo) and enter the Running SPL view, if it was enabled, otherwise enter the One Profile view.




2.6.1 Measurement mode

The measurement results can be displayed in several views, depending on the selected **Measurement Function**. You can switch between views by pressing the <ESC> key or by pressing the ▲ / ▼ keys together with <Shift>.

Measurement views



In the measurement views, the readings are displayed as well as additional information using icons relating to:

- instrument status: memory, power, real time, etc.,
- measurement status: measurement elapsed time, measurement start/stop/pause, trigger, logger, etc.,
- measurement parameters: measured result, channel number, file name, filter, etc.



Some views are always available, others can be activated or deactivated in Configuration mode.

Some views display numerical and some graphical results, as in the example on the right: time history plot and spectrum.




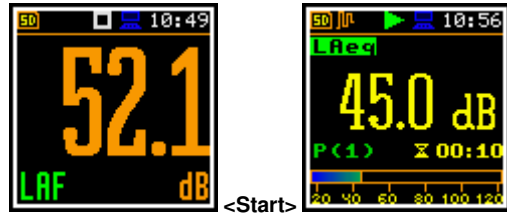
In some views you can switch between sub-views by pressing the **<Enter>** key.







All icons are described in Chapter 2.8, other fields and view control functions are described in Chapter 5.

Starting a measurement


To start a measurement, press the **<Start>** key. The flashing  icon will appear, and the measurement will be taken using the current settings, stored in the instrument's internal memory.




The time elapsed since the start of the measurement (elapsed time) is displayed in the lower right corner of the measurement screen in the format  **mm:ss** in the range from 00:00 to 59:59, or in the format  **hh:mm:ss** in the range from 01:00:00 to 99:59:59, or in the format  **xxxh** from 100h to 999h, and  **>999h** if the elapsed time exceeds 999 hours. Its maximum value is equal to the **Integration Period** and the elapsed time is reset to zero at the start of a new measurement cycle (see Chapter 4.1).



Pausing a measurement

To pause a measurement, press the **<Shift>** and **<ESC>** key together. The measurement will be paused and the  icon will appear along with the **Pause** screen.




In Pause mode, the  key can be used to erase up to 30 last seconds of the measurement. Each press deletes one second of the measurement, reducing the elapsed time.

This can be useful if, for example, the measurement is temporarily disturbed by an event that should not normally occur.

To continue the measurement, press **<Enter>**.

Stopping a measurement

To stop a measurement, press the **<Stop>** key. The  icon will appear.



2.6.2 Configuration mode

To configure a measurement or the instrument, use the Menu mode, which is entered using the **<Menu>** key. The menu consists of different types of screens, including main menu, submenu, lists of options, lists of parameters, text editor screens, information screens etc.

User interface options

There are three user interface options that determine the level of functionality available: **Start/Stop**, **Simple** or **Advanced**. These options can be selected from the **User Inter.** screen of the **Instrument** section. The **Simple** option allows basic instrument settings to be made, while the **Advanced** option allows the full range of settings to be made. Many screens can therefore have a different appearance depending on the selected option.

The **Start/Stop** option limits the menu to only one **User Interface** item in the main menu and measurement screens.



Note: For parameters that are hidden in the **Simple** interface, the instrument will use settings previously defined in the **Advanced** interface or default settings.

If the **Simple** interface is selected after **Advanced**, the instrument proposes to restore the default settings by asking the following question: **Do you restore the default value of the advanced settings?** If **No** is selected, all the parameters hidden in the **Simple** interface will have the settings defined in the **Advanced** interface. If **Yes** is selected, the instrument resets all the hidden parameters to their default values.



Note: Most of the screens in this manual are shown in the **Advanced** interface.

Main Menu

The main **Menu** contains six sections (submenu), grouping configuration settings: **Function**, **Measurement**, **Display**, **File**, **Instrument**, **Auxiliary Setup** and **Report**.

The main **Menu** is accessed by pressing the **<Menu>** key (**<Shift>** + **<Enter>**).

Recent Items list






A double press on the **<Menu>** key opens the list of recently used menu items. This provides quick access to the most frequently used lists of parameters and options, without having to scroll through the entire menu.

Selecting an item

Use the **▲ / ▼** key to select the desired item in the **Menu** list.

Entering an item

Press the **<Enter>** key to enter the desired item after selecting it from the menu list. This will display a new sub-menu, option list, parameter list or information screen.

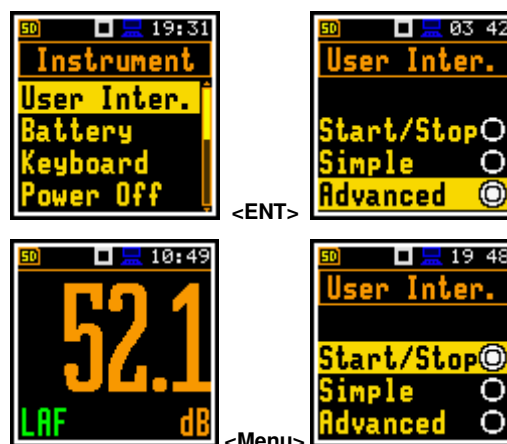

List of parameters

The list of parameters contains parameters whose value is selected from the available range or set.

- Use the ▲ / ▼ key to select the desired item in a list.
- Use the ◀ / ▶ key to change the value in of the selected item.
- Use the <Enter> key to save all changes made to the parameter list.



If the parameter has a numerical value, you can speed up the selection by pressing the ◀ or ▶ key for more than 2 seconds. The parameter will change automatically until you release the keys.

The numerical parameter value can be changed by a larger increment (10 or 20) by pressing the ◀ / ▶ key together with <Shift>.

Matrix of parameters


When a list of parameters consists of more than one column you may change:

- column with the ◀ / ▶ key
- line with the ▲ / ▼ key
- value in a selected position with the ◀ / ▶ key pressed with <Shift>
- all values in a line with the ▲ / ▼ key pressed with <Shift>
- all values in a column, if the cursor is on one of Profile positions, with the ◀ / ▶ key pressed with <Shift>
- all values in a matrix, if the cursor is on one of Profile positions, with the ▲ / ▼ key pressed with <Shift>.




List of options

The list of options consists of several items, only one of which can be selected. To select an option, proceed as follows. Highlight the required option using the ▲ / ▼ key, then press <Enter>. This option will become active, and the list will close. If you re-enter the list, the last option selected will be highlighted.



Complex parameters

For complex parameters consisting of more than one value item, such as **RTC**, first select the item with the ◀ / ▶ / ▲ / ▼ keys and then change the value with the ◀ / ▶ key pressed with <Shift>.



In all cases, the <Enter> key is used to confirm changes and to close the opened list of parameters. In most cases the <ESC> key closes the parameter list, ignoring any changes.

Text editor screen

The text editor screens allow you to edit lines of characters (file names, directory name, etc.) The text editor screen is opened with the ◀ / ▶ key when the item with the text parameter is selected. These screens provide help information on how to edit text.



- Use the ◀ / ▶ key to select the character in the edited text.
- Use the ▲ / ▼ key to select the ASCII character. The following digits, capital letters, underscore and space appear on the display in reverse after each time the above keys are pressed.
- Use the ◀ / ▶ key pressed together with <Shift> to insert or delete the character in the edited text.

Information screen

Some screens provide information about the status of the instrument, available memory, standards met by the instrument, etc.

Use the ▲ / ▼ keys to scroll through the screen.

To close such a screen, press <Enter> or <ESC>.

Help information



In most of the screens, the last line or several lines contain help information. It tells the user how to select or change the value of the parameter, change the character in the text line, etc.

For example, **Delete: Shift <** means that you can delete the selected item by pressing the ◀ key with <Shift>.

Inactive parameters

If some functions or parameters are not available, the menu items associated with that function will be inactive (their colour changes to grey).

For example, if **Logger** (path: <Menu> / Measurement / Logging / Logger Set.) is switched off, some other **Logging** items will be inactive!



2.7 DEFAULT SETTINGS

Factory settings

The instrument is supplied with default settings, which you can change, but always return to them using the **Factory Settings** function in the **Auxiliary Setup** section.

The following chapters of the manual describe in detail what each parameter means and how to change the instrument's settings.

Main default settings

By default, the instrument has the **Simple** interface and is configured as a Sound Level Meter (**Measurement Function: Level Meter**) to measure sound pressure level using three virtual meters, called profiles, with a 1 second delay from the <Start> key press (**Start Delay: 1 s**), infinite integration time (**Integration Period: Inf**), and linear Leq integration (**LEQ Integration: Linear**).


Sound pressure is measured with free field compensation for microphone noise and case effect in the free field (**Microphone: On**, **Field Comp.: Free Field**, **Windscreen: On**), active logging of the selected results (**Lpeak**, **Lmax**, **Lmin** and **Leq**) with 1 second step for all profiles and summary results saving.

Other functions such as measurement trigger, logger trigger, event recording and timer are disabled.


The logger and summary results are automatically saved to the file with the name specified in the **Logger Setup** screen (**Logger Name: Lxxxx**). The logger results are logged with 1 second step (**Logger Step: 1s**). Logger splitting is **Off**.

Default profile settings:

Profile 1 - **C** weighting filter for Peak results (**Filt.Peak(1)=C**), **A** weighting filter for other results (**Filter(1)=A**), **Fast** for the LEQ detector (**Detector(1)=Fast**);



- Profile 2** - **C** weighting filter for Peak results (**Filt.Peak(2)=C**), **C** weighting filter for other results (**Filter(2)=C**), **Fast** for the LEQ detector (**Detector(2)=Fast**);
- Profile 3** - **Z** weighting filter for Peak results (**Filt.Peak(3)=Z**), **Z** weighting filter for other results (**Filter(3)=Z**), **Fast** for the LEQ detector (**Detector(3)=Fast**);




You can change all the above settings using the **Profiles** item in the **Measurement** section. The instrument remembers all changes until the next time it is used. You can return to the default settings (set by the manufacturer) using the use of the **Factory Set.** item in the **Aux. Setup** section.

2.8 DESCRIPTION OF ICONS

Instrument status Indicators












Additional information on the status of the instrument is provided by the row of icons on the top line of the display.

The real time clock (RTC) is also displayed on the same line together with icons.



Meanings of icons are as follows:


<p>The „measurement” icon is displayed when the measurement is in progress and the icon shape changes from self to contoured.</p>	<p>The “SD card” icon is displayed when the SD card memory is in use and there is free space. The grey colour of the icon indicates that the card memory is full.</p>
<p>The “waiting” icon is displayed when the instrument is waiting for the measurement to start after the <Start> key has been pressed, due to a start delay or a delay caused by a trigger.</p>	<p>The “no card” icon is displayed when the SD memory card is not inserted.</p>
<p>The “stop” icon is displayed when the measurement is stopped.</p>	<p>The “pause” icon is displayed when the measurement is paused.</p>
<p>The “overload” icon is displayed if an overload was registered during the measurement.</p>	<p>The “underrange” icon is displayed if an underrange was registered during the measurement.</p>
<p>The “logger” icon is displayed when the current measurement results are being logged to the logger file.</p>	<p>“signal” icon is displayed during wave recording.</p>
<p>The grey colour of the icon indicates that the instrument is waiting for logging to start after the <Start> key is pressed, due to a start delay or a delay caused by a trigger.</p>	<p>Grey colour of the icon means that the instrument waits for the wave recording start after pressing <Start> key due to a start delay or a delay caused by a trigger.</p>
<p>The “battery” icon is displayed when the instrument is powered from the internal batteries. The colour of the icon corresponds to the state of charge of the batteries (green - 30÷100%, yellow – 10÷30%, red – less than 10%).</p>	<p>The “clock” icon is displayed when the timer is On. It is active when the instrument is waiting for the start of the measurement. When it is about to start, the icon turns green and starts flashing.</p>

	The “ level+ ” icon is displayed when the “ Level+ ” trigger is waiting for a condition to be met. The icon will alternate with the „wait”, “logger” or “wave” icons.		The “ level- ” icon is displayed when the “ Level- ” trigger is waiting for a condition to be met. The icon will alternate with the „play”, “logger” or “wave” icons.
	The “ slope- ” icon is displayed when the “ Slope- ” trigger is waiting for a condition to be met. The icon will alternate with the “wave” icons.		The “ slope+ ” icon is displayed when the “ Slope+ ” trigger is waiting for a condition to be met. The icon will alternate with the “wave” icons.
	The “ trigger ” icon is displayed when trigger other than Level or Slope is waiting for a condition to be met. The icon will alternate with the “play”, “logger” or “wave” icons.		The “ Bluetooth ” icon is displayed when <i>Bluetooth</i> ® is switched on. The color of the icon indicates the status state of the connection: green – connected, grey – disconnected.
	The “ RS232 ” icon is displayed when the RS232 port is active.		The “ plug ” icon is displayed when the instrument is powered from the USB-C port without using the USB interface.
	The “ USB ” icon is displayed when there is USB connection with a PC.		The “ shift ” icon is displayed when the <Shift> key is pressed.
	The “ vibration ” icon is displayed when high self-vibration level is registered.		

2.9 OVERLOAD AND UNDERRANGE DETECTION

Overload detectors

The instrument has built-in overload detectors. Overload conditions of both the A/D converter and the input amplifier are detected. Overload in the measuring channel (in its analogue part) and overload of the analogue/digital converter are both detected. The “overload” indication appears when the input signal amplitude is 0.5 dB above the declared “Peak measurement range”. This condition is checked once per second or with the logger step if it is less than 1 second.


An overload is indicated by the flashing  icon displayed from the time the overload is detected until the end of the integration period. If the overload disappears by the end of the integration period, the overload icon will not be displayed from the start of the next measurement cycle.

When an overload is detected, the special marker is recorded to the logger file with the data logging step.

The overload time is measured by the **OVL** result during the integration period and saved in the logger file as part of Summary Results.

Underrange detector

The instrument has a built-in underrange detector. The “underrange” indication appears when the RMS value for the elapsed time is below the lower linear operating range. This condition is checked once per second.

An underrange is indicated by the flashing  icon displayed during the underrange detection period. If an underrange is detected up to the integration period, the special marker will be recorded to the logger file with the Integration Period step. If the signal level increases during the integration period and the total RMS is greater than the minimum, the icon will disappear and the underrange marker will not be recorded.

2.10 SAVING DATA

The instrument creates files of the next types:

- Logger files containing measurement results (extension **.SVL**)
- Wave files containing signal waveform (extension **.WAV**)
- Setup files containing measurement and instrument configuration (extension **.SVT**)

A detailed description of the structures of all file types is given in Appendix B.

Memory type

All files are stored in the instrument's memory in the predefined or assigned directories. Setup files are stored in the predefined directory **SETUP**. The non predefined directories can be changed by the user or renamed.



- SD card is inserted



- no SD card


The **SD Card** memory is activated automatically after insertion of the card. The presence of the SD card is indicated by the icon with SD letters at the top left-hand corner of the display.

File Manager

File Manager is used to check the contents of memory and perform operations on files and directories such as renaming, deleting, viewing information and creating new directories.

The **SD Card** memory is organised as a standard memory with directories and subdirectories (FAT32 file system). It is possible to create or delete directories.

The contents of the memory can be checked using the **File Manager** item in the **File** section.

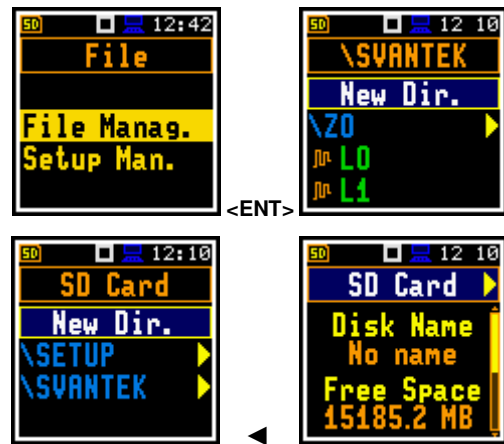

Automatic saving of logger and wave files

Logger and wave files are created and saved automatically. To enable automatic saving, the following conditions should be met:

1. SD card should be inserted and there should be enough free space on it.
2. The **Logger** (path: <Menu> / Measurement / Logging / Logger Set.) and/or **Recording** (path: <Menu> / Measurement / Logging / Wave Rec.) should be enabled.
3. The new file(s) should be given a unique name (path: <Menu> / Measurement / Logging / Logger Set. / Logger Name and path: <Menu> / Measurement / Logging / Wave Rec. / File Name).



Files are saved in the directory, which was set as a working directory. The default working directory (after using **Factory Settings** function) is called **SVANTEK**.



Note: The "logger" icon is displayed during the measurement run with data logging to the logger file. If the signal is recorded to the wave file, the "signal" icon is displayed.

The file name (Logger or Wave) is automatically generated using a pattern **LLdd**, where **LL** is the string of letters (called the prefix) and **dd** is a string of digits forming a number. Up to 8 characters can be used to name a file.

The default prefix is **L** for the logger files and **R** for the wave files.

The instrument assigns an individual counter to each prefix of files created by the user and saved in the working directory. The counter value is equal to the maximum number in the set of files with the same prefix. For example, if there are files named **L0**, **L15** and **L16**, the counter will be 16.

The number of the new automatically created file will increase the value of the counter by one. So, in the example above, the new file name will be **L17**.

You can change the automatically generated file name in the special screen that appears after pressing the ◀ / ▶ key.

If you change the number in the file name without changing the prefix and press <Enter>, the counter will be automatically adjusted.

The instrument will only accept the name whose number is greater than the prefix counter.

You can change the automatically proposed prefix. In this case the instrument will assign the new counter to the new prefix.



<ENT>



<Sh/ESC>

Saving Setup files

Setup files can be created using the **Setup Manager** or from the measurement screen by pressing <ESC> with <Shift> when a measurement is not in progress.

All Setup files are stored in the default **SETUP** directory.

2.11 DOWNLOADING AND UPLOADING FILES

Svantek provides the dedicated software that enables uploading and downloading as well as additional control and post-processing functions: *SvanPC++* and *Supervisor* software for PCs or *Assistant Pro* application for mobile devices



Note: Working with *SvanPC++* and *Supervisor* software is described in detail in “*SvanPC++ User Manual*” and “*Supervisor User Manual*”.

2.12 ACTIVATING OPTIONAL FUNCTIONS

The standard instrument firmware contains all the basic functions to perform measurements according to most international standards and methods. For more complex tasks, additional functions can be added to the instrument. These functions include 1/1 and 1/3 octave analyser, waveform recording, reverberation time and STIPA measurement.

If additional functions are not included in the instrument kit and have not been enabled by the supplier, such a task is the responsibility of the user who decides to purchase additional functions at a later date.

The optional function is activated the first time you try to use it. For example, if **1/1 Octave** was locked, but is later purchased, the first time you try to switch it on, the instrument will require you to enter the special code that unlocks this option. Once unlocked, the option is permanently available.

You can check and lock options that were previously unlocked in the special **Active Functions** and **Active Options** screen that opens when you press the **<Shift>** and **◀** keys immediately after switching on the instrument. You should hold keys down for the first half of the system initialisation until the **Active Fun.** screen opens. To access the **Active Opt.** screen, press the **<Enter>** key.



3 MEASUREMENT FUNCTIONS AND CALIBRATION – Function

The **Function** section allows you to select the measurement function (**Meas. Funct**) and to calibrate or check the instrument (**Calibration**).




3.1 ACTIVATING MEASUREMENT FUNCTIONS – MEASUREMENT FUNCTION

The main function of the instrument is to measure the broadband sound pressure level (**Lev. Met.**). The Sound Level Meter (SLM) function meets the IEC 61672-1:2013 standard for Class 1 accuracy. The instrument can also be used for medium to long term acoustic monitoring using the high capacity data logger which can store all measurement results.

You can also use the 1/1 and 1/3 octave band real-time analysis (**1/1 Oct.**, **1/3 Oct.**) and dosimeter (**Dosimeter**) options. These options extend the main Level Meter functionality of the instrument, by performing the 1/1 or 1/3 octave analysis and dose meter measurements are performed along with all calculations of the broadband Level Meter results (**1/1.&Dose** and **1/3.&Dose** functions provide 1/1 and 1/3 octave analysis along with dose calculations).

To activate a function, open the **Meas. Funct** list and select the required function: **Lev. Met.**, **1/1 Oct.**, **1/3 Oct.**, **Dosimeter**, **1/1.&Dose**, **1/3.&Dose**, **RT60** or **STIPA**.

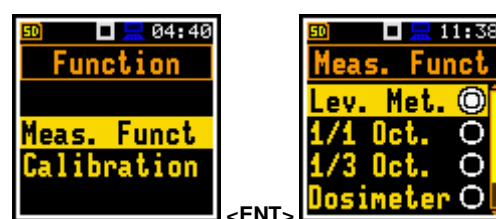

Note: The type of measurement function is not displayed on the screen, so the user should remember the currently selected function!



Note: The **1/1 Octave**, **1/3 Octave**, **Dosimeter**, **RT60** and **STIPA** functions are optional and should be unlocked by entering an activation code in the text editor screen that opens after the first attempt to select them. Once unlocked, these functions are permanently available.

The optional functions can be included with the instrument as supplied or purchased at a later date if required.



Note: It is not possible to change the measurement function during a measurement. In this case, the instrument displays the text: **“Measurement in Progress”**. To change the function of the instrument, the current measurement must be stopped!

3.2 CALIBRATION OF THE INSTRUMENT – CALIBRATION

The instrument is factory calibrated with the supplied microphone for the reference environmental conditions (see Appendix C). The sensitivity of the microphone is a function of the temperature, ambient pressure and humidity, and if the absolute value of the sound pressure is required, the absolute calibration of the measurement channel should be performed. To select the calibration function, open the **Calibration** menu.

The automatic calibration option allows the instrument to perform the sound calibration automatically when the calibrator is placed over the microphone (switched on or with the auto run function). The calibration signal is automatically detected, and the calibration measurement is automatically started. Simply press **<Enter>** to accept the calibration results. No measurement can be made while automatic calibration is in progress.





Note: SV 971A has two dynamic ranges – **Normal** and **Low**. In the SLM functions (**Level Meter**, **1/1 Octave**, **1/3 Octave**, **RT60** and **STIPA**) both ranges can be used for measurement, but in the Dosimeter functions (**Dosimeter**, **1/1.&Dose**, **1/3.&Dose**) only **Normal** can be used (see Chapter 4.6 and 11.4). For calibration, it does not matter which function and which range is selected.

In the **Simple** user interface, the **Calibration** list includes items that allow you to calibrate the instrument using the sound calibrator (**By Measurement**), review and clear previous calibration records (**Last Calibration**, **Calibration History**, **Clear History**), add current calibration results to the logger file (**Post Calibration**).



<ENT>



In the **Advanced** user interface, there is an additional item in the **Calibration** list (**Auto Calibration**), which allows you to enable the auto calibration function.



Note: It is recommended to calibrate the instrument each time before starting measurements. A single calibration at the beginning of each day is usually sufficient for most regulations.



Note: The calibration factor is always added to the measurement results and range limits of all measurement functions.



Note: The recommended factory calibration interval is 12 months to ensure continued accuracy and compliance with international regulations. Please contact your local Svantek representative for further details.



Note: It is possible to perform a “By Sensitivity” calibration by setting the calibration factor using a special command, see Appendix A.




Note: To check or calibrate the instrument, the current measurement must be stopped.

3.2.1 Calibration – By Measurement

To calibrate the instrument:

1. Set the calibration level (**Cal. Level**) – see Appendix C, Chapter C.1, par. Calibration.
2. Carefully place the sound calibrator (SV 36 or equivalent 94/114 dB @ 1000 Hz) over the microphone of the instrument.




Note: It is also possible to use an electromechanical pistonphone, which generates a signal (ca 124 dB), or another type of sound calibrator designed for ½” microphones.

3. Switch on the calibrator (if the used calibrator you are using doesn't have an auto run function) and wait about 30 seconds for the tone to stabilise before starting the calibration measurement.
4. Start the calibration measurement by pressing the <Enter> or <Start> key.


The calibration delay time is set to 3 seconds. While waiting for the measurement to start, the **Delay** will count down on the display.



During the calibration measurement, the level of the measured calibration signal is displayed. If the maximum difference between three consecutive 1-second L_{Ceq} results is less than **0.05 dB**, the calibration measurement is stopped, and the calibration factor will be calculated. The measurement can be stopped at any time by pressing the **<Stop>** key.



After stopping the calibration measurement, the **Calibration drift** (change in the calibration factor since last calibration, calculated in dB) is displayed and it is proposed to save the new calibration factor by pressing **<Enter>** or to reject it by pressing **<Esc>**. In both cases the instrument will exit the **Calibration** screen.



It is recommended to repeat the calibration measurements several times. The results obtained should be almost the same (with a difference of ± 0.1 dB). The reasons for unstable results are as follows:

- the calibrator is not properly attached to the instrument,
- there are external acoustic disturbances such as high noise levels nearby,
- damage to the calibrator or measurement channel (microphone, preamplifier or instrument itself).



Note: During the calibration measurement, external interference (acoustic noise or vibrations) should not exceed a value of 100 dB (when using a calibrator that generates 114 dB).

5. Press **<Enter>** to accept and save the new calibration factor.



6. Detach the calibrator from the microphone.



<ENT>




Note: If the calculated calibration drift is out of the ± 3 dB range, the warning "Microphone outside the tolerance. Accept?" will appear on the screen. If the calibration drift is outside the ± 20 dB range, the head of the screen turns red: **Calibration.**




Note: To exit the calibration procedure without saving the calibration factor, press **<ESC>**.

3.2.2 Last calibration record – Last Calibration

The **Last Cal.** screen displays the information about the last calibration record for the current measurement function: the type of calibration (*Factory Calibration*, *By Sensitivity* or *By Measurement*), the date of calibration and the calibration factor.




<ENT>



3.2.3 History of calibrations – Calibration History

The **Cal. History** screen displays a list of calibration records.

The calibration record has the same structure as the last calibration record.

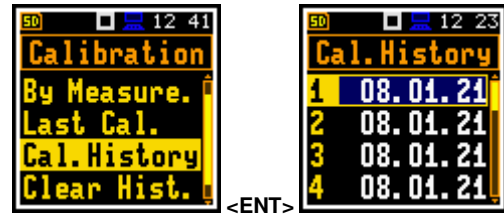

Note: Each time you return to the factory settings without keeping the last calibration (see Chapter 8.2), the new record appears in the list that indicates the Factory calibration of the instrument.

3.2.4 Erasing calibration records – Clear History

To delete all records in the calibration history list, select the **Clear Hist.** item and press **<Enter>**.


The instrument requests will ask you to confirm the deletion.



3.2.5 Post measurement calibration – Post Calibration

Some regulations require that post-measurement calibration information be added to measurement files created prior to such calibration. The post-calibration factor is for informational only, as it was not taken into consideration during the measurement.

The **Post Cal.** screen offers three options: no saving (**Off**), save in the last file created (**Last File**) or save in the files created after the last calibration (**After Cal.**).

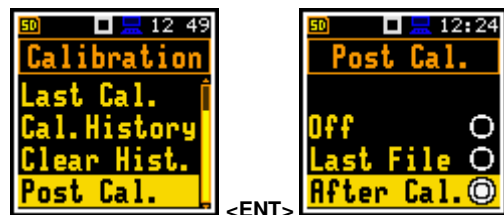

3.2.6 Automatic calibration – Auto Calibration

The **Auto Cal.** item allows you to perform automatic calibration when the sound calibrator is attached. In this case, the "Calibration by measurement" screen will appear automatically. If **Auto Cal.** is off, the user should access this screen from the menu.



The automatic calibration function has been implemented to make calibration as easy as possible and to allow the user to calibrate the instrument with a minimum of steps.

When Auto Calibration is enabled, the unit periodically compares the measured signal level (Running SPL for 1 second) with the reference calibration level when it's not performing a measurement and starts the calibration measurement if the stable SPL result is within $\pm 5\text{dB}$ of the calibration level.

To perform the automatic microphone calibration, follow the steps below:

1. Switch on the instrument.
2. Attach the SV 36 (or equivalent 94/114 dB @ 1000 Hz) calibrator to the microphone and switch it on (if the calibrator you are using doesn't have an automatic switch-on function).

Calibration starts automatically and the calibration process is similar to that of calibration By Measurement.





Note: Automatic calibration is performed in relation to the calibration level set in the **By Measurement** screen.

The sound pressure level generated by the calibrator will trigger the automatic calibration process if the difference between the **Calibration Level** value set in the **Calibration** screen and the measured SPL level generated by the calibrator is within ± 5 dB.

During the calibration measurement, the level of the measured calibration signal is displayed. If the maximum difference between three consecutive 1-second LCeq results is less than **0.05 dB**, the calibration measurement is stopped, and the calibration factor will be calculated. The measurement can be stopped at any time by pressing the **<Stop>** key.


When the calibration measurement is stopped, the **Calibration drift** (change in the calibration factor since the last calibration, calculated in dB) is displayed.

3. Press **<Enter>** to save the new calibration factor or **<Esc>** to discard it. In either case the instrument will exit the **Calibration** screen.
4. Detach the calibrator from the microphone.



4 CONFIGURING MEASUREMENT PARAMETERS – Measurement

The **Measurement** section combines elements related to the configuration of measurement parameters.

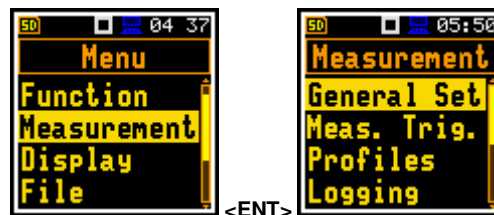

The contents of the **Measurement** list depend on the user interface (**Simple** or **Advanced**) and the measurement function selected. Two example **Measurement** screens are shown for the **Advanced** and **Simple** interfaces.



The **Measurement** section contains the following items which allow you to:

General Set	set general measurement parameters,
Meas. Trig.	set the measurement trigger; this item only appears in the Advanced interface,
Profiles	set profile specific parameters in the Level Meter function,
Profile 1 (2,3)	set profile specific parameters in the Dosimeter function;
Alarm	set alarms; this item only appears in the Dosimeter function and in the Advanced interface,
Logging	set the logger,
Spectrum	set the spectrum parameters; this item only appears in the 1/1 and 1/3 octave analysis functions,
Range	check the current measurement range,
Comp. Filter	switch on the required compensation filter,
Stat. Lev.	set 10 statistical levels,
Exp. Time	set the exposure time for dose measurements; this item only appears in the Dosimeter function and in the Advanced interface,
Timer	set the internal timer; this item only appears in the Advanced interface.

4.1 SETTING GENERAL MEASUREMENT PARAMETERS – GENERAL SETTINGS

The **General Set** screen allows you to set the general measurement parameters: delay of the start of the measurement (**Start Delay**), synchronisation with the instrument's RTC (**Start Sync.**), period of integration of the measurement results (**Integr. Per**), repetition of the measurement cycles (**Rep. Cycles**), type of the LEQ detector (**LEQ Integr.**) and duration of the day period (**Day Time L.**).

Start delay

The **Start Delay** item defines the delay time between pressing the **<Start>** key and to the actual start of the measurement (the instrument's digital filters of continue to analyse the input signal even when the measurement is stopped). This delay can be set between 0 seconds to 60 minutes. The default value is **1s**.





Note: In the **Simple** interface, the **Start Delay** item is hidden, but the instrument uses the settings previously defined in the **Advanced** interface or the default settings (**1s**).




Note: During calibration, the start delay is always 3 seconds.



Note: When the instrument is switched on, it takes 30 seconds to warm up. The instrument will not start a measurement until 30 seconds have elapsed if you press the **<Start>** key earlier.


Synchronisation of measurements

The **Start Sync.** item defines the points of synchronisation of the measurements with the RTC of the instrument. The **Start Sync.** item can be set to **Off**, **1m**, **15m**, **30m** and **1h**. For example, if **1h** is selected, the measurement will start from the beginning of the first second of the next hour after the **<Start>** key is pressed and will be repeated from the first second of the next hour after the integration period has elapsed if the number of cycles is greater than one. The default value is **Off**.



Integration period

The **Integr. Per** item defines the period over which the signal is measured (and for some results averaged/integrated) and the measurement results are logged to the logger file as **Summary Results** (see **Logger Setup** description). The integration period can be infinite (**Inf**) or selected from the set: **24h**, **8h**, **1h**, **15m**, **5m**, **1m**, from **1s** to **59s** with 1s increments, from **1m** to **59m** with 1m increments, from **1h** to **24h** with 1h increments.




During the integration period, the instrument takes a series of 1-second measurements and averages them with the results averaged over the n-1 seconds. The averaged results are displayed and updated every second for the elapsed measurement time (n seconds). At the end of the integration period, the averaged results are stored in the logger file, if such storage is enabled.

At the end of the integration period, the measurement is automatically stopped and restarted if the number of measurement repetitions (**Rep. Cycles**) is greater than one.

The definitions of the measurement results are given in Appendix D.

Number of measurement cycles

The **Rep. Cycles** item defines the number of measurements (made with the measurement period defined in the **Integr. Per** item) that the instrument will perform after the **<Start>** key is pressed. The values of **Rep. Cycles** are within the limits [Inf, 1÷1000]. The default value is **1**.



For example, if **Integr. Period** equals 8 hours and **Rep. Cycles** equals 2, the instrument will make a first measurement for the 8-hour period and a second measurement for the 8-hour period from the end of the first measurement. At the end of each cycle the 8-hour LEQ is stored in the logger file.




Note: In the **Simple** interface, the **Rep. Cycles** item is hidden, but the instrument uses the settings previously defined in the **Advanced** interface or the default settings (**1**).



Note: In the case of the infinite integration period or the infinite repetition cycles, the measurement should be stopped manually with the **<Stop>** key.

Day time limits

The **Day Time Limits** item defines the day and night time limits required by the local standards. These limits are used to calculate the **Lden** result (see Appendix D for definition). Two options are available: **6H-18H** and **7H-19H**. The default value is **6H-18H**.





Note: In the **Simple** interface, the **Day Time Limits** item is hidden, but the instrument uses the settings previously defined in the **Advanced** interface or default settings (**6H-18H**).

Detector type

The **LEQ Integration** item defines the detector type for calculating RMS based results: **Leq**, **Lden**, **LEPd**, **Ln** and **Sel**. Two options are available: **Exponential** and **Linear**. Default value is **Linear**.



Linear is required to obtain the true RMS value of the measured signal according to IEC 61672-1:2013. When this option is selected, the RMS based results do not depend on the detector time constant defined in the **Profiles** screen (path: <Menu> / Measurement / Profiles) (results are displayed without indication of the detectors selected in the profiles). In this case, the **Lin.** (or **L**) is displayed during the presentation of the results.

Exponential allows to meet the requirements of another standard for averaging **Leq**. When this option is selected, the RMS based results depend on the detector time constant defined in the **Profiles** screen (path: <Menu> / Measurement / Profiles): **Slow**, **Fast**, **Impulse**. The results are displayed with the detector type indicator selected for the profiles.



Note: In the **Simple** interface, the **LEQ Integration** item is hidden, but the instrument will use settings previously defined in the **Advanced** interface or default settings (**Linear**).


Rolling Leq

In the two items **LRx Time** you can define integration periods for the calculation of **LR1** and **LR2** results (see Appendix D). The default values are **30 m** and **60 m** respectively.



4.2 SETTING THE MEASUREMENT TRIGGER – MEASUREMENT TRIGGER

The **Meas. Trig.** item only appears in the **Advanced** interface and allows the measurement trigger parameters to be set. The **Meas. Trig.** is a contextual list of parameters in which the trigger (**Trigger**) can be switched **Off** or **On** by selecting the trigger type (**Slope+**, **Slope-**, **Level+**, **Level-** or **Gradient+**). If the trigger is on, additional parameters can be defined: the measurement result to be checked for a trigger condition (**Source**), the threshold level (**Level**) and the rate at which the source value changes (**Gradient**).

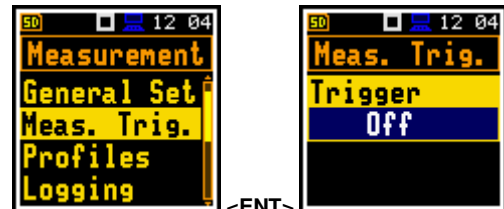

Note: In the **Simple** interface, the **Measurement Trigger** item is hidden, but the instrument uses the settings previously defined in the **Advanced** interface or the default settings (**Trigger: Off**).

The trigger condition is checked every 0.5 milliseconds.

Slope trigger


The **Slope + / Slope-** trigger starts the measurement with the duration of the **Integration Period** under the condition that the rising/falling value of the measured result (**Source**) integrated during 0.5 ms passes above/below the threshold value (**Level**).



At the start of a new measurement cycle (after pressing the **<Start>** key or automatically after stopping the previous measurement cycle) the instrument checks a trigger condition every 0.5 ms and if the condition is met, the instrument starts a continuous series of 1-second integrations, the number of which is equal to the number of seconds in the **Integration Period**.

After ending the **Integration Period**, the new measurement cycle can start with above logic.

The measurement can be stopped manually at any moment with the **<Stop>** key.

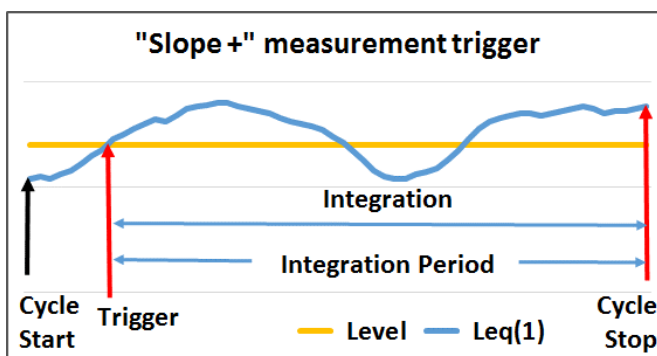

Note: When a measurement is waiting for the slope trigger, the flashing "slope" icon will overlay the „waiting" icon.




Level trigger

The **Level+** / **Level-** trigger starts the 1-second measurement under the condition: value of the RMS result (**Source**) integrated by 0.5 milliseconds is greater/lower than the threshold value (**Level**). In other cases, the instrument continues checking the trigger condition every 0.5 milliseconds.



At the start of the new cycle (after pressing the **<Start>** key or automatically after stopping the previous cycle) the instrument checks the trigger condition every 0.5 ms and starts 1-second integration if the condition is met.

After each 1-second integration, the instrument repeats the trigger condition check every 0.5 ms and starts the next 1 second integration if the condition is met. The instrument repeats this as often as there are seconds in the integration period and stops the measurement cycle. Therefore, the series of 1-second measurements may not be continuous, and the duration of the measurement cycle may be longer than the integration period.

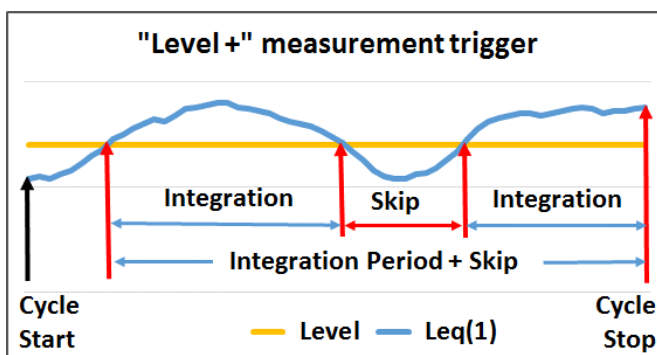

The measurement can be stopped manually at any time using the **<Stop>** key. Summary Results are calculated from a series of 1-second results measured during each measurement cycle and stored in a logger file.




Note: When a measurement is waiting for a level trigger, the flashing "level" icon will overlay the „waiting" icon.



Gradient trigger


The **Gradient +** trigger starts the 1-second measurement under the condition: the value of the RMS result (**Source**) integrated during 0,5 milliseconds is greater than the threshold (**Level**) and the gradient of the Source value is greater than the gradient threshold (**Gradient**). In other cases, the instrument continues to check the trigger condition every 0.5 milliseconds.



This type of trigger has the same logic as the **Level +** trigger, but the trigger condition also requires the gradient level to be exceeded.




Note: When a measurement is waiting for a gradient trigger, the flashing “trigger” icon will overlay the „waiting” icon.




Source

Only one measurement result (**Source**) can be used to check the trigger condition in the **Level Meter** mode, namely the instantaneous LEQ from the first profile (with appropriate filter and detector), which is denoted here as **Leq(1)**. This item cannot be changed.




Threshold

The threshold (**Level**) can be set in the range of **24 dB** to **136 dB**. The **Source** value is compared with the **Level** value every 0.5 milliseconds.



Rate of change of Source value


This item appears when the **Gradient+** trigger is selected. The rate of change of the **Source** value (**Gradient**) can be set in the range of **1 dB/ms** to **100 dB/ms**.




4.3 SETTING PARAMETERS FOR PROFILES – PROFILES

Parameters for three profiles can be set in the **Profiles** screen for the **Lev. Met.** function or in the **Profile x** screens for the **Dosimeter** function.

The following parameters can be set independently for each profile: the weighting filter for results other than peak (**Filter**), the weighting filter for peak results (**Filter Peak**) and the type LEQ detectors (**Detector**).




<ENT>



Weighting filter

Next weighting filters can be selected for the **Filter** and **Filter Peak** positions:


- Z** Class 1 according to IEC 61672-1:201,
- A** Class 1 according to IEC 651 and IEC 61672-1:2013,
- C** Class 1 according to IEC 651 and IEC 61672-1:2013,
- B** Class 1 according to IEC 651,
- LF** low frequency filter according to China requirements.



LEQ detector

The following LEQ detectors (time constants) are available: **Impulse**, **Fast** and **Slow**.

Time constants are always applied to the **Lmax**, **Lmin**, **L(SPL)**, **Ltm3** and **LTeq** results and to the **Leq**, **LE(SEL)**, **LEPd** and **Lden** results if the **Exponential** LEQ detector is selected in the **General Settings** list (see Appendix D).



4.4 SETTING ALARM THRESHOLDS FOR DOSE METER – ALARM

The **Alarm** item is only active in the **Dosimeter** function and is described in detail in Chapter 11.6.



4.5 CONFIGURING DATA LOGGING – LOGGING


Summary results (**L(SPL)**, **Leq**, **LE(SEL)**, **Lden**, **LEPd**, **Ltm3**, **Ltm5**, $10 \times \text{Ln}$, **OVL**, **Lpeak**, **Lmax**, **Lmin**, **EX**, **SD** and spectra) are measured and stored in the file with the step defined by the **Integration Period** item as many times as defined by the **Repetition Cycles** item (path: <Menu> / Measurement / General Settings).

The instrument also allows the additional recording of some results with a different step defined by the **Logger Step** item (path: <Menu> / Measurement / Logging / Logger Setup). It is therefore possible to store two sequences of measurement results in parallel – one for Summary results (SR) and another for Logger results or time history results (TH).

When **Logger** is switched on, selected logger results taken from three independent profiles are stored simultaneously with a time step down to **100 ms**. Recording of logger results to a file is stopped after a period equal to the **Integration Period** multiplied by the number of **Repetition Cycles**, or when the measurement is stopped manually.

The Summary Results are stored in the same file as the Logger Results. Blocks of summary results are written to the file at the end of each measurement cycle.

The figure below illustrates the principles for saving measurement results.

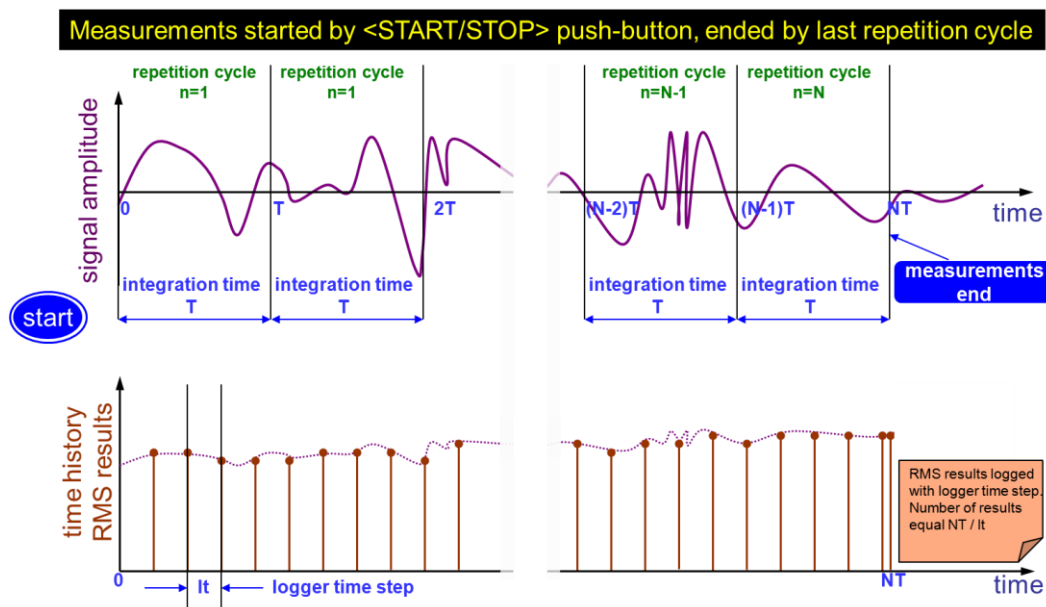

Summary Results and Logger Results saving

The **Logging** list allows you to program the logging functions: recording of Summary and Logger results in a logger file and recording of audio signal in a WAV file.

In the **Simple** interface, the **Logging** list includes only of one item - **Logger Set**.



4.5.1 Setting general logging parameters – Logger Setup

In the **Logger Set.** list you can enable logging (**Logger**) and set the general logger parameters: split the logger file (**Log. Split**), set the logging step (**Logger Step**), edit the file name (**Logger Name**) and enable logging of Summary results (**Summary Results**).

The **Logger** item switches logging **On** or **Off**.

Switching the logger on activates other items in the **Logging** list.



Note: If **Logger** is **Off**, logger files will not be created, logger results will not be measured, and summary results will not be stored!



Note: The **Wave Recording** function doesn't depend on the **Logger** status. Wave files have a different format and are created when **Wave Recording** is enabled – see Chapter 4.5.4.

Logger file split

The **Log. Split** item allows the logging data to be split into separate files. If **Log. Split** is **Off**, the data will be logged in one logger file with the name defined in the **Logger Name** item. The default value is **Off**.

In other cases, the logging is done in separate files and the logging in the new file starts at the end of the integration period (**Integr. Per**), or at every quarter of the RTC (**Sync. to 15m**), or at every half an hour of the RTC (**Sync. to 30m**), or at every hour of the RTC (**Sync. to 1h**), or at user defined times (**Spec. Time**). Whenever the split time is reached, the logger file is closed, and a new file is opened with the number incremented by one for subsequent measurement data.



Note: In the **Simple** interface, the **Logger Split** item is hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (**Off**).

If **Spec. Time** is selected in the **Log. Split** item, you can set six split times (**Split Time1**, **Split Time2**, **Split Time3**, **Split Time4**, **Split Time5** and **Split Time6**) changing **Off** to the desired time of the day when splitting should occur.



The **Logger Step** item defines the step for recording logger results to a file. It can be set in a range from **100ms** to **1h**. The default value is **1s**.



Note: For logger steps smaller than 1s, the running Leq results will be calculated with a step of 1s but stored to the logger file with the logger step. In such cases the logger curve for the running Leq results will be a stepped curve.




Note: In the **Simple** interface mode, the **Logger Step** parameter is hidden, but the instrument will use settings previously defined in the **Advanced** mode or default settings (**1s**).

Logger file name

The **Logger Name** item allows you to define the logger file name. The default logger file name is **Lnn**, where **nn** is a number. The name can be up to eight characters long. Pressing the ◀ / ▶ key opens the special screen with the text editor.

The edited name is accepted and saved when the <Enter> key is pressed. The special warning is displayed if the file with the same name already exists in the working directory. The instrument displays the message "Incorrect File Name" and waits for the <Enter> key to be pressed.

If the new name is correct, the instrument will display it in the **Logger Name** item.

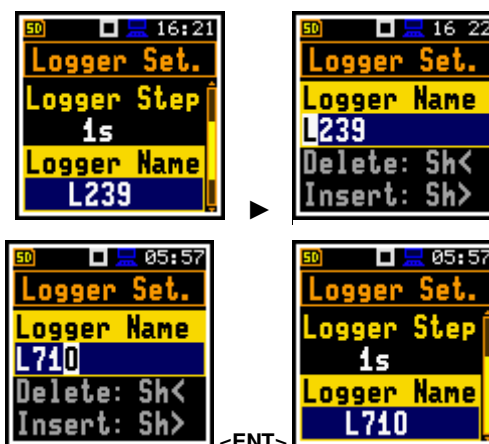

Logging Summary results

The **Summary Results** item switches on or off the storage of the full set of Summary results measured by the instrument with the **Integration Period** step: main results (**L**, **Leq**, **LE**, **Lden**, **LEPd**, **Ltm3**, **Ltm5**, **Ln**, **OVL**, **Lpeak**, **Lmax**, **Lmin**, **EX**, **SD**), statistics and spectra.



Note: In the **Simple** interface, the **Summary Results** item is hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (**On**).

4.5.2 Selecting results for logging – Logger Results

The **Logger Results** item allows you to select results for three independent profiles to be logged in the logger file during a measurement with the **Logger Step**.

The list of logger results depends on the measurement function. For the **Level Meter** function, the following results can be logged: **Lpeak** (**Lpk**), **Lmax**, **Lmin**, **Leq**, **LR1** and **LR2**.

Use the ◀ / ▶ or ▲ / ▼ keys to select the item.

To select results to be logged, press the ◀ / ▶ key with <Shift>.




Note: When the **Logger** is **Off** or no results have been selected for logging, the logger plot cannot be activated in **Display Modes** and will not appear on the display.



Note: In the **Simple** interface, the **Logger Results** item is hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (all results are selected).

4.5.3 Logger trigger settings – Logger Trigger

The **Logger Trigger** item allows you to define how the logger results are to be recorded in the logger file. The trigger can be disabled (**Off**) or enabled if you select the trigger type in the **Trigger** item. If the trigger is enabled, other parameters can be defined: the measurement result to be checked for a trigger condition (**Source**), the threshold (**Level**) and the number of readings to be stored in the logger before the trigger condition is met (**Pre Trigger**) and the number of readings to be stored in the logger after the last trigger during logging (**Post Trigger**).

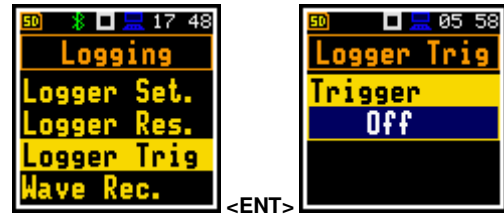

Note: In the **Simple** interface, the **Logger Trigger** item is hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (**Trigger: Off**).


Level trigger


The **Level +/Level -** trigger enables the logging of logger results with the **Logger Step** under the condition: the value of the LEQ result (**Source**) measured by the **Logger Step** period is greater/less than the threshold (**Level**). In other cases, the logging is skipped.

This type of trigger makes it possible to separate the results related to the low/high noise level.

Logging can only be performed when the Summary results are being measured, i.e., from the start of the measurement to the end of the measurement.

This means, for example, that if the measurement is waiting for a trigger condition, logging will be skipped, even if the logger trigger condition is met.

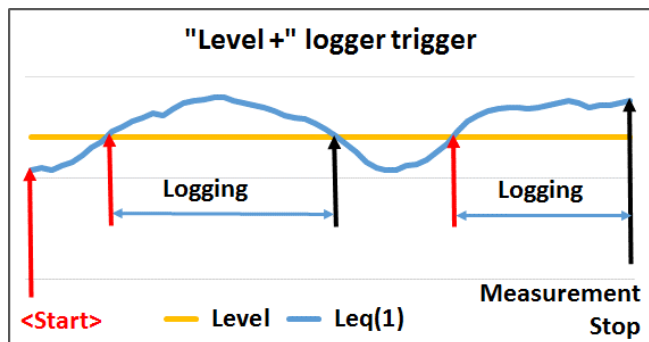


Note: When logging is waiting for a level trigger, the "level" icon will alternate with the "logging" icon. 

Source

Only the one measurement result (**Source**) can be used to check the trigger condition in the **Level Meter** mode, namely the instantaneous LEQ from the first profile (with appropriate filter and detector), denoted here as **Leq(1)**. This item cannot be changed.

Threshold

The threshold (**Level**) can be set in the range of **24 dB** to **136 dB**. The **Source** value is compared with the **Level** value every 0.5 milliseconds.



Pre and post trigger logging

The **Pre Trigger** item allows you to define the number of readings to be recorded in the logger file before the trigger condition is met. This number is limited to 0..10.



The **Post Trigger** item allows you to define the number of readings to be recorded in the logger file after the last trigger condition is met. This number is limited to 0..200.

These parameters can serve a dual purpose. Firstly, if you want to collect data immediately after or before the event that triggered the logger. Secondly, when it is necessary to have continuous logging, but the source oscillates close to the threshold. Extending the logging window allows you to avoid the effects of pulsation.

Periods of logging before or after the trigger condition are shown to the right of the number in minutes and seconds (in the format **0 m 00 s**) as a result of multiplying the number of results by the **Logger Step**.

4.5.4 Configuring signal recording – Wave Recording

The **Wave Rec.** item allows you to enable and configure a recording of the signal waveform to a WAV file.

WAV files are saved automatically in the working directory of the instrument's memory.



Note: In the **Simple** interface, the **Wave Recording** item is hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (**Recording: Off**).



Note: The **Wave Recording** function is optional and should be unlocked by entering the activation code in the text editor screen, opened with the ► key. Once unlocked, this function is always available.

The **Recording** item, if it is not disabled (**Off**), defines the type of trigger for a signal recording: from the start and throughout the measurement period (**Continuous**), manual start (**Trig.manual**), from a slope, level or gradient trigger or from the start of a measurement with a given recording interval (**Integr. Per.**).



The **File Name** item allows you to edit the name of the WAV file.

The **Format** item defines a type of the WAV file format: **PCM** or **Extensible**.




Slope trigger

The **Slope+** / **Slope-** trigger starts a signal recording on the condition: the rising value of the Leq result (**Source**), integrated by 0.5 ms, passes above/below the threshold level (**Level**).



When the **<Start>** key is pressed, the instrument checks the trigger condition with the steps defined by the **Trigger Period** parameter, and, if the condition is met, starts a signal recording. The recording lasts for the minimum **Recording Time**, and during this time the instrument continues to check the trigger condition with the **Trigger period** step. Provided that the **Trigger Period** is shorter than the **Recording Time**, if the next trigger condition is met during the **Recording Time**, the instrument triggers the recording again, so that from this moment it continues with the additional **Recording Time** and so on. If there are no triggers during the next recording time, recording will stop after the last trigger plus **Recording Time**. Assuming that trigger conditions continue to be checked after the first recording, a new signal recording can start during the same measurement time.

The attached example shows that two records have been created between the start and stop of the measurement. The first record is equal to **Recording Time** because no second trigger condition was met during this period. During the second record, the measurement was stopped, and the record is shorter than **Recording Time**.

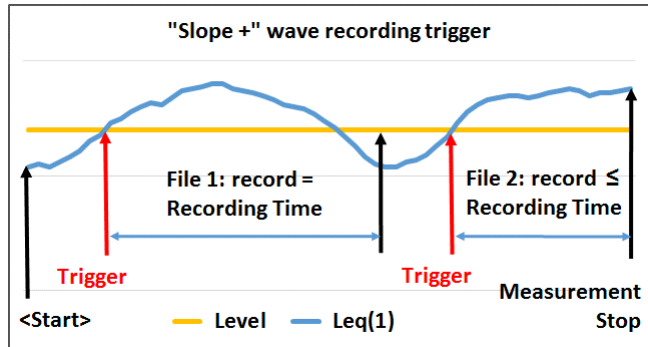


Note: When a wave recording is waiting for the slope trigger, the "slope" icon will overlay on the grey „wave” icon.



Level trigger

The **Level + / Level -** trigger starts a signal recording that will last for the **Recording Time** under the condition: the value of the Leq result (**Source**) integrated by 0.5 ms is greater/less than the threshold (**Level**). In other cases, the recording doesn't start, but if it has been already started, it can be continued until the **Recording Time** has elapsed.

If a trigger condition occurs during the **Recording Time**, the recording will be extended for another **Recording Time** from the moment of the trigger condition, and so on.

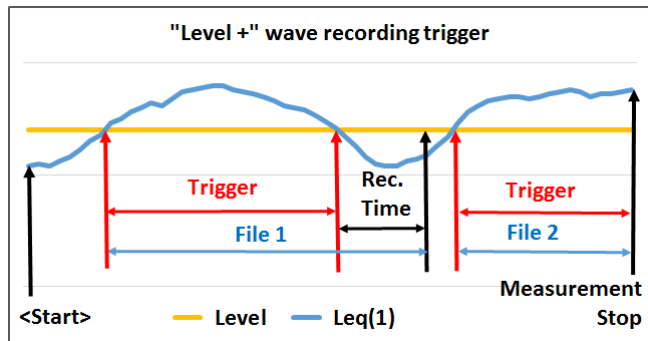

Note: When the wave recording is waiting for the level trigger, the "trigger" icon will overlay on the grey „wave” icon.



Gradient trigger

The **Gradient +** trigger starts a signal recording for the **Recording Time** under the condition: the value of the Leq result (**Source**) averaged by 0.5 ms is greater than the threshold (**Level**) and the rate of change of this Source result (gradient) is greater than the gradient threshold (**Gradient**). In other cases, the recording doesn't start, but if it has been already started, it can be continued until the **Recording Time** has elapsed. The instrument also checks the trigger condition during recording and if the condition is met, the recording is continued for another **Recording Time**.



Integration period trigger

If the **Integr. Period** trigger is selected, the signal recording is triggered at the start of each measurement and the recording lasts for the minimum **Recording Time**. If the trigger condition occurs during recording (when the **Integration Period** is shorter than the **Recording Time**), the recording will continue from that moment for the next **Recording Time** and so on.



Manual trigger

If the **Trig.manual** trigger is selected, the signal recording starts and stops when the ◀ and ▶ keys are pressed simultaneously during the measurement. When these keys are pressed, the screen with the corresponding message appears. Recording always stops after the time set by the **Rec. Time** parameter.



Note: When a wave recording is waiting for the gradient trigger manual trigger or "integration period" trigger, the flashing "trigger" icon will overlay on the grey „wave" icon.

The **Filter** item allows the user to select the broadband frequency filter during a waveform recording: **Z**, **A**, **C**, **B** or **LF**.

The **Sampling** parameter defines the sampling frequency of the waveform recording: **48kHz**, **24kHz** or **12kHz**.

The **Signal Gain** item allows the user to select the gain of the recorded signal: **0 dB ... 40 dB**.

Source result

Only one measured result (**Source**) can be used to check the trigger condition in the **Level Meter** mode, namely the LEQ from the first profile averaged for the **Trigger Period** with appropriate filter and detector here denoted as **Leq(1)**. This item cannot be changed.

Threshold level






The threshold (**Level**) can be set in the range of 24 dB to 136 dB.

Checking the trigger condition

The **Source** value is compared with the **Level** value at the step defined by the **Tr. Period** parameter, which can be set as follows: **Logger Step**, **0.5ms**, **100ms** and **1s**.


Gradient

Rate of triggering signal change (**Gradient**) can be set in the range of **1 dB/ms** to **100 dB/ms**.




Recording before trigger

If the **Pre Trigger** item is set to a value other than **Off**, the instrument will start recording the waveform before the first trigger. The interval of this recording is equal to the **Trigger period** (0.5 s in the example attached).

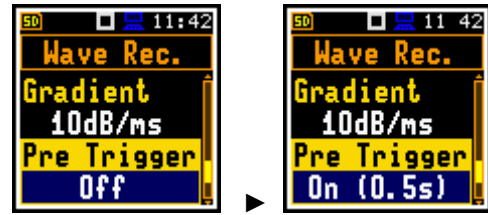

Signal recording time

The **Rec. Time** item allows you to set the time of signal recording after triggering. If the trigger condition appears during the recording time, the signal is recorded for an additional **Rec. Time**. The available values are from **1s** to **8h** or infinitive (**Inf**).



Wave file size control

The **LengthLimit** item allows you to define the maximum time during which recording to a file is allowed. After this time, the current file is closed, but the signal recording continues in the new file. You can disable the limitation selecting **Off**. This option allows you to control the size of the waveform files.



Note: When a measurement is paused, either manually or automatically (in the case of programmed pauses in Dosimeter mode), the Wave file is closed at the start of the pause and a new Wave file is opened when the pause is released.

4.6 SELECTING MEASUREMENT RANGE – RANGE

The **Range** position is used to set one of the measurement ranges available in the instrument: **Normal** and **Low**.

The absolute values of the range depend on the calibration factor and are shown in the **Range** screen.



In the attached screens it is assumed that the calibration factor is equal to zero.

The detailed description of the measurement ranges parameters is given in Appendix C.




Note: The ranges in the above screens correspond to the microphone with the declared sensitivity of $25 \div 37$ mV/Pa (see Appendix C). If the microphone sensitivity is other than $25 \div 37$ mV/Pa, the range will change automatically.

4.7 SELECTING MICROPHONE COMPENSATION – COMPENSATION FILTER

The **Comp. Filter** item is only available in the **Advanced** interface and allows you to switch on/off the compensation filters used in the instrument.

The **Microphone** compensation filter (microphone inner noise compensation) is switched on by default but can be switched off for electrical measurements (e.g., for laboratory calibration).

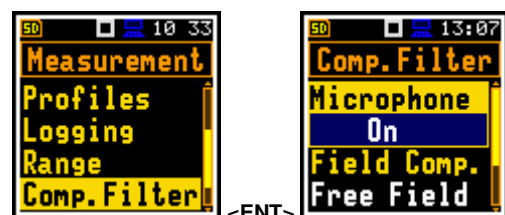

The **Field Compensation** item allows you to switch off (**Off**) the compensation filter for laboratory tests or to select the compensation filter for sound measurements in the free-field (**Free Field**), diffuse field (**Dif. Field**) conditions or for the permanent outdoor monitoring application as a part of the **SV 271** monitoring station: **Environment** (when the acoustic signal is parallel to the microphone's grid) or **Airport** (when the acoustic signal is perpendicular to the microphone's grid). The default setting is **Free Field**.

The **Windscreen** item is active when the field compensation is **On**. It switches on the compensation when the windscreen is applied. The default setting is **On**.



Note: In the **Simple** interface, the **Comp. Filter** position is hidden, but the instrument will use the settings previously defined in the **Advanced** mode or the default settings (**Microphone: On; Field Comp.: Free Field; Windscreen: On**).




Note: For laboratory instrument's tests, the compensation filters should be set according to Appendix C.

4.8 SETTING STATISTICAL LEVELS – STATISTICAL LEVELS

In the **Stat. Levels** list, you can define ten statistical levels, named from **N1** to **N10**, to be calculated, displayed, and stored in the files together with Summary Results (see Appendix D).

The default statistical levels have the following settings: **1, 10, 20, 30, 40, 50, 60, 70, 80** and **90**. All values should be within the integer range [1, 99]. Each value can be set independently from others.

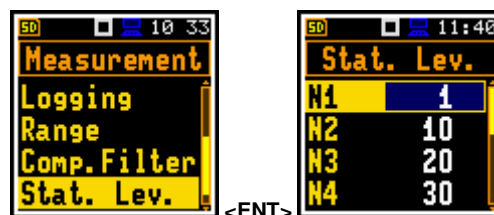

4.9 PROGRAMMING INSTRUMENT'S INTERNAL TIMER – TIMER

The **Timer** function is used to program the automatic start of the measurement (and switch on the instrument if it is switched off) at a given time and day of the week, and the automatic stop of the measurement and switch off the instrument.



Note: In the **Simple** interface, the **Timer** item is hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (**Timer: Off**).

The measurement is performed with the parameters set in the **Measurement** section with one exception (see Note below).



Note: When the **Timer** is **On**, the measurements are performed from the defined **Start** to **Stop** times because the **Repetition Cycles** parameter is automatically set to **Inf** (path: <Menu> / Measurement / General Set.). The last integration can be truncated.


Setting the start and stop of the measurement

The **Start (hh:mm)** and **Stop (hh:mm)** items define the start and stop times of measurement.

In the items: **Monday, Tuesday, ..., Sunday**; you can select the days of the week on which the measurements are to start.

The timer can be programmed for a maximum number of days ahead (**Max days**) (up to 100) or without limit (**Inf**). During these days, the instrument refers to the time of the **Real Time Clock (RTC)**. The measurements stop when the number of days in the day counter reaches **Max days**. If the **Inf** value is selected, the measurement series can only be stopped manually (if power is available). If more than one day per week is selected, the day counter increases with each measurement day.

Once the timer has been programmed, you can switch off the instrument. However, if you try to switch off the instrument when the time remaining to the first timer start point is less than 10 minutes, the instrument will ask you if you really want to switch off the instrument, as this will also disable the timer.



Note: Before using the timer, check that the real time clock settings are correct.



Note: Ensure that there is sufficient internal battery power and memory for the instrument to perform the required measurements when it wakes up.

4.9.1 Example of timer execution


Let us assume that you want to switch on the measurement on Monday at 8:00, measure the noise level for 20 minutes and save the results in the file named L4.

To do this you should configure the **Timer** function as shown in the attached screen and to set the measurement parameters (path: <Menu> / Measurement / General Settings) and define the file name (path: <Menu> / Measurement / Logging / Logger Setup). Then turn off the instrument.

The instrument turns on and starts to warm up during the 30 seconds before the measurement start time at 8:00 on the nearest Monday.

The measurement is carried out over a period of 20 minutes. The results are then automatically stored in a file named L4. The instrument will turn off at 8:20 and wait for the next Monday to start the next measurement at 8.00. The next file is automatically named L5, and so on.

Such cycle will be repeated as many times as is defined by **Max days** parameter. If more than one day in a week is selected, the day counter is increased with each measurement performed. The measurement cycle will stop when the day counter reaches the **Max days** value. If **Inf** value is selected, the measurement cycles can only be stopped by the user (if the power supply is guaranteed, of course).



5 CONFIGURING DATA VIEWING – Display

The **Display** section contains the elements for setting the views of the measurement result and the display parameters.

The content of the **Display** list depends on the selected measurement function.




The **Display** section contains the items that allow you to:

- Disp. Modes** enable views in Measurement mode,
- Disp. Scale** adjust the **Logger** and **Spectrum** views,
- Spect. View** select the spectra to be viewed; this item becomes available only in the 1/1 and 1/3 octave analysis functions,
- Meas. Res.** select the measurement results to be displayed,
- Logger Res.** select time history results to be plotted,
- Screen Set.** enable/disable screen rotation and set the power save function.

5.1 ENABLING VIEWS – DISPLAY MODES


The One Result view is always enabled. Other views can be enabled or disabled in the **Disp. Modes** list.

You can switch between the views enabled in the **Display Modes** screen.

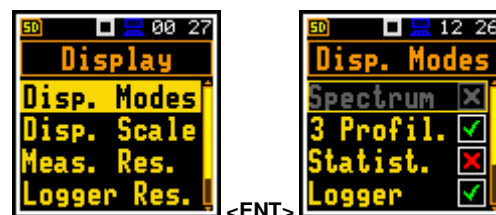

In the **Level Meter** function, the following views are available: **3 Profiles**, **Statistics**, **Logger**, **Running SPL** and **File Info**.

An additional view (**Spectrum**) is available in the **1/1 Octave** and **1/3 Octave** functions.



Changing views


The view is changed with the **<ESC>** key or with the **▲ / ▼** key pressed with **<Shift>**.



5.1.1 One Result view

In the One Result view, any measurement result selected in the **Disp. Res** list, can be viewed.

The One Result view can have different sub-views. You can change the sub-view of the One Result view by pressing **<Enter>**.

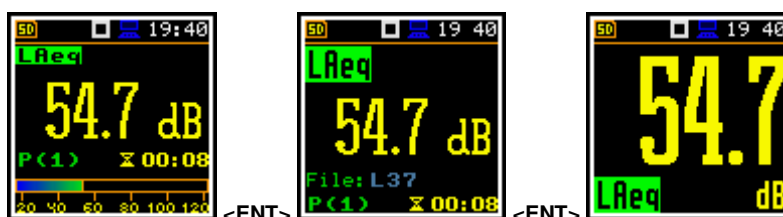

One Result view fields

1. Result name for:

- **Level Meter**, 1/1 Oct. and 1/3 Oct. functions: OVL, Lpeak, Lmax, Lmin, L, Leq, LE, Lden, LEPd, Ltm3, Ltm5, Ln, EX, SD, LR1, LR2
- **Dosimeter** function: OVL, Lpeak, Lmax, Lmin, L, DOSE, D_8h, PrDOSE, LAV, Leq, LE, SEL8, E, E_8h, LEPd, PSEL, Ltm3, Ltm5, Ln, PTC, PTP, ULT, TWA, PrTWA, Lc-a, EX, SD, LR1, LR2

2. Value of the measured result

3. Current profile number

4. Quasi analogue value indicator

5. Implemented weighting filter: **Z**, **A**, **C**, **B** or **LF**

6. Detector time constant: **Imp.**, **Fast**, **Slow** for the exponential detector or **Lin.** for the linear detector

7. Units of measured value


Elapsed time showing the current second of measurement in the range [0, **Integration Period**].



Note: For some results, the weighting filter and detector type are shown in the result name. For example, the **Lmax** result with **A** filter and **Fast** detector will be presented as **LAFmax**. For such results, there is no indication in the filter and detector fields.

Changing the result for the current profile

Use the ◀ / ▶ key to change the measurement result for the current profile.

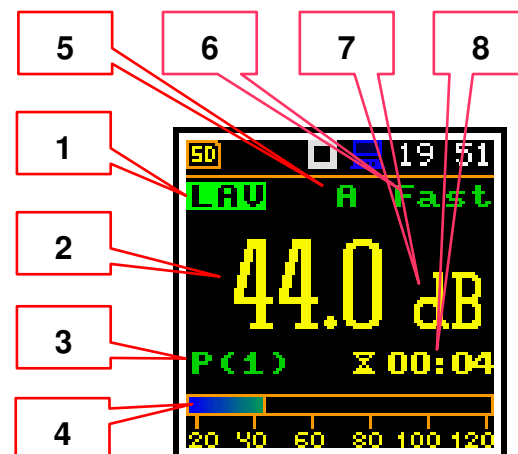

Changing statistical levels (Ln)

The statistical levels, which are set in the **Stat. Lev.** list (path: <Menu> / Measurement / Stat. Lev.), can be changed with the ◀ / ▶ key pressed with <Shift>.



Changing current profile

Use the ▲ / ▼ key to change a current profile.




5.1.2 Three profiles view

In the **3 Profiles** view, any three measurement results, selected in the **Disp. Res** list, may be presented for three profiles. You may change the **3 Profiles** sub-view by pressing the <Enter> key.



3 Profiles view fields


1. Result name for the first profile
2. Weighting filter and detector time constant
3. Value of the measured result
4. Quasi analogue value indicator for the selected result

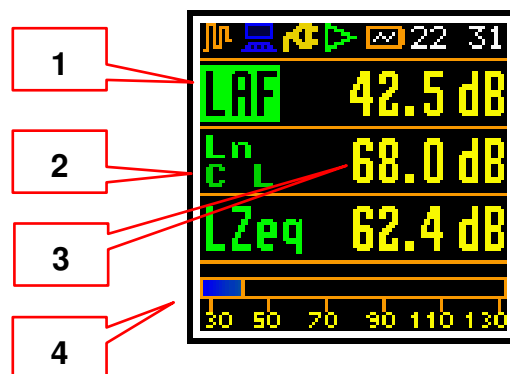

Changing the result for the current profile

Use the ◀ / ▶ key to change the measurement result for the current profile.

The statistical levels can be changed with the ◀ / ▶ key pressed with <Shift>.

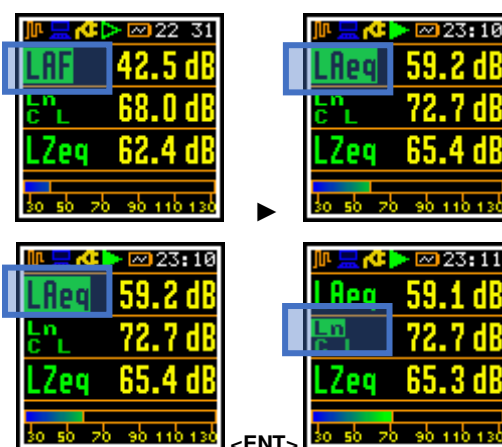

Changing current profile

Use the ▲ / ▼ key pressed with <Shift> to change the current profile.

5.1.3 Logger view


Logger view fields

1. Logger Plot
2. Result value for cursor position
3. Result name (Profile number)
4. Cursor time position

In the **Logger** view, the time history results, selected in the **Logger View** list, are displayed as a plot.

Use the ◀ / ▶ key to change the cursor position.

Press <Enter> to change the active plot for reading cursor values.

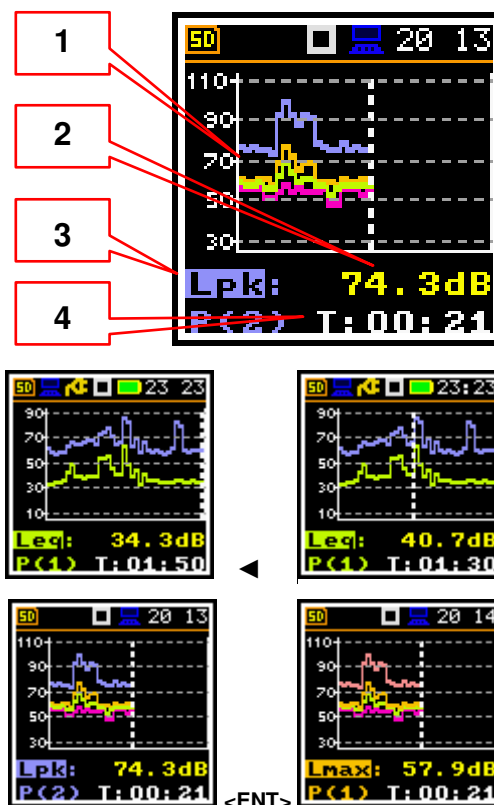



Note: If **Logger** (path: <Menu> / Measurement / Logging /Logger Set.) is switched off the **Logger** presentation mode is disabled! Therefore, to have this presentation mode active, switch the **Logger** on!




Note: When **Logger** is switched on, but results were not selected for logging the **Logger** presentation mode is disabled!

5.1.4 Statistics view

"Statistics" is the cumulative probability density function of exceeding the noise level during the measurement period. The X-axis defines the probability of exceeding the noise level, the statistical level **Ln**, and the Y-axis defines the calculated noise level in dB.


Statistics view fields

1. Cursor position
2. Statistics plot
3. Type of the plot (**Ln's**), active profile, LEQ detector (Linear, Fast, **Slow** or **Impulse**), used weighting filter name (**A**, **C**, **Z** or **B**)
4. Value (in dB) of the selected statistical level **Ln** for the cursor position
- 5.

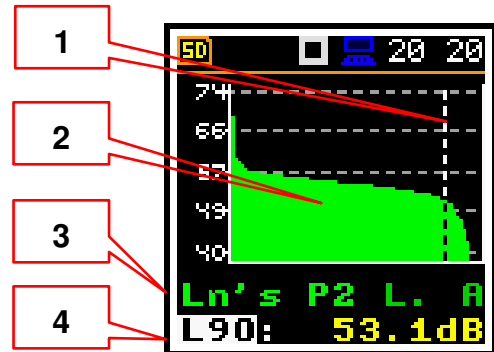


Changing the cursor position

Use the ◀ / ▶ key to change the cursor position.

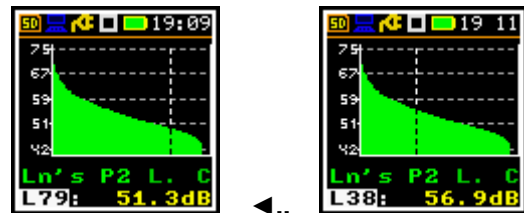

Changing current profile

Use the ▲ / ▼ key pressed with <Shift> to change the active profile.

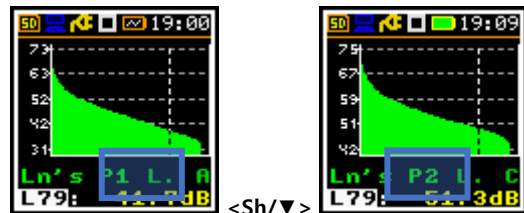

5.1.5 Running SPL view


The **Running SPL** view shows the SPL result when the measurement is not currently running. In this view, the SPL result is calculated and displayed, but not stored in the instrument's memory. The purpose of this mode is to give the user an initial indication of the signal being measured.



5.1.6 File information view

The **File Info** item provides the information about the last logger file saved.

The **File Info** view shows file name and size. When **Logger** is **Off** (path: <Menu> / Measurement /Logging / Logger Setup) the **File Info** item is disabled.

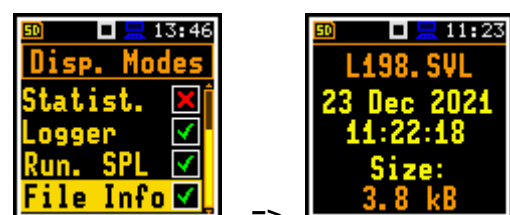

5.2 ADJUSTING PLOT SCALE – DISPLAY SCALE

The **Display Scale** list of parameters allows you to adjust the scale of the plot and switch a grid on/off in the **Logger**, **Statistics** or **Spectrum** display modes.

Scaling the vertical axis

The **Dynamics** item allows you to select the desired dynamic range scaling of the plot (Y-axis).

You can select the range from the set: **10 dB**, **20 dB**, **40 dB**, **80 dB** and **120 dB**.


Switching grid on/off

The **Grid** item allows you to switch on/off the horizontal grid lines of the plot.

Automatic Y-scale adjustment

The **Autoscale** item allows you to switch on/off the automatic scale adjustment of the dynamic range of the Y-axis to the initial level of the input signal from the microphone as soon as the measurement is started.

The example shows the changes in the scale after a sudden increase in sound pressure level.

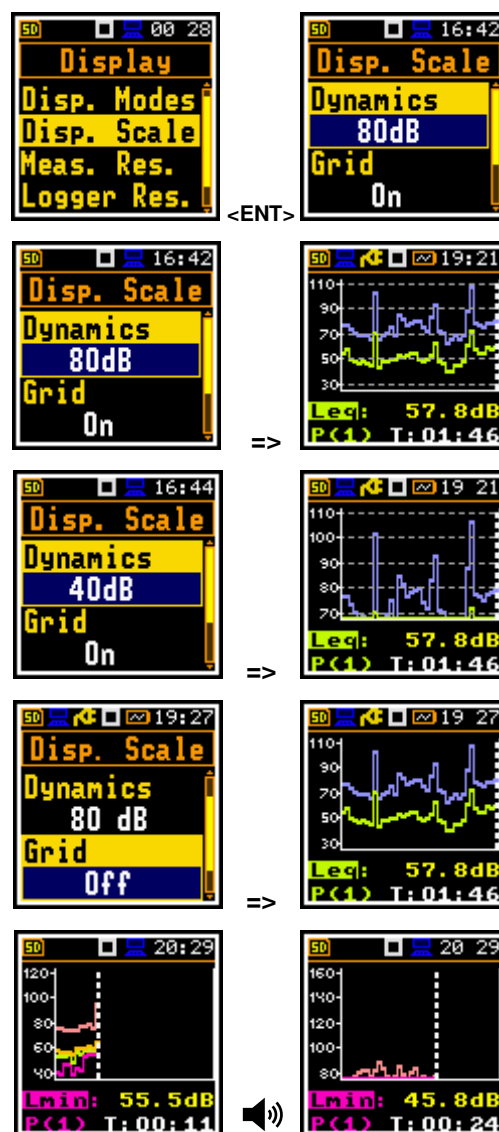


5.3 SELECTING MEASUREMENT RESULTS TO BE DISPLAYED – MEASUREMENT RESULTS

The **Meas. Res.** item allows you to select the Sound Level Meter (**SLM Results**) or Dose Meter (**Dosim. Res.**) measurement results to be displayed in different views.


The result can be selected from:

- **SLM Results** list: **TIME**, **Lpeak**, **Lmax**, **Lmin**, **L**, **Leq**, **LE**, **Lden**, **LEPd**, **Ltm3**, **Ltm5**, **Ln**, **LR1**, **LR2**, **EX**, **SD**, **OVL**;
- **Dosim. Res.** list: **TIME**, **Lpeak**, **Lmax**, **Lmin**, **L**, **DOSE**, **D_8h**, **PrDOSE**, **LAV**, **Leq**, **LE**, **SEL8**, **E**, **E_8h**, **LEPd**, **PSEL**, **Ltm3**, **Ltm5**, **Ln**, **PTC**, **PTP**, **ULT**, **TWA**, **PrTWA**, **Lc-a**, **EX**, **SD**, **OVL**.

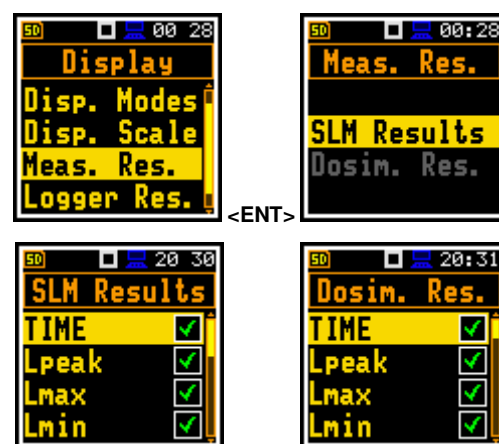




Note: The **EX** and **SD** results are optional and should be unlocked by entering the activation code in the text editor screen that opens after the first attempt to select them. Once unlocked, these results are permanently available!



5.4 SELECTING LOGGER RESULTS TO BE DISPLAYED – LOGGER RESULTS

The **Logger Results** item allows you to select the Logger results (time history results) to be displayed in the **Logger** view.



<ENT>

You can select Logger results for the:

- **Level Meter**, 1/1 Oct. and 1/3 Oct. functions: **Lpk**(Lpeak), **Lmax**, **Lmin**, **Leq**, **LR1**, **LR2**
- **Dosimeter** function: **Lpk**(Lpeak), **Lmax**, **Lmin**, **Leq**, **LAV**



5.5 CONFIGURING POWER SAVER – SCREEN SETUP

The **Screen Set.** item allows you to configure the power saver function (**Dim Mode**) and switching on the screen auto rotation.

Power saver function



The consumption of the instrument's internal power source can be minimising by reducing the screen brightness when possible.

There are two options for **Dim Mode**. The screen can be switch off (**Screen Off**) or dimmed with different levels (**Level 1, 2 or 3**). If one of these options is set, the screen will be dimmed or switched off after a delay set by the **Dim Delay** parameter when any key is pressed. Once this has happened, pressing any key will switch the screen back on.



If **Dim Mode** is **Off**, the screen always remains bright.

By default, **Dim Mode** is set to **Level 2** (medium dim).

The power saver delay defines the delay time between the last use of any key and the start of the power saver mode. This delay period can be set from **5s** to **60m** with **Dim Mode** active.




<ENT>



Changing the colour scheme

The **Col. Scheme** item allows you to change the colour scheme of the screen from **Colorful** to **Black/white**.



6 MANAGING FILES – File

The **File** section allows you to manage the data and setup files stored in the instrument's memory.

The memory structure and files saving methods are described in Chapter [2.10](#).



The **File** section contains the following items that allow you to:

File Manager manage measurement results files,


Setup Manager manage only setup files located in the predefined SETUP directory.



Note: Items in the **File** list are only active when an SD card is inserted into the card slot behind the bottom cover of the instrument.



Note: Data files can only be saved on the SD card. Therefore, if there is no SD card in the instrument, no file can be created and **Logging** item is not available in the **Measurement** list.



There are three types of files generated by the instrument:

- Logger files containing measurement results (extension **.SVL**, icon)
- Wave files containing signal recording (extension **.WAV**, icon)
- Setup files containing measurement and instrument configuration (extension **.SVT**, icon)

Logger and Wave files are automatically created and saved with default names. You can define a specific logger file names in the **Logger Name** item (path: <Menu> / Measurement / Logging / Logger Set.) and a specific wave file name in the **File Name** item (path: <Menu> / Measurement / Logging / Wave Rec.).

The elements of the logger file structure depend on the selected function (**Lev. Met.**, **1/1 Oct.**, **1/3 Oct.**, **RT60**, **Dosimeter**, **STIPA**) and logging settings. These elements are as follows:

- main results, including results of statistical analysis,
- time histories of the measurement results,
- marker recordings,
- 1/1 or 1/3 octave analysis results,
- dosimeter results,
- RT60 analysis results,
- STIPA analysis results.

A detailed description of the structures of all file types is given in Appendix B.

6.1 MANAGING FILES – FILE MANAGER

The **File Manager** is used to check the contents of memory and to perform operations on the measurement files and directories such as: opening, renaming, deleting, viewing information, creating a new directory/file, and clearing memory.

In the **File Manager**, all file and directory names are in upper case. Directory names are blue and file names are green. Measurement files have icons and no extensions, other files have no icons but extensions.

The list of files and directories is displayed in the **File Manager** screen. Files are stored in hierarchically organised directories.

Pressing **<Enter>** on the highlighted directory/file will open the screen with the list of operations available for that directory/file.

Changing directories

To open a directory, select it and press the **►** key.

To return to the upper directory, press the **◀** key.


Creating a new directory

The first item in the **File Manager** list is **New Dir.**, which allows you to create a new directory.


To create a new directory, enter the directory in which the new one is to be created, select the **New Dir.** item and press **<Enter>**. The text editor screen will appear for entering the new directory name.

Memory properties

The last screen after pressing the **◀** key shows information about the instrument's memory (**SD Card**): name (**Disk Name**), free space (**Free Space**) and total memory space (**Capacity**).

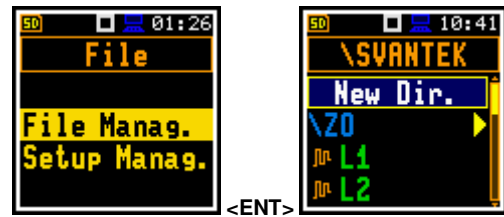

<ENT>



<ENT>




►



<ENT>



▼



6.1.1 Assigning the directory for saving data files – Working Directory

You can specify a directory for automatic saving of the measurement files. To do this, select the required directory and press **<Enter>**. Select the **Work. Dir.** item in the command list and press **<Enter>**.

All logger and wave files are then stored in this directory.



<ENT>



Note: The working directory name is not displayed on the screen, so you should remember the selected working directory!

6.1.1 Opening file/directory – Open


To open a file or directory, select the file/directory you wish to open and press **<Enter>**. Select **Open** from the command list and press **<Enter>**.

The **Open** command for a directory act as the **►** key (see Chapter 6.1).

The **Open** command for a file displays Summary results records.

You can change views and change displayed results as shown.

You can change the record to be displayed in the **File Info** view by selecting the record with the **◀/▶** key and switching to the desired view.

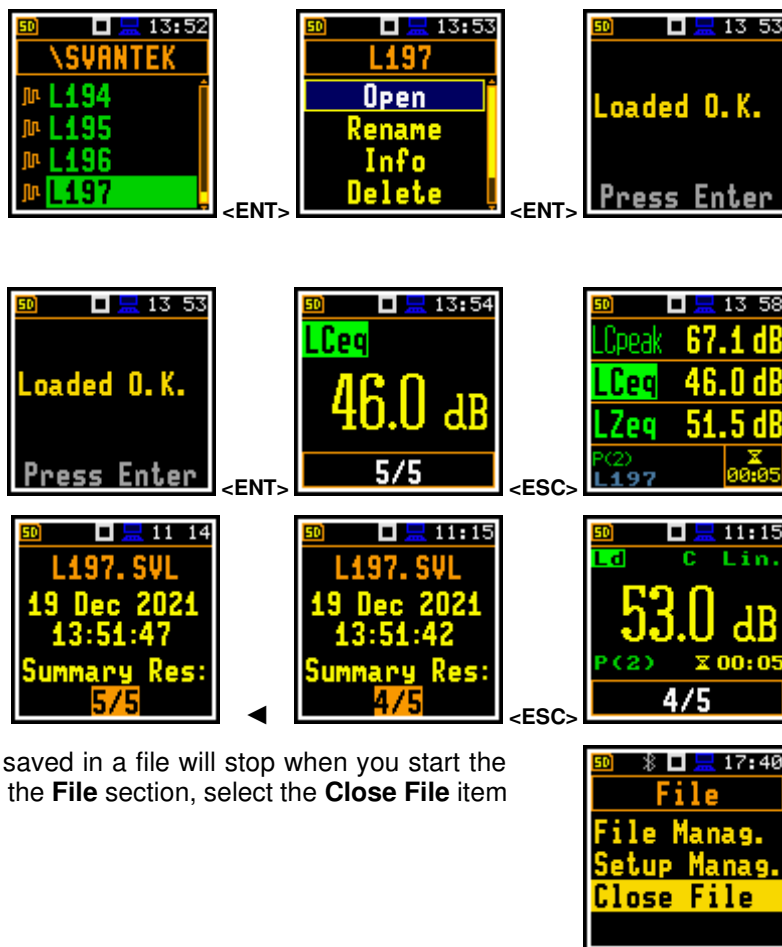

The preview of the summary results saved in a file will stop when you start the new measurement or when you open the **File** section, select the **Close File** item and press **<Enter>**.

6.1.2 Renaming file/directory – Rename

To rename a file or directory, select the file/directory to be renamed and press **<Enter>**. Select the **Rename** item from the command list and press **<Enter>**. The text editor screen will appear for you may enter the new file/directory name.



6.1.3 Viewing information about file/directory – Info

To obtain information about a file/directory, select the file/directory and press **<Enter>**. Select the **Info** item from the command list and press **<Enter>**. The instrument will display the information about the selected file/directory.



6.1.4 Deleting file/directory – Delete

To delete a file/directory from the file/directory list, select the file/directory to be deleted and press **<Enter>**. Select the **Delete** item from the command list and press **<Enter>**. The instrument will ask you to confirm this action as it cannot be undone.



6.1.5 Erasing memory – Erase Disk

To erase all files and directories from memory, select any file and press the **<Enter>** key. Select the **Erase Disk** item from the command list and press **<Enter>**. You should confirm this action as it cannot be undone.



Once the disc has been erased, the default directories will be restored.

6.2 MANAGING SETUP FILES – SETUP MANAGER

The **Setup Manager** allows you to save new setup files, load and delete them, view file information, and select the setup files that will be displayed in the setup screen when the instrument starts up.

All setup files are stored in the default **SETUP** directory.

The screen with the list of available operations on the setup files opens when the **<Enter>** key is pressed on the highlighted setup file.

Loading the setup file means that the settings stored in the loaded file become the active settings of the instrument.

If the right box of the setup file is checked, this setup will be in the list of setups when the instrument starts up, so that you can select a predefined setup at the beginning of the measurement session.




7 CONFIGURING INSTRUMENT – Instrument

The **Instrument** section is mainly related to the configuration of the hardware components of the instrument.

The **Instrument** section contains the following items that allow you to:

User Inter.	select the user interface option,
Battery	display information about current power source,
Keyboard	program keyboard functions,
Power Off	switch off the power to the unit when inactive,
USB	configure the USB interface; this item is available only in the Advanced interface,
Comm. Ports	configure the serial interface,
RS232 Stat.	check the status of the RS232 interface,
Self Vibr.	set the marker registration threshold for instrument self-vibration; this item is only available in the Advanced user interface,
RTC	set the Real Time Clock,
Unit Label	display instrument properties.

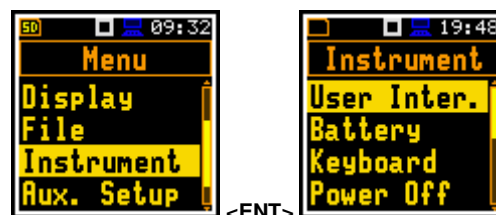

7.1 CHOOSING USER INTERFACE MODE – USER INTERFACE

The **User Inter.** item allows you to select the user interface option: **Start/Stop**, **Simple** or **Advanced**.

The **Simple** interface allows basic instrument settings, while the **Advanced** interface allows the full range of settings. Many screens therefore have different views in different interface options. The default value is **Simple**.

The **Start/Stop** option limits the user interface to only one **User Interface** item in the main **Menu** and measurement screens.




Note: If you change the interface from **Advanced** to another, you will always be asked “Do you restore the default value of the advanced settings?” If the answer is **No**, all settings of parameters that are not active in the **Simple** interface will remain unchanged. If the answer is **Yes**, these parameters will be reset to their default values.



7.2 CHECKING POWER – BATTERY

The **Battery** item allows you to check the status of the power source. The instrument can be powered by four rechargeable or standard alkaline AAA batteries or the USB-C interface.

The view on the display depends on the current power source.

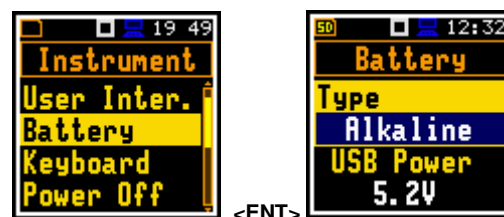


If the instrument is powered by internal batteries, the current battery voltage is displayed along with an approximate charge level.

Select the correct battery type for the correct detection of the battery state of charge: **Alkaline** or **Rechargeable**.



Note: Rechargeable batteries must be removed and charged using an external charger. They cannot be charged inside the instrument.

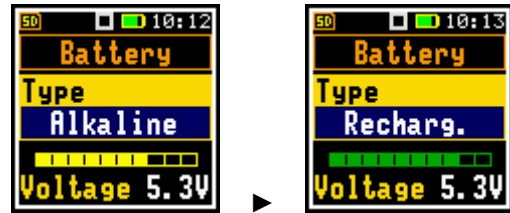

7.3 PROGRAMMING KEYBOARD FUNCTIONS – KEYBOARD

The **Keyboard** item allows you to program the operation of the **<Shift>** key and enable the keyboard to be locked and unlocked using four keys.



<Shift> key mode

In the **Shift** item you can choose between **Direct** and **2nd Function**. If the **Direct** option is selected, the **<Shift>** key works like a computer keyboard – to achieve the desired result, the second key should be pressed at the same time as **<Shift>**. If the **2nd Function** option is selected, the **<Shift>** key works like the virtual keyboard on a smartphone – the **<Shift>** key should be pressed first and then the second key. This allows you to operate the instrument with one hand. The default value is **Direct**.



Keyboard lock

The **Key Lock** item allows you to enable the keyboard lock. When **On** is selected, the **Fast Unlock** function becomes available. This function allows you to program the keyboard unlock code. The default value is **Off**.



Keyboard unlock

The unlock code can be programmed the following four items: **First Key**, **Second Key**, **Third Key** and **Fourth Key**. In each item, the user can select one of four arrow keys: **Left Key**, **Right Key**, **Up Key** or **Down Key**, the sequence of which generates the unlock code.




7.4 AUTOMATIC POWER OFF – POWER OFF

The **Power Off** item allows you to set the time after which the instrument automatically switches off if no key has been pressed during this time.

If **Inf** (infinite) value is selected, the instrument will not switch off automatically, but only manually.

The default value is **5 m**.

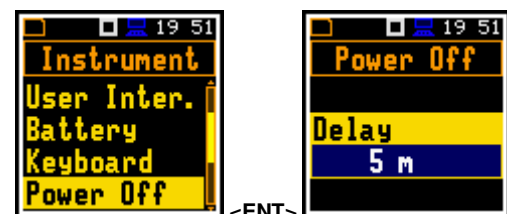

7.5 CONFIGURING THE USB INTERFACE – USB

The **USB** item allows you to select the transfer rate of the USB interface: **Full 12 Mbps** and **High 480 Mbps**. The default value is **High 480 Mbps**.



Note: For effective operation with the USB, the **High 480Mbps** speed mode should be used, however when the interference RF field strength may exceed the value of 3V/m, then it is recommended to switch to the **Full 12Mbps** speed mode.

7.6 SETTING INTERFACE PARAMETERS – COMMUNICATION PORTS

The **Communication Ports** item allows you to select the type of the **Serial Port** (**RS232** or **Bluetooth**) and set its parameters. The default value is **RS232**.

The **Serial Port** item allows you to toggle between **RS232** interface and **Bluetooth**.

In the case of **Bluetooth**, you must enter the **PIN** to pair another device with the instrument.

In the case of **RS232**, you must select the **Interface** type (interface cable **SP75/76** or SV 271 monitoring station controller **SD270(A)**), **Baud Rate** (1200, 2400, 4800, 9600, 19200, 38000, 57600 or 115200 bits/s) and the time limit for data transmission (**Time Out**). The default value of the **Time Out** parameter is 1 second, but this may be too short for printers that are not fast enough. In such cases the **Time Out** parameter should be increased.

Other RS 232 transmission parameters are fixed at **8 bits for data**, **No parity** & **1 Stop bit**.



7.1 CHECKING THE RS232 STATUS – RS232 STATUS

The **RS232 Stat.** item allows you to check the RS232 connection with the device set in the **Interface** item (path: <Menu> / Instrument / Communication Ports).

For example, if SV 971A is working with the SV 271 monitoring station, this screen should display the controller type, its firmware version, the transmission speed and the battery charge level.

If the RS232 port is not in use, the screen is blank.



7.2 SELF-VIBRATION MARKER – SELF VIBRATION


The **Self Vibr.** position allows you to define the self-vibration threshold of the instrument for marker registration. The special marker will be written to the file when instrument's self-vibration is higher than that defined in the **Marker Thr.** item.

This item is only available in the **Advanced** user interface.



7.3 PROGRAMMING THE INTERNAL REAL TIME CLOCK – RTC

The **RTC** item enables programming the internal Real Time Clock of the instrument. This clock is displayed in the top right corner of the display.

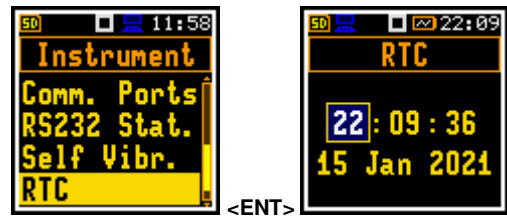

To edit the time or date, select the time or date field with the ◀ / ▶ or ▲ / ▼ key.




Use the ▲ / ▼ key pressed with <Shift> to change the value in the selected field.

Press <Enter> to confirm the selection. If you exit this screen with <ESC> will also save the new time.



7.4 CHECKING INSTRUMENT PROPERTIES – UNIT LABEL

The **Unit Label** item allows you to check the instrument model, the instrument and microphone serial numbers, the current software version installed and the relevant standards that the instrument complies with.

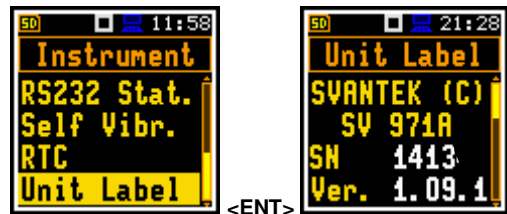

Note: The contents of the **Unit Label** should always be sent to SvanTek service department or official representative in the event of any problems encountered by the user during the normal operation of the instrument.

8 AUXILIARY SETTINGS – Auxiliary Setup

The **Auxiliary Setup** section provides additional functions that, for example, allow the user interface to be customised to meet specific user requirements and are not directly related to the hardware components of the instrument.




The **Auxiliary Setup** section contains the following items that allow you to:

- Language** select the language of the interface,
- Factory Set** restore the factory default settings,
- Comments** define the file name for recording voice comments; this item is only available in the **Advanced** interface,
- Leq & Lav** select the option to display the **Leq** and **Lav** results; this item is only available in the **Dosimeter** function and in the **Advanced** interface,
- Warnings** enable/disable the warnings displayed during normal operation of the instrument.

8.1 SELECTING THE INTERFACE LANGUAGE – LANGUAGE

The **Language** item allows you to select the language of the interface. The default language is **English**.

If the display shows an interface in an unknown language when the unit is switched on, the user can reset the unit by pressing three **<Shift/Enter/Start>** keys together while switching on the instrument. This will return the instrument to the default setup with the English interface.

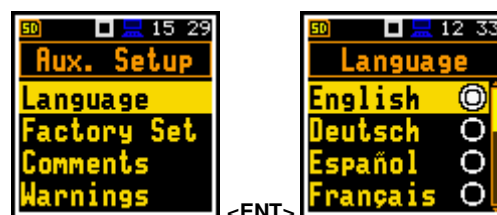

8.2 RESTORING FACTORY SETTINGS – FACTORY SETTINGS

The **Factory Set.** Item allows you to restore the default settings of the instrument.


Factory settings can be also restored by pressing three **<Shift/Enter/Start>** keys together while switching on the instrument.

After restoring the factory settings, the instrument asks if you want to keep the last calibration. If you select **No**, the factory calibration is restored and the new calibration record with the *Factory calibration* of the instrument is created in the **Calibration History** list (see Chapter [3.2.2](#)).




8.3 VOICE COMMENTS – COMMENTS

The **Comments** item allows you to specify the file name for the voice comments recording. This item is only available in the **Advanced** interface mode. You can record voice comments in all interface options.

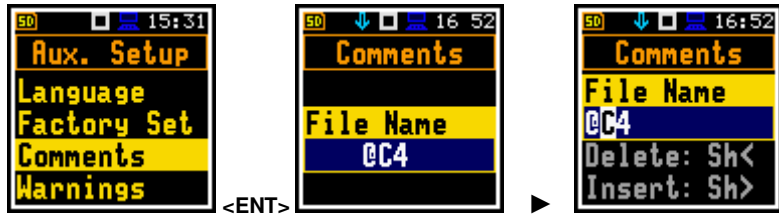


To record a comment, press the ◀, ▶ keys simultaneously when a measurement is stopped. This will bring up a screen asking which logger file is to be linked to the comment file - the previous one (**Prev.**) or the next one (**Next**). Pressing <Enter> will display the screen with the record command.

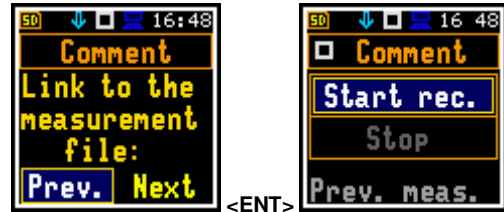

After starting the recording (**Start rec.**) with the <Enter> key, a red circle will start to flashing on the top line of the screen to indicate that the recording is in progress. This allows you to comment on the measurement. Press <Enter> to end the recording. The end of the recording is confirmed with the message "Saved O.K.".



The voice comment file is saved in the same working directory as a connected logger file with a name starting with @ and the icon .



8.4 DISPLAYING LEQ & LAV RESULTS – LEQ & LAV

The **Leq & Lav** item allows you to select the option to display the **Leq** and **Lav** results.

This item is only available in the **Dosimeter** function and in the **Advanced** interface. See the description of this function in Chapter [11.7.1](#).



8.5 ACTIVATING WARNINGS – WARNINGS


The **Warnings** item allows you to enable messages to be displayed during the normal operation of the instrument.



If **Logging** is enabled, the instrument will generate a warning if you start a measurement without logging the results to a file (i.e., if the **Logger** is disabled).




If **Power Off** is enabled, any attempt to switch off the instrument during a measurement will result in a "Measurement in progress" warning. You should stop the measurement to be able to switch off the instrument. When the measurement is complete, the "Power Off" warning will become active. You should then confirm that you wish to switch off the instrument.




If **Preampl.** is enabled, a warning is displayed if the instrument detects that there is no preamplifier attached to the instrument's input.

If **Changes** is enabled, the instrument displays the warning message in the case when some parameters were changed, but the list of parameters was exit with the <ESC> key.



9 PRINTING REPORTS – Report

The **Report** section allows you to configure and print measurement reports in a predefined format.

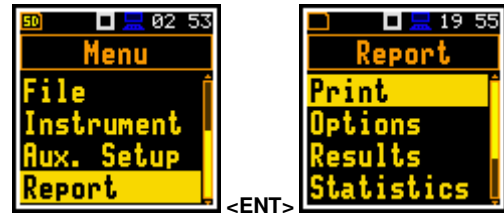


The **Report** section contains the following items that allow you to:

Print	print measurement results to the default printer,
Options	set report options,
Results	select the measurement results to be included in the report,
Statistics	select statistics to be included in the report,
Spectrum	select 1/3 octave bands to be included in the report,
Printer	select the number of characters in the report line.

To obtain a report, connect the instrument to the RS 232 port of the printer using the **SV 76** interface. This hardware interface is hidden inside the Cannon type 9-pin RS 232 connector. At the other end of the **SV 76** interface, which itself looks like a cable, is the USB-C connector which should be plugged into the USB-C socket on the instrument.

Make sure that the RS232 port is correctly configured.

To do this, in the **Communication Ports** screen (*path: <Menu> / Instrument*), select **RS232** in the **Serial Port** item and set the transmission speed (**Baud Rate**) and the time limit for data transmission (**Time Out**).

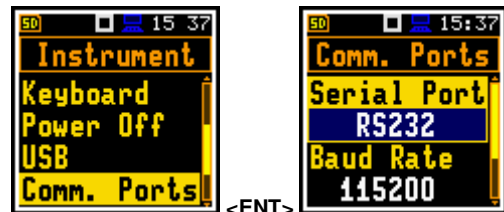

Printers with a USB interface only are not currently controlled by the instrument.



Note: Switch off the instrument before connecting it to an external device (e.g., printer or PC).



Note: All reports are printed in the character format using the ASCII set on either A4 or A5 size paper.

9.1 PRINTING MEASUREMENT RESULTS – PRINT

The **Print** item starts a report print on the connected printer or PC.


After pressing **<Enter>** the instrument checks its status. If the measurement is in progress, printing is not possible and a message to this effect is displayed.

If the measurement has already been performed and results are available, the data will be transferred from the instrument to the connected printer. The instrument returns to the **Report** list when all the data has been transferred.

If no measurements have been taken, the next message is displayed.

The timeout message is displayed if the printer (or PC) is not connected or there is some other reason for not receiving data. The instrument waits for a reaction from the user (any key should be pressed except **<Shift>**) and when a key is pressed it returns to the **Report** list.

Below is an example of a report printout.



SVANTEK (C) SV 971A S/N:39039

2017-05-22 13:59:24 T:00:00:05

Profile 1 Slow A

LCpeak:	82.9	Ld	:	55.9
LASmax:	77.0	LEPd	:	55.9
LASmin:	58.8	Ltm3	:	74.2
LAS	: 58.8	Ltm5	:	77.0
LAeq	: 55.9	OVL	:	0.0
LAE	: 62.9			

Profile 2 Slow C


LCpeak:	82.9	Ld	:	60.8
LCFmax:	80.0	LEPd	:	60.8
LCFmin:	53.3	Ltm3	:	77.2
LCF	: 60.3	Ltm5	:	80.0
LCeq	: 60.8	OVL	:	0.0
LCE	: 67.8			

Profile 3 Slow Z

LZpeak:	83.3	Ld	:	68.7
LZFmax:	81.4	LEPd	:	68.7
LZFmin:	60.1	Ltm3	:	78.8
LZF	: 65.6	Ltm5	:	81.4
LZeq	: 68.7	OVL	:	0.0
LZE	: 75.7			

9.2 SELECTING PRINT OPTIONS – OPTIONS

The **Options** item allows you to specify the report content, select profiles, results for those profiles, statistics and spectra to be included in the report.

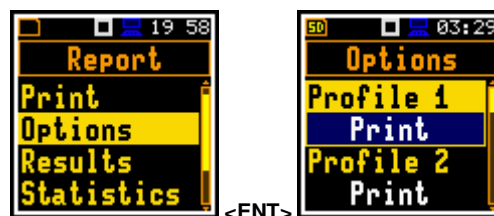

You can include (**Print**) or exclude (**Off**) results for each profile (**Profile x**) from the report.

You can exclude all the main results (**Results**) from the report (**Off**), include them all (**Print All**) or select results for the report (**Pr.Selected**). In the latter case the **Results** item appears in the **Report** menu.



You can exclude all statistics (**Statistics**) from the report (**Off**), include them all (**Print All**) or select essential statistics for the report (**Pr.Selected**). In the latter case, the **Statistics** item appears in the **Report** menu.



In case of 1/1 octave or 1/3 octave analysis functions, it is also possible to exclude all Leq, Lmax, Lmin and Lpeak spectra (items: **Leq Spect.**, **Lmax Spect.**, **Lmin Spect.**, **Lpeak Spect.**) from the report (**Off**), to include all bands of 1/1 or 1/3 spectra in the report (**Print All**) or selected bands (**Pr.Selected**). In the latter case the **Spectrum** item appears in the **Report** menu.

You can include (**Print**) or exclude (**Off**) units of the results from the report.




9.3 SELECTING RESULTS FOR THE REPORT – RESULTS

The **Results** item allows you to select the results to be included in the report for the selected profiles: **Lpeak**, **Lmax**, **Lmin**, **L**, **DOSE**, **D_8h**, **PrDOSE**, **LAV**, **Leq**, **LE**, **SEL8**, **E**, **E_8h**, **Lden**, **LEPd**, **PSEL**, **Ltm3**, **Ltm5**, **PTC**, **PTP**, **ULT**, **TWA**, **PrTWA**, **Lc-a**, **LR1**, **LR2** and **OVL**.




9.4 SELECTING STATISTICS FOR THE REPORT – STATISTICS

The **Statistics** item allows you to select the statistic levels from **N1** to **N10** to be included in the report.

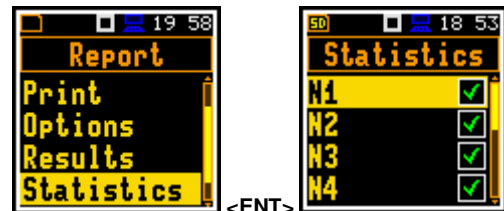

9.5 SELECTING SPECTRA FOR THE REPORT – SPECTRUM

The **Spectrum** item allows you to select the 1/1 or 1/3 octave bands to be included in the report for the **Leq**, **Lmax**, **Lmin** and **Lpeak** spectra, based on their centre frequencies.

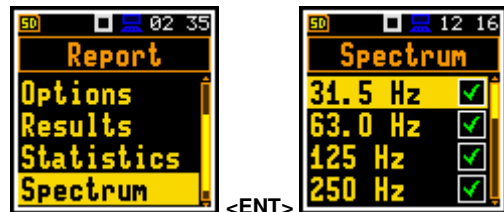

9.6 PRINTER SETTINGS – PRINTER

The **Printer** item allows you to set the number of characters in the report lines – from 20 to 500. The default value is 32.




10 1/1 AND 1/3 octave ANALYSER

The real-time 1/1 octave or 1/3 octave analysis is performed in parallel with the SLM or Dosimeter measurements. All digital band-pass filters (eleven 1/1 octave filters with centre frequencies from 16.0 Hz to 16 kHz and thirty-five 1/3 octave filters with centre frequencies from 8 Hz to 20 kHz; in the “base ten” system) work in real-time with the weighting filters (**Z**, **A**, **B** or **C**) and the LEQ detector (**Linear**, **Fast** or **Slow**). This allows pre-weighting of the spectrum with one of the selected broadband filters if required by the application, e.g., to provide hearing protection when controlling high noise levels in the workplace.

For each 1/1 octave or 1/3 octave band, the Leq, Peak, Min or Max result is calculated and displayed as a bar on the spectrum graph. The results of 1/1 and 1/3 octave analysis (spectra) can be examined on a display in the **Spectrum** view.


A vertical cursor can be used to read the spectrum value.

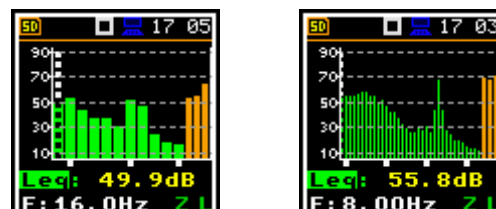

In addition to the band results, three totals are measured and displayed as three additional bars on the spectrum plot. Parameters for Total values (e.g., filters) are set by default and cannot be changed: Total 1 – A filter, Total 2 – C filter, Total 3 – Z filter.

10.1 SELECTING 1/1 OCTAVE OR 1/3 OCTAVE FUNCTION

To select the 1/1 octave or 1/3 octave analysis function, open the **Meas. Funct** item, select the **1/1 Octave (1/1.&Dose)** or **1/3 Octave (1/3.&Dose)** option and press **<Enter>**.

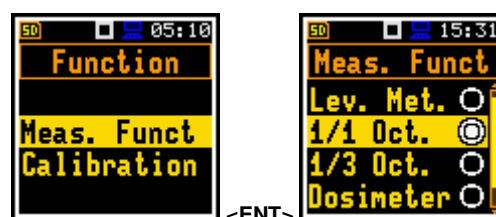

Note: The 1/1 octave and 1/3 octave analysis functions are optional and should be unlocked by entering the activation code in the text editor screen that opens after the first attempt to select them. Once unlocked, these options are permanently available.


10.2 1/1 OCTAVE OR 1/3 OCTAVE ANALYSER CONFIGURATION

10.2.1 General settings for 1/1 and 1/3 octave analysis – General Settings

The execution of 1/1 or 1/3 octave analysis depends on a set of parameters configured in the **Measurement** section.

The averaging of the results for each band is performed during the **Integration Period** and is repeated the number of times set in **Repetition Cycles**.

Both parameters are defined in the **General Settings** list.



10.2.2 Selecting measurement range for 1/1 and 1/3 octave analysis – Range

For the **1/1 Octave** or **1/3 Octave** functions, you can select the measurement ranges specified in Appendix C, named as **Normal** and **Low**.

The input range is selected in the **Range** screen of the **Measurement** list.



For the **1/1.&Dose** or **1/3.&Dose** functions, the measurement range is set to **Normal** and cannot be changed.



Note: The ranges in the above screens correspond to the microphone with the sensitivity within the declared range $25 \div 37$ mV/Pa (see Appendix C). If the microphone sensitivity is other than $25 \div 37$ mV/Pa, the range will change automatically.

10.2.3 Logging of the 1/1 and 1/3 octave spectra – Logging

Spectra are always logged together with Summary results in a logger file with **Integration Period** step. The first requirement is that the **Logger** is switched on (path: <Menu> / Measurement / Logging / Logger Setup / Logger: On).




The **Leq** and **Lpeak** results of the 1/1 or 1/3 octave analysis can also be stored in the logger file with the step defined by the **Logger Step** parameter (path: <Menu> / Measurement / Logging / Logger Setup). Activation of spectrum storage in the logger file with the **Logger step** is done by checking the **Peak Spectrum** or **Leq Spectrum** item.




10.2.4 Setting parameters of the 1/1 and 1/3 octave analysis – Spectrum

If the **1/1 Octave** or **1/3 Octave** functions are active, the additional item (**Spectrum**) appears in the **Measurement** list.

The **Spectrum** item allows you to select the pre-weighting broadband frequency filter and LEQ detector for the 1/1 or 1/3 octave analysis.



<ENT>




The following weighting filters are available for the 1/1 and 1/3 octave analysis in the **Filter** item:


- **A** class 1 according to IEC 651 and IEC 61672-1:2013,
- **C** class 1 according to IEC 651 and IEC 61672-1:2013,
- **Z** class 1 according to IEC 61672-1:2013,
- **B** class 1 according to IEC 651.

Filter characteristics are given in Appendix C.

The **Detector** item defines the RMS detector for the 1/1 octave or 1/3 octave bands and Total values: **Linear**, **Fast** or **Slow**.



<ENT>



Note: Total values for 1/1 octave or 1/3 octave analysis may differ from the results for a level meter if the RMS detector settings are different.

10.3 CONFIGURING 1/1 AND 1/3 OCTAVE SPECTRA VIEWS

The **Display** section contains items that allow you to customise the spectrum view:

Display Modes switch on the **Spectrum** view,

Display Scale adjust the scale of the spectrum plot and switch the grid on/off,


Spectrum View select the spectra to be viewed: instantaneous, averaged, maximum or minimum.

10.3.1 Presentation of the 1/1 and 1/3 octave spectra


The **Spectrum** item in the **Display Modes** list becomes available for the **1/1 Octave** and **1/3 Octave** functions and allows you to enable the spectrum view (**Spectrum**).

Spectrum view fields


1. Spectrum graph
2. Type of filter and RMS detector
3. Type of result and its value for the cursor position
4. Central frequency for the cursor position
5. Cursor position
6. Total values

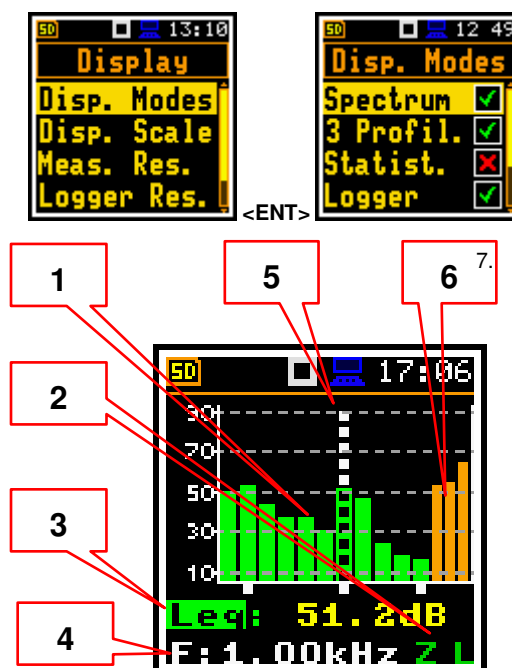


Use the **▲ / ▼** keys to move the spectrum plot up or down in relation to the X-axis.

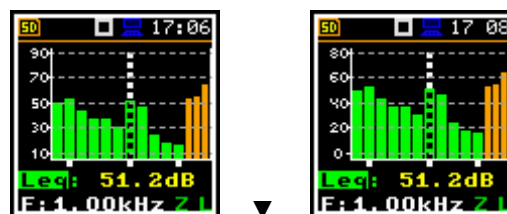


Use the **◀ / ▶** key to change the cursor position. The central frequency of the band and corresponding dB value are displayed in the line below the plot.

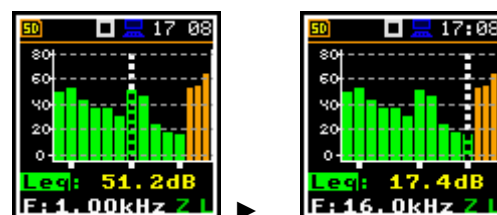

Spectrum view can be changed with the **<Enter>** key. The second spectrum view doesn't have the Y scale and therefore has wider bars.

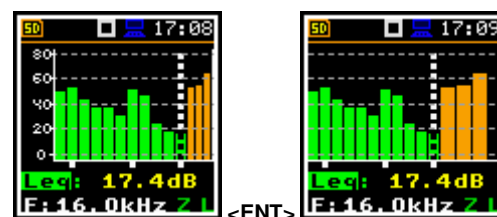

The **Total** values are calculated using the **A**, **C** and **Z** filters and their values are displayed at the bottom line of the screen when the cursor is placed on the corresponding orange bar.

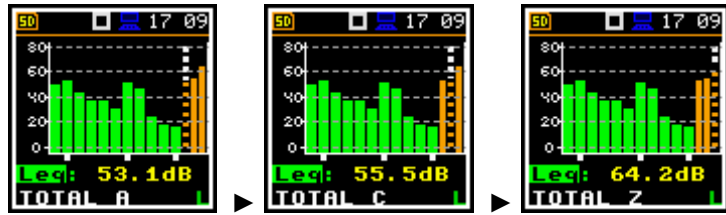

10.3.2 Adjusting the spectrum plot scale – Display Scale

The **Display Scale** item allows you to change the scale of the spectrum plot and toggle the grid and automatic scale on/off.




Scaling vertical axis

The **Dynamics** item allows you to select the desired dynamic range of the spectrum plot: **10dB**, **20dB**, **40dB**, **80dB** and **120dB**.

The attached example shows a spectrum view with 80 dB and 40 dB ranges.


Switching the grid on/off

The **Grid** item switches the grid on/off in the spectrum view.

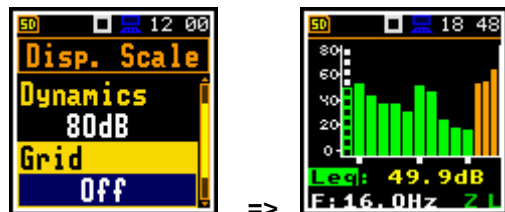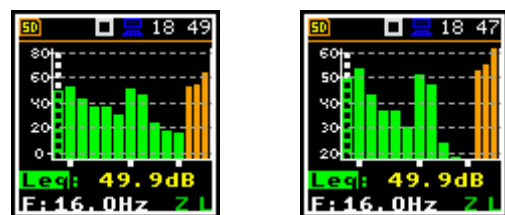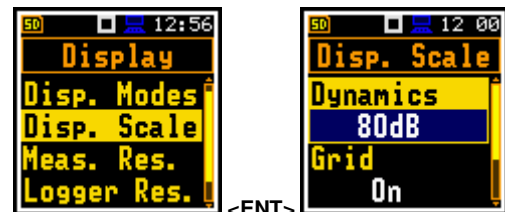

Automatic Y-scale adjustment

The **Autoscale** item switches on or off the automatic adjustment of the dynamic range of the Y-axis scale to the actual difference between the lowest and highest measured octave or third octave results. The example shows the changes in the scale after a sudden increase in sound pressure level.

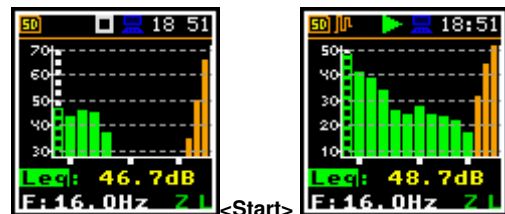


10.3.3 Selecting spectra to view – Spectrum View

The **Spectrum View** item, which appears in the **1/1 Octave** or **1/3 Octave** functions, allows you to select different spectra to be displayed in the **Spectrum** view.


In the **Spectrum Type** item, you can select the type of spectrum to be displayed as a bar plot:

- **Instantaneous**, obtained for the Leq results integrated over 100 ms,
- **Averaged**, obtained by averaging the instantaneous spectra for the elapsed time [0, Integration Period],
- **Lp-k**, obtained for the Lpeak results for the elapsed time [0, Integration Period],

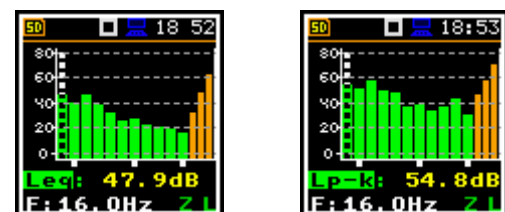

- **Max**, obtained as the maximum instantaneous spectrum for the elapsed time [0, Integration Period] or
- **Min**, obtained as the minimum instantaneous spectrum for the elapsed time [0, Integration Period].

Minimum and maximum spectra can be displayed in the same plot as the main spectrum if the **Max** and/or **Min** parameter are enabled.

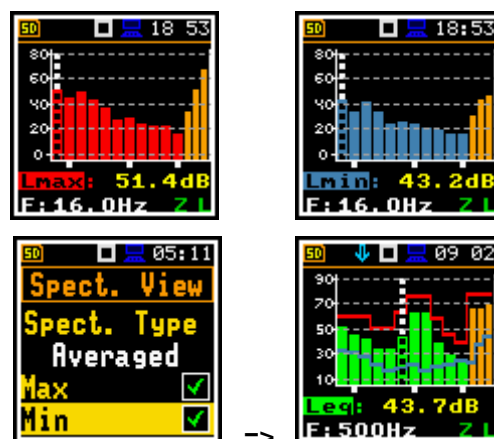


11 SOUND EXPOSURE METER – DOSIMETER

The instrument operates as a Sound Exposure Meter (Dosimeter) in much the same way as a Sound Level Meter (SLM) measuring basic dose parameters in addition to SLM results. This chapter describes settings specific to the Dosimeter.

11.1 SELECTING THE DOSIMETER FUNCTION

To select the **Dosimeter** function, enter the **Function** section, select the **Meas. Funct** item and press <Enter>. From the **Meas. Funct** list, select the **Dosimeter** function and press <Enter>.

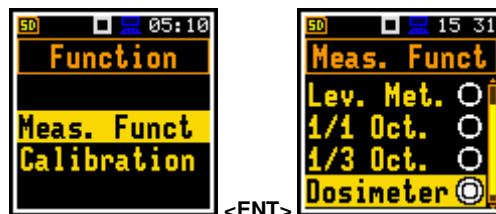


11.2 SETTING GENERAL PARAMETERS – GENERAL SETTINGS

Most of the general settings of the **Dosimeter** function are similar to those of the **Level Meter** function (see Chapter 4.1). In addition, the dosimeter has five programmable automatic pauses.

Programmable automatic pauses

The automatic pauses can be switched off (**Off**) or can be programmed based on the RTC time (**On**).

If **Pause** is **On**, two additional items appear allowing you to set the **Pause Begin** and **Pause End** times.

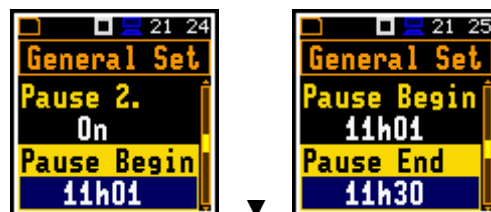

Note: In the **Simple** interface, the **Pause** parameters are hidden, but the instrument uses settings previously defined in the **Advanced** interface or default settings (**Off**).


11.3 SETTING PROFILE PARAMETERS – PROFILE X

The parameters of the three profiles can be set in the **Profile x** lists of parameters.

The following parameters can be programmed independently for each profile: weighting filter (**Filter**), peak filter (**Filter Peak**) and LEQ detector type (**Detector**), criterion level (**Crit. Level**), threshold level (**Thr. Level**), exchange rate (**Exch. Rate**), thresholds - **ULT Thresh.** and **PTC Thresh.**

Weighting filter

- Z** Class 1 according to IEC 61672-1:201,
- A** Class 1 according to IEC 651 and IEC 61672-1:2013,
- C** Class 1 according to IEC 651 and IEC 61672-1:2013,
- B** Class 1 according to IEC 651,
- LF** low frequency filter according to China requirements.

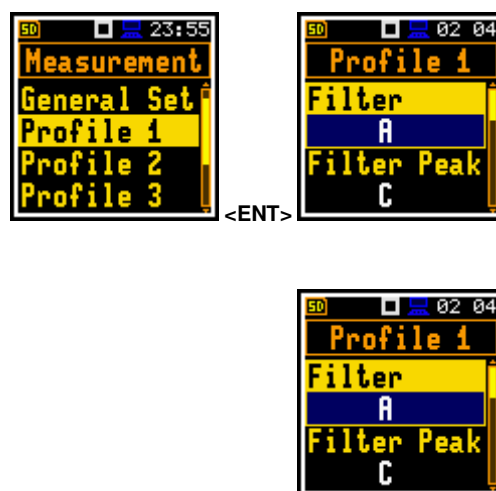

LEQ detector

The following LEQ detectors are available in the instrument: **Imp.**, **Fast** and **Slow**.

Dosimeter specific parameters can be set in accordance with the OSHA HC (Occupational Safety and Health Administration - Hearing Conversation), OSHA PEL (Occupational Safety and Health Administration – Permissible Exposure Level) and ACGIH standards.


Criterion Level is a steady noise level permitted for a full eight-hour work shift: **60dB, 65dB, 70dB, 75dB, 80dB, 84dB, 85dB, 87dB, 90dB**.

Threshold Level is a noise level limit below which the dosimeter does not accumulate noise dose data: **None, 60dB, 65dB, 70dB, 75dB, 80dB, 85dB, 90dB**.

Exchange Rate is an amount by which the permissible sound level may increase if the exposure time is halved: **2, 3, 4, 5, 6**.


ULT Threshold Level (Upper Level Time) is a threshold level for calculating of the ULT results: **70dB ÷ 140dB**.

PTC Threshold Level (Peak Threshold Counter) is a threshold level for calculating of the PTC results: **70dB ÷ 140dB**.




11.4 CHECKING THE MEASUREMENT RANGE – RANGE

The measurement range for the **Dosimeter** function is set to **Normal** and cannot be changed. See Appendix C for a detailed description of the measurement range parameters.




<ENT>



11.5 SETTING THE EXPOSURE TIME – EXPOSURE TIME

The **Exp. Time** item allows you to set the workday exposure time used to calculate the **LEPd** results (see Appendix D).



<ENT>




11.6 SETTING ALARM THRESHOLDS FOR DOSE METER RESULTS – ALARM

The **Alarm** item is active only in the **Dosimeter** function and allows you to program the alarm thresholds for three profiles (**Thresh. P1 (2,3)**).



The thresholds can be set for the following measurement results in ranges:

- DOSE:** 1÷200%,
- D_8h:** 1÷200%,
- PTC:** 1÷1000,
- ULT:** 1÷60s.


If **Off** is selected, the alarm is disabled.



<ENT>




<ENT>



The alarm is signalled on a special screen with the **Alarm** text in a flashing frame and exceeded the profile thresholds.

For example, with these settings, the alarm screen will look like this.


To exit the alarm screen, press any key.

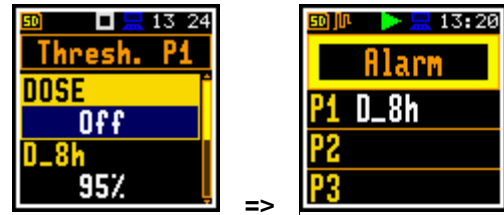

11.7 DISPLAYING DOSIMETER RESULTS

The **Dose Meter** function measures and displays the following results: **TIME**, **Lpeak**, **Lmax**, **Lmin**, **L**, **DOSE**, **D_8h**, **PrDOSE**, **LAV**, **Leq**, **LE**, **SEL8**, **E**, **E_8h**, **LEPd**, **PSEL**, **Ltm3**, **Ltm5**, **Ln**, **PTC**, **PTP**, **ULT**, **TWA**, **PrTWA**, **Lc-a**, **EX**, **SD** and **OVL**.

Results can be enabled or disabled in the **Dosimeter results** screen (*path: <Menu> / Display / Meas. Res. / Dosim. Res.*).

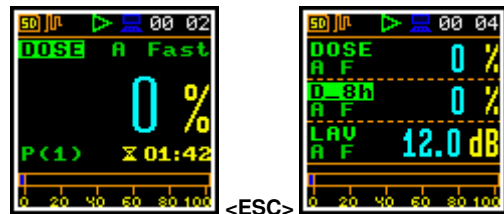


11.7.1 Displaying of Leq & Lav results – Leq & Lav

The **Leq & Lav** item allows you to select the way the **Leq** and **Lav** results are to be displayed.

If **Both** is selected, **Leq** and **Lav** will always be displayed together.

If **Mutual Exclusive** is selected, the rule is:

- for an **Exchange Rate** equal to 3, **Leq** is displayed and **Lav** is not,
- for an **Exchange Rate** other than 3, **Lav** is displayed and **Leq** is not.

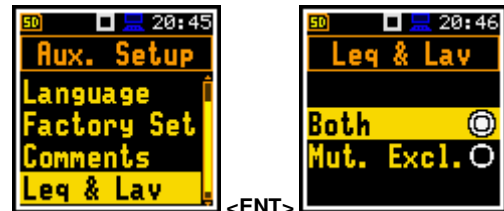

12 REVERBERATION TIME MEASUREMENTS – RT60

The **RT60** analysis is an optional function of the SV 971A that provides reverberation time calculation for 1/1 octave bands (from 63 Hz to 8 kHz) or 1/3 octave bands (from 50 Hz to 10 kHz) and three total RMS levels (**A**, **C** and **Z** weighted). The entire measurement process and calculations implemented in the SV 971A comply with the ISO 3382 standard.

The reverberation time of a room can be measured with the SV 971A using two measurement methods: Impulse Response Method (**Impulse**) and Interrupted Noise Method (**Decay**). The choice of method depends on the type of sound source used. The **Impulse** method is intended for measurements with an impulsive sound source (e.g., gunshot, petard explosion), whereas the **Decay** method is intended for measurements when the room is excited by a broadband or narrowband sound noise source (usually pink noise). For more details on the measurement and calculation process, see Appendix E.

The reverberation time analysis used in the instrument consists of two parts:


1. The measurement part in which the acoustic response of the room is registered.
2. The calculation part in which the reverberation time (**EDT**, **RT20** and **RT30**) is calculated for the measured room response.



Note: It is recommended that you familiarise yourself with Appendix E before proceeding. This chapter only describes how to navigate the instrument, while Appendix E provides definitions and describes reverberation time measurements.

12.1 SELECTING THE RT60 FUNCTION

To activate the **RT60** function, enter the **Function** section, select the **Meas. Funct** item and press <Enter>. In the **Meas. Funct** screen, select the **RT60** function and press <Enter>.

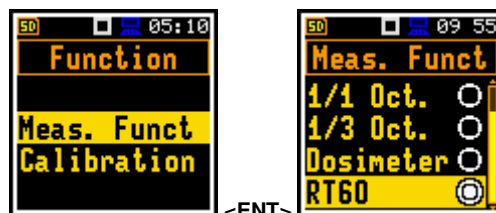

Note: The **RT60** function is optional and should be unlocked by entering the activation code in the text editor screen that opens after the first attempt to select this function. Once unlocked, this option is permanently available.

12.2 SETTING RT60 PARAMETERS – RT60 SETTINGS


The execution of the **RT60** analysis depends on certain parameters that can be set in the **Measurement** section screens: **RT60 Settings**, **Compensation Filter** and **Range**.

The **Range** screen only displays the **Normal** measurement range, which cannot be changed (see Chapter 4.6).

The **Compensation Filter** item, which only appears in the **Advanced** interface, allows you to switch on the required compensation filter (see Chapter 4.7). When the **RT60** function is enabled, the **Field Compensation** is always set to **Free Field**.

Other measurement parameters are set by default:



- **LEQ Integration:** Linear
- **Profiles / Detector:** Slow
- **Spectrum / Filter:** Z
- **Spectrum / Detector:** Linear



The **RT60 Settings** list allows you to select the method for **RT60** calculations, define the name of the file where the registered data will be collected, and other parameters for **RT60** calculations.

The **Start Delay** item defines the delay between the moment the **<Start>** key is pressed and the start of the actual measurement.

The **Method** item allows you to select the method for **RT60** calculations: **Decay** or **Impulse**. Both methods are described in Appendix E.

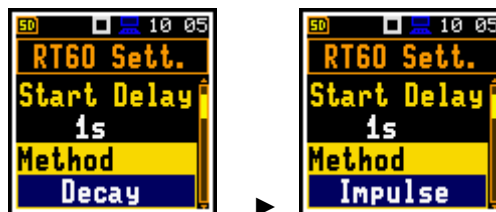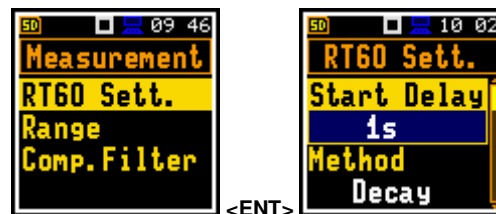

The **Recording Time** item allows you to define the recording time of the measurement data (sound pressure level decay curve). Data recording starts when the trigger condition occurs. The recording time can be set in the range **1s ÷ 30s** or **Auto**.


If **Auto** is selected, the instrument decides when to stop recording. The default time step is 2ms.

The **Time Step** item allows you to define the time step of the data recording (sound pressure level) in the file: **2, 5, 10, 20, 50 ms**.



The **Averaging** item allows you to enable averaging of the reverberation time results from several measurements.

When this item is **On**, the new **RT60 Aver.** screen is available in the measurement mode.




=>



The **Noise Mar.** item allows you to define the margin value for the calculated noise level (for more detail see Appendix E). This parameter can be set in the range **0.0 dB ÷ 20.0 dB** with 0.1 dB step (default value is **10.0 dB**).

The **Octave** item allows you to define the bands (**1/1** or **1/3**) the **RT60** analysis is performed.



The **Freq. Range** item allows you to define the frequency range for 1/1 or 1/3 octave calculations:

- for 1/1 octave: **63Hz-4kHz** (7 bands) or **63Hz-8kHz** (8 bands).
- for 1/3 octave: **50Hz-5kHz** (21 bands) or **50Hz-10kHz** (24 bands).



The **Logger Name** item allows you to specify the name of the logger file in which the **RT60** analysis data will be recorded. The name can be up to eight characters long. Press the **< / >** key to open the screen with the text editor.



▶






The **Level** item allows you to define the threshold level of the sound source for triggering the RT60 measurement. If the measured sound is below the **Level** value, the RT60 measurement will not start. The parameter can be set in the range $24 \div 136$ dB with 1 dB step (default value is **100dB**).



12.3 STARTING RT60 MEASUREMENTS

Measurements using the Decay method

- Set parameters for **Decay** RT60 measurements. The most commonly used setup is as follows.
 - Method:** Decay
 - Recording Time:** Auto
 - Time Step:** 2ms
 - Averaging:** On
 - Noise Mar.:** 10.0dB
 - Level:** 100dB.
- Place the sound source in the room to be measured (for the location of the sound source, see the ISO standard for measuring reverberation time).
- Place the microphone at one of the selected measurement points (for the location of the measurement points, see the ISO standard for measuring reverberation time).
- Switch on the sound source.
- Start the measurement by pressing the **<Start>** key. While the instrument is waiting for the trigger condition to be met, the **LAeq** result will be displayed and when the signal has stabilised, the instrument will prompt you to turn off the sound source.
- Switch off the sound source (the source should be left on long enough for the acoustic field to stabilise). Once the trigger condition has been met, the instrument collects data and returns the RT60 table for 1/1 octave or 1/3 octave bands.

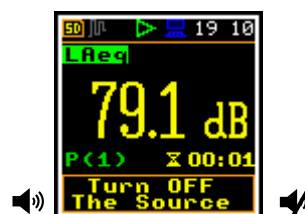

Note: It is necessary to switch on the sound source before starting the measurement due to the trigger requirements (see Appendix E for details). If it is necessary to start the instrument before switching on the sound source, it is recommended to use the higher **Start Delay** value.

Measurements using the Impulse method



- Set parameters for **Impulse** RT60 measurements. The most commonly used setup is as follows.
 - Method:** Impulse
 - Recording Time:** Auto
 - Time Step:** 10ms
 - Averaging:** On
 - Noise Mar.:** 10.0dB
 - Level:** 100dB
- Place the microphone at one of the selected measurement points (for the location of the measurement points, see the ISO standard for measuring reverberation time).





Note: The correct value of the sound level trigger threshold should be set well above the background noise and well below the maximum sound level emitted by the impulse source.



3. Start the measurement by pressing the **<Start>** key. While the instrument is waiting for the trigger condition to be met, the **LAeq** result will be displayed.
4. Release the impulse sound source. When the trigger condition is met, the instrument collects data and returns the RT60 table for 1/1 octave or 1/3 octave bands.



Note: During data collection, all other sound sources in the tested room should be suppressed to avoid affecting the measurement results.



12.4 VIEWING RT60 RESULTS

The **RT60** measurement results for all 1/1 or 1/3 octave bands and three Total values are presented in a table.



The table shows the next results of the reverberation time for:

- **EDT** - early decay time,
- **RT20** - reverberation time calculated at 20 dB dynamics,
- **RT30** - reverberation time calculated at 30 dB dynamics.




Note: If "- N -" text appears in the RT indicator field, it means that for this band with the selected parameters (**Noise Mar.**) the required measurement conditions were not fulfilled to obtain the results (for more details see Appendix E).

12.5 AVERAGING RT60 RESULTS


If **Averaging** is On, you can average the results of successive measurements by following the steps below:

1. While in the RT60 view, press the **<Left>** key from the **EDT** column or the **<Right>** key from the **RT30** column to access the **RT60 Aver.** screen.




The **Meas.No** item displays the number of the measurement that has been averaged so far.

2. From the **RT60 Aver.** screen, press the **<Enter>** key to confirm averaging.




<ENT>



As a result, three additional columns appear in the RT60 table: **AEDT**, **A20** and **A30**.

When you start a new measurement and obtain results, you can perform averaging with previously averaged results as per steps 1 and 2 above. The **Meas.No** will be increased by one and columns **AEDT**, **A20** and **A30** will show new results averaged with previous results.

To clear averaging, select **Clear** from the **RT60 Aver.** screen, press **<Enter>** and confirm to clear.



<ENT>



13 STI CALCULATIONS – STIPA

The Speech Transmission Index (STI) is used to measure the deterioration of speech intelligibility caused by the transmission channel. The STI method uses a test signal applied to the transmission channel and an analysis of the received test signal. The speech transmission quality of the channel is determined and expressed as an STI value between 0 and 1.

Applications of STI include evaluation of sound reinforcement and emergency systems, communication channels, speech intelligibility, communication in rooms and auditoriums, etc.

STIPA (speech transmission index for public address systems) is an STI derived approach developed for fast measurement of electro-acoustic and acoustic environmental effects that affect speech intelligibility in room acoustics and/or public address systems.

STIPA calculations are performed in SV 971A according to IEC 60268-16:2011.



Note: *Svantek also provides applications (BA Assistant or Building Acoustics Pro) for mobile devices that perform STIPA measurements using Svantek measuring instruments (including SV 971A) with a more convenient user interface (see user manuals for these applications).*

13.1 STI METHOD BACKGROUND

The STI method is based on measurements of the STI test signal comprising seven octave band noise signals corresponding with the octave bands from 125 Hz up to 8 kHz. Each noise carrier is modulated with one or more modulation frequencies at one-third octave intervals ranging from 0,63 Hz up to and including 12,5 Hz. Such a test signal which simulates speech fluctuations is reproduced in a room or through a communication channel and received at a listener position (superimposed by distortions presented in the room like echoes or noise) by means of omnidirectional microphone.

The STI method determines the modulation transfer function $m(F)$ – the reduction in modulation depth per modulation frequency - of the transmission channel for the seven octave bands. The RMS level of each octave band carrier matches the relative level of the average, long-term spectrum of the speech material. Each octave band has a contribution to speech intelligibility which is weighted according to that band. The weighted sum of these transmission index values is used to determine the overall STI value for the transmission channel.

The STIPA method uses two modulation frequencies per octave band, generated simultaneously, giving a total of 14 modulation indices.

13.2 SELECTING THE STIPA FUNCTION

To activate the **STIPA** function, enter the **Function** section, select the **Meas. Funct** item and press <Enter>. In the **Meas. Funct** screen, select the **STIPA** function and press <Enter>.



Note: *The **STIPA** function is optional and should be unlocked by entering the activation code in the text editor screen that opens after the first attempt to select this function. Once unlocked this function is permanently available.*

13.3 STIPA MEASUREMENT AND CALCULATION PROCESS

STI measurements usually refer to objects (buildings), which may consist of several areas (rooms), in which measurements are made at a certain number of points (in practice, from 1 up to several dozen). In addition, especially when assessing speech intelligibility in a room directly, i.e. without an amplification system, tests are performed for a given number of source positions (in practice from one to several). A given area may be tested in several configurations, for example, a theatre auditorium with the curtain raised and lowered, or a railway vehicle at rest and in motion. The result for a given point is obtained from several measurements (in practice from 1 to 6) - most often as an average. Analyses are performed independently for areas in a given configuration.

13.3.1 Measured results

The **STIPA** function allows measurement and calculation of the following results:

- **STI** - Speech Transmission Index representing the speech transmission quality in terms of intelligibility over a speech transmission channel, ranging from 0 to 1. STI is calculated for individual measurements and averaged for the measurement point and for the area.
- **Avg.** – averaged STI or CIS result for the measurement point.
- **Δ** – difference between maximum and minimum values of the STI index obtained for the measurement point of the tested area.
- **LAeq** – A-weighted time-averaged sound level over a 15-seconds integration period, in dB.
- **LCeq** – C-weighted time-averaged sound level over a 15-seconds integration period, in dB.
- **LZeq** – Z-weighted time-averaged sound level over a 15-seconds integration period, in dB.
- **LAS** – time-weighted sound level expressed at observation time (15 second integration period), in dB.
- **m(f1), m(f2)** - modulation transfer ratios as a function of two modulation frequencies for each of the 7 octave bands, between 0 and 1.
- **CIS** - Common Intelligibility Scale $CIS = 1 + \log(STI)$.
- **σ** - standard deviation of the measured STI indices for the tested area.
- **Min** – minimum STI value obtained with the measurements.

There are some additional indications:

- The STI qualification band: **A+** to **U** (see Annex G of IEC 60268-16:2011).

These results are displayed in different views:


- **Area view** is a main STIPA view that allows you to create new measurement points, delete measurement points or exclude them from the calculation of averaged indices for the Area, as well as to switch to the **Point** view for the selected point. This view shows a list of measurement points and the next results:



- Averaged **STI** or **CIS** indices taking into account the Ambient noise distortion for the measurement points.
- The STI qualification band (**A+** to **U**) is displayed for each measurement point.


The red colour of the STI/CIS result indicates errors or distortions detected during measurements in that point.

- *Area summary* view is a main STIPA view that shows summary results for the current area:

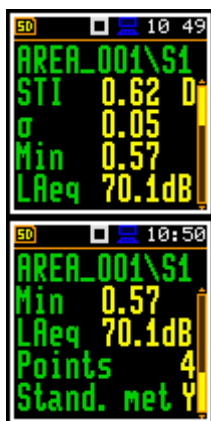

- Averaged **STI** or **CIS** index considering Ambient noise distortions.
- σ - standard deviation of the measured STI indices for the area.
- **Min** – minimum STI value.
- **LAeq** – averaged LAeq for the area.
- Number of measurement points (**Points**) considered for the summary results calculations.
- Conformity of the measurements with the selected standard (**Stand. met**): Yes (**Y**) or No (**N**).

- *Point* view is a main STIPA view that allows you to see the modulation function, to delete measurements (only for the last measurement point) and to exclude measurement results from the calculation of the averaged STI index. This view corresponds to the measurement point selected in the *Area* view and displays measurement results for this point:



- Averaged STI or CIS index considering Ambient noise distortions (**Avg.**) and the index spread ($\Delta\text{STI}/\Delta\text{CIS}$).
- **STIx** results with considered ambient noise, STI qualification band, **LAeq** and **LCeq** results for the measurement (**x: 1, 2, ..**). The red colour of the STIx result indicates errors or disturbances detected during the measurement.



Note: Averaged **CIS** is displayed instead of **STI** in the *Area summary* view and in the *Point* view when this parameter is selected as **Index** in the **STIPA Settings** screen.

- *Measurement* view appears when a new measurement is started (manually or automatically). This view shows the results, which are updated every second and a 15-second progress bar:



- **STI** index with or without considered Ambient noise (**Meas.**) and STI qualification band.
- **LAeq** and **LAS** for the current measurement time.

At the end of the measurement, the instrument automatically switches to the *Point* view and the measurement results are placed in the measurement list. If you stop the measurement manually, the instrument switches to the *Point* view, but the measurement result is not included in the measurement list (see Chapter 13.3.6).

- *Modulation function* view corresponds to the measurement selected in the *Point* view and displays LZeq and modulation transfer ratios ($m(f1)$, $m(f2)$) for seven octave bands with a centre frequency from 125 Hz up to 8 kHz:



Use the ◀ / ▶ key to change columns.

If the modulation ratios are greater than 1 due to errors or disturbances detected during the measurement, they are given a value of 1 and the results for this band are highlighted in red.

To return the *Point* view press <Enter> or <ESC>.




Note: You can switch between views by the pressing the ▼/▲ key together with <Shift>.

13.3.2 Project structure

Speech intelligibility measurements are organised in a project structure. The project name is the name of the directory in the instrument's memory. Test areas are the names of its subdirectories. The test signal positions (called sources) are named in the next lower-level directories. The source position directory contains measurement point directories with predefined names (**P1**, **P2** etc.) where the measurement files are saved. The measurement file contains the measurement results for the single measurement. Projects are saved in the pre-defined STIPA catalogue in the instrument memory. Projects can be accessed from the **File Manager**.

For example, in the screenshots below, the project directory (**PROJ_001**) contains an area directory (**AREA_001**), which contains a source position directory (**S1**) which contains two directories (**P1** and **P2**) and an Ambient noise file (**NOISE.SVL**). The **P1** directory contains files with measurement results (**M1.SVL**, **M2.SVL** ...).

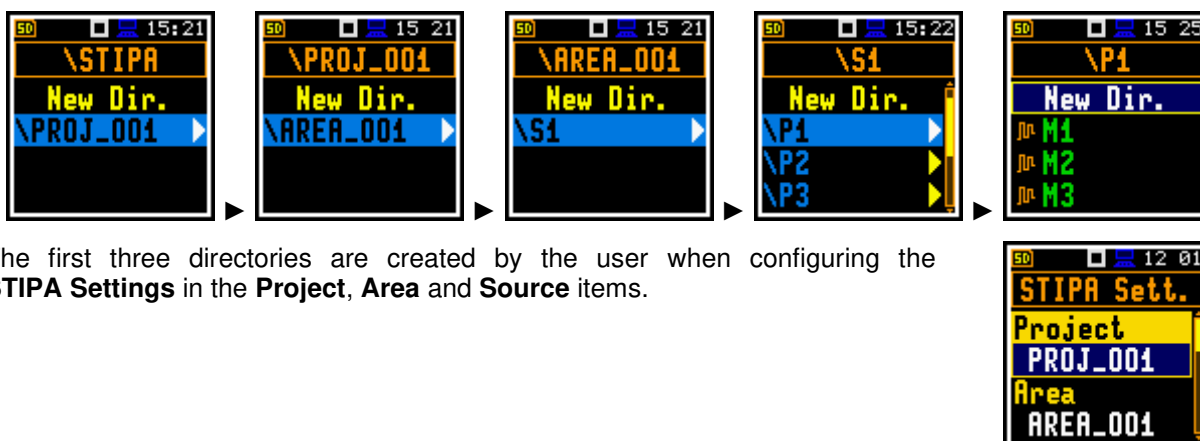

The first three directories are created by the user when configuring the **STIPA Settings** in the **Project**, **Area** and **Source** items.



Note: Project, Area and Source directories can be created, renamed or deleted using the **File Manager** (see Chapter 6.1).

Point directories are created automatically after the **Next** measurement point for the Area has been created during the measurement process. Measurement files are automatically at the start of each measurement (see Chapter 13.3.6).



Note: You cannot delete or rename point directories and measurement files using the **File Manager**. You can delete a point directory and a measurement file using the mechanism described in Chapter 13.3.6.

13.3.3 Results averaging

STIPA measurements require averaging of the STI/CIS indices. There are two aspects to this averaging:

- 1) Averaging the results for a measurement point.

The averaged **STI/CIS** for the measurement point is displayed in the first row of the *Point* view and in the measurement point list of the *Area* view.



- 2) Averaging the results for a tested area.

The averaged **STI/CIS** for the tested area is displayed in the second row of the *Area summary* view.



According to most standards, it is good practice to average the results for measurement points for two or three measurements. In the case of noise fluctuations during measurements, it is recommended to take at least three measurements and check that the spread of the STI index does not exceed 0.03.

13.3.4 STIPA settings

The performance of STIPA measurements depends on certain parameters that can be set in the **Measurement** section: **STIPA Settings**, **Ambient noise**, **Range** and **Compensation Filter**.

The **Range** screen allows you to select the **Normal** or **Low** measurement range (see Chapter 4.6).

The **Compensation Filter** item, which appears only in the **Advanced** interface, allows the required compensation filter to be switched on (see Chapter 4.7).

The other measurement parameters are set by default:

- **Synchronization of start: Off**
- **LEQ integration: Linear**
- **LEQ detector for profiles: Slow**
- **Spectrum filter: Z**
- **Spectrum detector: Linear**

The **STIPA Settings** and **Ambient noise** items are used to configure STIPA parameters. Follow the next steps to configure a STIPA project:

1. In the **Measurement** section, select the **STIPA Sett.** item and press **<Enter>**.




2. Select the **Project** item, press the **►** key and in the **File Manager** screen select:

- a. **New Dir.** to create a new project directory or
- b. the directory of the previously created project and press **<Enter>**.




In the case of **New Dir.**, the instrument will suggest a default name for the new Project directory, which can be modified in the editor screen that opens after pressing **<Enter>**.

Once the directory name has been edited it should be confirmed with **<Enter>**.

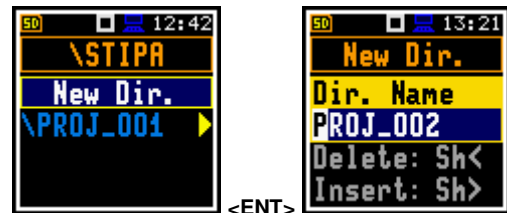


At the newly created directory line in the **File Manager**, press **<Enter>** to return to the **STIPA Sett.** screen.

The selected project name will be displayed in the **Project** item of the **STIPA Sett.** screen.

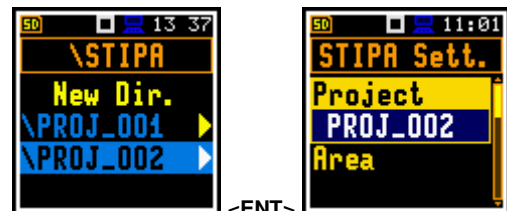


- Go to the **Area** item and press the ► key. In the **File Manager** screen, create a new area directory (**New Dir.**) or select the directory of the previously created Area in the selected Project.

After creating a new area directory or selecting the existing one, press <Enter> and the selected area name will be displayed in the **Area** item of the **STIPA Sett.** screen.

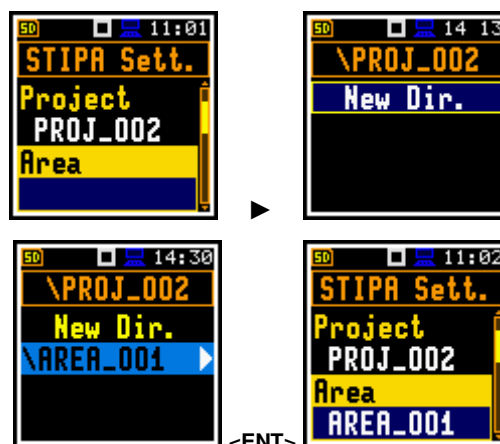


- Go to the **Source** item and press the ► key. In the **File Manager** screen, create a new source directory (**New Dir.**) or select the directory of the previously created Source in the selected Area.

After creating a new source directory or selecting the existing one, press <Enter> and the selected source name will be displayed in the **Source** item of the **STIPA Sett.** screen.

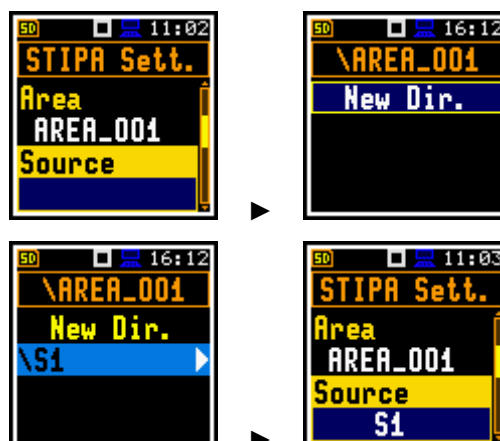

- Select the **Averaging** type: **Manual** or **Auto**.

Manual averaging means that you can carry out as many measurements in the measurement point as necessary and you decide when to stop the series of measurements by using the **Complete** command (see Chapter 13.3.6).

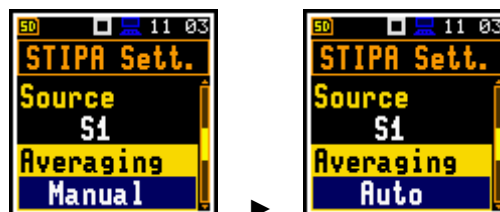

Automatic averaging assumes that the measurements are averaged according to IEC 60268-16:2011, which assumes two averaging procedures – for standard measurements (**60268-16x2**) and for measurements with fluctuating noise (**60268-16x3**). In the name of the standard, the abbreviation **x2** means that at least two measurements should be made, and **x3** means that at least three measurements should be made. When automatic averaging is selected, an additional item **Standard** appears in the **STIPA Settings** screen.

- In the case of automatic averaging, select the **Standard** that defines the type of averaging: **60268-16x2** or **60268-16x3**.

In automatic averaging mode, you perform measurements in the same way as in manual mode. The difference is that in automatic mode the instrument decides when to stop the series of measurements and stops it automatically when a certain condition is met.




7. In the **Index** item, select the **STI** or **CIS** result to be displayed in the main STIPA views.



8. In the **Source Calibration** item, adjust the level of the STIPA reference signal to the level of a real speech signal in the tested area.


The LAeq of both signals must be measured, and if the difference between the real signal and the STIPA signal is different from -3 dB, enter it as the Source calibration.



13.3.5 Considering ambient noise distortion

During the measurement, the effect of ambient noise distortion can be considered in combination with the STIPA signal in the 1/1 octave bands with centre frequencies from 125 to 8000 Hz. These sound pressure levels should not necessarily be the result of some measurements. They can be defined based on the user's knowledge, design assumptions, literature, etc.


The **Ambient noise** item allows you to set the noise levels for the octave bands to be included in the STIPA calculations.

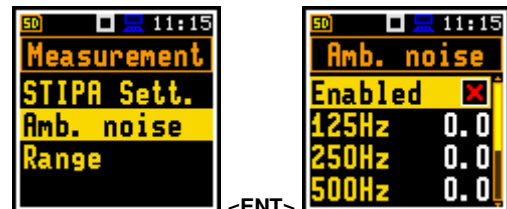

To set the ambient noise, select the 1/1 octave band and use the **◀/▶** key to set the desired value in dB.



The **Enable** item allows you to include/exclude the ambient noise in subsequent measurements.

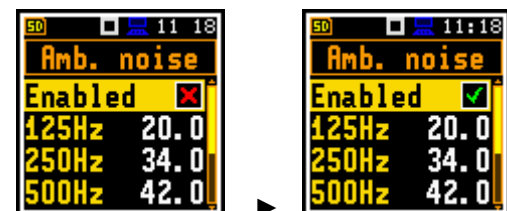

13.3.6 STIPA measurements

When the STIPA settings are complete, you can start measurement.

1. To take a measurement, enter the measurement mode (exit the configuration menu).

When you start a measurement, the *Area* view will show the first measurement point with a zero STI value.

If you have already taken the measurements for some of the measurement points, you should create a new measurement point – see step 5.



- Press the **<Start>** key to start the measurement. The *Measurement* view will appear showing the progress bar of the measurement and the STI index calculated with the ambient noise considered (**STI**), the measured STI index (**Meas.**), the STI qualification band next to the index, the **LAeq** and **LAS** results.

The measurement lasts 15 seconds, with results updated every 1 second.



Note: Ambient noise distortion is considered according to the values set in the **Ambient noise** table (see Chapter 13.3.5).



Note: Pressing the **<Stop>** key during the measurement will abort the measurement without recording the results.




When the measurement is complete, the instrument displays the *Point* view with the current measurement results. Use the **▲ / ▼** key to scroll through the results.

- Press the **<Start>** key if you want to take another measurement.
- To end the series of measurements for the measurement point, you should complete them.

To complete the measurement series at the measurement point, press the **<Enter>** key, select **Complete** and in the command list and press **<Enter>**.

The instrument switches automatically to the *Area* view.

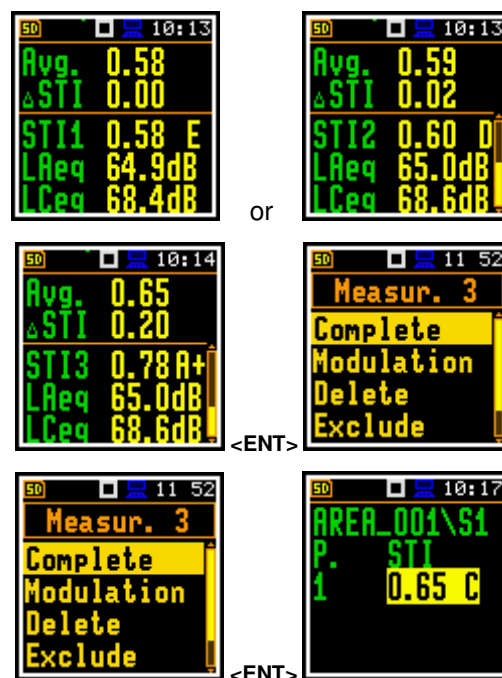


Note: In the case of automatic averaging, the series of measurements is automatically completed when the conditions specified in the selected standard are met.

If you select the measurement in the *Point* view and open the command list, you can view the modulation function coefficients (**Modulation**) for the selected measurement and delete (**Delete**) or exclude from the averaging (**Exclude**) the selected measurement.

If you select **Modulation** and press **<Enter>**, the instrument will switch to the *Modulation* function view.

Use the **◀ / ▶** key to change columns in this view.

Press **<Enter>** or **<ESC>** to return to the *Point* view

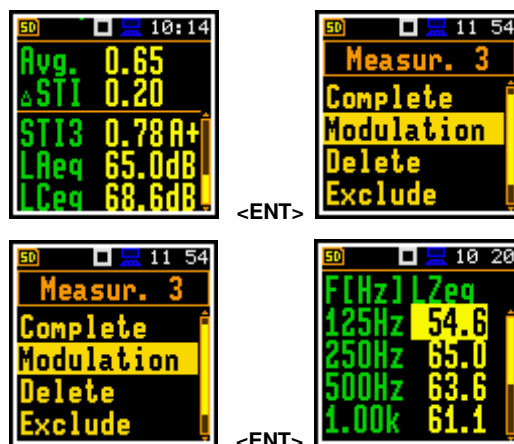

If you select **Delete** and press **<Enter>**, the instrument will delete the selected measurement from the measurement list and change the numbering in the *Point* view. At the same time, the file containing the measurement results is deleted from the Points directory.

If you select **Exclude** and press **<Enter>**, the instrument will exclude the selected measurement from averaging and the excluded measurement results will be grey in the *Point* view.

When you select the excluded measurement and open the command list, the last command is named **Include**.

You can also exclude/include the selected measurement from averaging directly in the *Point* view by pressing the **<Left> / <Right>** key together with **<Shift>**.

The file with the excluded measurement results will have the character “_” instead of “M”.

- Once you have completed the series of measurements for the measurement point, you can create a new point.

To do this, press **<Enter>** in the *Area* view and select **New point** from the command list and press **<Enter>**. The instrument will create a new point directory and switch to the *Point* view.

To start measurements at the new measurement point, press the **<Start>** key and follow steps 2 – 4.


If you wish to change the ambient noise levels for a new measurement point, open the **Ambient noise** item and make the necessary adjustments to the octave noise levels. After confirming the changes with **<Enter>**, you can return to the measurement mode with the new ambient noise distortion parameters.



Note: Any confirmed changes to the **Ambient noise** table will replace the previous ones and new ambient noise distortions will be considered in the next measurements.

The summary results for the Area are presented in the *Area summary* view, which can be accessed from the *Area* view by pressing the **<Down> / <Up>** key together with **<Shift>**.

If you select the measurement point in the *Area* view and open the command list, you can also switch to the *Point* view (**View point**) and delete (**Delete**) or exclude (**Exclude**) the selected measurement point from the averaging.



If you select **View point** and press **<Enter>**, the instrument will open the *Point* view for the selected measurement point.

If the selected point is not the last measurement point, in the *Point* view, you can only view the measurement results together with the modulation function and exclude/include the selected measurements from the averaging. The **Delete** command is disabled.


If you select **Delete** and press **<Enter>**, the instrument will delete the selected measurement point and return to the *Area* view with a new point numbering. The point directory will be deleted from the Source directory along with any data files it contains.

If you select **Exclude** and press **<Enter>**, the instrument will exclude the selected measurement point from averaging and excluded measurement point will be grey in the *Area* view.

If you select the excluded measurement point and open the command list, the last command is named **Include**.

You can also exclude/include the selected measurement point from the averaging directly in the *Area* view by pressing the **◀ / ▶** key together with **<Shift>**.

The directory of the excluded point will have the character **_** instead of **P**.

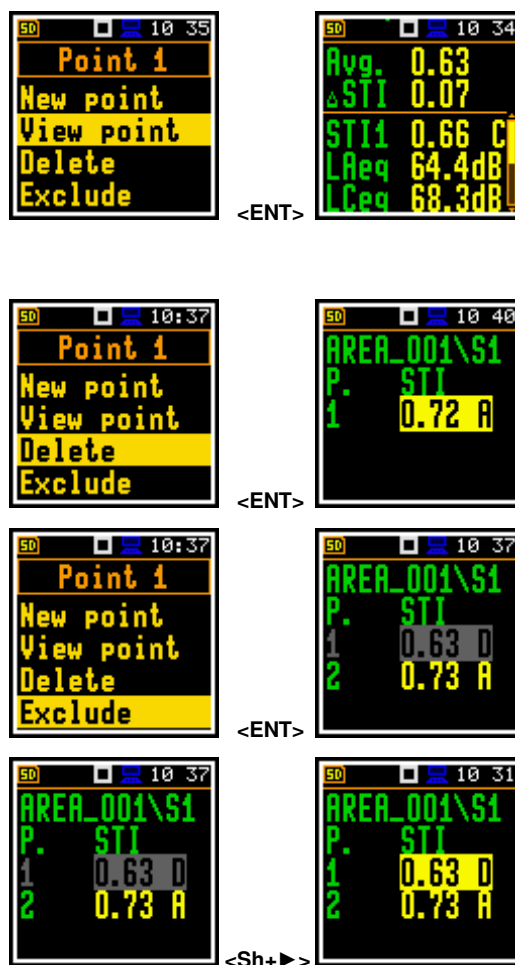

You can stop the measurements for the selected **Project/Area/Source** at any time and, if necessary, create the next **Project/Area/Source** combination in the **STIPA Settings** screen.


13.4 DOWNLOADING FILES AND PROCESSING DATA

The measurement files created by the instrument during STIPA measurements can be downloaded and analysed using the *SvanPC++* software.

SvanPC++ allows you to download and analyse measurement files created directly by the instrument, as well as projects created by the Building Acoustics applications.

13.4.1 Measurement with Building Acoustics application


Building Acoustics is an application for mobile devices (smartphones, tablets) that uses SvanTek instruments to measure building acoustics, including STIPA speech intelligibility.

After performing measurements with *Building Acoustics* application, a project (zip file containing files with results obtained during the measurement) is automatically copied to the instrument. The project zip file is called BAXxx.ZIP and you can download it to a PC and open it with the program *SvanPC++* using the option "SVAN Files" (available in the menu "SVAN -> SVAN Files" or using the meter icon  in the toolbar). Once the *SvanPC++* software is installed on your PC, you can open the project directly by double clicking on it.

To open the project:

- Connect your Svanтек instrument to the PC,
- Start SvanPC++,
- Select the project file from the list on the left side of the window and use the right arrow button to download the file to the PC.

Double click on the downloaded file and it will automatically open in SvanPC++. The STIPA results window will appear.

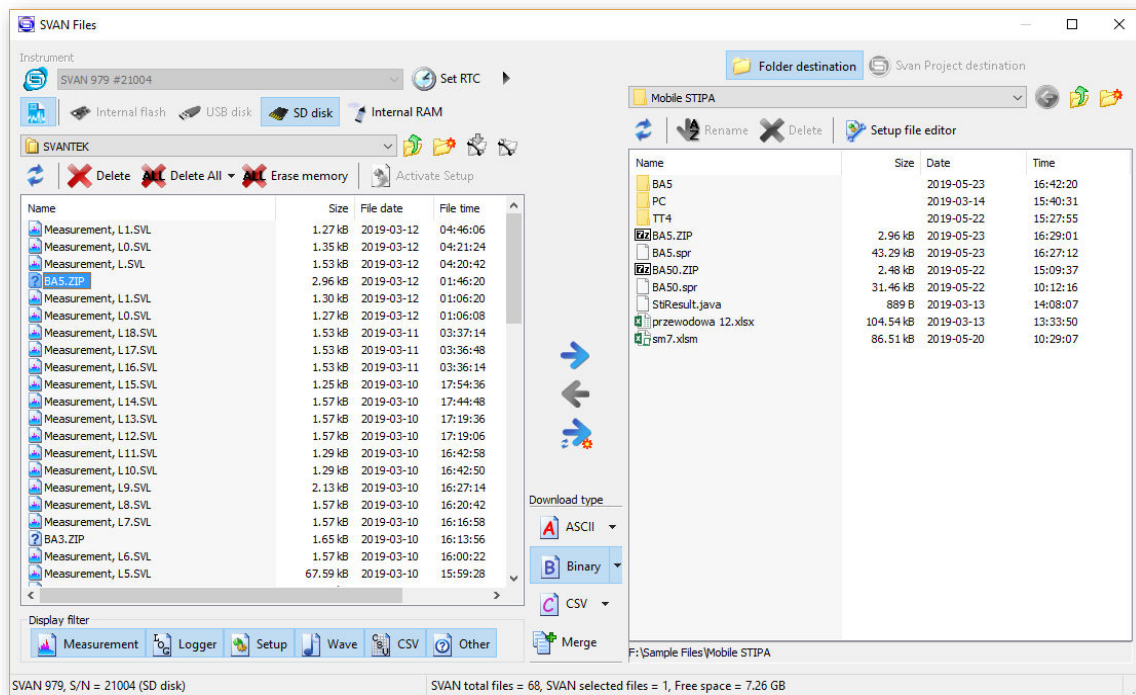


You can click on the file in the list on the left. The file will be downloaded to the temporary folder and opened.

13.4.2 Direct measurement with the instrument (without Building Acoustics application)


When the instrument is used directly for STIPA measurements, the measurement files are grouped into point catalogues. Point catalogues are grouped into source catalogues. These in turn are grouped into the area catalogues and the area catalogues are grouped into the project catalogue.

To download files with *SvanPC++*, use the "SVAN Files" window. Select the appropriate catalogue with the required data in the instrument left panel and then click on the right arrow to download it. You can select the whole project catalogue or only a catalogue for the area or point (or even a single SVL file).

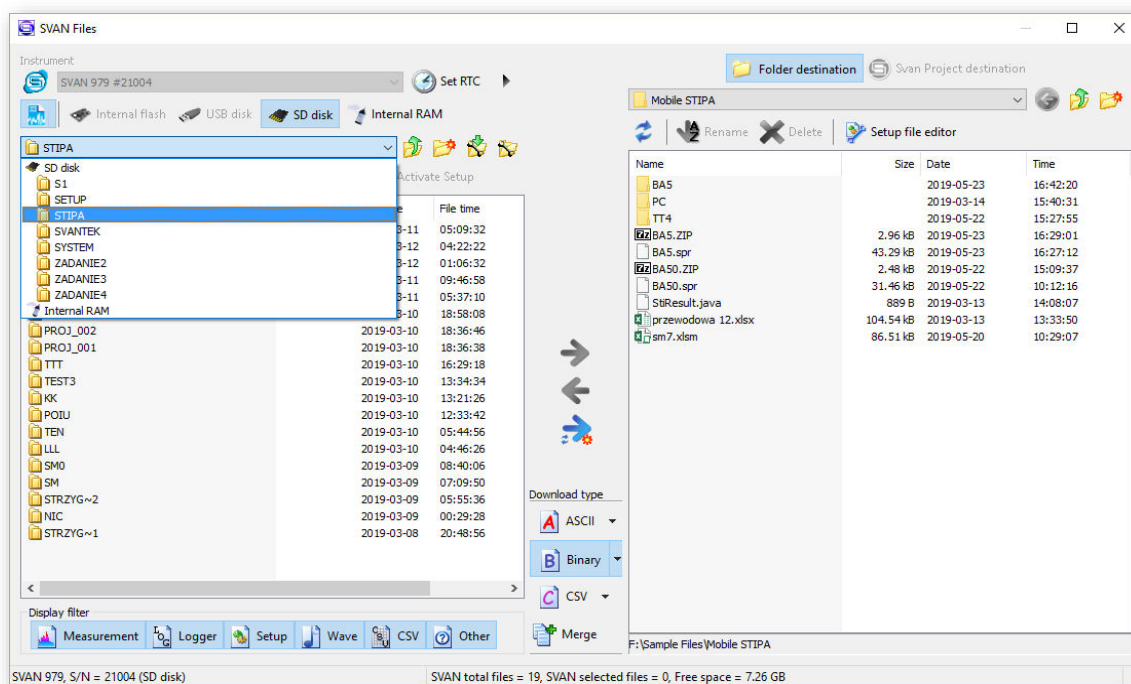

If you have downloaded the file, you can open it with a double click. If you have downloaded the whole folder, you have to link the downloaded dataset. The easiest way to do this is to use the SvanPC++ project functionality. Close the "SVAN Files" window and create a new project ("File -> New Project" and select "Simple project" as the project type).

A window will appear on the left panel with a list of project files (empty for now). Add the folders/files you want to combine to the project. The easiest way to do this is by drag & drop from the file explorer, by selecting the folder/files and dragging them into the SvanPC++ window. The program will automatically link all files from the folder, whereby the program may ask you how to link files - in the case of STIPA, the option you choose is irrelevant, as STIPA measurements are linked by grouping on matching projects/areas/sources/points. After this operation the STIPA results window will automatically appear.

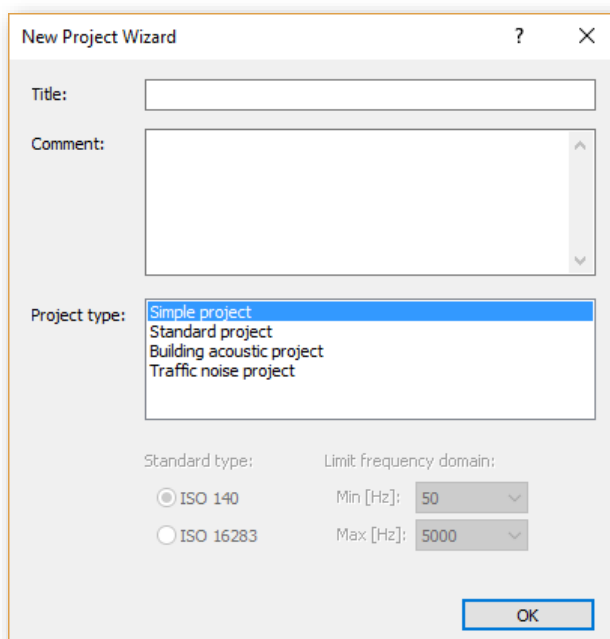

Speech transmission index											
Project	TENO										
Area	DLAPAW~1										
Source	STI	Category	σ	Δ	CIS	STI (Measure)	Category (Measure)	CIS (Measure)	L _{Aeq} [dB]	L _{Ceq} [dB]	Status
S1	0,59	E	0,10	0,20	0,77	0,62	D	0,79	112,85	113,49	E
[-]P1	0,69	B	0,05	0,11	0,84	0,71	B	0,85	71,15	80,97	✓
<input checked="" type="checkbox"/> 1	0,63	D	-	-	0,80	0,65	C	0,81	71,14	81,07	✓
<input checked="" type="checkbox"/> 2	0,74	A	-	-	0,87	0,77	A+	0,89	70,77	80,68	✓
<input checked="" type="checkbox"/> 3	0,70	B	-	-	0,85	0,72	A	0,86	71,50	81,14	✓
Background noise	-	-	-	-	-	-	-	-	-	-	-
[+]P2	0,49	G	0,13	0,34	0,69	0,53	F	0,72	115,86	116,50	E

13.4.4 Changing background noise values


The cells containing the background noise results are editable, i.e., you can manually enter values for individual octaves (simply double click on the selected background noise value). Such a change will automatically convert the results for all points above.

You can also import background values using the paste option (CTRL+V or menu "Edit -> Paste"), after selecting the value from which you want to paste the results. Data that are in the clipboard will be pasted for the next octaves starting from the selected cell. You can copy data to the clipboard from Excel, from another program as well as you can copy values from another view of *SvanPC++* (thanks to which you can import results from another SVL file). If the clipboard contains numerical values separated by a white space (space, tab, enter), the program will accept them correctly.

13.4.5 Generating reports

There are two ways to create a report:

1. Using the Excel icon in the top left corner of the view, this will automatically open an Excel spreadsheet with all the data visible in the view.
2. By selecting cells in the table and using the copy-paste option (CTRL+C or menu "Edit -> Copy" or from the right-click context menu), you can transfer a fragment or the whole view to, for example, Word.

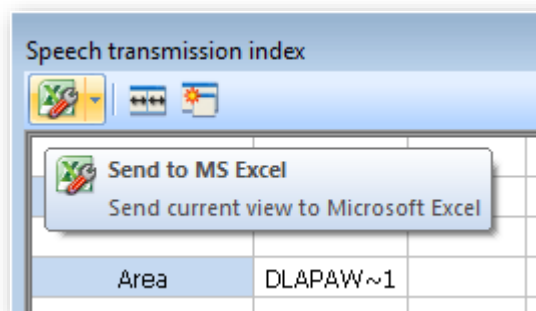

14 PC SOFTWARE AND SMARTPHONE APPLICATIONS

SVANTEK offers PC software for data download and processing as well as remote control and communication with SV 971A, depending on the user's needs:

- *SvanPC++* - data download and upload, data post-processing, reporting and remote control via the USB or RS232 connection with a PC,
- *Supervisor* - data download and upload via the USB or RS232 connection with a PC, reporting, and applications for smartphones and tablets that are equipped with Bluetooth®:
- *Assistant* – general purpose application for current result viewing and remote control,
- *Building Acoustics* – application dedicated to building acoustics and speech intelligibility measurements (STIPA).

The *SvanPC++* and *Supervisor* installation packages can be downloaded from the Svantek's official website, smartphone applications – from *Play Store*.

PC software are described in the user manuals that can be downloaded from Svantek's official website, the *Assistant* and *Building Acoustics* applications are described in Appendix E of this manual.

15 MAINTENANCE

15.1 REPLACING BATTERIES

SV 971A is supplied with four AAA alkaline batteries, but you may also use AAA rechargeable batteries.

The “**battery**” icon indicates the status of the internal batteries.

The instrument is not equipped with an internal charger, so the batteries can only be recharged after they have been removed from the instrument.

To change or charge the batteries, switch off the instrument, unscrew the coin slot screw, remove the black bottom cover of the instrument, and slide out the battery tubes.



Note: When replacing the batteries, ensure that the polarity is correct.

15.2 EXTRACTING AND INSERTING THE MEMORY CARD

SV 971A is supplied with a 16 GB Kingston Industrial micro-SD card - (SDCIT/8GBSP).

It can be replaced with the higher capacity card (up to 128GB), but the card must be formatted as FAT32 before use.




Note: The memory card supplied has been tested by SVANTEK and this type of card is strongly recommended for use when replacing the original card.



Note: If you wish to use a higher capacity card, please contact your local distributor.

To change the memory card, switch off the instrument, unscrew the screw and remove the black bottom cover of the instrument.

The card is installed in the slot. To remove the card, press on the card and pull it out of the slot.

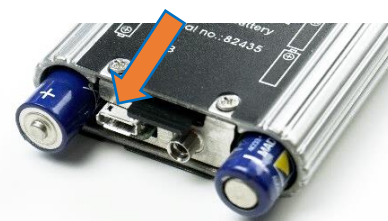

After inserting the SD card, a click should be heard to indicate that the card has been inserted correctly. If necessary, use a tool (such as a pen) to push the card into the slot.

15.3 REPLACING THE MICROPHONE AND MICROPHONE PREAMPLIFIER

SV 971A is equipped with a special connector for the input of the measurement signal from the microphone preamplifier.

The SV 971A set includes a pre-polarised ½” microphone (ACO 7152) and a microphone preamplifier (SV 18A).



Note: The kit includes a protective microphone cap which should be kept on the microphone at all times when the instrument is not being used for measurements.

To change the microphone cartridge, simply unscrew the previous microphone and screw on the new one. When unscrewing the microphone, be careful not to drop it. To avoid this, unscrew the microphone so that it rests in the palm of your hand.




Note: After replacing the microphone, you must calibrate the instrument! Due to the significant difference in the sensitivity between the microphones, the calibration drift may also be significant, but this does not mean that the unit is malfunctioning.

The instrument is supplied with the preamplifier connected. However, it is sometimes necessary to remove the preamplifier (e.g., when SV 971A is to be used with the SV 271 monitoring station).

To remove the preamplifier from the instrument, unscrew the preamplifier's threaded ring and pull the preamplifier out of the instrument.

To connect the preamplifier (with microphone) to the instrument, position the instrument socket and the preamplifier plug so that the mark on the instrument socket is aligned with the pilot slot on the preamplifier plug. Then insert the preamplifier plug into the socket and tighten the threaded ring.

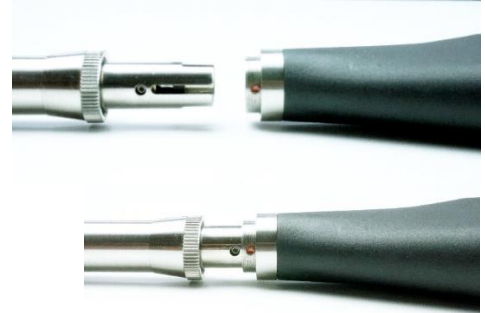

15.4 RESETTING THE INSTRUMENT

- **SYSTEM RESET:** internal software reset clears any setup configuration and restores the default factory settings (*path: <Menu> / Auxiliary Setup / Factory Settings*).
- **HARDWARE RESET:** internal hardware reset doesn't change any settings. Make sure that the battery is not exhausted and that the instrument is switched off. Press and hold the **<Shift>** and **<Start/Stop>** keys for 20 seconds, then release. Switch the instrument on.



Note: The hardware reset should only be used in extreme situations, such as when an instrument has hung up.

Note that a hardware reset:

- will stop any pre-programmed auto-run modes,
- will stop the measurement run!

15.5 UPGRADING THE FIRMWARE

Svantek is committed to continuous innovation and therefore reserves the right to provide firmware enhancements based on user feedback.

To update the instrument firmware:

- Unpack the supplied firmware package (provided as a suitable compressed file).
- Make sure that the instrument is switched off.
- Switch off all Svantek PC software
- Connect the SC 158 cable to the instrument and then to the PC.
- Press and hold the **<Enter>** and **<ESC>** keys while switching on the instrument with **<Shift>** and **<Start/Stop>** keys. The following message should appear on the instrument's screen: Bootstrap ver: x.xx.
- Wait for the "<USB>" message to appear on the instrument's screen and run the *go-usb.bat* file on the PC.
- The changing number and final message "..... o.k." should appear on the PC screen.
- A successful firmware update is indicated by the message "Program loaded!"
- Switch off the instrument.



Note: Using the **SvanPC++** software it is very easy to check if there are new firmware releases available for download.

15.6 PRESERVATION OF INTERNAL BATTERIES

- To prolong the life of the internal batteries, it is recommended to switch off the instrument when storing it. In the case of alkaline batteries, it is recommended to remove them from the instrument.
- When the instrument is switched off, it still uses a small amount of battery power. It is therefore recommended that rechargeable batteries are recharged every few months if they are not used regularly.

15.7 TRANSPORTATION AND STORAGE

For transport or storage, we recommend using the packaging provided by the manufacturer. In a potentially dirty industrial environment, it is advisable to use the carrying case provided by the manufacturer, such as waterproof case (SA 72) or the pocket soft bag (SA 80), which offer excellent mechanical and environmental protection and long-term storage conditions.

15.8 CLEANING

Clean the surface of the instrument with a damp, soft cloth.

The instrument sockets should be cleaned with compressed air.



Note: In cases of larger dirt, such as oil or grease, contact your Local Authorized Distributor or Svantek Service Office.

15.9 TROUBLESHOOTING

- If the instrument does not switch on, connect the USB power supply. Then perform a hardware reset.
- If the instrument is switched on but does not respond to any key, perform a hardware reset.
- If the reset does not help call your Local Authorized Distributor or Svantek Service Office.

Should your Svantek professional measurement equipment need to be returned for repair or for calibration, please contact the service office at the following number or contact via the Svantek website.

Service Office: +48 (22) 51-88-320 or +48 (22) 51-88-322.

Office hours are 9:00 a.m. to 5:00 p.m. Central European Time.

Internet: www.svantek.com

Address: [SVANTEK Sp. z o.o.](#)








[Strzygłowska 81](#)

[04-872 Warszawa,](#)


[Poland](#)

16 GLOSSARY

16.1 MODES AND MEASUREMENT FUNCTIONS


Position	Description	Screen	Reference
<i>Function</i>	The menu section that enables selecting the <i>Measurement Function</i> and performing <i>Calibration</i> of the instrument.		Chapter 3
<i>Measurement Function</i>	Type of calculations the instrument currently performs: - <i>Level Meter</i> , - <i>1/1 Octave</i> , - <i>1/3 Octave</i> , - <i>Dosimeter</i> , - <i>RT60</i> , - <i>STIPA</i> .		Chapter 3.1
<i>Level Meter</i>	<i>Measurement Function</i> enabling calculation of broad band results (<i>Summary Results</i>) and time-history for sound measurements in accordance with Class 1 IEC 61672-1:2013 accuracy. All results can be calculated in parallel by three virtual meters (so called profiles) using different weighting filters and LEQ detectors.		Chapter 3.1
<i>1/1 Octave</i>	<i>Measurement Function</i> enabling calculation of <i>Level Meter</i> results and 1/1 octave sound results in accordance with Class 1 IEC 61260-1:2014. 1/1 octave results are presented as a spectrum graph - a function of result value vs central band frequency. 1/1 octave results can be saved as a time-history.		Chapter 3.1 , 10
<i>1/3 Octave</i>	<i>Measurement Function</i> enabling calculation of <i>Level Meter</i> results and 1/3 octave sound results in accordance with Class 1 IEC 61260-1:2014. 1/3 octave results are presented as a spectrum graph - a function of result value vs central band frequency. 1/3 octave results can be saved as a time-history.		Chapter 3.1 , 10
<i>Dosimeter</i>	<i>Measurement Function</i> enabling calculation of broad band (<i>Level Meter</i>) and sound exposure results.		Chapter 3.1 , 11
<i>1/1.&Dose</i>	<i>Measurement Function</i> enabling calculation of <i>Dose Meter</i> results and 1/1 octave sound results in accordance with Class 1 IEC 61260-1:2014. 1/1 octave results are presented as a spectrum graph - a function of result value vs central band frequency. 1/1 octave results can be saved as a time-history.		Chapter 3.1 , 10

1/3.&Dose *Measurement Function* enabling calculation of *Dose Meter* results and 1/3 octave sound results in accordance with Class 1 IEC 61260-1:2014. 1/3 octave results are presented as a spectrum graph - a function of result value vs central band frequency. 1/3 octave results can be saved as a time-history.




Chapter
[3.1, 10](#)

RT60 *Measurement Function* enabling calculation of reverberation time in 1/1 octave bands or 1/3 octave bands including three total RMS levels (A, C and Z weighted). Two methods can be applied: Impulse Response Method and Interrupted Noise Method. Results are presented for 1/1 or 1/3 octave bands.







Chapter
[3.1, 12](#)

STIPA *Measurement Function* enabling analysis of the speech intelligibility with the STIPA method.




Chapter
[3.1, 13](#)

16.2 CALIBRATION

Position	Description	Screen	Reference
Calibration	Position on the <i>Function</i> screen that opens a screen with positions allowing you to perform calibration of the instrument: <i>By Measurement</i> , <i>Last Calibration</i> , <i>Calibration History</i> , <i>Clear History</i> , <i>Post Calibration</i> and <i>Auto Calibration</i> .		Chapter 3.2
By Measurement	Type of calibration based on the reference signal measurement with the use of a sound calibrator.		Chapter 3.2.1
Calibration Measure	Measured by the instrument reference signal level without calibration factor correction.		Chapter 3.2.1, 3.2.6
Calibration Level	Level of the reference signal generated by used calibrator.		Chapter 3.2.1

Calibration drift Difference between the new calibration factor and the previous one.




Chapter
[3.2.1](#), [3.2.6](#)

Last Calibration Recent calibration record: measurement function for which calibration was performed (*Level Meter* or *Dosimeter*), type of calibration (*Factory Calibration*, *By Sensitivity* or *By Measurement*), date of calibration and calibration factor.




Chapter
[3.2.2](#)

Calibration History List of calibration records which you can view by pressing the **<Enter>** key.




Chapter
[3.2.3](#)

Clear History Operation that clears all calibration records.




Chapter
[3.2.4](#)

Post Calibration Feature that enables adding the new calibration factor to some files already saved in the instrument's memory or to the files that will be created in the future.



Chapter
[3.2.5](#)









Auto Calibration Feature that enables automatic calibration when the reference sound signal is detected by the instrument.


















Chapter
[3.2.6](#)








16.3 MEASURED RESULTS

Position	Description	Screen	Reference
Elapsed time	Time from the measurement start, that is displayed under the result in the format mm:ss in the range from 00:00 to 59:59, or in the format hh:mm:ss in the range from 01:00:00 to 99:59:59, or in format xxxh from 100h to 999h, and >999h if the elapsed time exceeds 999 hours. Its maximum value is equal to the <i>Integration Period</i> and the elapsed time is zeroed when new measurement cycle starts.		Chapter 5.1.1

<i>OVL</i>	Percentage of the overloaded input signal, which occurred within the elapsed measurement time.		Appendix D
<i>Lpeak</i>	Peak Sound Level, the greatest instantaneous value of a standard frequency weighted sound pressure level within the elapsed measurement time. It is measured with frequency weighting A, C or Z and accordingly displayed as LApeak, LCpeak or LZpeak.		Appendix D
<i>Lmax</i>	Maximal value of the time-weighted sound pressure level at the exponential RMS detector output within the elapsed measurement time. The Max result for the 1 second period is equal to the Spl result. It is measured with frequency weighting A, C or Z and time weighting F, S, I and displayed as LAFmax, LASmax, LCFmax, LCSmax etc.		Appendix D
<i>Lmin</i>	Minimal value of the time-weighted sound pressure level at the exponential RMS detector output within the elapsed measurement time. It is measured with frequency weighting A, C or Z and time weighting F, S, I and displayed as LAFmax, LASmax, LCFmax, LCSmax etc.		Appendix D
<i>Leq</i>	Equivalent continuous sound level, time-averaged sound level for the elapsed measurement time (equivalent sound level). It is measured with frequency weighting A, C or Z and accordingly displayed as LAeq, LCEq or LZeq.		Appendix D
<i>L</i>	Time weighted sound level expressed at observation time, expressed in dB. It is measured with frequency weighting A, C or Z and time weighting F, S, I and displayed as LAF, LAS, LCF, LCS etc.		Appendix D
<i>LE</i>	Sound Exposure Level (SEL), the constant sound level that has the same amount of energy in one second as the original noise event and is the subset of the <i>Leq</i> result so, for the integration time equal to 1 s, <i>SEL</i> is always equal to <i>Leq</i> . It is measured with frequency weighting A, C or Z and accordingly displayed as LAE, LCE or LZE.		Appendix D
<i>LEPd</i>	Daily Personal Noise Exposure, the noise exposure level for a nominal 8-hour working day, used for assessing the noise exposure of a worker during a working day. The <i>LEPd</i> result is calculated on the base of the <i>Leq</i> .		Appendix D









<i>L_{tm3}</i>	Takt-Maximal Level calculated according to the German standard TA Lärm.		Appendix D
<i>L_{tm5}</i>	Takt-Maximal Level calculated according to the German standard TA Lärm.		Appendix D
<i>L_n</i>	Statistical Noise Levels, the certain boundary level surpassed by the temporary noise level values in not more than n% of the observation period. <i>L_n</i> are calculated on the base of 100ms <i>Leq</i> results and renewed every second on the display as cumulated statistics over the current measurement time.		Appendix D
<i>L_(den)</i>	Day-evening-night equivalent level, <i>Leq</i> . Sound Level, measured over the 24 hour period, with a 10 dB penalty added to the levels between 23.00 and 07.00 hours and a 5 dB penalty added to the levels between 19.00 and 23.00 hours to reflect people's extra sensitivity to noise during the night and the evening. The instrument displays: <i>L_d</i> , <i>L_e</i> , <i>L_n</i> , <i>L_{de}</i> , <i>L_{en}</i> , <i>L_{nd}</i> , or <i>L_{den}</i> depending on the day and night time which the measurement covers. Due to different country requirements, it is possible to shift day time from 7h-19h to 6h-18h.		Appendix D
<i>PSEL</i>	Individual Sound Exposure Level to the noise is equal to the standing sound level in a measurement period. The <i>PSEL</i> result is calculated on the base of the <i>LEQ</i> .		Appendix D
<i>DOSE</i>	Quantity of noise received by the worker, expressed as the percentage of the whole day acceptable value.		Appendix D
<i>D_{8h}</i>	Quantity of noise received by the worker for 8 hours.		Appendix D








<i>PrDOSE</i>	Quantity of noise received by the worker during exposure time.		Appendix D
<i>LAV</i>	Average level of the acoustic pressure for the given time period of the measurement.		Appendix D
<i>SEL8</i>	<i>SEL</i> result corresponding to the integration time equal to 8 hours. The <i>SEL8</i> result is calculated on the base of the LEQ.		Appendix D
<i>E</i>	Exposition represents the amount of the acoustical energy received by the worker.		Appendix D
<i>E_8h</i>	Exposition in 8 hours represents the amount of the acoustical energy received by the worker for 8 hours. The <i>E_8h</i> result is expressed in the linear units [Pa²h].		Appendix D
<i>PTC</i>	Peak Threshold Counter – the number of the overpasses of the Threshold Level by <i>Lpeak</i> result. This result is incremented in 100 ms intervals.		Appendix D
<i>PTP</i>	PTC result expressed in percent.		Appendix D
<i>TWA</i>	Time Weighted Average - average A-weighted sound level for a nominal 8-hour workday with Time Weighting S and Exchange Rate 5. TWA is usually measured with A-weighting and Slow response detector type. TWA is calculated from the measured LAV (taking Threshold Level into account) and a Reference time of 8 h. Mainly used in		Appendix D









	the USA for assessing the noise exposure for a worker during a workday.		
<i>ULT</i>	Upper Limit Time - time that SPL exceeded the "ULT Threshold Level" set during configuration.		Appendix D
<i>PrTWA</i>	Projected Time Weighted Average is calculated from the measured LAV (taking THRESHOLD LEVEL into account) and the exposure time.		Appendix D
<i>Lc-a</i>	<i>Leq</i> that enhances the low-frequency components of the sound signal. It is the result of subtracting an A-weighted LAeq from a simultaneously collected C-weighted Leq.		Appendix D
<i>EX</i>	Expected value. Calculated on the basis of 100ms Leq results.		Appendix D
<i>SD</i>	Standard deviation. Calculated on the basis of 100ms Leq results.		Appendix D
<i>LR1</i>	First rolling <i>Leq</i> - Leq for the window of the last xx seconds/minutes of the measurement moving with 1 second step.		Appendix D
<i>LR2</i>	Second rolling <i>Leq</i> - Leq for the window of the last yy seconds/minutes of the measurement moving with 1 second step.		Appendix D








16.4 MEASUREMENT PARAMETERS








Position	Description	Screen	Reference
----------	-------------	--------	-----------








<i>Measurement</i>	Section of the Main Menu that enables selecting the measurement parameters in the screens: <i>General Settings</i> , <i>Measurement Trigger</i> , <i>Profiles</i> , <i>Logging</i> , <i>Spectrum</i> , <i>Range</i> , <i>Compensation Filter</i> , <i>Statistical Levels</i> , <i>Exposure Time</i> , <i>Timer</i> and <i>Alarm</i> .		Chapter 4
<i>General Settings</i>	General measurement settings: <i>Start Delay</i> , <i>Start Sync.</i> , <i>Integration Period</i> , <i>Repetition Cycles</i> , <i>RMS Integration</i> and <i>Day Time Limits</i> .		Chapter 4.1
<i>Start Delay</i>	Delay between pressing the <Start> key and the start of measurement integration.		Chapter 4.1
<i>Start Sync.</i>	Synchronization of the measurement/integration start to the nearest full minute or hour of the instrument real-time clock. It helps to measure in full cycles.		Chapter 4.1
<i>Integration Period</i>	Time of averaging of <i>Summary Results</i> : from 1 second to Infinite. For example, with 8 hours integration period the LEQ result will be averaged for 8 hours. In the case of Infinite, the measurement will last until the user presses the <Stop> key.		Chapter 4.1
<i>Repetition Cycles</i>	Number of measurement/integration repetitions after the <Start> key pressure. This enables to make a series of measurements without pressing the <Start> key and save this series in the results file.		Chapter 4.1
<i>LEQ Integration</i>	Type of integration of RMS based results (RMS detector): <i>Linear</i> or <i>Exponential</i> . The IEC 61672-1:2013 standard requires Linear integration, without time weighting, however in some countries old regulation refers to the Exponential RMS integration with standard time weighting: Fast or Slow.		Chapter 4.1
<i>Linear</i>	Linear type of integration of RMS based results (RMS detector), without time weighting according to the IEC 61672-1:2013 standard.		Chapter 4.1









<i>Exponential</i>	Exponential type of integration of RMS based results (RMS detector), where averaging is a continuous averaging process that weighs current and past data differently. The amount of weight given to past data as compared to current data depends on the exponential time constant. In exponential averaging, the averaging process continues indefinitely.		Chapter 4.1
<i>Day Time Limits</i>	Definition of the day and night periods required by local standards: 6–18h and 7–19h. These limits are used for the calculation of the L(den) function.		Chapter 4.1
<i>LRx Time</i>	Definition of the integration periods for calculating the LR1 and LR2 results.		Chapter 4.1
<i>Profiles</i>	Virtual broadband level meters, which calculate the set of results with own weighting filter (<i>Filter</i>) and exponential detector time constant (<i>Detector</i>). Profiles can be programmed together in the <i>Profile</i> screen if the instrument works in the <i>Level Meter</i> , <i>1/1 Octave</i> or <i>1/3 Octave</i> modes, or individually if the instrument works in the <i>Dosimeter</i> mode.	 	Chapter 4.3 , 11.3
<i>Filter</i>	Weighting filter applied in the profile for all results except <i>Lpeak</i> in accordance with most applicable world standards: Z, A, C, B, LF.		Chapter 4.3 Appendix C Appendix D
<i>Filter Peak</i>	Weighting filter applied in the profile for <i>Lpeak</i> results calculation in accordance with most applicable world standards: Z, A, C, B, LF.		Chapter 4.3 Appendix C Appendix D








<i>Detector</i>	Exponential RMS detector time constant applied in the profile: <i>Impulse</i> , <i>Fast</i> or <i>Slow</i> for such results like <i>Leq</i> , <i>Lmax</i> , <i>Lmin</i> , <i>LE</i> , <i>LEPd</i> , <i>Lden</i> , <i>L</i> , <i>Ltm3</i> and <i>Ltm5</i> .		Chapter 4.3 Appendix D
<i>Compensation Filter</i>	Digital filter that compensates some effect: <i>Microphone</i> , <i>Diffuse Field</i> , <i>Windscreen</i> , <i>Outdoor Environment</i> and <i>Outdoor Airport</i> .		Chapter 4.7
<i>Microphone</i>	Digital filter that compensates the microphone inner noise. It is switched On by default, however it should be switched Off for electrical measurements (e.g. for laboratory calibration measurements).		Chapter 4.7
<i>Field Compensation</i>	Digital filter that compensates the free-field (Free Field) or diffuse field (Dif. Field) effects as well as compensation of the outdoor microphone kit SA 271A (Environmental and Airport). The user may switch off (Off) all compensations for laboratory purposes.		Chapter 4.7
<i>Windscreen</i>	Digital filter that compensates the effect of the SA 22 windscreen.		Chapter 4.7
<i>Range</i>	Position that enables selecting the linear operating range for the sinusoidal signal selection: <i>Low</i> or <i>Normal</i> . The calibration factor is always added to the range limits. The ranges depend on the selected <i>Compensation Filter</i> .		Chapter 4.6
<i>Low</i>	Low linear operating range for the sinusoidal signal. The calibration factor is always added to the range limits. The range depends on the selected <i>Compensation Filter</i> .		Chapter 4.6 Appendix C
<i>Normal</i>	Normal linear operating range for the sinusoidal signal. The calibration factor is always added to the range limits. The range depends on the selected <i>Compensation Filter</i> .		Chapter 4.6 Appendix C

Measurement Trigger	Screen that enables configuring triggering of the measurement/integration process with parameters: <i>Trigger</i> , <i>Source</i> , <i>Level</i> and <i>Gradient</i> .		Chapter 4.2
Trigger	Position that switches <i>Off</i> or on the measurement trigger by selecting its type: <i>Level+</i> , <i>Level-</i> or <i>Gradient+</i> . If the instrument is waiting for the trigger condition, the appropriate trigger icon is flashing on the display alternatively with the „play” icon.		Chapter 4.2
Slope+	Type of trigger that starts the measurement/ integration by the duration of the <i>Integration Period</i> on condition: rising value of the RMS result (<i>Source</i>) integrated during 0,5 ms passes above the threshold value (<i>Level</i>).		Chapter 4.2
Slope -	Type of trigger that starts the measurement/ integration by the duration of the <i>Integration Period</i> on condition: falling value of the RMS result (<i>Source</i>) integrated during 0,5 ms passes below the threshold value (<i>Level</i>).		Chapter 4.2
Level+	Type of trigger that starts the 1-second measurement/ integration under the condition: value of the RMS result (<i>Source</i>) integrated during 0,5 ms is greater than the threshold value (<i>Level</i>). In other cases, the instrument continues checking the trigger condition every 0.5 ms. During one measurement cycle the instrument performs as many 1-second integrations as many seconds the <i>Integration Period</i> consists and stops the measurement cycle.		Chapter 4.2
Level-	Type of trigger that starts the 1-second measurement/ integration under the condition: value of the RMS result (<i>Source</i>) integrated during 0.5 ms is lower than the threshold value (<i>Level</i>). In other cases, the instrument continues checking the trigger condition every 0.5 ms. During one measurement cycle the instrument performs as many 1-second integrations as many seconds the <i>Integration Period</i> consists and stops the measurement cycle.		Chapter 4.2
Gradient+	Type of trigger that starts the 1-second measurement/ integration under the condition: value of the RMS result (<i>Source</i>) integrated during 0,5 ms is greater than the threshold level (<i>Level</i>) and the gradient of this Source is greater than the threshold level (<i>Gradient</i>). In other cases, the instrument continues checking the trigger condition every 0.5 ms. During one measurement cycle the instrument performs as many 1-second integrations as many seconds the <i>Integration Period</i> consists and stops the measurement cycle.		Chapter 4.2

	This type of trigger has the same logic as Level+ trigger, but the trigger condition requires also gradient level to be exceeded.		
<i>Source</i>	Measured result that is compared with the threshold level (<i>Level</i>) for triggering – RMS measured in the first profile: Leq(1).		Chapter 4.2
<i>Level</i>	Threshold level of the <i>Source</i> for triggering condition fulfilment.		Chapter 4.2
<i>Gradient</i>	Threshold level of the source signal value speed of changing (Gradient) for trigger condition fulfilment.		Chapter 4.2
<i>Statistical Levels</i>	Screen that enables setting a boundary level (<i>Ln</i>) surpassed by the temporary noise level values in not more than nn% of the observation period. The user can define ten statistical levels, named from N1 to N10, to be calculated, displayed and saved in the files together with the main results.		Chapter 4.8 Appendix D
<i>Timer</i>	Screen that enables configuring automatic switching On the instrument and performing the measurement on the programmed time with defined setup. Timer can be <i>Single</i> or repeatable (<i>Multiple</i>). After every timer cycle, the instrument automatically switches itself off.		Chapter 4.9
<i>Logging</i>	Screen that enables configuring saving of the <i>Summary Results</i> , <i>Logger Results</i> and a waveform signal in files with the use of the next screens: <i>Logger Setup</i> , <i>Logger Results</i> , <i>Logger Trigger</i> and <i>Event Recording</i> .		Chapter 4.5
<i>Logger Setup</i>	Screen that enables switching the logger function on and setting the main logging parameters: <i>Logger</i> , <i>Split</i> , <i>Logger Step</i> and <i>Logger Name</i> .		Chapter 4.5.1

<i>Logger</i>	Position in the <i>Logger Setup</i> list that switches On or Off the <i>Logging</i> functionality. If <i>Logger</i> is Off no data recording is available.		Chapter 4.5.1
<i>Logger Split</i>	Position in the <i>Logger Setup</i> screen that enables saving of the logger records in separate files according to different rules: after the integration period, or every quarter/half an hour/hour, or on specific times of a day.		Chapter 4.5.1
<i>Logger Step</i>	Time of measuring/integrating <i>Logger Results</i> and recording them to the logger file (same meaning as <i>Integration Period</i> for <i>Summary Results</i>). <i>Logger Step</i> can be selected from the set: 100 ms, 200 ms, 500 ms or from 1 second to 59 seconds with 1-second step or from 1 minute to 59 minutes with 1-minute step and up to 1 hour.		Chapter 4.5.1
<i>Logger Name</i>	Position in the <i>Logger Setup</i> screen that enables defining the name of file in which <i>Logger Results</i> , <i>Summary Results</i> , <i>Markers</i> and <i>Event Recordings</i> will be saved.		Chapter 4.5.1
<i>Summary Results</i>	Main measurement results: <i>Leq</i> , <i>Lpeak</i> , <i>Lmax</i> , <i>Lmin</i> , <i>L</i> , <i>LE</i> , <i>Lden</i> , <i>LEPd</i> , <i>Ltm3</i> , <i>Ltm5</i> , <i>LR1</i> , <i>LR2</i> statistics <i>Ln</i> , <i>EX</i> , <i>SD</i> and <i>OVL</i> ; that are measured, displayed and saved in the file with the <i>Integration Period</i> step as many times as defined by the <i>Repetition Cycles</i> parameter. They are renewed and displayed every second when the measurement is running. The saving of the <i>Summary Results</i> can be switched on or off in the <i>Logger Setup</i> screen.		Chapter 4.5.1
<i>Logger Results</i>	Screen in the <i>Logging</i> list enabling selecting results that will be logged to the logger file as a time-history with the <i>Logger Step</i> : <i>Lpeak</i> , <i>Lmax</i> , <i>Lmin</i> , <i>Leq</i> , <i>LR1</i> , <i>LR2</i> . For the 1/1 <i>Octave</i> and 1/3 <i>Octave</i> functions also spectra can be saved.		Chapter 4.5.2
<i>Logger Trigger</i>	Screen that enables configuring parameters for triggering of <i>Logger Results</i> recording to the logger file: <i>Trigger</i> , <i>Source</i> , <i>Level</i> , <i>Pre Trigger</i> and <i>Post Trigger</i> .		Chapter 4.5.3

<i>Trigger</i>	Position that switches Off or On the logger trigger by selecting its type: <i>Level+</i> or <i>Level-</i> . If the instrument is waiting for the trigger condition, the appropriate trigger icon is flashing on the display alternatively with the „logger” icon.		Chapter 4.5.3
<i>Level+</i>	Type of trigger, that starts logging of <i>Logger Results</i> under the condition: value of the Leq result (<i>Source</i>) integrated by the <i>Logger Step</i> period is greater than the threshold level (<i>Level</i>). In other cases, the logging is skipped.		Chapter 4.5.3
<i>Level-</i>	Type of trigger, that starts logging of <i>Logger Results</i> under the condition: value of the Leq result (<i>Source</i>) integrated by the <i>Logger Step</i> period is lower than the threshold level (<i>Level</i>). In other cases, the logging is skipped.		Chapter 4.5.3
<i>Source</i>	Measured result that is compared with the threshold level (<i>Level</i>) for triggering – LEQ measured in the first profile (Leq(1)).		Chapter 4.5.3
<i>Level</i>	Threshold level of <i>Source</i> for triggering condition fulfilment.		Chapter 4.5.3
<i>Pre Trigger</i>	Period of additional logging before triggering condition fulfilment.		Chapter 4.5.3
<i>Post Trigger</i>	Period of additional logging after triggering condition fulfilment.		Chapter 4.5.3
<i>Wave Recording</i>	Recording of the waveform signal in the wave file.		Chapter 4.5.4

<i>Recording</i>	Switching on the signal recording: <i>Continuous</i> or on trigger: <i>Slope+</i> , <i>Slope -</i> , <i>Level+</i> , <i>Level-</i> , <i>Gradient+</i> , <i>Trigger Chapter</i> or <i>Integr. Period</i> . Continuous means that the waveform signal will be recorded continuously from the start of the measurement till its end. On trigger recording put additional conditions for triggering and ending of the recording. If the instrument is waiting for the trigger condition, the appropriate trigger icon is flashing on the display alternatively with the „signal” icon.		Chapter 4.5.4
<i>Slope+</i>	Type of trigger that starts the signal recording for <i>Recording Time</i> under the condition: rising value of the LEQ result (<i>Source</i>) integrated during 0,5 ms passes above the threshold level (<i>Level</i>).		Chapter 4.5.4
<i>Slope -</i>	Type of trigger that starts the signal recording for <i>Recording Time</i> under the condition: falling value of the LEQ result (<i>Source</i>) integrated during 0,5 ms passes below the threshold level (<i>Level</i>).		Chapter 4.5.4
<i>Level+</i>	Type of trigger that starts the signal recording for <i>Recording Time</i> under the condition: value of the LEQ result (<i>Source</i>) integrated by the 0,5 ms period is greater than the threshold level (<i>Level</i>).		Chapter 4.5.4
<i>Level-</i>	Type of trigger that starts the signal recording to start for <i>Recording Time</i> under the condition: value of the LEQ result (<i>Source</i>) integrated by the 0,5 ms period is lower than the threshold level (<i>Level</i>).		Chapter 4.5.4
<i>Gradient+</i>	Type of trigger that starts the signal recording for <i>Recording Time</i> under the condition: value of the LEQ result (<i>Source</i>) integrated by the 0,5 ms period is greater than the threshold level (<i>Level</i>) and the gradient of this Source is greater than the threshold level (<i>Gradient</i>).		Chapter 4.5.4
<i>Trigger manual</i>	Type of trigger that starts manual triggering of the signal recording start after pressing simultaneously ◀ and ▶ keys during the measurement.		Chapter 4.5.4

Integr. Period Type of trigger that starts the signal recording for *Recording Time* every time the measurement starts. If *Integration Period* is shorter than *Recording Time*, the event recording will be continued for additional *Recording Time*.




Chapter
[4.5.4](#)

Filter Weighting filter used during signal recording: Z, A, C, B or LF.




Chapter
[4.5.4](#)

Sampling Sampling frequency of the event recording: 24 kHz or 12 kHz.



Chapter
[4.5.4](#)

Signal Gain Gain of the recorded signal: 0 dB ... 40 dB.




Chapter
[4.5.4](#)

Source Measured result that is compared with the threshold level for triggering (*Level*) – LEQ measured in the first profile: Leq(1).




Chapter
[4.5.4](#)

Level Threshold level of the *Source* for the trigger condition fulfilment.




Chapter
[4.5.4](#)

Trigger Period Time interval of checking the triggering conditions. This parameter can be set as: Logger Step, 0.5 ms, 100.0 ms and 1 s.











Chapter
[4.5.4](#)

Gradient Threshold level of the source signal value speed of changing (Gradient) for trigger condition fulfilment.



Chapter
[4.5.4](#)

<i>Pre Trigger</i>	Period of signal recording before the first trigger condition moment: Off or 1 s.		Chapter 4.5.4
<i>Recording Time</i>	Time of the signal recording after meeting every trigger condition. The available values can be selected from 1 s to 8 h. Recording stops after <i>Recording Time</i> or earlier if the measurement is stopped manually.		Chapter 4.5.4
<i>Spectrum</i>	Screen that enables setting the <i>1/1 Octave</i> or <i>1/3 Octave</i> spectrum parameters setup: <i>Filter</i> and <i>Detector</i> .		Chapter 10.2.4
<i>Peak Sp.</i>	Position in the <i>Logger Results</i> screen that switches on/off the Lpeak spectra saving as a time-history in a logger file.		Chapter 10.2.3
<i>Leq Sp.</i>	Position in the <i>Logger Results</i> screen that switches on/off the Leq spectra saving as a time-history in a logger file.		Chapter 10.2.3
<i>Filter</i>	Weighting filters for the <i>1/1 Octave</i> and <i>1/3 Octave</i> analysis: A, B, C, Z.		Chapter 10.2.4
<i>Detector</i>	Type of integration of RMS based results for <i>1/1 Octave</i> and <i>1/3 Octave</i> analysis: Linear, Fast or Slow.		Chapter 10.2.4
<i>Pause</i>	Automatic pause(s) in the <i>Dosimeter</i> mode, that can be programmed based on absolute time.		Chapter 11.2

Exposure Time Total time during working day in which the worker is exposed to the noise. This time is considered for the LEPd result calculation.



Chapter
[11.5](#)
Appendix D

Criterion Level Steady noise level permitted for a full eight-hour work shift.



Chapter
[11.3](#)

Threshold Level Noise level limit below which the dosimeter does not accumulate noise dose data.




Chapter
[11.3](#)

Exchange Rate Amount by which the permitted sound level may increase if the exposure time is halved.




Chapter
[11.3](#)

ULT Threshold Level Threshold level for calculation of ULT results.




Chapter
[11.3](#)

PTC Threshold Level Threshold level for calculation of PTC results.



Chapter
[11.3](#)

RT60 Settings Screen that enables setting the reverberation time measurement parameters: *Start Delay*, *Method*, *Recording Time*, *Time Step*, *Averaging*, *Noise Mar.*, *Octave*, *Freq. Range*, *Logger Name* and *Level*.











Chapter
[12.2](#)

Start Delay Delay between pressing the <Start> key and the start of the RT60 measurement.



Chapter
[12.2](#)

<i>Method</i>	Method of the RT60 calculation: <i>Decay</i> (Interrupted Noise Method) or <i>Impulse</i> (Impulse Response Method). The selection of the method depends on the used type of the sound source.		Chapter 12.2
<i>Recording me</i>	<i>Ti</i> Time of measurement data (sound pressure level decay curve) registration during RT60 calculations: 1s .. 30 s or <i>Auto</i> .		Chapter 12.2
<i>Time Step</i>	Time-step of data registration (sound pressure level) in the file during RT60 calculations: 2, 5, 10, 20, 50 ms.		Chapter 12.2
<i>Averaging</i>	Averaging of the reverberation time results from several measurements during RT60 calculations.		Chapter 12.2
<i>Noise Mar.</i>	Margin value to the calculated noise level for RT60 calculations: 0 ÷ 20 dB.		Chapter 12.2
<i>Octave</i>	Type of spectrum (1/1 octave or 1/3 octave) based on which the RT60 analysis is performed.		Chapter 12.2
<i>Freq. Range</i>	Frequency range for RT60 calculations: 63Hz-4kHz (7 bands) and 63Hz-8kHz (8 bands) for 1/1 octave ; 50Hz-5kHz (21 bands) and 50Hz-10kHz (24 bands) for 1/3 octave.		Chapter 12.2
<i>Logger Name</i>	Name of the Logger file in which data of the RT60 analysis will be recorded.		Chapter 12.2







Level

Threshold level of the sound source for triggering the RT60 measurement. If the measured sound is below the *Level* value, the RT60 measurement will not start.




Chapter
[12.2](#)

16.5 DISPLAY PARAMETERS


Name	Description	Screen	Reference
<i>Display</i>	Section of the Main Menu that enables setting of the measurement views.		Chapter 5
<i>Display Mode</i>	Mode of measurement results presentation - view. Views can be activated in the <i>Display Modes</i> screen.		Chapter 5.1
<i>One Result view</i>	View of the one result. This view is always available and cannot be disabled.		Chapter 5.1.1
<i>Running SPL view</i>	View of the running SPL result. This view is used before the measurement start for the noise level estimation.		Chapter 2.6 , 5.1.5
<i>3 Profiles view</i>	View of three results on the display at the same time.		Chapter 5.1.2
<i>Logger view</i>	View of time-history (logger) results.		Chapter 5.1.3

Statistics view View of statistics of sound results.




Chapter
[5.1.4](#)

Spectrum view View spectra: 1/1 Octave and 1/3 Octave.




Chapter
[5.1](#), [10.3](#)

RT60 results view View of RT60 results calculated for octave or third-octave bands: EDT, RT20, RT30; and averaged results: AEDT, ART20, ART30.




Chapter
[12.4](#)

Display Scale Screen that enables setting parameters of the results presentation: *Dynamics*, *Grid* and *Autoscale*.




Chapter
[5.2](#)

Dynamics Range of the plot scale: 10 dB, 20 dB, 40 dB, 80 dB, 100 dB and 120 dB.




Chapter
[5.2](#)

Grid Toggle of the grid on the graph views.




Chapter
[5.2](#)

Autoscale Switching automatic scale adjustment of the Y axis.



Chapter
[5.2](#)

Measurement Results Screen that enables selecting the Sound Level Meter and/or Dose Meter results, which will be presented on the display.



Chapter
[5.3](#)

SLM Results Screen that enables selecting the Sound Level Meter results, which will be presented on the display.



Chapter
[5.3](#)

Dosimeter Results Screen that enables selecting the Dose Meter results, which will be presented on the display.




Chapter
[5.3](#)

Logger Results Screen that enables selecting time-history results, which will be presented on the display.




Chapter
[5.4](#)

Spectrum View Screen that enables selecting types of spectra for displaying: Averaged, Instantaneous, Max, Min and Peak.




Chapter
[10.3.3](#)

Instantaneous Spectrum of instantaneous *Leq* results for the 1/1 Octave or 1/3 Octave bands.




Chapter
[10.3.3](#)

Averaged Spectrum of averaged *Leq* results for the 1/1 Octave or 1/3 Octave bands.




Chapter
[10.3.3](#)

Max Spectrum of *Lmax* results for the 1/1 Octave or 1/3 Octave bands.




Chapter
[10.3.3](#)

Min Spectrum of *Lmin* results for the 1/1 Octave or 1/3 Octave bands.




Chapter
[10.3.3](#)

Peak Spectrum of *Lpeak* results for the *1/1 Octave* or *1/3 Octave* bands.




Chapter
[10.3.3](#)

Screen Setup Screen that enables setting the screen brightness and power saving.




Chapter
[5.5](#)

Auto Rotation Switching on the adjustment of the screen image on the display according to the instrument's physical orientation in space.




Chapter
[5.5](#)

Dim Mode Screen dimming in no activity after delay. The screen may be switch off (*Screen Off*) or dimmed with different levels (*Level 1, 2 or 3*).



Chapter
[5.5](#)

Dim Delay Screen dimming time delay in no activity after last key pressing.




Chapter
[5.5](#)









Col. Scheme Colour scheme of the screen.



Chapter
[5.5](#)

16.6 INSTRUMENT PARAMETERS

Name	Description	Screen	Reference
Instrument	Section in the Main Menu that enables setting the hardware components of the instrument in the screens: <i>User Interface</i> , <i>Battery</i> , <i>Keyboard</i> , <i>Power Off</i> , <i>USB</i> , <i>Communication Ports</i> , <i>Self Vibration</i> , <i>RTC</i> and <i>Unit Label</i> .		Chapter 7

<i>User Interface</i>	Screen that allows to select the user interface - a set of functions that are available for the user. Instrument offers three types of user interface: limited to start and stop of the measurement (<i>Start/Stop</i>), narrow set of functions for novice users (<i>Simple</i>) and full set of functions (<i>Advanced</i>).		Chapter 7.1
<i>Start/Stop</i>	User interface mode that limits the menu to only one <i>User Interface</i> position in the main <i>Menu</i> and measurement screens		Chapter 7.1
<i>Simple</i>	User interface that limits instrument's settings to the most frequent used positions, hiding other positions. Before activation of the <i>Simple</i> mode the user may decide whether to leave settings of hiding positions as they were set before the activation of the <i>Simple</i> mode or to reset them to the factory default settings.		Chapter 7.1
<i>Advanced</i>	User interface that enables full scope of instrument settings.		Chapter 7.1
<i>Battery</i>	Position in the <i>Instrument</i> list that enables checking of the instrument power source status.		Chapter 7.2
<i>Keyboard</i>	Position in the <i>Instrument</i> list that enables setting of the Shift, Alt, Start/Stop keys functionality and programming of locking/unlocking the keyboard.		Chapter 7.3
<i>Power Off</i>	Position in the <i>Instrument</i> list that enables selecting of the period after which the instrument will automatically switches off in case there was no any key pressed during this period.		Chapter 7.4
<i>USB</i>	Position in the <i>Instrument</i> list that enables selecting the transmission speed of the USB interface. There are two options: <i>Full 12Mbps</i> and <i>High 480Mbps</i> .		Chapter 7.5


Communication Ports Position in the *Instrument* list that enables selecting and programming the serial port of the instrument (*Serial Port*).



Chapter
[7.6](#)

Serial Port Position in the *Communication Ports* list which enables selecting the serial port of the instrument – *RS232* or *Bluetooth*.

In the case of the *RS232* serial port, you can set the transmission speed (*Baud Rate*) and the time limit during for the data transfer (*Time Out*). In the case of *Bluetooth*, you can set the PIN.




Chapter
[7.6](#)

Self Vibration Position in the *Instrument* list that enables defining the threshold level for the self-vibration of the instrument for marker registration. The special marker will be written to the file when the self-vibration of the instrument is higher than defined in the *Marker Thr.* position.



Chapter
[7.2](#)

RTC Instrument's Real Time Clock. This clock is displayed in the upper right corner places of the display.





Chapter
[7.3](#)

Unit Label Information about the instrument type, its serial number, the current software version installed and the relevant standards, which the instrument fulfils.



Chapter
[7.4](#)

16.7 AUXILIARY PARAMETERS

Name	Description	Screen	Reference
Auxiliary Setup	Section in the Main Menu that enables customizing the instrument interface to specific user requirements in the screens: <i>Language</i> , <i>Factory Settings</i> , <i>Comments</i> , <i>Leq & Lav</i> and <i>Warnings</i> .		Chapter 8
Language	Screen that enables selecting the user interface language.		Chapter 8.1

Factory Settings

Restoration of the default settings of the instrument.



Chapter
[8.2](#)

Comments

Definition of the file name for recording of voice comments.



Chapter
[8.3](#)

Leq & Lav


Position in the *Auxiliary Setup* screen that enables to control displaying of Leq and Lav results: *Both* or *Mutually Exclusive*.



Chapter
[8.4](#)




Warnings

Activation of the warning messages, which are to be displayed during the normal operation of the instrument.



Chapter
[8.5](#)

16.8 REPORT

Name	Description	Screen	Reference
<i>Report</i>	Section in the Main Menu that enables configuring and printing measurement reports in the predefined format and includes positions: <i>Print</i> , <i>Options</i> , <i>Results</i> , <i>Statistics</i> , <i>Spectrum</i> and <i>Printer</i> .		Chapter 9
<i>Print</i>	Position in the <i>Report</i> screen that enables printing of the report.		Chapter 9.1
<i>Options</i>	Position in the <i>Report</i> screen that enables specifying the report content, selecting profiles, results for these profiles, statistics and spectra which will be included in the report.		Chapter 9.2

Results


Position in the *Report* screen that allows you to select results to be included in the report for the selected profiles.



Chapter
[9.3](#)

Statistics


Position in the *Report* screen that allows you to select statistic levels from *N1* to *N10* to be included in the report.



Chapter
[9.4](#)

Spectrum


Position in the *Report* screen that allows you to select based on their central frequencies the 1/1 or 1/3 octave bands which will be included in the report for the *Leq*, *Lmax*, *Lmin* and *Lpeak* spectra.



Chapter
[9.5](#)

Printer

Position in the *Report* screen that enables setting the number of characters in the report lines – from 20 to 500.



Chapter
[9.6](#)

APPENDIX A. REMOTE CONTROL

The **USB 2.0 interface** is the Type C serial interface working with 480 MHz clock which enables one to control remotely the unit. Its speed is relatively high, and it ensures the common usage of USB-C in most produced nowadays Personal Computers.

Alternatively, all commands described in this appendix are valid for any other kinds of interfaces (if present) like **Bluetooth** communication **or RS232**.

Functions, which are developed in order to control data flow in the serial interfaces, ensure:

- Bi-directional data transmission,
- Remote control of the instrument.

In order to program the serial interface, the user has to:

1. send a "function code",
2. get a response to the "function code"
3. send/receive a data file (optionally)

A.1 INPUT/OUTPUT TRANSMISSION TYPES

Following basic input/output transmission types (called functions) are available:

- #1** – general control functions,
- #2** – read out of the measurement results in the **SLM** mode,
- #3** – read out of the measurement results in the **1/1** or **1/3 Octave** analysis mode,
- #4** – read out data from the setup file,
- #5** – read out of the statistical analysis results,
- #7** – special control functions,
- #9** – writing data to the setup file,
- #D** – data files access,
- #S** – direct setup access.

A.2 FUNCTION #1 – GENERAL CONTROL FUNCTIONS

#1 function enables the user to send the control setting codes to the instrument and read out a file containing the current control state. A list of the control setting codes is given in A.3 **Control setting codes**. The format of #1 function is defined as follows:

#1,Xccc,Xccc,(...),Xccc; (1)

or

#1,Xccc,X?,Xccc,(...),X?,Xccc; (2)

or

#1,X?,X?,(...),X?; (3)

where:

X - group code, **ccc** – new code value,

X? - request to send the current X code setting.

In the first case (1) the instrument does not respond to a command, even if an error occurs.

In the second and third cases (2), (3) the instrument outputs control settings for all requests X? in the following format:

#1,Xccc,Xccc,(...),Xccc;



Note: All bytes of that transmission are ASCII characters.



Note: Changing settings using #1 functions during measurements running state (#1,S1;) is blocked. Stop the measurements (#1,S0;) before changing the settings.

In order to read out all current control settings the user should send to the device the following sequence of characters:

#1;

In this case the instrument outputs all control settings given in A.3 **Control setting codes** in the format:

#1,Xccc,Xccc,(...),Xccc;

Example: The instrument sends the following sequence of characters as an answer for the mentioned above request:

#1,U971,N1234,W1.05.1,Q0.01,M1,R1,F2:1,F3:2,F1:3,F2:4,F3:5,F1:6,J2:1,J3:2,J1:3,J3:4,J3:5,J1:6,f1,C1:1,C0:2,C2:3,C1:4,C0:5,C2:6,B0:1,B3:2,B15:3,b0,d1s,D10s,K5,L0,Y3,y0,XT0,XL100,XQ0,Xq0,XC115:1,XC115:2,XC115:3,XI115:1,XI115:2,XI115:3,XA0,XD-1:1,XD-1:2,XD-1:3,XD-1:4,XD-1:5,XD-1:6,S0,T1,e480,c1:1,c1:2,c1:3,h0:1,h0:2,h0:3,x3:1,x3:2,x5:3,m0,s0,l100,O10,o0,t0;

means that:

- SV 971A is investigated (**U971**); see #7,US; command for unit subtype information;
- its number is 1234 (N1234);
- software version number is 1.05.1 (W1.05.1);
- calibration factor is equal to 0.01 dB (Q0.01);
- **Level Meter** is selected as the measurement function (M1);
- range is **Low** (R1);
- **A** filter is selected in profile 1, SLM function (F2:1);
- **C** filter is selected in profile 2, SLM function (F3:2);
- **Z** filter is chosen in profile 3, SLM function (F1:3);
- **A** filter is selected in profile 1, Dosimeter function (F2:4);
- **C** filter is selected in profile 2, Dosimeter function (F3:5);
- **Z** filter is chosen in profile 3, Dosimeter function (F1:6);
- **A** Peak filter is selected in profile 1, left channel, SLM function (J2:1);
- **C** Peak filter is selected in profile 2, left channel, SLM function (J3:2);
- **Z** Peak filter is selected in profile 3, left channel, SLM function (J1:3);
- **C** Peak filter is selected in profile 1, both channels, Dosimeter function (J3:4);
- **C** Peak filter is selected in profile 2, both channels, Dosimeter function (J3:5);
- **Z** Peak filter is selected in profile 3, both channels, Dosimeter function (J1:6);
- **Z** filter is selected for **1/1 Octave** or **1/3 Octave** analysis (f1)
- **Fast** detector is selected in profile 1, SLM function (C1:1);
- **Impulse** detector is chosen in profile 2, SLM function (C0:2);
- **Slow** detector is selected in profile 3, SLM function (C2:3);
- **Fast** detector is selected in profile 1, Dosimeter function (C1:4);
- **Impulse** detector is chosen in profile 2, Dosimeter function (C0:5);
- **Slow** detector is selected in profile 3, Dosimeter function (C2:6);
- logger's buffer is not filled by the results from profile 1 (B0:1);
- **Lpeak** and **Lmax** values are stored in the files of the logger from profile 2 (B3:2);
- **Lpeak**, **Lmax**, **Lmin** and **Leq** values are stored in the files of the logger from profile 3 (B15:3);
- results of **1/1 Octave** or **1/3 Octave** analysis are not stored in the files of the logger (b0);

- results are stored in a logger's file every 1 second (d1s);
- integration period is equal to 10 seconds (D10s);
- the measurement has to be repeated 5 times (K5);
- linear detector is selected to the **Leq** calculations (L0);
- .. and so on.

See A.3 **Control setting codes** for more details.



Note: Control settings presented in the instrument's response and not described in A.3 **Control setting codes** considered as reserved. Do not change these settings!

A.3. FUNCTION #2 – MEASUREMENT RESULTS READ-OUT IN THE SLM MODE

#2 function enables one to read out the current measurement results from the selected profile.

#2 function has the format defined as follows:

#2 [<aver>] [<profile>] [[[,X?] ,X?] ,(...)];

where:

<aver> – type of results:

- i** – instantaneous results, i.e. results from the current cycle (default),
- a** – averaged results, i.e. results from the previous cycle,

<profile> – profile number:

1, 2 or 3 – one of the profile, i.e. only results from the given profile will be sent;

X – code of the specified result (see below); if no codes are specified all results will be sent;

In the case of **<profile> = 1, 2 or 3** the instrument sends results in the format defined as follows:

#2 [<aver>],<profile>,Xccc,(...);

where **ccc** is the value of the result **X** or question mark (?) if result **X** is not available;

If no results are available, the instrument returns:

#2,?;

The **X** codes of the results from the **SLM** mode are defined as follows:

- v** under-range flag (ccc equals to 0 when the overload did not occur, 2 when the under-range took place during the last measurement period but did not occur in the last second of the measurement and 3 when the under-range took place during the last measurement period and it lasted in the last second of the measurement);
- V** overload flag (ccc equals to 0 or 1);
- T** time of the measurement (ccc – value in seconds);
- x** start date of the measurement in format **dd/mm/yyyy** (**dd** – day, **mm** – month, **yyyy** - year)
- t** start time of the measurement in format **hh/mm/ss** (**hh** – hour, **mm** – minute, **ss** - second)
- P** **Lpeak** value (ccc – the value in dB);
- M** **Lmax** value (ccc – the value in dB);
- N** **Lmin** value (ccc – the value in dB);
- S** **L** result (ccc – the value in dB);
- R** **Leq** result (ccc – the value in dB).
- U** **LE** result (ccc – the value in dB);
- B(k)** **Lden** result (ccc – the value in dB; k – flag determining the kind of the result);

l(nn) **LEPd** result (ccc – the value in dB, nn – the value of Exposure Time in minutes);
Y **Ltm3** result (ccc – the value in dB);
Z **Ltm5** result (ccc – the value in dB);
L(nn) **L** result of the nn statistics (ccc – the value in dB).
g **LR1** result (ccc – the value in dB);
G **LR2** result (ccc – the value in dB);
s **SD** result (ccc – the value in dB);
k **EX** result (ccc – the value in dB);



Note: In the case of **Lden**, the value *k* placed in the parenthesis after the code **B**, denotes the kind of the currently measured result. The kind of the **Lden** result depends on the time during which the measurements were performed (**d** denotes day, **e** denotes evening and **n** denotes night). The corresponding values of *k* parameter and the kind of the measured **Lden** result are presented below:

k = 1 **Ld** result,
k = 2 **Le** result,
k = 3 **Lde** result,
k = 4 **Ln** result,
k = 5 **Lnd** result,
k = 6 **Len** result,
k = 7 **Lden** result.

The codes of the results from the **DOSE METER** mode are defined as follows:

v under-range flag (ccc equals to 0 when the overload did not occur, 2 when the under-range took place during the last measurement period but did not occur in the last second of the measurement and 3 when the under-range took place during the last measurement period and it lasted in the last second of the measurement);
V overload flag (ccc equals to 0 or 1);
T time of the measurement (ccc – value in seconds);
x start date of the measurement in format *dd/mm/yyyy* (*dd* – day, *mm* – month, *yyyy* - year)
t start time of the measurement in format *hh/mm/ss* (*hh* – hour, *mm* – minute, *ss* - second)
P **Lpeak** value (ccc – the value in dB);
M **Lmax** value (ccc – the value in dB);
N **Lmin** value (ccc – the value in dB);
S **L** result (ccc – the value in dB);
D **DOSE** result (ccc – the value in %);
d **D_8h** result (ccc – the value in %);
p **PrDOSE** result (ccc – the value in %);
A **LAV** result (ccc – the value in dB);
R **Leq** result (ccc – the value in dB);
U **LE** result (ccc – the value in dB);
u **SEL8** result (ccc – the value in dB);
E **E** result (ccc – the value in Pa²h);
e **E_8h** result (ccc – the value in Pa²h);
l(nn) **LEPd** result (ccc – the value in dB, nn – the value of Exposure Time in minutes);
J **PSEL** result (ccc – the value in dB);
Y **Ltm3** result (ccc – the value in dB);
Z **Ltm5** result (ccc – the value in dB);

L(nn) value L of the nn statistics (ccc – the value in dB);

C **PTC** result (ccc – the counter value);

c **PTP** result (ccc – the value in %);

I **ULT** result (ccc – value in seconds);

W **TWA** result (ccc – the value in dB);

w **PrTWA** result (ccc – the value in dB);

a **Lc-a** result (ccc – the value in dB);

The exemplary results of the instrument's response after sending to it the following sequence of characters: **#2,1**; coming from the first profile are given below:

a) for the case of the **SLM** mode:

#2,1,x17/03/2014,t13:44:28,v0,V0,T10,P79.97,M52.92,N38.50,S46.35,R43.91,U53.91,B(1)43.91,I(480)43.92,Y50.67,Z51.15,L(01)55.00,L(10)45.60,L(20)44.30,L(30)42.80,L(40)41.50,L(50)40.80,L(60)40.40,L(70)40.00,L(80)39.50,L(90)39.00,g?,G?,k?,s?;

b) and for the case of the **Dosimeter** mode:

#2,1,x17/03/2014,t13:48:36,v0,V0,T7,P124.39,M99.26,N41.54,S42.05,D0,d389,p389,A85.86,R85.86,U94.31,u130.45,E0.00,e1.23,I(480)85.87,J49.72,Y95.62,Z99.22,L(01)100.30,L(10)89.50,L(20)78.60,L(30)68.50,L(40)60.30,L(50)54.00,L(60)51.00,L(70)46.50,L(80)44.00,L(90)42.40,C4,c6,I0,W49.72,w85.87,a-0.55;



Note: The presented above order of the measurement results sent out by the instrument does not depend about the characters sent to the unit.

Example: After sending to the instrument the string:

#2,1,T?,R?,V?,P?,L?;

the unit sends out the results of measurement coming from the first profile in predefined, described above, order:

#2,1,V0,T1,P65.80,R43.99,L(01)52.00,L(10)51.10,L(20)46.10,L(30)44.10,L(40)38.60,L(50)38.10,L(60)37.60,L(70)37.10,L(80)36.60,L(90)36.10;

Read-out the RT60 results

In the case of RT60 function there are additional codes:

#2,EDT; this function allows you to read the current EDT results.

#2,T20; this function allows you to read the current RT20 results.

#2,T30; this function allows you to read the current RT30 results.

The function's answer is in the one of the following format:

#2,<type>,0,<status>; when results are not available

#2,<type>,1,<results>; when results are available.

<type> accepts the following values: EDT/T20/T30

<status> is the status of device

0 – no results,

1 – waiting for trigger,

2 – measurement in progress,

3 – calculations

<results> is the full list of frequencies with corresponding results in the format:

freq1:value1,freq2:value2,...,freqN:valueN

The exemplary answer:

```
#2,T30,1,50.0Hz:0.36s,63.0Hz:0.41s,80.0Hz:0.20s,100Hz:---
,125Hz:0.07s,160Hz:0.09s,200Hz:0.32s,250Hz:0.33s,315Hz:0.44s,400Hz:0.29s,500Hz:0.39s,630Hz:0.49
s,800Hz:0.44s,1.00k:0.47s,1.25k:0.46s,1.60k:0.34s,2.00k:0.42s,2.50k:0.40s,3.15k:0.42s,4.00k:0.42s,5.
00k:0.41s,TOT.A:0.42s,TOT.C:0.42s,TOT.Z:0.42s;
```

A.2.3. Read-out the STIPA results

#2,STI,CP; this command creates new project and returns new project name.

#2,STI,CA; this command creates new area and returns new area name.

#2,STI,CS; this command creates new source and returns new source name. e.g. **#2,STI,CS,"S2";**

#2,STI,PL; this command returns the project list. e.g. **#2,STI,PL,2,"PROJ0001","PROJ0002";**

#2,STI,AL; this command returns the area list. e.g. **#2,STI,AL,2,"AREA1","AREA2";**

#2,STI,SL; this command returns the source list. e.g. **#2,STI,SL,2,"S1","S2";**

The following list of commands require prior setting of the project, area and source.

#2,STI,NP; this command adds the new point and returns the new point ID.

#2,STI,PC; this command returns the count of the measurement points and list of point IDs. e.g.

#2,STI,PC,n,1,2,3;

#2,STI,MC,p; this command returns the count of the measurements at the point **p**.

#2,STI,AP,p; this command allows you to read and set average flag at the point **p**.

#2,STI,AM,p,m; this command allows you to read and set average flag for the **m** measurement at the point **p**.

#2,STI,DP,p; this command deletes the point **p**.

#2,STI,DM,p,m; this command deleted the measurement **m** at the point **p**.

#2,STI,MR,p,m,mrn; this command allows you to read the results of the **m** measurement at the point **p**.

#2,STI,FR,p,m,frn; this command allows you to read the modulation results of the **m** measurement at the point **p**.

#2,STI,SN; this command allows you to read and write Ambient Noise parameters. e.g.

#2,STI,SN,enabled,90.0,91.0,...,95.0;

p: 0..PointCount-1

m: 0..MeasurementCount-1

mrn: STI,LAQ,LCQ,LAS,STM,FLG

frn: LZQ,MF1,MF2,ERR

enabled: 0/1

flags: UNDERRANGE = 1, OVERLOAD = 2



Note: All bytes of that transmission are ASCII characters.

A.4. FUNCTION #3 – MEASUREMENT RESULTS READ-OUT IN 1/1 AND 1/3 OCTAVE MODES

#3 function enables one to read out the current measurement results in **1/1 Octave** or **1/3 Octave** modes, depends on device function selected.

#3 function format is defined as follows:

#3; - displayed spectrum

#3,A; - averaged spectrum

#3,I; - instantaneous spectrum

#3,M; - max spectrum

#3,N; - min spectrum

#3,P; - peak spectrum

The device responds, sending the last measured spectrum (when the instrument is in STOP state) or currently measured spectrum (when the instrument is in RUN state) in the following format:

#3[,T<time>];<Status Byte> <LSB of the transmission counter> <MSB of the transmission counter> <data byte> (...) <data byte>

<time> is the measurement time given in seconds

<Status Byte> gives the information about the current state of the instrument.

D7	D6	D5	D4	D3	D2	D1	D0
----	----	----	----	----	----	----	----

where:

- D7 = 0 means that "overload does not happen",
= 1 means that "overload appeared",
- D6 = 0 means that "spectrum is not averaged",
= 1 means that "spectrum is averaged",
- D4 = 0 the instantaneous current result (RUN State),
= 1 the final result (STOP State),
- D3 = 1 results in **1/3 Octave** mode,
- D2 = 1 results in **1/1 Octave** mode,
- D5, D1, D0 reserved bits.



Note: ASCII part of the response ends with semicolon ";". Status byte, transmission counter and data bytes are coded in binary form.



Note: The measurement result is coded in binary form as dB•100 (e.g. 34.5 dB is sent as binary number 3450).

A.5. FUNCTION #4 – SETUP FILE READ-OUT

#4 function enables the user to read-out a file from the internal Flash-disk or RAM memory. The data file formats are given in Appendix B.

#4 function formats are defined as follows:

- #4,0,\;** file containing the catalogue,
- #4,0,?;** count of the files,
- #4,0,index,count;** part of the file containing the catalogue,

where:

index - first record,

count - number of records in the catalogue.

The catalogue of the files is a set of the records containing 16 words (16 bits each). Each record describes one file saved in the instrument's Flash-disk or RAM. The record structure is as follows:

- words 0 - 3 8 characters of the file name,
- word 4 type (binary number),
- word 5 reserved,
- word 6 least significant word of the file size,
- word 7 most significant word of the file size,
- words 8 - 15 reserved.

- #4,4;** current setup file,
- #4,4,?;** size of the current setup file,

#4,4,offset,length; part of current setup file,

where:

offset - offset from the beginning of the current setup file,

length - number of bytes to read,



Note: The "\" character is treated as the file name of the catalogue and must be sent to the instrument.

All data words are sent **<LSB>** (least significant byte) first.

When an error is detected in the file specification or data, the instrument responds with:

#4,?;



Note: Current setup file placed in RAM is serviced by this command in SV 971A only. For data files access see A.1 **Function #D – data files access**.

A.6. FUNCTION #5 – STATISTICAL ANALYSIS RESULTS READ-OUT

#5 function enables one to read out the statistical analysis results.

#5 function format is defined as follows:

#5,p;

where:

p - the number of the profile (1, 2 or 3)

The device responds, sending the current classes of the statistics in the following format:

**#5,p;<Status Byte> <LSB of the transmission counter> <MSB of the transmission counter>
<NofClasses><BottomClass><ClassWidth><Counter of the class> (...) <Counter of the class>**

Status Byte gives the information about the current state of the instrument.

D7	D6	D5	D4	D3	D2	D1	D0
----	----	----	----	----	----	----	----

where:

D7 = 0 means "overload does not happen",

= 1 means "overload appeared",

D5 = 0 instantaneous current result (RUN State),

= 1 final result (STOP State),

D6, D0 to D4 reserved bits.



Note: There is no any succeeding transmission in the case when the **Status Byte** is equal to zero.

The **transmission counter** is a two-byte word denoting the number of the remaining bytes to be transmitted. Its value is calculated from the formulae:

Transmission counter = 6+n * (4 * the number of the classes in the statistics)

where:

n is a number of the transmitted statistics. For p = 1, 2 or 3 only one statistic is transmitted (n = 1).

NofClasses is a two-byte word denoting the number of classes in the statistic.

BottomClass is a two-byte word denoting the lower limit of the first class (*10 dB).

ClassWidth is a two-byte word denoting the width of the class (*10 dB).

Counter of the class is a four-byte word containing the number of the measurements belonging to the current class.



Note: The bytes in the words are sent **<LSB>** (least significant byte) first.



Note: ASCII part of the response ends with semicolon “;”. Status byte, transmission counter and data bytes are coded in binary form.

A.7. FUNCTION #7 – SPECIAL CONTROL FUNCTIONS

#7 function enables the user to perform special control functions. **Some of them should be used with the extreme care.**

#7 function format is defined as follows.

To read settings a query should be send to the device:

#7,<code>;

where **<code>** is a two ASCII letter code.

The device responds with a control settings:

#7,<code>,set1[,set2[,set3[,...[,setN]]]];

where **<code>** is the same code sent in the query and **set1, set2,... setN** are settings.

To write settings to the device follow the opposite procedure. Send to the device:

#7,<code>,set1[,set2[,set3[,...[,setN]]]];

In the case of success the device responds with:

#7,<code>;

In the case of an unknown function or error the device returns:

#7,?;

Codes and settings for #7 function are described in the A.3 **Control setting codes**.



Note: #7 function protocol consist of ASCII characters only.



Note: Some of the #7 functions are blocked during measurements running state (#1,S1;). Stop the measurements (#1,S0;) before changing these settings.

A.8. FUNCTION #9 – SETUP FILE WRITE-IN

#9 function enables the user to write a configuration file into the instrument's storage or non-volatile memory. The data file formats are given in Appendix B.

#9 function formats are defined as follows:

#9,<FILE_TYPE>,<FILE_LENGTH>,<DATA>

where:

<FILE_TYPE>	type of the file
	2 - setup file (file is saved on SD card; does not change current setup),
	4 - current setup file,
<FILE_LENGTH>	length of the file in bytes,
<DATA>	binary content of the file.



Note: #9 function is blocked during measurements running state (#1,S1;). Stop the measurements (#1,S0;) before using the function.

A.1 FUNCTION #D – DATA FILES ACCESS

#D functions are used to access data files in the instrument's storage like microSD card or USB Flash Disc with FAT file system. A basic knowledge of FAT file system is necessary to use these functions.

#D functions take the following parameters:

<disk>	logical disk number: 0 – SD card, 1 – USB Disk (not implemented), 2 – Internal Memory (not implemented)
<address>	directory address (cluster number),
<offsetB>	offset of the first byte to read (an even number),
<nB>	number of bytes to read (an even number),
<data>	binary data,
<count>	directory size in bytes,
<name>	filename in the format XXXXXXXX.YYY (XXXXXXX – filename, YYY- filename extension),
<dirName>	directory name,
<nBwr>	number of bytes to write.

- 1) **#D,c,?;** this function returns a list of available disks in format:

#D,c,<disk1>[,<disk2>[,<disk3>]];

- 2) **#D,d,?;** this function returns parameters of the working directory in format:

#D,d,<disk>,<address>,<count>;

- 3) **#D,d,<disk>,<address>;** this function enables to change the working directory.

Response:

#D,d; - command was executed
#D,d,?; - command cannot be executed

- 4) **#D,r,<disk>,<address>,<offsetB>,<nB>;** the function enables to read a file from the working directory.

Response:

#D,r,<disk>,<address>,<offsetB>,<nB>;[<data>]

- 5) **#D,w,<name>,<nBwr>;<data>** the function enables to write a file to the working directory.

Response:

#D,w; - command was executed
#D,w,?; - command cannot be executed

- 6) **#D,e,<name>;** function enables to delete a file in working directory.

Response:

#D,e; - command was executed
#D,e,?; - command cannot be executed

- 7) **#D,e;** function enables to delete all files in the working directory.

Response:

#D,e; - command was executed
#D,e,?; - command cannot be executed

- 8) **#D,m,<address>,<dirName>;** function enables to create a subdirectory in the directory defined by <address>.

Response:

#D,m; - command was executed
#D,m,?; - command cannot be executed

- 9) **#D,f,<address>;** function enables to delete directory and its contents (files and subdirectories).

Response:

#D,f; - command was executed
#D,f,?; - command cannot be executed

- 10) **#D,s,?;** this function returns parameters of the setup directory in format:

#D,s,<disk>,<address>;

- 11) **#D,i,?;** this function returns parameters of the STIPA function directory in format:

#D,i,<disk>,<address>;



Note: Only read functions are available during measurements running state (#1,S1;). Stop the measurements (#1,S0;) to unlock all the functions.

A.2 FUNCTION #S – DIRECT SETUP ACCESS

#S function enables to read/write instrument's settings in a direct manner. Any settings changed by this command affect current setup, are written into non-volatile memory and are available on the next power up.

#S function format is defined as follows.

To read settings a query should be send to the device:

#S[,<code1>[,<code2>[,<code3>[,...]]]];

where <codeN> is a two to four ASCII letter setting code.

The device responds with the control settings:

#S[,<code1>:<set1>[,<code2>:<set2>[,<code3>:<set3>[,...]]]];

where <codeN> is the same settings code sent in the query and <setN> is a settings value.

To return all settings available send:

#S;

To write settings to the device follow the opposite procedure. Send to the device:

#S,<code1>:<set1>[,<code2>:<set2>[,<code3>:<set3>[,...]]];

In the case of success the device responds with the same ASCII string:

#S,<code1>:<set1>[,<code2>:<set2>[,<code3>:<set3>[,...]]];

In the case of an error (e.g. settings code does not exist or parameter value is out of range) the device respond with “?” instead of <setN> value:

#S,<codeN>:?;

For example if three parameters are set and <set2> is out of range the device response is:

#S,<code1>:<set1>,<code2>:?,<code3>:<set3>;

Codes and settings for #S function are described in the A.3 **Control setting codes**.



Note: #S function protocol consist of ASCII characters only.



Note: Some of the #S functions are blocked during measurements running state (#1,S1;). Stop the measurements (#1,S0;) before changing these settings.

A.3 CONTROL SETTING CODES

The control setting codes used in the SV 971A instrument are given in the below tables:

Table A.1 Unit information

Table A.2 Measurements settings and control

Table A.3 Calibration and microphone settings

Table A.4 Profile settings

Table A.5 Spectrum settings

Table A.6 Dosimeter settings

Table A.7 RT60 settings

Table A.8 STIPA settings

Table A.9 Statistical settings

Table A.7 Audio settings

Table A.8 Logger settings

Table A.9 CSV export settings

Table A.10 Programmable pauses (valid only in Dosimeter function)

Table A.11 Audio settings

Table A.12 Logger settings

Table A.13 Display and keyboard settings

Table A.14 Setup settings

Table A.15 Alarms settings (valid only in the Dosimeter function)

Table A.16 General settings

Table A.17 Power settings

Table A.18 Position and time settings

Table A.19 Report printing settings

Notes:

- function codes marked in green are **read only!**



- function codes marked in red are **locked during measurements run state!** Stop measurements before changing these settings.

- values in square brackets are **[optional]!**

- values are written in the form of numbers or in the form of a bit number (prefix 'b') or hexadecimal (prefix '0x') e.g. the b5 is equal to the number $32 = 2^5$ or hexadecimal 0x20.

Table A.1 Unit information

Group name	#1 code	#7 code	#S code	Code description
Unit type	U			971
Unit subtype		US		Returns unit subtype. 2 – SV 971A
Serial number	N			xxxxxx
Software version	W			a.bb.c – firmware version a.bb.0c – beta firmware version
			AA	abbc - firmware version in hex format
Files system version		FS		a.bb - file system version
PIC version		PI		x.xx - version of auxiliary microcontroller
Hardboot version		VH		x.xx - version of hardboot program
Bootstrap version		VB		x.xx - version of bootstrap program

Table A.2 Measurements settings and control

Group name	#1 code	#7 code	#S code	Code description
Measurement function	M		BB	1 - Level Meter 2 - 1/1 Octave 3 - 1/3 Octave 4 - Dosimeter 102 - 1/1 Octave & Dosimeter 103 - 1/3 Octave & Dosimeter 8 - RT60 19 - STIPA
Measurement Range	R		BC	1 - Low 2 - Normal
Measurement state	S			0 - Stop 1 - Start 2 - Pause 4 - Delay before START (read only)
Start delay	Y		BD	nn - nn delay given in seconds $\in (0 \div 59)$ and $(60 \div 3600)$ with step 60s
Start synchronization	y		BN	0 - switched off (OFF) -1 - synchronization to full second 1 - synchronization to 1 min. 15 - synchronization to 15 min. 30 - synchronization to 30 min. 60 - synchronization to 1 hour.
Integration period	D			0 - infinity (measurement finished by pressing the Stop or remotely - by sending S0 control code) nns - nn number in seconds nnm - nn number in minutes

Group name	#1 code	#7 code	#S code	Code description
				nnh - nn number in hours
			BE	0 - infinity (measurement finished by pressing the Stop or remotely - by sending S0 control code) 1 - 24 hours 2 - 8 hours 3 - 1 hour 4 - 15 minutes 5 - 5 minutes 6 - 1 minute x \in (7 ÷ 65) - (x-6) seconds x \in (66 ÷ 124)- (x-65) minutes x \in (125÷148)- (x-124) hours 149 - infinity
Repetition number	K		BF	Repetition number of the measurement cycles. 0 - infinity (measurement finished by pressing the Stop or remotely - by sending S0 control code) nnnn - nnnn number of repetitions \in (1 ÷ 1000)
Detector type in the LEQ function	L		BG	0 - Linear 1 - Exponential
Day time limits		DL	BH	0 - 6h-18h 1 - 7h-19h
Rolling time (1)			BU	nn- nn time in seconds \in (1 ÷ 60) nn- nn time in minutes multiplied by 60 \in (60 ÷ 3600)
Rolling time (2)			BW	nn- nn time in seconds \in (1 ÷ 60) nn- nn time in minutes multiplied by 60 \in (60 ÷ 3600)
Exposure Time	e		EA	x - time in minutes \in (1 ÷ 720)
Microphone compensation		MC	JD	0 - Off 1 - On
Free field compensation		FF	BT	Free Field compensation. 0 - Off 1 - Free Field 2 - Diffuse Field 3 - Outdoor Environmental 4 - Outdoor Airport
Windscreen compensation		WD	BP	0 - Off 1 - On
Measure trigger mode	m		FA	0 - Off 2 - Slope+ 3 - Slope- 4 - Level+ 5 - Level- 6 - Gradient+
Measure trigger level	I		FI	x - level [dB] \in (24 ÷ 136); default 100dB

Group name	#1 code	#7 code	#S code	Code description
Measure trigger gradient	O		FK	x - gradient [dB] $\in (1 \div 100)$; default 10dB/(trigger period)
Auto-Run		AS		#7,AS,<e>,<HH>,<MM>,<hh>,<mm>,<dW>,<mR>; where: <e> - On (e=1), Off (e=0), <HH> - hour of the measurement start, <MM> - minutes of the measurement start, <hh> - hour of the measurement stop, <mm> - minutes of the measurement stop, <dW> - day of week in which the measurement will be done defined as a sum of flags: b0 - Monday b1 - Tuesday b2 - Wednesday b3 - Thursday b4 - Friday b5 - Saturday b6 - Sunday <mR> - maximum number of the measurement days,
			MR	<e> - On (e=1), Off (e=0)
			MJ	<HH> - hour of the measurement start
			MK	<MM> - minutes of the measurement start
			ML	<hh> - hour of the measurement stop
			MM	<mm> - minutes of the measurement stop
			MN	<dW> - day of week
			MO	<mR> - maximum number of the measurement days

Table A.3 Calibration and microphone settings

Group name	#1 code	#7 code	#S code	Code description
Calibration factor	Q		AJ	nn.nn - calibration factor [dB] represented as real number $\in (-10.00 \div 10.00)$
Calibration history		CH		#7,CH; Get number of records calibration history. Response format: #7,CH,n; n – number of records calibration history, #7,CH,n; Get n record from calibration history. Response format: #7,CH,n,cT,hh,mm,ss,DD,MM,YYYY,cF,cL; n – record number in the history of calibration,

Group name	#1 code	#7 code	#S code	Code description
				cT – type of calibration: 0 - none, 1 - by measurement, 2 - by sensitivity, 3 - factory calibration, hh:mm:ss – time of calibration, DD/MM/YYYY – date of calibration, cF – calibration factor in dB. cL – calibration level in dB. Response #7,CH,-1; denotes incorrect data in the selected record
Last calibration type			AF	Previously performed calibration type 0 - none 1 - By Measurement (manual) 2 - Remote 3 - Factory Calibration 4 - Auto Calibration
Last calibration date and time		CT		Function returns calibration date and time in the format: #7,CT,DD-MM-YYYY, hh:mm:ss ; where hh:mm:ss denotes the time and DD/MM/YYYY gives the date
			AG	Last calibration date d - coded data $\in (0 \div 65535)$ Date decoding in C language: day = $(d \& 0x1F)$; month = $((d >> 5) \& 0x0F)$; year = $((d >> 9) \& 0x7F) + 2000$;
			AH	Last calibration time t - t coded time $\in (0 \div 65535)$ Time decoding in C language: sec = $(t \% 30)$; min = $((t / 30) \% 60)$; hour = $(t / 1800)$; <i>Note: time resolution is 2 seconds!</i>
Calibration level			AI	nnnn - calibration reference level [dB] multiplied by 100
Auto calibration settings		AC	JF	0 - Off 1 - On
Post calibration settings			JA	0 - Off 1 - Last file 2 - Files after last calibration
Preamplifier TEDs type		TT		Returns type of the preamplifier saved in TEDS memory. Where -1 - unknown, 18 - SV18
Preamplifier TEDs serial number		TS		Returns serial number of the preamplifier saved in TEDS memory in format.

Group name	#1 code	#7 code	#S code	Code description
				#7,TS,<sn>; Where <sn> - microphone serial number,
Load TEDs		LF		Load TEDS memory.

Table A.4 Profile settings

Group name	#1 code	#7 code	#S code	Code description
Filter type in profile n	F			Fk:n - k filter in profile n k: 1 - Z filter, 2 – A filter, 3 – C filter, 5 – B , 6 – LF filter n: 1, 2, 3 – profile number: 1, 2 or 3 for function other than Dosimeter n: 4, 5, 6 – profile number: 1, 2 or 3 for Dosimeter function.
			BIn	k - k filter in profile n+1, $n \in (0 \div 2)$ Valid for function other than Dosimeter.
			EGn	k - k filter in profile n+1, $n \in (0 \div 2)$ Valid for Dosimeter function.
Peak Filter type in profile n	J			Jk:n - k filter in profile n k: 1 - Z filter, 2 – A filter, 3 – C filter, 5 – B , 6 – LF filter n: 1, 2, 3 – profile number: 1, 2 or 3 for function other than Dosimeter n: 4, 5, 6 – profile number: 1, 2 or 3 for Dosimeter function.
			BJn	k - k filter in profile n+1, $n \in (0 \div 2)$ Valid for function other than Dosimeter.
			EHn	k - k filter in profile n+1, $n \in (0 \div 2)$ Valid for Dosimeter function.
Detector type in profile n	C			Ck:n - k detector in profile n k: 0 - Impulse , 1 – Fast , 2 – Slow n: 1, 2, 3 – profile number: 1, 2 or 3 for function other than Dosimeter n: 4, 5, 6 – profile number: 1, 2 or 3 for Dosimeter function.
			BKn	k - k filter in profile n+1, $n \in (0 \div 2)$ Valid for function other than Dosimeter.
			EIn	k - k filter in profile n+1, $n \in (0 \div 2)$ Valid for Dosimeter function.

Table A.5 Spectrum settings

Group name	#1 code	#7 code	#S code	Code description
Filter type in 1/x OCTAVE analysis	f		BL	1 - Z filter 2 - A filter 3 - C filter 5 - B filter
Detector type in 1/x OCTAVE analysis	XB		BS	0 - Linear 1 - Fast 2 - Slow

Table A.6 Dosimeter settings

Group name	#1 code	#7 code	#S code	Code description
Criterion Level	c			c1:p - 80 dB c2:p - 84 dB c3:p - 85 dB c4:p - 90 dB c5:p - 60 dB c6:p - 65 dB c7:p - 70 dB c8:p - 75 dB c9:p - 87 dB p: 1, 2, 3 - profile number
				criterion level in profile n+1, $n \in (0 \div 2)$ 0 - 80 dB 1 - 84 dB 2 - 85 dB 3 - 90 dB 4 - 60 dB 5 - 65 dB 6 - 70 dB 7 - 75 dB 8 - 87 dB
Threshold Level	h			h0:p - None h1:p - 70 dB h2:p - 75 dB h3:p - 80 dB h4:p - 85 dB h5:p - 90 dB h6:p - 60 dB h7:p - 65 dB p: 1, 2, 3 - profile number
				threshold level in profile n+1, $n \in (0 \div 2)$ 0 - None 1 - 70 dB 2 - 75 dB 3 - 80 dB 4 - 85 dB 5 - 90 dB 6 - 60 dB 7 - 65 dB
Exchange Rate	x			xk:n - k exchange rate in profile n, $k \in (2 \div 6)$ n: 1, 2, 3 – profile number

Group name	#1 code	#7 code	#S code	Code description
			EDn	k - k exchange rate in profile n+1, $n \in (0 \div 2)$, $k \in (2 \div 6)$
Threshold level for ULT calculation	XI			xk:n - k threshold level in profile n, $k \in (70 \div 140)$ dB n: 1, 2, 3 – profile number
			EE n	k - k threshold level in profile n+1, $n \in (0 \div 2)$, $k \in (70 \div 140)$ dB
Threshold level for PCT calculation	XC			xk:n - k threshold level in profile n, $k \in (70 \div 140)$ dB n: 1, 2, 3 – profile number
			EFn	k - k threshold level in profile n+1, $n \in (0 \div 2)$, $k \in (70 \div 140)$ dB

Table A.7 RT60 settings

Group name	#1 code	#7 code	#S code	Code description
RT60 Method			VA	1 - Decay 2 - Impulse
Octave			VG	1 - 1/1 octave 2 - 1/3 octave
Frequency Range in 1/1 mode			VH	1 - 63Hz÷4kHz 2 - 63Hz÷16kHz
Frequency Range in 1/3 mode			VI	1 - 50Hz÷5kHz 2 - 50Hz÷20kHz
Recording Time			VB	0 - Auto n - n = time in seconds $\in (1 \div 30)$
Time Step			VC	0 - 2ms 1 - 5ms 2 - 10ms 3 - 20ms 4 - 25ms 5 - 50ms
Averaging			VD	0 - Off 1 - On
Smoothing			VE	n - n = graph smoothing factor $\in (1 \div 15)$
Noise Margin			VF	n - n = Value in dB multiplied by 10 $\in (0 \div 200)$

Table A.8 STIPA settings

Group name	#1 code	#7 code	#S code	Code description
Project Name			QR	xxxxx - xxxxx up to 8 characters (permitted characters: 0-9, A-Z and ' _')
Area Name			QS	xxxxx - xxxxx up to 8 characters (permitted characters: 0-9, A-Z and ' _')
Source Name			QX	xxxxx - xxxxx up to 8 characters (permitted characters: 0-9, A-Z and ' _')
Source Level			QZ	x - source calibration level in dB multiple by 10 $\in (-300 \div 300)$
Averaging			QT	0 - Manual 1 - Auto
Standard			QU	0 - 60268x2 1 - 60268x3
Index			QV	0 - STI 1 - CIS
Ambient noise			QY	0 - Off 1 - On

Table A.9 Statistical settings

Group name	#1 code	#7 code	#S code	Code description
Statistical levels		SL		Reading (response from the instrument): #7,SL,<sl1>,<sl2>,<sl3>,<sl4>,<sl5>,<sl6>,<sl7>,<sl8>,<sl9>,<sl10>; Writing: #7,SL,<sl_index>,<sl_level>; This function sets statistical levels where <sl_index> is the statistical index $\in (1 \div 10)$, <sl_level> is the statistical level [%] $\in (1 \div 99)$
			RA	<sl1> - statistical level 1
			RB	<sl2> - statistical level 2
			RC	<sl3> - statistical level 3
			RD	<sl4> - statistical level 4
			RE	<sl5> - statistical level 5
			RF	<sl6> - statistical level 6
			RG	<sl7> - statistical level 7
			RH	<sl8> - statistical level 8
			RI	<sl9> - statistical level 9
			RJ	<sl10> - statistical level 10

Table A.10 Programmable pauses (valid only in Dosimeter function)

Group name	#1 code	#7 code	#S code	Code description
Pause 1			CA	0 - Off 1 - On
Pause 1 - start hour			CB	hour $\in (0 \div 23)$
Pause 1 - start minute			CC	minute $\in (0 \div 59)$
Pause 1 - stop hour			CD	hour $\in (0 \div 23)$
Pause 1 - stop minute			CE	minute $\in (0 \div 59)$
Pause 2			CF	0 - Off 1 - On
Pause 2 - start hour			CG	hour $\in (0 \div 23)$
Pause 2 - start minute			CH	minute $\in (0 \div 59)$
Pause 2 - stop hour			CI	hour $\in (0 \div 23)$
Pause 2 - stop minute			CJ	minute $\in (0 \div 59)$
Pause 3			CK	0 - Off 1 - On
Pause 3 - start hour			CL	hour $\in (0 \div 23)$
Pause 3 - start minute			CM	minute $\in (0 \div 59)$
Pause 3 - stop hour			CN	hour $\in (0 \div 23)$
Pause 3 - stop minute			CO	minute $\in (0 \div 59)$
Pause 4			CP	0 - Off 1 - On
Pause 4 - start hour			CR	hour $\in (0 \div 23)$
Pause 4 - start minute			CS	minute $\in (0 \div 59)$
Pause 4 - stop hour			CT	hour $\in (0 \div 23)$
Pause 4 - stop minute			CU	minute $\in (0 \div 59)$
Pause 5			CW	0 - Off 1 - On
Pause 5 - start hour			CV	hour $\in (0 \div 23)$
Pause 5 - start minute			CX	minute $\in (0 \div 59)$
Pause 5 - stop hour			CY	hour $\in (0 \div 23)$
Pause 5 - stop minute			CZ	minute $\in (0 \div 59)$

Table A.11 Audio settings

Group name	#1 code	#7 code	#S code	Code description
Wave file name			IB	xxxxxxx – up to 8 characters (permitted characters: 0:9, A:Z, and '_'). Default name "R1"
Last wave file name		LW		a name of a previous wave file
Wave recording mode			IA	0 - Off 1 - continuous 2 - slope+ 3 - Slope– 4 - level+ 5 - Level– 6 - gradient+ 7 - manual 8 - integration period
Format			IC	0 - PCM 1 - Extensible
Sampling			IE	0 - 48 kHz 1 - 24 kHz 2 - 12 kHz
Filter			ID	1 - Z filter 2 - A filter 3 - C filter 5 - B filter
Gain			IO	x - x gain [dB] used in 16 bit mode $\in (0 \div 40)$
Trigger level			II	x - x level [dB] $\in (24 \div 136)$; default 100dB
Trigger period			IJ	0 - logger step 5 - 0.5 ms 1000 - 100 ms 10000 - 1 s
Trigger gradient			IK	x - x gradient [dB] $\in (1 \div 100)$; default 10dB/(trigger period)
Pre trigger			IL	x - x pre trigger time [s] (default 1s) \in (0 \div 30) - for 12 kHz sampling (0 \div 15) - for 24 kHz sampling (0 \div 8) - for 48 kHz sampling
Recording time			IN	x - x recording time [s]; $\in (1 \div 59)$, (60 \div 3600) with 60s steps and (3600 \div 28800) with 3600s steps
Length Limit			IP	0 - file size limit 4GB x - file size limit in minutes; $\in (1 \div 480)$

Table A.12 Logger settings

Group name	#1 code	#7 code	#S code	Code description
Logger file name			DC	xxxxxxx – up to 8 characters (permitted characters: 0:9, A:Z, and '_'). Default name "L1"
Last logger file name		LB		a name of a previous logger file
Next logger file name		NB		a name of a next logger file

Group name	#1 code	#7 code	#S code	Code description
Logger step	d			nn - nn number of milliseconds \in (100,200,500) nns - nn number of seconds \in (1 ÷ 60) nnm - nn number of minutes \in (1 ÷ 60)
				nn - nn number of milliseconds \in (100,200,500), (1000 ÷ 60000) with 1000ms steps and (60000 ÷ 3600000) with 60000ms steps
Logger	T		DA	0 - Off 1 - On <i>Note: this setting must be on in order to create a logger data file!</i>
Logger results in profile n	B			Bx:n - x – sum of the following flags: b0 - logger with Lpeak values in profile n b1 - logger with Lmax values in profile n b2 - logger with Lmin values in profile n b3 - logger with Leq values in profile n b4 - logger with Lav values in profile n b5 - logger with LR1 values in profile n b6 - logger with LR2 values in profile n n – profile \in (1 ÷ 3)
			DDn	x - x logger results in profile n+1, n \in (0 ÷ 2)
Summary results	XXE		DG	0 - Off 1 - On <i>Note: this is a main switch for all summary results.</i>
1/x Octave analysis results	b		DE	x - x – sum of the following flags: b0 - logger with Lpeak spectrum b3 - logger with Leq spectrum
Logger File Splitting Mode	XA		DH	0 - switched off (OFF) -1 - file is created for each measurement cycle. 15 - file is created every 15 min, synchronized to RTC. 30 - file is created every 30 min, synchronized to RTC. 60 - file is created every 1 hour, synchronized to RTC. 1440 - file is created on the specified times, see next parameter <i>Note: for “-1” – integration period must be at least 60s</i>
Specified Time for Logger File Splitting	XD			XDx:n – x = -1 (switched off) x = 0 ÷ 1439 (time in minutes) n = 1 ÷ 6 (specified time number)

Group name	#1 code	#7 code	#S code	Code description
				<i>Note: valid only if Split Mode is equal to 1440</i>
			DI	Active split time number x - x – sum of the following flags b0 - split on time number 1 b1 - split on time number 2 b2 - split on time number 3 b3 - split on time number 4 b4 - split on time number 5 b5 - split on time number 6
			DJn	Split hour (0 ÷ 23) for time number n-1, n ∈ (0 ÷ 5)
			DKn	Split minute (0 ÷ 59) for time number n-1, n ∈ (0 ÷ 5)
User text			UB	text – up to 128 characters of user text added to each data file. Default text “ ”. Permitted characters: 0-9, a-z, A-Z, space and the following characters !"#%&'()*+-./:<=>?@[\\]^_`{ }~
Logger trigger mode	XT		GA	0 - Off 4 - level+ 5 - Level–
Logger trigger level	XL		GI	x - level [dB] ∈ (24 ÷ 136); default 100dB
Logger pre-trigger	XQ		GL	x - number of the records taken into account before the fulfilment of the triggering condition ∈ (0 ÷ 10); default 0
Logger post-trigger	Xq		GM	x - number of the records taken into account after the fulfilment of the triggering condition ∈ (0 ÷ 200); default 0

Table A.13 Display and keyboard settings

Group name	#1 code	#7 code	#S code	Code description
Key shift mode			NA	0 - 2nd function 1 - Direct
Make Key Lock			NB	0 - Off 1 - On
Fast Unlock			NC	0 - Off 1 - On
Unlock 1 st key			ND	1 - Esc 2 - Left 4 - Enter 8 - Right 16 - Down 32 - Up
Unlock 2 nd key			NE	1 - Esc 2 - Left 4 - Enter 8 - Right

Group name	#1 code	#7 code	#S code	Code description
				16 - Down 32 - Up
Unlock 3 rd key			NF	1 - Esc 2 - Left 4 - Enter 8 - Right 16 - Down 32 - Up
Unlock 4 th key			NG	1 - Esc 2 - Left 4 - Enter 8 - Right 16 - Down 32 - Up
Keyboard lock		KL		0 - Unlock 1 - Lock
Files lock		FL	XE	0 - Unlock 1 - Lock
Main View Mode			SG	0 - Normal 1 - Full 2 - Large
Spectrum View			SA	0 - Off 1 - On
Spectrum View Mode			SI	0 - Normal 1 - Full
3-profiles View			SB	0 - Off 1 - On
3-profiles View Mode			SH	0 - Normal 1 - Full
Statistics View			SC	0 - Off 1 - On
Statistics View Mode			SJ	0 - Normal 1 - Full
Time History View			SD	0 - Off 1 - On
Time History View Mode			SK	0 - Normal 1 - Full
Running SPL View			SE	0 - Off 1 - On
File Info View			SF	0 - Off 1 - On
Display Time result in the main and 3-profile views			OA	0 - Off 1 - On Valid for function other than Dosimeter.
Display Lpeak result in the main and 3-profile views			OB	0 - Off 1 - On Valid for function other than Dosimeter.
Display Lmax result in the main and 3-profile views			OC	0 - Off 1 - On Valid for function other than Dosimeter.

Group name	#1 code	#7 code	#S code	Code description
Display Lmin result in the main and 3-profile views			OD	0 - Off 1 - On Valid for function other than Dosimeter.
Display L result in the main and 3-profile views			OE	0 - Off 1 - On Valid for function other than Dosimeter.
Display Leq result in the main and 3-profile views			OF	0 - Off 1 - On Valid for function other than Dosimeter.
Display LE result in the main and 3-profile views			OG	0 - Off 1 - On Valid for function other than Dosimeter.
Display Lden result in the main and 3-profile views			OH	0 - Off 1 - On Valid for function other than Dosimeter.
Display LEPd result in the main and 3-profile views			OI	0 - Off 1 - On Valid for function other than Dosimeter.
Display Ltm3 result in the main and 3-profile views			OJ	0 - Off 1 - On Valid for function other than Dosimeter.
Display Ltm5 result in the main and 3-profile views			OK	0 - Off 1 - On Valid for function other than Dosimeter.
Display Ln result in the main and 3-profile views			OL	0 - Off 1 - On Valid for function other than Dosimeter.
Display LR1 result in the main and 3-profile views			OM	0 - Off 1 - On Valid for function other than Dosimeter.
Display LR2 result in the main and 3-profile views			ON	0 - Off 1 - On Valid for function other than Dosimeter.
Display EX result in the main and 3-profile views			OR	0 - Off 1 - On Valid for function other than Dosimeter.
Display SD result in the main and 3-profile views			OS	0 - Off 1 - On Valid for function other than Dosimeter.
Display OVL result in the main and 3-profile views			OO	0 - Off 1 - On Valid for function other than Dosimeter.
Display Time result in the main and 3-profile views			PA	0 - Off 1 - On Valid for Dosimeter function.
Display Lpeak result in the main and 3-profile views			PB	0 - Off 1 - On Valid for Dosimeter function.

Group name	#1 code	#7 code	#S code	Code description
Display Lmax result in the main and 3-profile views			PC	0 - Off 1 - On Valid for Dosimeter function.
Display Lmin result in the main and 3-profile views			PD	0 - Off 1 - On Valid for Dosimeter function.
Display L result in the main and 3-profile views			PE	0 - Off 1 - On Valid for Dosimeter function.
Display Dose result in the main and 3-profile views			PF	0 - Off 1 - On Valid for Dosimeter function.
Display D_8h result in the main and 3-profile views			PG	0 - Off 1 - On Valid for Dosimeter function.
Display PrDose result in the main and 3-profile views			PQ	0 - Off 1 - On Valid for Dosimeter function.
Display Lav result in the main and 3-profile views			PH	0 - Off 1 - On Valid for Dosimeter function.
Display Leq result in the main and 3-profile views			PI	0 - Off 1 - On Valid for Dosimeter function.
Display LE result in the main and 3-profile views			PJ	0 - Off 1 - On Valid for Dosimeter function.
Display SEL8 result in the main and 3-profile views			PK	0 - Off 1 - On Valid for Dosimeter function.
Display E result in the main and 3-profile views			PL	0 - Off 1 - On Valid for Dosimeter function.
Display E_8h result in the main and 3-profile views			PM	0 - Off 1 - On Valid for Dosimeter function.
Display LEPd result in the main and 3-profile views			PN	0 - Off 1 - On Valid for Dosimeter function.
Display PSEL result in the main and 3-profile views			PO	0 - Off 1 - On Valid for Dosimeter function.
Display Ltm3 result in the main and 3-profile views			PP	0 - Off 1 - On Valid for Dosimeter function.
Display Ltm5 result in the main and 3-profile views			PR	0 - Off 1 - On Valid for Dosimeter function.

Group name	#1 code	#7 code	#S code	Code description
Display Ln result in the main and 3-profile views			PS	0 - Off 1 - On Valid for Dosimeter function.
Display PTC result in the main and 3-profile views			PT	0 - Off 1 - On Valid for Dosimeter function.
Display PTP result in the main and 3-profile views			PU	0 - Off 1 - On Valid for Dosimeter function.
Display ULT result in the main and 3-profile views			PW	0 - Off 1 - On Valid for Dosimeter function.
Display TWA result in the main and 3-profile views			PV	0 - Off 1 - On Valid for Dosimeter function.
Display PrTWA result in the main and 3-profile views			PY	0 - Off 1 - On Valid for Dosimeter function.
Display Lc-a result in the main and 3-profile views			PZ	0 - Off 1 - On Valid for Dosimeter function.
Display EX result in the main and 3-profile views			OT	0 - Off 1 - On Valid for Dosimeter function.
Display SD result in the main and 3-profile views			OW	0 - Off 1 - On Valid for Dosimeter function.
Display OVL result in the main and 3-profile views			PX	0 - Off 1 - On Valid for Dosimeter function.
Graph Y axis for 1/x OCTAVE			SM	0 - 10dB 1 - 20dB 2 - 40dB 3 - 80dB (default) 4 - 120dB
Graph grid for 1/x OCTAVE			SN	0 - Off 1 - On (default)
Spectrum type for 1/x OCTAVE			SP	0 - Averaged 1 - Instantaneous 2 - Max 3 - Min 4 - Peak
Spectrum view Min. for 1/x OCTAVE			SR	0 - Off 1 - On
Spectrum view Max. for 1/x OCTAVE			SS	0 - Off 1 - On
Chart auto-scale			SO	0 - Off 1 - On (default)

Group name	#1 code	#7 code	#S code	Code description
Displayed result in the main and 3-profile views (function other than Dosimeter)			LDn	x - x result in profile n+1, $n \in (0 \div 2)$ 1 - Time 2 - Lpeak 3 - Lmax 4 - Lmin 5 - LF 6 - Leq 7 - LAE 8 - Lden 9 - LEPd 10 - Ltm3 11 - Ltm5 12 - Ln 13 - LR1 14 - LR2 15 - EX 16 - SD 17 - OVL
Displayed result in the main and 3-profile views (Dosimeter function)			LEn	x - x result in profile n+1, $n \in (0 \div 2)$ 1 - Time 2 - Lpeak 3 - Lmax 4 - Lmin 5 - LF 6 - Dose 7 - D_8h 8 - PrDOSE 9 - Lav 10 - Leq 11 - LE 12 - SEL8 13 - E 14 - E_8h 15 - LEPd 16 - PSEL 17 - Ltm3 18 - Ltm5 19 - Ln 20 - PTC 21 - PTP 22 - ULT 23 - TWA 24 - PrTWA 25 - Lc-a 26 - EX 27 - SD 28 - SD

Group name	#1 code	#7 code	#S code	Code description
Results displayed on the Time history view			STn	<p>x - x logger results in profile n+1, $n \in (0 \div 2)$</p> <p>x – sum of the following flags:</p> <p>b0 - logger with Lpeak values in profile n</p> <p>b1 - logger with Lmax values in profile n</p> <p>b2 - logger with Lmin values in profile n</p> <p>b3 - logger with Leq values in profile n</p> <p>b4 - logger with L values in profile n</p> <p>b5 - logger with LR1 values in profile n</p> <p>b6 - logger with LR2 values in profile n</p>
Display dim mode			SU	<p>0 - Off</p> <p>1 - Level 1</p> <p>2 - Level 2 (default)</p> <p>3 - Level 3</p> <p>4 - Screen Off</p>
Display dim timeout			SW	<p>0 - disabled, display stays on all the time</p> <p>nn - timeout [s] for display dim; nn delay given in seconds $\in (5 \div 59)$ with 1s step and $\in (60 \div 3600)$ with 60s step; default is 60s</p> <p><i>Note: it is not recommended to disable this feature!</i></p>
Display auto rotate			SV	<p>0 - Off</p> <p>1 - On</p>
Colour Scheme			SX	<p>0 - Colourful</p> <p>1 - Black/White</p>
Warning: Logger Off			TA	<p>0 - Off</p> <p>1 - On (default)</p>
Warning: Power Off			TB	<p>0 - Off</p> <p>1 - On (default)</p>
Warning: Preamplifier disconnected			TC	<p>0 - Off</p> <p>1 - On (default)</p>
Warning: Save changes			TD	<p>0 - Off</p> <p>1 - On (default)</p>

Table A.14 Setup settings

Group name	#1 code	#7 code	#S code	Code description
Load setup		LS		<p>name - a name of a setup file to be loaded (activated)</p> <p><i>Notes:</i></p> <ul style="list-style-type: none"> - name is given without "svt" extension - a setup file must be placed into the SETUP directory of the instrument's SD card prior using this command; see 0 or A.1 on file upload
Save setup		SS		<p>name - a current instrument setup will be saved as a "name.svt" file in the SETUP directory of the instrument's SD card; 8 characters is a maximum name length</p>

Group name	#1 code	#7 code	#S code	Code description
				<i>Notes:</i> - name is given without “svt” extension
Clear setup		CS		This command restores factory defaults of the instrument. To execute command send #7,CS[,<sel>]; where <sel> is settings selector: 0 - inquiry, clear and ask to save the calibration 1 - TEDS, clear and read TEDs 2 - Memory, 3 - Factory (set factory calibration)
Delete setup		DS		name - a name of a setup file to be deleted from the SETUP directory of the instrument's SD card <i>Notes:</i> - name is given without “svt” extension

Table A.15 Alarms settings (valid only in the Dosimeter function)

Group name	#1 code	#7 code	#S code	Code description
Alarm Dose threshold			WAn	threshold in dB for profile n+1, $n \in (0 \div 2)$
Alarm D_8h threshold			WDn	threshold in dB for profile n+1, $n \in (0 \div 2)$
Alarm PTC threshold			WBn	threshold for profile n+1, $n \in (0 \div 2)$
Alarm ULT threshold			WCn	threshold in seconds for profile n+1, $n \in (0 \div 2)$

Table A.16 General settings

Group name	#1 code	#7 code	#S code	Code description
Interface mode		IM	AE	0 - Start/Stop 1 - Simple (default) 2 - Advanced
Language		LA	JC	0 - English (default) 1 - German 2 - Spanish 3 - French 4 - Hungarian 5 - Italian 6 - Dutch 7 - Polish 8 - Portuguese 9 - Russian 10 - Turkish
Leq & Lav			JE	0 - Both 1 - Mutual exclusive
USB		UF	JG	0 - USB High Speed (480 MHz) 1 - USB Full Speed (12 MHz) (default)

Group name	#1 code	#7 code	#S code	Code description
Serial interface mode		BT	JN	0 - RS232 1 - Bluetooth
Bluetooth PIN		BP	JL	0 - PIN off PIN $\in (1 \div 9999)$
RS232 Baud Rate			JH	7 - 115200 6 - 57600 5 - 38400 4 - 19200 3 - 9600 2 - 4800 1 - 2400 0 - 1200
RS232 Time Out			JI	n - n = time in seconds $\in (1 \div 60)$
Unit Name		UN		Up to 12 characters (permitted characters: 0:9, a:z, A:Z, space, and '_').
Display Unit Name		DN		k - display unit name on the instruments screen for k seconds
Comment file name			UA	Qxxxxxxx – up to 7 characters (permitted characters: 0:9, A:Z, and '_'). Default name "@C1"
SD card: erase disk		ED		Erase all files from SD card.
SD card: version of Fat file system		FT		-1 - SD disk not ready 1 - FAT16 2 – FAT32
SD card: number of sectors		NS		n - number of sectors. <i>Sector is 512 bytes in size</i>
SD card: number of free sectors		NF		n - number of free sectors. <i>Sector is 512 bytes in size</i>
Measurement files number		BN		n - number of "*.svl" files in the instrument's working directory
Instrument temperature		TP		xx.x - temperature of the instrument [°C]
Microphone temperature		TM		xx.x - temperature of the microphone [°C]
Vibration threshold			JJ	x - vibration threshold in [g]
Instrument orientation		OR		Returns orientation of the device in the format: #7,OR,x<a.aa>,y<b.bb>,z<c.cc>; where a.aa - gravitational acceleration in [g] for axes x b.bb - gravitational acceleration in [g] for axes y c.cc - gravitational acceleration in [g] for axes z
SPL on stop		LL		Reading (response from the instrument): #7,LL,<L1>; where <L1> - L value from profile 1 in [dB] <i>Notes: function is not available during measurements.</i>
Station status		II		This function provides cumulative station status. Reading (response from the instrument): #7,II,[L1],Fx<flags>,B<bat>,D<disk>;

Group name	#1 code	#7 code	#S code	Code description
				<p>where</p> <p><L1> - L value from profile 1 in [dB] (on STOP only)</p> <p><flags> - station status flags defined in hexadecimal format as a sum of the following flags:</p> <p>b0 - measurements are running, b1 - pause is active, b2 - programed pause id active, b5 - USB power supply is present, <bat> - battery relative state of charge [%] <disk> - SD card occupation [%]</p>

Table A.17 Power settings

Group name	#1 code	#7 code	#S code	Code description
Battery type			JB	<p>0 - Alkaline 1 - Rechargeable</p>
Power status		BS		<p>To read settings send #7,BS;. Response: #7,BS,<bat>;</p> <p>where <bat>: 1 ÷ 100 – battery state in [%] -1 - external USB power supply</p>
Battery voltage		BV		volt - battery voltage [mV] multiplied by 10;
USB voltage		UV		volt - USB voltage [mV] multiplied by 10;
Power off		PO		Power off the instrument.
Reset		XR		Hardware reset of the instrument (power off and on).
Automatic power off			JK	<p>0 - disabled, display stays on all the time nn - timeout [s] for instrument power off; nn delay given in seconds ∈ (300 ÷ 3600) with 60s step and ∈ (3600 ÷ 14400) with 3600s step; default is 14400s</p> <p><i>Note: instrument automatically power off only if doesn't measurement!</i></p> <p><i>Automatic power off is blocked when instrument is powered from USB supply</i></p>

Table A.18 Position and time settings

Group name	#1 code	#7 code	#S code	Code description
Set GPS marker		MG		<p>#7,MG,p1,p2,p3,p4,p5,p6,p7,p8,p9,p10,p11,p12,p13,p14,p15,p16,p17,p18,p19,p20;</p> <p>All parameters are optional.</p> <p>where:</p> <p>p1 – signal quality, p1 = 0 - no signal, p1 = 1 - GPS fix, p2 – Seconds part of time, p3 – Minutes part of time, p4 – Hours part of time, p5 – Day, p6 – Month, p7 – Year, p8 – Degree part of latitude, p9 – Minutes part of latitude, p10 – Seconds part of latitude, p11 – Milliseconds part of latitude, p12 – Latitude direction: N, S, p13 – Degree part of longitude, p14 – Minutes part of longitude, p15 – Seconds part of longitude, p16 – Milliseconds part of longitude, p17 – Longitude direction: E, W, p18 – Altitude in meters, p19 – Decimal part of altitude, p20 – Speed * 100 (km/h),</p>
Real Time Clock (RTC)		RT		<p>Current instrument's date/time settings.</p> <p>Reading (response from the instrument): #7,RT,<hour>,<min>,<sec>,<day>,<month>,<year>;</p> <p>Writing: #7,RT,<hour>,<min>,<sec>,<day>,<month>,<year>;</p> <p>where</p> <p><hour> - hour ∈ (0 ÷ 23) <min> - min ∈ (0 ÷ 59) <sec> - sec ∈ (0 ÷ 59) <day> - day ∈ (1 ÷ 31) <month> - hour ∈ (1 ÷ 12) <year> - hour ∈ (2000 ÷ 2099)</p>

Table A.19 Report printing settings

Group name	#1 code	#7 code	#S code	Code description
Print data from profiles			QAn	k - k print in profile n+1, $n \in (0 \div 2)$, 0 - Off 1 - On
Print profile results			QB	0 - Off 1 - All results 2 - Selected results
Print statistics			QC	0 - Off 1 - All results 2 - Selected results
Print Aver spectrum			DD	0 - Off 1 - All results 2 - Selected results
Print Max spectrum			QE	0 - Off 1 - All results 2 - Selected results
Print Min spectrum			QF	0 - Off 1 - All results 2 - Selected results
Print Peak spectrum			QG	0 - Off 1 - All results 2 - Selected results
Printer chars per line			QH	$n \in (20 \div 500)$
Units			QJ	0 - Off 1 - Print
Print Lpeak profiles result			QK1	0 - Off 1 - On
Print Lmax profiles result			QK2	0 - Off 1 - On
Print Lmin profiles result			QK3	0 - Off 1 - On
Print L profiles result			QK4	0 - Off 1 - On
Print Dose profiles result			QK5	0 - Off 1 - On
Print D_h8 profiles result			QK6	0 - Off 1 - On
Print PrDose profiles result			QK7	0 - Off 1 - On
Print Lav profiles result			QK8	0 - Off 1 - On
Print Leq profiles result			QK9	0 - Off 1 - On
Print LE profiles result			QL1	0 - Off 1 - On
Print SEL8 profiles result			QL2	0 - Off 1 - On
Print E profiles result			QL3	0 - Off 1 - On

Group name	#1 code	#7 code	#S code	Code description
Print E_8h profiles result			QL4	0 - Off 1 - On
Print Lden profiles result			QL5	0 - Off 1 - On
Print LEPd profiles result			QL6	0 - Off 1 - On
Print PSEL profiles result			QL7	0 - Off 1 - On
Print Ltm3 profiles result			QL8	0 - Off 1 - On
Print Ltm5 profiles result			QL9	0 - Off 1 - On
Print PTC profiles result			QM1	0 - Off 1 - On
Print PTP profiles result			QM2	0 - Off 1 - On
Print ULT profiles result			QM3	0 - Off 1 - On
Print TWA profiles result			QM4	0 - Off 1 - On
Print PrTWA profiles result			QM5	0 - Off 1 - On
Print Lc-a profiles result			QM6	0 - Off 1 - On
Print LR1 profiles result			QM7	0 - Off 1 - On
Print LR2 profiles result			QM8	0 - Off 1 - On
Print OVL profiles result			QN1	0 - Off 1 - On
Print EX profiles result			QN2	0 - Off 1 - On
Print SD profiles result			QN3	0 - Off 1 - On
Print statistics			QOn	k - print statistic for statistical level n, 0 - Off 1 - On n $\in (0 \div 9)$,
Print 20Hz octave result			QP1	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 25Hz octave result			QP2	0 - Off 1 - On Valid for 1/3 Octave function.
Print 31.5Hz octave result			QP3	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 40Hz octave result			QP4	0 - Off 1 - On

Group name	#1 code	#7 code	#S code	Code description
				Valid for or 1/3 Octave function.
Print 50Hz octave result			QP5	0 - Off 1 - On Valid for 1/3 Octave function.
Print 63Hz octave result			QP6	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 80Hz octave result			QP7	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 100Hz octave result			QP8	0 - Off 1 - On Valid for 1/3 Octave function.
Print 125Hz octave result			QP9	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 160Hz octave result			QR1	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 200Hz octave result			QR2	0 - Off 1 - On Valid for 1/3 Octave function.
Print 250Hz octave result			QR3	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 315Hz octave result			QR4	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 400Hz octave result			QR5	0 - Off 1 - On Valid for 1/3 Octave function.
Print 500Hz octave result			QR6	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 630Hz octave result			QR7	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 800Hz octave result			QR8	0 - Off 1 - On Valid for 1/3 Octave function.
Print 1kHz octave result			QR9	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 1.25kHz octave result			QS1	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 1.6kHz octave result			QS2	0 - Off 1 - On

Group name	#1 code	#7 code	#S code	Code description
				Valid for 1/3 Octave function.
Print 2kHz octave result			QS3	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 2.5kHz octave result			QS4	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 3.15kHz octave result			QS5	0 - Off 1 - On Valid for 1/3 Octave function.
Print 4kHz octave result			QS6	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 5kHz octave result			QS7	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 6.3kHz octave result			QS8	0 - Off 1 - On Valid for 1/3 Octave function.
Print 8kHz octave result			QS9	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 10kHz octave result			QT1	0 - Off 1 - On Valid for or 1/3 Octave function.
Print 12.5kHz octave result			QT2	0 - Off 1 - On Valid for 1/3 Octave function.
Print 16kHz octave result			QT3	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print 20kHz octave result			QT4	0 - Off 1 - On Valid for or 1/3 Octave function.
Print total A result			QT5	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print total C result			QT6	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.
Print total Z result			QT7	0 - Off 1 - On Valid for 1/1 Octave or 1/3 Octave function.

APPENDIX B. DATA FILE STRUCTURES

B.1 GENERAL STRUCTURE OF THE SV 971A FILES

Each file containing data from the SV 971A instrument consists of several groups of words. In the case of SV 971A (the internal file system rev. **1.08**), there are two different types of files containing:

- the results stored in the file in the instrument's logger (cf. App. B.2);
- setup data (cf. App. B.3).

Each file has the following elements:

- SvanPC file header (cf. [Table B.1](#));
- file header (cf. [Table B.2](#));
- unit and internal software specification (cf. [Table B.3](#));
- calibration settings (cf. [Table B.4](#));
- user's text (a header) stored together with the measurement data (cf. [Table B.5](#));
- parameters and global settings, common for all profiles (cf. [Table B.6](#));
- parameters for measurement trigger (cf. [Table B.7](#));
- parameters for logger trigger (cf. [Table B.8](#));
- parameters for Wave-file recording (cf. [Table B.9](#));
- special settings for profiles (cf. [0](#));
- display settings of the main results (cf. [Table B.11](#));
- header of the statistical analysis (cf. [0](#));
- header of the file from the logger (cf. [Table B.13](#));
- contents of the file from the logger (cf. [Table B.14](#));
- parameters for RT60 analysis (cf. [Table B.23](#));
- parameters for STIPA analysis (cf. [Table B.27](#)).

Other elements of the file structure are not obligatory for each file type stated above. They depend on the file type (**SLM**, **Dosimeter**, file from the logger) and on the setting of the **FULL STAT**. These elements are as follows:

- Header of the Summary Results Record (saved in Summary Results Record) (cf. [Table B.15](#));
- main results (saved in Summary Results Record) (cf. [Table B.16](#), [Table B.17](#));
- statistical levels (saved in Summary Results Record) (cf. [Table B.18](#));
- 1/1 Octave analysis results (saved in Summary Results Record) (cf. [Table B.19](#));
- 1/3 Octave analysis results (saved in Summary Results Record) (cf. [Table B.20](#));
- results of the statistical analysis (saved in Summary Results Record) (cf. [Table B.21](#));
- settings of the instrument saved in the setup file (cf. [Table B.22](#));
- results of the RT60 analysis (cf. [Table B.24](#), [Table B.25](#));
- results of the STIPA analysis (cf. [Table B.28](#), [Table B.29](#));
- file-end-marker (cf. [Table B.30](#)).

Below, all file structure groups are described separately in Tab. B.1.1 – Tab. B.1.30. The format used in the columns, named **Comment** with the square parenthesis ([xx, yy]), means the contents of the word with; **xx** is the most significant byte (MSB) and **yy** the lowest significant byte (LSB) of the word. The format 0xnnnn means that the nnnn is four-digit number in hexadecimal form.

Table B.1 SvanPC file header

Word number	Name	Comment
0..2	“SvanPC”	reserved
3	26	reserved
4	32	reserved
5	73	reserved
6..15	reserved	reserved
...

Table B.2 File header

Word number	Name	Comment
0	0xnn01	[01, nn=header's length]
1..4	FileName	name of the file (8 characters)
5	reserved	reserved
6	CurrentDate	file creation date (cf. App. B.4)
7	CurrentTime	file creation time (cf. App. B.4)
8..13	reserved	reserved
...		...

Table B.3 Unit and software specification

Word number	Name	Comment
0	0xnn02	[02, nn=specification's length]
1	UnitNumberL	unit number (LSB word)
2	UnitType	type of the unit: 971 – SV 971A
3	SoftwareVersion	software version: 105
4	SoftwareIssueDate	software issue date
5	DeviceMode	mode of the instrument
6	UnitSubtype	subtype of the unit: 2 – SV 971A
7	FileSysVersion	file system version: 105
8	SoftwareBetaSubv	software beta subversion
9	SoftwareSubversion	software subversion: 01
10	UnitNumberH	unit number (MSB word)
11	PreNumberL	preamplifier number (LSB word)
12	PreNumberH	preamplifier number (MSB word)
...		...

Table B.4 Calibration settings

Word number	Name	Comment
0	0xnn47	[47, nn=header's length]
1	PreCalibrType	type of calibration performed prior to measurement: 0 - none 1 - By Measurement (manual) 2 - Remote 3 - Factory Calibration 4 - Auto Calibration
2	PreCalibrDate	date of calibration performed prior to measurement (cf. App. B.4)
3	PreCalibrTime	time of calibration performed prior to measurement (cf. App. B.4)
4	PreCalibrFactor	factor (*100 dB) of calibration performed prior to measurement
5	PreCalibrLevel	level (*100 dB) of calibration performed prior to measurement
6	PostCalibrType	type of calibration performed prior to measurement: 0 - none 1 - By Measurement (manual) 2 - Remote 3 - Factory Calibration 4 - Auto Calibration 0xFFFF - Calibration not performed
7	PostCalibrDate	date of calibration performed after the measurement (cf. App. B.4)
8	PostCalibrTime	time of calibration performed after the measurement (cf. App. B.4)
9	PostCalibrFactor	factor (*100 dB) of calibration performed after the measurement
10	PostCalibrLevel	level (*100 dB) of calibration performed after the measurement
...

Table B.5 USER's text

Word number	Name	Comment
0	0xnn03	[03, nn=specification's length]
1...	title text	user's text (two characters in a word) finished with one or two null bytes

Table B.6 Parameters and global settings

Word number	Name	Comment
0	0xnn04	[04, nn=block's length]
1	MeasureStartDate	measure start date (cf. App. B.4)
2	MeasureStartTime	measure start time (cf. App. B.4)
3	DeviceFunction	device function: 1 - Sound Level Meter , 2 - 1/1 Octave , 3 - 1/3 Octave , 4 - Dosimeter 102 - 1/1 Octave & Dosimeter ,

		103 - 1/3 Octave & Dosimeter , 8 - RT60 19 - STIPA
4	MeasureInput	measurement input type: 2 - Microphone
5	Range	measurement range: 1 - Low 2 - Normal
6	UnitFlags	calibration flags: b0 - if set to 1: calibration coefficient is used b3 - if set to 1: overload occurred b7,b6,b5: type of the result Lden 000 – Lden result is not available 001 – Ld result 010 – Le result 011 – Lde result 100 – Ln result 101 – Lnd result 110 – Len result 111 – Lden result B9 - if set to 1: preamplifier disconnected
7	RepCycle	repetition cycle: 0 - infinity nnnn - number of repetitions $\in (1 \div 1000)$
8	NofChannel	number of channels (1)
8	NofProf	number of profiles (3)
10	StartDelay	start delay time
11..12	IntTimeSec	integration time specified in seconds
13	InterfaceMode	user interface mode: 0 - Start/Stop , 1 - Simple , 2 - Advanced
14	LeqInt	detector's type in the Leq function: 0 - Linear , 1 - Exponential
15	SpectrumFilter	1/1 or 1/3 Octave analysis filter: 1 - Z , 2 - A , 3 - C 5 - B in other cases: Reserved
16	SpectrumBuff	1/1 or 1/3 Octave logger: sum of the following flags: 1 - logger with Lpeak values 8 - logger with Leq values in other cases: reserved
17	ExposureTime	exposure time: 1..720 (min)
18	Leq & Lav	method of viewing results Leq and Lav 0 - Both

		1 - Mutually exclusive (visibility depends of the EXCHANGE RATE parameter)
19	MicComp	compensating filter for microphones: 0 - switched off, 1 - switched on
20	SpectrumRMSDetector	spectrum RMS detector type: 0 - LINEAR , 1 - Fast , 2 - Slow
21	Reserved	reserved
22	CriterionLevel[0]	1 st profile criterion level (only Dosimeter): 60, 65, 70, 75, 80, 84, 85, 87, 90 (*10 dB)
23	ThresholdLevel[0]	1 st profile threshold level (only Dosimeter): 0, 60, 65, 70, 75, 80, 85, 90 (*10 dB)
24	ExchangeRate[0]	1 st profile exchange rate (only Dosimeter): 2, 3, 4, 5, 6
25	CriterionLevel[1]	2 nd profile criterion level (only Dosimeter): 60, 65, 70, 75, 80, 84, 85, 87, 90 (*10 dB)
26	ThresholdLevel[1]	2 nd profile threshold level (only Dosimeter): 0, 60, 65, 70, 75, 80, 85, 90 (*10 dB)
27	ExchangeRate[1]	2 nd profile exchange rate (only Dosimeter): 2, 3, 4, 5, 6
28	CriterionLevel[2]	3 rd profile criterion level (only Dosimeter): 60, 65, 70, 75, 80, 84, 85, 87, 90 (*10 dB)
29	ThresholdLevel[2]	3 rd profile threshold level (only Dosimeter): 0, 60, 65, 70, 75, 80, 85, 90 (*10 dB)
30	ExchangeRate[2]	3 rd profile exchange rate (only Dosimeter): 2, 3, 4, 5, 6
31	MainResBuff	Summary results. Contents defined as a sum of: 0 - none 1 - Main Results 2 - Spectrum 4 - Spectrum MAX 8 - Spectrum MIN 16 - Spectrum PEAK 32 - Statistical levels 64 - Statistical analysis in profiles 128 - Statistical analysis in 1/1 or 1/3 Octave mode
32	StartSync	synchronization the start of measurement with RTC 0 - switched off -1 - synchronization to 1 sec 1 - synchronization to 1 min 15 - synchronization to 15 min 30 - synchronization to 30 min 60 - synchronization to 1 hour .
33	reserved	reserved
34	Windscreen	Windscreen compensation: 0 - off. 1 - on.

35	FieldCompensation	Field Compensation: 0 – Off 1 – Free Field 2 – Diffuse Field 3 – Outdoor Environmental 4 – Outdoor Airport
36	UL Th. Level[0]	1 st profile threshold level for ULT calculation 70 ÷ 140 dB (*10)
37	UL Th. Level[1]	2 nd profile threshold level for ULT calculation 70 ÷ 140 dB (*10)
38	UL Th. Level[2]	3 rd profile threshold level for ULT calculation 70 ÷ 140 dB (*10)
39	PEAK Th. Level[0]	1 st profile threshold level for PTC calculation 70 ÷ 140 dB (*10)
40	PEAK Th. Level[1]	2 nd profile threshold level for PTC calculation 70 ÷ 140 dB (*10)
41	PEAK Th. Level[2]	3 rd profile threshold level for PTC calculation 70 ÷ 140 dB (*10)
42	SplitMode	logger files splitting mode: 0 - off. -1 - The file is created for each measurement cycle. 15 - The file is created every 15 min synchronized to RTC. 30 - The file is created every 30 min synchronized to RTC. 60 - The file is created every 1 hour synchronized to RTC. 1440 - The file is created on the specified times.
43	SplitTime[1]	logger files splitting time: -1 - off. 0:1439 - Time in minutes. Valid only if SplitMode is equal 1440.
44	SplitTime[2]	logger files splitting time: -1 - off. 0:1439 - Time in minutes. Valid only if SplitMode is equal 1440.
45	SplitTime[3]	logger files splitting time: -1 - off. 0:1439 - Time in minutes. Valid only if SplitMode is equal 1440.
46	SplitTime[4]	logger files splitting time: -1 - off. 0:1439 - Time in minutes. Valid only if SplitMode is equal 1440.
47	SplitTime[5]	logger files splitting time: -1 - off. 0:1439 - Time in minutes. Valid only if SplitMode is equal 1440.
48	SplitTime[6]	logger files splitting time: -1 - off. 0:1439 - Time in minutes. Valid only if SplitMode is equal 1440.
49	Pause[1]	programmable pause no. 1.
50	PauseBegin[1]	start time of the pause no. 1 in format 0xhhmm hh – hour mm – minute
51	PauseEnd[1]	end time of the pause no. 1 in format 0xhhmm: hh – hour mm – minute
52	Pause[2]	programmable pause no. 2.

53	PauseBegin[2]	start time of the pause no. 2 in format 0xhhmm hh – hour mm – minute
54	PauseEnd[2]	end time of the pause no. 2 in format 0xhhmm: hh – hour mm – minute
55	Pause[3]	programmable pause no. 3.
56	PauseBegin[3]	start time of the pause no. 3 in format 0xhhmm hh – hour mm – minute
57	PauseEnd[3]	end time of the pause no. 3 in format 0xhhmm: hh – hour mm – minute
58	Pause[4]	programmable pause no. 4.
59	PauseBegin[4]	start time of the pause no. 4 in format 0xhhmm hh – hour mm – minute
60	PauseEnd[4]	end time of the pause no. 4 in format 0xhhmm: hh – hour mm – minute
61	Pause[5]	programmable pause no. 5.
62	PauseBegin[5]	start time of the pause no. 5 in format 0xhhmm hh – hour mm – minute
63	PauseEnd[5]	end time of the pause no. 5 in format 0xhhmm: hh – hour mm – minute
64..65	MeasureStartTimeMS	measure start time in ms (cf. App. B.4)
66	RollLeq1	Rolling time (1) in seconds
67	RollLeq2	Rolling time (2) in seconds
...		

Table B.7 Measurement trigger parameters

Word number	Name	Comment
0	0xnn2B	[2B, nn=block's length]
1	TriggerMode	trigger mode: 0 - Off , 2 - measurement on trigger Slope+ 3 - measurement on trigger Slope- 4 - measurement on trigger Level+ 5 - measurement on trigger Level- 6 - measurement on trigger Gradient+
2	TriggerSource	source of the triggering signal: 0 - Leq(1) the Leq result from the first profile
3	TriggerLevel	level of triggering: 24 ÷ 136 dB (*10)
4	TriggerGrad	gradient of triggering: 1 dB/ms ÷ 100 dB/ms (*10)
5	TriggerPre	reserved
6	TriggerPost	reserved

7	TriggerSampling	reserved
8	TriggerRecTime	reserved
9	TriggerStep	trigger period given in 0.1 ms. If zero Step is equal to logger time-step (cf. Tab. B.1.15)
10	TriggerFilter	reserved
11	BitsPerSample	reserved
12	Range	reserved
13	Gain	reserved
14	LengthLimit	reserved
...		

Table B.8 Logger trigger parameters

Word number	Name	Comment
0	0xnn2C	[2C, nn=block's length]
1	TriggerMode	trigger mode: 0 - Off , 4 - measurement on trigger Level+ , 5 - measurement on trigger Level-
2	TriggerSource	source of the triggering signal: 0 - Leq(1) the Leq result from the first profile
3	TriggerLev	level of triggering: 24 ÷ 136 dB (*10)
4	TriggerGrad	reserved
5	TriggerPre	number of the records taken into account before the fulfilment of the triggering condition ∈(1 ÷ 10)
6	TriggerPost	number of the records taken into account after the fulfilment of the triggering condition ∈(1 ÷ 200)
7	TriggerSampling	reserved
8	TriggerRecTime	reserved
9	TriggerStep	trigger period given in 0.1 ms. If zero Step is equal to logger time-step (cf. Tab. B.1.15)
10	TriggerFilter	reserved
11	BitsPerSample	reserved
12	Range	reserved
13	Gain	reserved
14	LengthLimit	reserved
...		

Table B.9 Wave-file recording parameters

Word number	Name	Comment
0	0xnn2D	[2D, nn=block's length]
1	TriggerMode	trigger mode: 0 - Off , 1 - recording whole measurement 2 - recording on trigger Slope+ 3 - recording on trigger Slope- 4 - recording on trigger Level+ 5 - recording on trigger Level- 6 - recording on trigger Gradient+ 7 - recording on trigger Manual
2	TriggerSource	source of the triggering signal: 0 - Leq(1) the Leq result from the first profile
3	TriggerLevel	level of triggering: 24 ÷ 136 dB (*10)
4	TriggerGrad	gradient of triggering: 1 dB/ms ÷ 100 dB/ms (*10)
5	TriggerPre	pretrigger time given in 10ms
6	TriggerPost	reserved
7	TriggerSampling	sampling frequency given in 10Hz
8	TriggerRecTime	recording time of single data block: 0 - recording to the end of measurement 1..28800 (sec)
9	TriggerStep	trigger period given in 0.1 ms. If zero Step is equal to logger time-step (cf. Tab. B.1.15)
10	TriggerFilter	filter type: 1 - Z , 2 - A , 3 - C 5 - B
11	BitsPerSample	bits/sample: 16
12	Range	full scale signal range in 0.01dB
13	Gain	signal gain in dB
14	LengthLimit	wave file length limit in minutes
...		

Table B.10 Special settings for profiles

Word number	Name	Comment
0	0xnn05	[05, nn=block's length]
1	0x0307	[used_profile, profile's mask]
2	0xmm06	[06, mm=sub-block's length]

3	DetectorP[1]	detector type in the 1 st profile: 0 - Imp. , 1 - Fast , 2 - Slow
4	FilterP[1]	filter type in the 1 st profile: 1 - Z , 2 - A , 3 - C 5 - B 6 - LF
5	BufferP[1]	logger contents in the 1 st profile defined as a sum of: 0 - none, 1 - L_{xpeak}^1 2 - $L_{xy}max^2$ 4 - $L_{xy}min^2$ 8 - L_{xyeq}^{23} 16 - LAV 32 - LR1 64 - LR2
6	FilterPeakP[1]	filter type for Peak result calculation in the 1 st profile: 1 - Z , 2 - A , 3 - C 5 - B 6 - LF
7	reserved	reserved
8	0xmm06	[06, mm=sub-block's length]
9	DetectorP[2]	detector type in the 2 nd profile: 0 - Imp. , 1 - Fast , 2 - Slow
10	FilterP[2]	filter type in the 2 nd profile: 1 - Z , 2 - A , 3 - C 5 - B 6 - LF
11	BufferP[2]	logger contents in the 2 nd profile defined as a sum of: 0 - none, 1 - L_{xpeak}^1 2 - $L_{xy}max^2$ 4 - $L_{xy}min^2$ 8 - L_{xyeq}^{23} 16 - LAV 32 - LR1 64 - LR2

12	FilterPeakP[2]	filter type for Peak result calculation in the 2 nd profile: 1 - Z , 2 - A , 3 - C 5 - B 6 - LF
13	reserved	reserved
14	0xmm06	[06, mm=sub-block's length]
15	DetectorP[3]	detector type in the 3 rd profile: 0 - Imp. , 1 - Fast , 2 - Slow
16	FilterP[3]	filter type in the 3 rd profile: 1 - Z , 2 - A , 3 - C 5 - B 6 - LF
17	BufferP[3]	logger contents in the 3 rd profile defined as a sum of: 0 - none, 1 - L_{xpeak}^1 2 - $L_{xy}max^2$ 4 - $L_{xy}min^2$ 8 - L_{xyeq}^{23} 16 - LAV 32 - LR1 64 - LR2
18	FilterPeakP[3]	filter type for Peak result calculation in the 3 rd profile: 1 - Z , 2 - A , 3 - C 5 - B 6 - LF
19	reserved	reserved
...		
¹	x - depends of the filter type for Peak result calculation in selected profile: A, C, Z, B (cf. Tab. B.1.10)	
²	x - depends of the filter type in selected profile: A, C, Z, B, LF (cf. Tab. B.1.10) y - depends of the detector type in selected profile: I (imp.), F (fast), S (slow) (cf. Tab. B.1.10)	
³	y - only for exponential detector's type (cf. Tab. B.1.6)	

Table B.11 Display settings of the main results

Word number	Name	Comment
0	0xnn48	[48, nn=header's length]
1	TIME	0 – TIME result not displayed, 1 - TIME result displayed
2	Lpeak	0 – L_{xpeak}^1 result not displayed, 1 – L_{xpeak}^1 result displayed
3	Lmax	0 – $L_{xy}^{max^2}$ result not displayed, 1 – $L_{xy}^{max^2}$ result displayed
4	Lmin	0 – $L_{xy}^{min^2}$ result not displayed, 1 – $L_{xy}^{min^2}$ result displayed
5	L	0 – L_{xy}^2 result not displayed, 1 – L_{xy}^2 result displayed
6	DOSE	0 – DOSE result not displayed, 1 - DOSE result displayed
7	D_8h	0 – D_8h result not displayed, 1 - D_8h result displayed
8	LAV	0 – LAV result not displayed, 1 - LAV result displayed
9	Leq	0 – L_{xveq}^{23} result not displayed, 1 – L_{xveq}^{23} result displayed
10	LE	0 – $L_{xy}E^{23}$ result not displayed, 1 - $L_{xy}E^{23}$ result displayed
11	SEL8	0 – SEL8 result not displayed, 1 - SEL8 result displayed
12	E	0 – E result not displayed, 1 – E result displayed
13	E_8h	0 – E_8h result not displayed, E_8h 1 - result displayed
14	Lden	0 – Lden result not displayed, 1 - Lden result displayed
15	LEPd	0 – LEPd result not displayed, 1 - LEPd result displayed
16	PSEL	0 – PSEL result not displayed, 1 - PSEL result displayed
17	Ltm3	0 – Ltm3 result not displayed, 1 - Ltm3 result displayed
18	Ltm5	0 – Ltm5 result not displayed, 1 - Ltm5 result displayed
19	Ln	0 – Ln result not displayed, 1 - Ln result displayed
20	PTC	0 – PTC result not displayed, 1 - PTC result displayed
21	PTP	0 – PTP result not displayed, 1 - PTP result displayed
22	ULT	0 – ULT result not displayed, 1 - ULT result displayed
23	TWA	0 – TWA result not displayed, 1 - TWA result displayed
24	PrDOSE	0 – PrDOSE result not displayed, 1 - PrDOSE result displayed
25	PrTWA	0 – PrTWA result not displayed, 1 - PrTWA result displayed
26	LR1	0 – LR1 result not displayed, 1 - LR1 result displayed
27	LR2	0 – LR2 result not displayed, 1 – LR2 result displayed
28	LCA	0 – Lc-a result not displayed, 1 – Lc-a result displayed
29	OVL	0 – OVL result not displayed, 1 - OVL result displayed
30	LeqLF	0 – LeqLF result not displayed, 1 - LeqLF result displayed
...
¹	x - depends of the filter type for Peak result calculation in selected profile: A, C, Z, B (cf. Tab. B.1.10)	
²	x - depends of the filter type in selected profile: A, C, Z, B, LF (cf. Tab. B.1.10) y - depends of the detector type in selected profile: I (imp.), F (fast), S (slow) (cf. Tab. B.1.10)	
³	y - only for exponential detector's type (cf. Tab. B.1.6)	

Table B.12 Header of the statistical analysis

Word number	Name	Comment
0	0xnn09	[09, nn=block's length]
1	0x0307	[03=number of profiles, 07=active profiles mask]
2	0xmm0A	[0A, mm=sub-block's length]
3	NofClasses[1]	number of classes in the first profile (120)
4	BottomClass[1]	bottom class boundary (*10 dB) in the first profile
5	ClassWidth[1]	class width (*10 dB) in the first profile
6	0xmm0A	[0A, mm=sub-block's length]
7	NofClasses[2]	number of classes in the second profile (120)
8	BottomClass[2]	bottom class boundary (*10 dB) in the second profile
9	ClassWidth[2]	class width (*10 dB) in the second profile
10	0xmm0A	[0A, mm=sub-block's length]
11	NofClasses[3]	number of classes in the third profile (120)
12	BottomClass[3]	bottom class boundary (*10 dB) in the third profile
13	ClassWidth[3]	class width (*10 dB) in the third profile
...

Table B.13 Header of the file from the logger

Word number	Name	Comment
0	0xnn0F	[0F, nn=header's length]
1	BuffTSec	logger time step - full seconds part
2	BuffTMillicsec	logger time step - milliseconds part
3	LowestFreq	lowest 1/1 Octave or 1/3 Octave frequency (*100 Hz)
4	NOctTer	number of 1/1 Octave or 1/3 Octave results
5	NOctTerTot	number of TOTAL values
6..7	BuffLength	logger length (bytes)
8..9	RecsInBuff	number of records in the logger
10..11	RecsInObserv	number of records in the observation period equal to: number of records in the logger + number of records not saved
12..13	AudioRecords	number of audio records in the logger
...



Note: The current logger time step in seconds can be obtained from the formulae:

$$T = \text{BuffTSec} + \text{BuffTMillicsec} / 1000$$

Table B.14 Contents of the file from the logger

Word number	Name	Comment
0..(BuffLength/2-1)		result#1, result#2, ... result#(BuffLength/2-1)

Table B.15 Header of the Summary Results Record (saved in Summary Results Record)

Word number	Name	Comment
0	0xnn59	[59, nn=header's length]
1..2	RecNumber	Summary Results Record number: 1..
...

Table B.16 Main results in the SLM mode (saved in Summary Results Record)

Word number	Name	Comment
0	0xnn07	[07, nn=block's length]
1	0x0307	[used_profile, profile's mask]
2	0xmm08	[08, mm=sub-block's length]
3..4	MeasureTime	time of the measurement
5	Result[1][1]	L_{xpeak}^1 value in the 1 st profile (*100 dB)
6	Result[1][2]	$L_{xy}E^{23}$ value in the 1 st profile (*100 dB)
7	Result[1][3]	maximal value (L_{xymax}^2) in the 1 st profile (*100 dB)
8	Result[1][4]	minimal value (L_{xymin}^2) in the 1 st profile (*100 dB)
9	Result[1][5]	L_{xy}^2 value in the 1 st profile (*100 dB)
10	Result[1][6]	L_{xyeq}^{23} value in the 1 st profile (*100 dB)
11	Result[1][7]	Lden value in the 1 st profile (*100 dB)
12	Result[1][8]	Ltm3 value in the 1 st profile (*100 dB)
13	Result[1][9]	Ltm5 value in the 1 st profile (*100 dB)
14	Result[1][10]	LR1 value in the 1 st profile (*100 dB)
15	Result[1][11]	LR2 value in the 1 st profile (*100 dB)
16	UnderRes[1]	under-range value in the 1 st profile
17..18	ULTime[1]	reserved
19..20	PTC[1]	reserved
21	UnitFlags	flags word for measurement cycle (definition in table B.1.6)
22	EX[1]	EX (Expected Value) in the 1 st profile (*100 dB)
23	SD[1]	SD (Standard Deviation) in the 1 st profile (*100 dB)
24	0xmm08	[08, mm=sub-block's length]
25..26	OVL	overload time
27	Result[2][1]	L_{xpeak}^1 value in the 2 nd profile (*100 dB)

28	Result[2][2]	$L_{xy}E^{23}$ value in the 2 nd profile (*100 dB)
29	Result[2][3]	maximal value ($L_{xy}max^2$) in the 2 nd profile (*100 dB)
30	Result[2][4]	minimal value ($L_{xy}min^2$) in the 2 nd profile (*100 dB)
31	Result[2][5]	L_{xy}^2 value in the 2 nd profile (*100 dB)
32	Result[2][6]	L_{xyeq}^{23} value in the 2 nd profile (*100 dB)
33	Result[2][7]	Lden value in the 2 nd profile (*100 dB)
34	Result[2][8]	Ltm3 value in the 2 nd profile (*100 dB)
35	Result[2][9]	Ltm5 value in the 2 nd profile (*100 dB)
36	Result[2][10]	LR1 value in the 2 nd profile (*100 dB)
37	Result[2][11]	LR2 value in the 2 nd profile (*100 dB)
38	UnderRes[2]	under-range value in the 2 nd profile
39..40	ULTime[2]	reserved
41..42	PTC[2]	reserved
43	UnitFlags	flags word for measurement cycle (definition in table B.1.6)
44	EX[2]	EX (Expected Value) in the 2 nd profile (*100 dB)
45	SD[2]	SD (Standard Deviation) in the 2 nd profile (*100 dB)
46	0xmm08	[08, mm=sub-block's length]
47..48	Reserved	reserved
49	Result[3][1]	L_{xpeak}^1 value in the 3 rd profile (*100 dB)
50	Result[3][2]	$L_{xy}E^{23}$ value in the 3 rd profile (*100 dB)
51	Result[3][3]	maximal value ($L_{xy}max^2$) in the 3 rd profile (*100 dB)
52	Result[3][4]	minimal value ($L_{xy}min^2$) in the 3 rd profile (*100 dB)
53	Result[3][5]	L_{xy}^2 value in the 3 rd profile (*100 dB)
54	Result[3][6]	L_{xyeq}^{23} value in the 3 rd profile (*100 dB)
55	Result[3][7]	Lden value in the 3 rd profile (*100 dB)
56	Result[3][8]	Ltm3 value in the 3 rd profile (*100 dB)
57	Result[3][9]	Ltm5 value in the 3 rd profile (*100 dB)
58	Result[3][10]	LR1 value in the 2 nd profile (*100 dB)
59	Result[3][11]	LR2 value in the 2 nd profile (*100 dB)
60	UnderRes[3]	under-range value in the 3 rd profile
61..62	ULTime[3]	reserved
63..64	PTC[3]	reserved
65	UnitFlags	flags word for measurement cycle (definition in table B.1.6)
66	EX[3]	EX (Expected Value) in the 3 rd profile (*100 dB)
67	SD[3]	SD (Standard Deviation) in the 3 rd profile (*100 dB)
...

¹ x - depends of the filter type for Peak result calculation in selected profile: A, C, Z, B (cf. Tab. B.1.10)

²	x - depends of the filter type in selected profile: A, C, Z, B (cf. Tab. B.1.10)
	y - depends of the detector type in selected profile: I (imp.), F (fast), S (slow) (cf. Tab. B.1.10)
³	y - only for exponential detector's type (cf. Tab. B.1.6)

Table B.17 Main results in Dosimeter mode (saved in Summary Results Record)

Word number	Name	Comment
0	0xnn07	[07, nn=block's length]
1	0x0307	[used_profile, profile's mask]
2	0xmm08	[08, mm=sub-block's length]
3..4	MeasureTime	time of the measurement
5	Result[1][1]	L_{xpeak}^1 value in the 1 st profile (*100 dB)
6	Result[1][2]	$L_{xy}E^{23}$ value in the 1 st profile (*100 dB)
7	Result[1][3]	maximal value ($L_{xy}max^2$) in the 1 st profile (*100 dB)
8	Result[1][4]	minimal value ($L_{xy}min^2$) in the 1 st profile (*100 dB)
9	Result[1][5]	L_{xy}^2 value in the 1 st profile (*100 dB)
10	Result[1][6]	L_{xyeq}^{23} value in the 1 st profile (*100 dB)
11	Result[1][7]	Lc-a (LCeq-LAeq) value (*100 dB)
12	Result[1][8]	Ltm3 value in the 1 st profile (*100 dB)
13	Result[1][9]	Ltm5 value in the 1 st profile (*100 dB)
14	Result[1][10]	LAV value in the 1 st profile (*100 dB)
15	Result[1][11]	TLAV value in the 1 st profile (*100 dB)
16	UnderRes[1]	under-range value in the 1 st profile
17..18	ULTime[1]	ULT value in the 1 st profile (sec.)
19..20	PTC[1]	PTC value in the 1 st profile
21	UnitFlags	flags word for measurement cycle (definition in table B.1.6)
22	EX[1]	EX (Expected Value) in the 1 st profile (*100 dB)
23	SD[1]	SD (Standard Deviation) in the 1 st profile (*100 dB)
24	0xmm08	[08, mm=sub-block's length]
25..26	OVL	overload time
27	Result[2][1]	L_{xpeak}^1 value in the 2 nd profile (*100 dB)
28	Result[2][2]	$L_{xy}E^{23}$ value in the 2 nd profile (*100 dB)
29	Result[2][3]	maximal value ($L_{xy}max^2$) in the 2 nd profile (*100 dB)
30	Result[2][4]	minimal value ($L_{xy}min^2$) in the 2 nd profile (*100 dB)
31	Result[2][5]	L_{xy}^2 value in the 2 nd profile (*100 dB)
32	Result[2][6]	L_{xyeq}^{23} value in the 2 nd profile (*100 dB)
33	Result[2][7]	reserved

34	Result[2][8]	Ltm3 value in the 2 nd profile (*100 dB)
35	Result[2][9]	Ltm5 value in the 2 nd profile (*100 dB)
36	Result[2][10]	LAV value in the 2 nd profile (*100 dB)
37	Result[2][11]	TLAV value in the 2 nd profile (*100 dB)
38	UnderRes[2]	under-range value in the 2 nd profile
39..40	ULTime[2]	ULT value in the 2 nd profile (sec.)
41..42	PTC[2]	PTC value in the 2 nd profile
43	UnitFlags	flags word for measurement cycle (definition in table B.1.6)
44	EX[1]	EX (Expected Value) in the 1 st profile (*100 dB)
45	SD[1]	SD (Standard Deviation) in the 1 st profile (*100 dB)
46	0xmm08	[08, mm=sub-block's length]
47..48	Reserved	reserved
49	Result[3][1]	L_xpeak¹ value in the 3 rd profile (*100 dB)
50	Result[3][2]	L_{xy}E²³ value in the 3 rd profile (*100 dB)
51	Result[3][3]	maximal value (L_{xy}max²) in the 3 rd profile (*100 dB)
52	Result[3][4]	minimal value (L_{xy}min²) in the 3 rd profile (*100 dB)
53	Result[3][5]	L_{xy}² value in the 3 rd profile (*100 dB)
54	Result[3][6]	L_{xyeq}²³ value in the 3 rd profile (*100 dB)
55	Result[3][7]	reserved
56	Result[3][8]	Ltm3 value in the 3 rd profile (*100 dB)
57	Result[3][9]	Ltm5 value in the 3 rd profile (*100 dB)
58	Result[3][10]	LAV value in the 3 rd profile (*100 dB)
59	Result[3][11]	TLAV value in the 3 rd profile (*100 dB)
60	UnderRes[3]	under-range value in the 3 rd profile
61..62	ULTime[3]	ULT value in the 3 rd profile (sec.)
63..64	PTC[3]	PTC value in the 3 rd profile
65	UnitFlags	flags word for measurement cycle (definition in table B.1.6)
66	EX[1]	EX (Expected Value) in the 1 st profile (*100 dB)
67	SD[1]	SD (Standard Deviation) in the 1 st profile (*100 dB)
...
¹ x - depends of the filter type for Peak result calculation in selected profile: A, C, Z, B (cf. Tab. B.1.10) ² x - depends of the filter type in selected profile: A, C, Z, B, LF (cf. Tab. B.1.10) y - depends of the detector type in selected profile: I (imp.), F (fast), S (slow) (cf. Tab. B.1.10) ³ y - only for exponential detector's type (cf. Tab. B.1.6)		

Table B.18 Statistical levels (saved in Summary Results Record)

Word number	Name	Comment
0	0xnn17	[17, nn=block's length]
1	0xpprr	[pp=used_profile, rr=profile's mask]
2	N_stat_level	number of statistical levels = N
3+i*(pp+1)	nn[i]	number of the Ln statistics; i=0..N-1
3+i*(pp+1)+p	Lnn[i,p]	value of the Ln statistics for profile p (p=1..pp) (*100 dB)
...

Table B.19 1/1 Octave analysis results (saved in Summary Results Record)

Word number	Name	Comment
0	0xnn0E, 0xnn26, 0xnn27, 0xnn30	[block_id, nn=block_length] 0xnn0E - averaged spectrum results, 0xnn26 - min. spectrum results, 0xnn27 - max. spectrum results 0xnn30 - peak spectrum results
1	0x0101	[used_profile, profile's mask]
2	LowestFreq	lowest 1/1 Octave frequency (*100 Hz): 3150
3	NOct	number of 1/1 Octave values: 10
4	NOctTot	number of TOTAL values: 3
5÷20	Octave[i]	1/1 Octave[i] value (*100 dB); i=1÷NOct+NoctTot (1÷13)
...

Table B.20 1/3 Octave analysis results (saved in Summary Results Record)

Word number	Name	Comment
0	0xnn10, 0xnn28, 0xnn29, 0xnn32	[block_id, nn=block_length] 0xnn10 - averaged spectrum results, 0xnn28 - min. spectrum results, 0xnn29 - max. spectrum results 0xnn32 - peak spectrum results
1	0x0101	[used_profile, profile's mask]
2	LowestFreq	lowest 1/3 Octave frequency (*100 Hz): 2000
3	NTer	number of 1/3 Octave values: 31
4	NTerTot	number of TOTAL values: 3
5÷50	Tercje[i]	1/3 octave[i] value (*100 dB); i=1÷NTer+NTerTot (1÷34)
...

Table B.21 Results of the statistical analysis in profiles (saved in Summary Results Record)

Word number	Name	Comment
0	0x010B	[0B, prof_mask#1]
1	SubblockLength	2 * number of classes in the first profile + 2
2..3	Histogram[1][1]	first counter in the first profile
4..5	Histogram[1][2]	second counter in the first profile
.....
0	0x020B	[0B, prof_mask#2]
1	SubblockLength	2 * number of classes in the second profile + 2
2..3	Histogram[2][1]	first counter in the second profile
4..5	Histogram[2][2]	second counter in the second profile
.....
0	0x040B	[0B, prof_mask#3]
1	SubblockLength	2 * number of classes in the third profile + 2
2..3	Histogram[3][1]	first counter in the third profile
4..5	Histogram[3][2]	second counter in the third profile
.....

Table B.22 Setup file

Word number	Name	Comment
0	0x0020	[20, 00=block's length in the second word]
1	BlockLength	length of the block
2..BlockLength-1	SetupTextData	saved setup values

Table B.23 RT60 parameters

Word number	Name	Comment
0	0xnn1A	[1A, nn=block's length]
1	ResultsType	type of results in block 1B: 1 - results, 2 - averaged results
2	Method	calculation method: 1 - Decay , 2 - Impulse
3	Spectrum	type of spectrum: 1 - 1/1 Octave , 2 - 1/3 Octave
4	TimeStep	logger time step in milliseconds
5	MeasureTime	measure time in seconds

6		reserved
7	DispSmooth	smoothing parameter (0 means no smoothing)
8	NoiseMargin	noise margin level (*10 dB)
9	Reserved	reserved
10	AverNo	number of averaged results
...		

Table B.24 RT60 results

Word number	Name	Comment
0	0x001B	[1B, 00= block's length in the second word]
1	BlockLength	length of the block
2	LowestFreq	lowest 1/3 Octave frequency (*100 Hz)
3	NTer	Number of 1/3 Octave values
4	NTotal	Number of TOTAL values
5	N1_rt60_freq	first frequency
6	N2_rt60_freq	last frequency
7+i	calculated[i]	i=N1_rt60_freq+N2_rt60_freq; i=N_tercje+N_tercje+N_max_total-1
8+i	EDT[i]	i=N1_rt60_freq+N2_rt60_freq; i=N_tercje+N_tercje+N_max_total-1
9+i	RT20[i]	i=N1_rt60_freq+N2_rt60_freq; i=N_tercje+N_tercje+N_max_total-1
10+i	RT30[i]	i=N1_rt60_freq+N2_rt60_freq; i=N_tercje+N_tercje+N_max_total-1
11+i	RT_user[i]	i=N1_rt60_freq+N2_rt60_freq; i=N_tercje+N_tercje+N_max_total-1
12+i	Cor_EDT[i]	reserved
13+i	Cor_RT20[i]	reserved
14+i	Cor_RT30[i]	reserved
15+i	Cor_RT_user[i]	reserved
...		reserved

Table B.25 RT60 averaged results

Word number	Name	Comment
0	0x001C	[1C, 00= block's length in the second word]
1	BlockLength	length of the block
2	LowestFreq	lowest 1/3 Octave frequency (*100 Hz)

3	NTer	number of 1/3 Octave values
4	NTotal	number of TOTAL values
5	N1_rt60_freq	first frequency
6	N2_rt60_freq	last frequency
7+i	calculated[i]	$i = N1_rt60_freq \div N2_rt60_freq$; $i = N_tercje \div N_tercje + N_max_total - 1$
8+i	EDT[i]	$i = N1_rt60_freq \div N2_rt60_freq$; $i = N_tercje \div N_tercje + N_max_total - 1$
9+i	RT20[i]	$i = N1_rt60_freq \div N2_rt60_freq$; $i = N_tercje \div N_tercje + N_max_total - 1$
10+i	RT30[i]	$i = N1_rt60_freq \div N2_rt60_freq$; $i = N_tercje \div N_tercje + N_max_total - 1$
11+i	RT_user[i]	$i = N1_rt60_freq \div N2_rt60_freq$; $i = N_tercje \div N_tercje + N_max_total - 1$
12+i	N_EDT[i]	number of averaging for the EDT[i]
13+i	N_RT20[i]	number of averaging for the RT20[i]
14+i	N_RT30[i]	number of averaging for the RT30[i]
15+i	N_RT_user[i]	number of averaging for the RT_user[i]
...		reserved

Table B.26 RT60 T0 offset parameters

Word number	Name	Comment
0	0xnn71h	71h = block identifier 0nnh = block length in words
1	SystemBase	filter database (2 or 10)
2	OctaveDivider	octave division (type of filters): 1 – octave filters 3 – 1/3 octave filters
3	FirstFreqIndex	index of the first filter; the exact centre filter frequency in Hertz according to its index is given by the following formula: $f = 1000 \cdot G^{i/b}$ – for odd value b $f = 1000 \cdot G^{(2i+1)/(2b)}$ – for even value b where: $G = 2$ – for filter base 2 $G = 10^{0.3}$ – for filter base 10 i – filter index b – octave division
4	N	number of values
5	T0_Offset[1]	First offset value

...
5+N-1	T0_Offset[N]	Last offset value
...		reserved

Table B.27 STIPA parameters

Word number	Name	Comment
0	0x0063	[63, 00= block's length in the second word]
1	BlockLength	length of the block
2	Standard	standard: 0 – IEC 60268-16x2, 1 – IEC 60268-16x3
3	Averaging	averaging type: 0 – Manual, 1 – Auto
4	N	project name length
5..	ProjectName[N]	project name
5+N	M	area name length
6+N..	AreaName[M]	area name
6+N+M	PointId	point Id
7+N+M	K	source name length
8+N+M..	SourceName[K]	source name
8+N+M+K	CalibrLevel	Calibration factor level (*10 dB)
...		reserved

Table B.28 STIPA results

Word number	Name	Comment
0	0x0061	[61, 00= block's length in the second word]
1	BlockLength	length of the block
2	STI	STI result (*100)
3	LAeq	LAeq result (*100 dB)
4	LCeq	LCeq result (*100 dB)
5	N	STIPA analysis frequency count
6	LZeq[1]	LZeq result for the first frequency (*100 dB)
7	Err1[1]	error flag of m(f1) for the first frequency (0,1)
8	Mf1[1]	result of m(f1) for the first frequency (*100 dB)
9	Err2[1]	error flag of m(f2) for the first frequency (0,1)

10	Mf2[1]	result of m(f2) for the first frequency (*100 dB)
i*5+1	LZeq[i]	LZeq result for the next frequency (*100 dB)
i*5+2	Err1[i]	error flag of m(f1) for the next frequency (0,1)
i*5+3	Mf1[i]	result of m(f1) for the next frequency (*100 dB)
i*5+4	Err2[i]	error flag of m(f2) for the next frequency (0,1)
i*5+5	Mf2[i]	result of m(f2) for the next frequency (*100 dB)
N*5+6	Flags	bit 0 – underrange flag bit 1 – overload flag
N*5+7	STI-Measured	STI result not including Ambient Noise
...		reserved

Table B.29 STIPA noise results

Word number	Name	Comment
0	0x0062	[62, 00= block's length in the second word]
1	BlockLength	length of the block
2	N	STIPA analysis frequency count
3..	Distortion[N]	STIPA distortion table (*100 dB)
...		reserved

Table B.30 File-end-marker

Word number	Name	Comment
0	0xFFFF	file end marker

B.2 STRUCTURE OF THE FILE CONTAINING RESULTS FROM LOGGER'S FILE

SvanPC file header - cf. [Table B.1](#)

File header - cf. [Table B.2](#)

Unit and software specification - cf. [Table B.3](#)

Calibration settings - cf. [Table B.4](#)

User's text - cf. [Table B.5](#)

Parameters and global settings - cf. [Table B.6](#)

Measurement trigger settings - cf. [Table B.7](#)

Logger trigger settings - cf. [Table B.8](#)

Wave-file recording parameters - cf. [Table B.9](#)

Special settings for profiles - cf. [0](#)

Display settings of the main results - cf. [Table B.11](#)

Header of the statistical analysis - cf. [0](#)

Header of the file from the logger - cf. [Table B.13](#)

Contents of the file from the logger - cf. [Table B.14](#) and the description in Chapter B.2.1.

RT60 parameters – cf. [Table B.23](#)

STIPA parameters – cf. [Table B.27](#)

B.2.1. The contents of the files in the logger

The records with the results and the records with the state of the markers as well as the records with the breaks in the results registration are saved in the files in the logger. All results are written in dB*100.

B.2.1.1. Record with the results

The contents of the record with the results depends on the selected measurement function and the value set in the **Logger** position of the **Profile x** and **Spectrum** sub-lists. The following elements can be present (in the given sequence):

(1) flag record

< flags > :

b0: 1- the overload detected, 0 - the overload not detected

b1: 1- the excessive self-vibration detected, 0 - the excessive self-vibration overload not detected

(2) results of the measurement from the first profile if the corresponding **LOGGER** position was active (*paths: Measurement / Logging / Logger Res. / Prof. 1*); up to seven words are written (cf. [0](#)):

<result1> - L_{xpeak}^1 result, depending on the value of BufferP[1]

<result2> - $L_{xy\max}^2$ result, depending on the value of BufferP[1]

<result3> - $L_{xy\min}^2$ result, depending on the value of BufferP[1]

<result4> - L_{xyeq}^{23} result, depending on the value of BufferP[1]

<result5> - **LAV** result, depending on the value of BufferP[1]

<result6> - **LR1** result, depending on the value of BufferP[1]

<result7> - **LR2** result, depending on the value of BufferP[1]

(3) results of the measurement from the second profile if the corresponding **LOGGER** position was active (*paths: Measurement / Logging / Logger Res. / Prof. 2*); up to five words are written (cf. [0](#)):

<result1> - L_{xpeak}^1 result, depending on the value of BufferP[2]

<result2> - $L_{xy\max}^2$ result, depending on the value of BufferP[2]

<result3> - $L_{xy\min}^2$ result, depending on the value of BufferP[2]

<result4> - L_{xyeq}^{23} result, depending on the value of BufferP[2]

<result5> - **LAV** result, depending on the value of BufferP[2]

<result6> - **LR1** result, depending on the value of BufferP[2]

<result7> - **LR2** result, depending on the value of BufferP[2]

(4) results of the measurement from the third profile if the corresponding **LOGGER** position was active (*paths: Measurement / Logging / Logger Res. / Prof. 3*); up to five words are written (cf. [0](#)):

<result1> - L_{xpeak}^1 result, depending on the value of BufferP[3]

<result2> - $L_{xy\max}^2$ result, depending on the value of BufferP[3]

<result3> - $L_{xy\min}^2$ result, depending on the value of BufferP[3]

<result4> - L_{xyeq}^{23} result, depending on the value of BufferP[3]

<result5> - **LAV** result, depending on the value of BufferP[3]

<result6> - **LR1** result, depending on the value of BufferP[3]

<result7> - **LR2** result, depending on the value of BufferP[3]

- | | |
|---|--|
| 1 | x - depends of the filter type for Peak result calculation in selected profile: A, C, Z, B |
| 2 | x - depends of the filter type in selected profile: A, C, Z, B
y - depends of the detector type in selected profile: I (imp.), F (fast), S (slow) |
| 3 | y - only for exponential detector's type |

(5) results of **1/1 Octave** analysis or **1/3 Octave** analysis if **1/1 Octave** analysis or **1/3 Octave** analysis was selected as the measurement function and the **Logger** was active (*paths: Measurement / Logging / Logger Res. / Peak Sp. [N] and Leq Sp. [N]*); the sequence of words is written:

<Octave Peak[1]> <Octave Peak [2]> ... <Octave Peak [NOct+NOctTot]> <Octave Leq[1]> <Octave Leq[2]> ... <Octave Leq[NOct+NOctTot]>

where:

Octave Peak[i] - the result of **1/1 Octave** or **1/3 Octave** Peak analysis (*100 dB);
i = 1..NOct+NOctTot

Octave Leq[i] - the result of **1/1 Octave** or **1/3 Octave** Leq analysis (*100 dB);
i = 1..NOct+NOctTot

B.2.1.2. Record with the state of the markers

The record with the state of the markers consists of one word:

<0x8nnn>

in which 12 bits nnn denote the state of the markers:

b11 = state of #12 marker

b10 = state of #11 marker

...

b1 = state of #2 marker

b0 = state of #1 marker

B.2.1.3. Record with the breaks in the results registration

The record with the breaks in the results registration consists of four words:

<0xB0ii> <0xB1jj> <0xB2kk> <0xB3nn>

in which ii, jj, kk, nn bytes denote 4-bytes counter of left or skipped records: nnkkjjii (ii is the least significant byte, nn – the most significant byte).

B.2.1.4. Record with the breaks account PAUSE in the results registration

The record with the breaks in the results registration consists of four words:

<0xA0ii> <0xA1jj> <0xA2kk> <0xA3nn>

in which ii, jj, kk, nn bytes denote 4-bytes counter duration of PAUSE in milliseconds:

nnkkjjii (ii is the least significant byte, nn - the most significant byte).

B.2.1.5. Record with the wave file name

The record with the wave file name consists of six words:

<0xC2aa>

<0xccbb>

<0xeedd>

<0xggff>

<0xiihh>

<0xCAaa>

in which:

aa - size of records,

bb cc dd ee ff gg hh ii - 8-bytes name of wave file name

B.2.1.6. Record with Summary Results

The format of the data frame is as follows:

HS	L (optional)	D	L (optional)	HE
----	--------------	---	--------------	----

where:

HS starting header (1 word)

L length of the block (field is optional and occurs only when b7..b0 in header are set to zero)

D Summary Data:

- Main results (cf. [Table B.16](#), [Table B.17](#))
- Statistical levels (optional, cf. [Table B.18](#))
- 1/1 Octave analysis results (optional, cf. [Table B.19](#))
- 1/3 Octave analysis results (optional, cf. [Table B.20](#))
- The results of the statistical analysis in profiles (optional, cf. [Table B.21](#))

HE ending header (1 word), which differs from the HS only on b11 bit (thanks to it, it is possible to analyse the recorded file starting from its end)

The HEADER format is as follows:

b15	b14	b13	b12	b11	b10	b9	b8	b7	b6	b5	b4	b3	b2	b1	b0
-----	-----	-----	-----	-----	-----	----	----	----	----	----	----	----	----	----	----

where:

b15 - 1

b14 - 1

b13 - 0

b12 - 0,

b11 - header type:

0 - HS

1 - HE

b10 - 0

b9 - 1

b8 - 1

b15÷b8 – HS (0xC3), HE (0xCB)

b7÷b0 – length of the block (if zero length of the block is saved in additional word L)

B.2.1.8. Record with name of the comment file

The format of the data frame is as follows:

HS	D	HE
----	---	----

where:

HS starting header (1 word)

D The full name of the comment file (e.g. "REC62.WAV").

HE ending header (1 word), which differs from the HS only on b11 bit (thanks to it, it is possible to analyse the recorded file starting from its end)

The HEADER format is as follows:

b15	b14	b13	b12	b11	b10	b9	b8	b7	b6	b5	b4	b3	b2	b1	b0
-----	-----	-----	-----	-----	-----	----	----	----	----	----	----	----	----	----	----

where:

b15 - 1

b14 - 1

b13 - 0

b12 - 0,

b11 - header type:

0 - HS

1 - HE

b10 - 1

b9 - 0

b8 - 0

b15÷b8 – HS (0xC4), HE (0xCC)

b7÷b0 – length of the block

B.2.1.9. Record with GPS data

The value equal to -12288 (0xd000) denotes the undefined value.

Word number	Name
0	0xC703
1	Length
2	Quality
3	Time.Sec
4	Time.Min
5	Time.Hour
6	Date.Day
7	Date.Month
8	Date.Year
9	Latitude.Deg
10	Latitude.Min
11	Latitude.Sec
12	Latitude.MiliSec
13	Latitude.Dir
14	Longitude.Deg
15	Longitude.Min
16	Longitude.Sec
17	Longitude.MiliSec
18	Longitude.Dir
19	Altitude
20	Altitude.10
21	Speed
22	Length
23	0xCF03
...	...

B.3 STRUCTURE OF THE SETUP FILE

SvanPC file header - cf. [Table B.1](#)

File header - cf. [Table B.2](#)

Unit and software specification - cf. [Table B.3](#)

Setup data - cf. [Table B.22](#)

File-end-marker - cf. [Table B.30](#)

B.4 DATE AND TIME

Following function written in C explain how the date and time are coded:

```
void ExtractDateTime(int date, unsigned int time, int dt[])
{
    dt[0] = time % 30;                /* sec */
    dt[1] = (time/30) % 60;           /* min */
    dt[2] = time/1800;                /* hour */

    dt[3] = date & 0x001F;            /* day */
    dt[4] = (date>>5) & 0x000F;       /* month */
    dt[5] = ((date>>9) & 0x007F) + 2000; /* year */
}
```

APPENDIX C. TECHNICAL SPECIFICATIONS

C.1 SPECIFICATION OF SV 971A AS SOUND LEVEL METER (SLM)

C.1.1 Specification of SV 971A as SLM in the standard configuration

Statement of performance

SV 971A working as SLM with all listed below accessories meets requirements of IEC 61672-1:2013 for the Class 1 Group X instruments.

Configuration of the complete SLM in its normal mode of operation

SV 971A	sound level meter and analyser comprising:
SV 18A	microphone preamplifier
ACO 7152	prepolarised free-field microphone (1/2", typical sensitivity 32 mV/Pa, polarization 0 V)
Recommended calibrator:	
SV 36	Class 1 sound calibrator 94/114 dB @ 1000 Hz or equivalent (not included in the standard set)

Accessories included in the SV 971A instrument set

SC 158	USB-C cable
SA 22	windscreen

Accessories available

SV 36	Class 1 sound calibrator: 94/114 dB @ 1000 Hz
SP 75	RS232 interface option
SA 271A	outdoor microphone kit

Measured quantities

The measured quantities for SLM mode are: **LXpeak**, **LXYmax**, **LXYmin**, **LXY**, **LXeq**, **LXE**, **Lden**, **LEPd**, **Ltm3**, **Ltm5**, **Ln** (Leq statistics), **EX** (expected Leq value), **SD** (standard Leq deviation), **OVL** (overload time %), two rolling Leq (**LR1** and **LR2**). Definitions for above mentioned parameters are given in Appendix D.

Additional functions

- Overload indication
- Underrange indication
- Battery state indication

Normal operating mode

SV 971A in configuration with the **SV 18A** microphone preamplifier and **ACO 7152** microphone with following settings: **Normal** or **Low** measurement range (*path: <Menu> / Measurement / Range* – see Chapter 4.6), **Microphone compensation - On**, **Field Compensation - Free Field**, **Windscreen compensation - Off** (*path: <Menu> / Measurement / Compensation Filter* – see Chapter 4.7).

Conformance testing

This chapter contains the information needed to conduct conformance testing according to the specified standards.

Mounting for acoustical tests

The microphone must be mounted on the preamplifier.

Electrical substitute for the microphone

To obtain a BNC type electrical input, the microphone must be replaced by an microphone electrical equivalent impedance ST 03 with $18 \text{ pF} \pm 10\%$.



Note: For acoustic conformance tests with the installed SA 22 windscreen, the **Windscreen compensation must be On**.

Periodical test upper frequency

8 kHz

Linear operating ranges

Two measuring ranges are available: **Normal** and **Low**.

The starting point at which tests of level linearity shall begin is 94.0 dB for the frequencies specifies below. For the **Low** measurement range and A weighting linearity test at 31.5 Hz, the starting point is 79 dB.

Table C.1.1. Linear operating ranges for the **Normal** measurement range (for the sinusoidal signal and microphone sensitivity 32 mV/Pa)

[dB]	L _{AS/F}		L _{BS/F}		L _{CS/F}		L _{ZS/F}		L _{AeqT}		L _{BeqT}		L _{CeqT}		L _{AE} (t _{int} = 2 s)		L _{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31.5 Hz	27	97	27	120	27	134	34	137	27	97	27	120	27	134	30	100	53	137
500 Hz	27	133	27	136	27	137	34	137	27	133	27	136	27	137	30	136	53	140
1 kHz	27	137	27	137	27	137	34	137	27	137	27	137	27	137	30	140	53	140
4 kHz	27	138	27	136	27	136	34	137	27	138	27	136	27	136	30	141	53	139
8 kHz	27	136	27	134	27	134	34	137	27	136	27	134	27	134	30	139	53	137
12.5 kHz	27	132	27	131	27	131	34	137	27	132	27	131	27	131	30	135	53	134

Table C.1.2. Linear operating ranges for the **Low** measurement range (for the sinusoidal signal and microphone sensitivity 32 mV/Pa)

[dB]	$L_{AS/F}$		$L_{BS/F}$		$L_{CS/F}$		$L_{ZS/F}$		L_{AeqT}		L_{BeqT}		L_{CeqT}		L_{AE} ($t_{int} = 2\text{ s}$)		L_{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31.5 Hz	24	83	24	106	24	120	32	123	24	83	24	106	24	120	27	86	50	123
500 Hz	24	119	24	122	24	123	32	123	24	119	24	122	24	123	27	122	50	126
1 kHz	24	123	24	123	24	123	32	123	24	123	24	123	24	123	27	126	50	126
4 kHz	24	124	24	122	24	122	32	123	24	124	24	122	24	122	27	127	50	126
8 kHz	24	122	24	120	24	120	32	123	24	122	24	120	24	120	27	125	50	123
12.5 kHz	24	118	24	117	24	117	32	123	24	118	24	117	24	117	27	121	50	120



Note: For the signals with the crest factor $n > 1.41$ upper measuring range of the RMS (LEQ and SPL) is reduced. The valid upper limit can be calculated according to the below given formula: $A_n = 137 - 20 \log(n/\sqrt{2})$, where A is the upper limit for the sinusoidal signal

Example: For the crest factor $n = 10$ the upper limit is $A_{10} = 120\text{ dB}$

Measuring ranges

Reference measuring range of the acoustic pressure

Normal

Measuring frequency range of the acoustic pressure (-3 dB) 5 Hz ÷ 20 000 Hz.

Basic measurement error of the acoustic pressure < 0.7 dB (measured for the reference conditions, see below).

Weighting filters (see Chapter C.3)

Z meeting requirements of the IEC 61672-1:2013 standard for the Class 1 “Z” filter

A meeting requirements of the IEC 651 and IEC 61672-1:2013 standard for the Class 1 “A” filter

B meeting requirements of the IEC 651 and IEC 61672-1:2013 standard for the Class 1 “B” filter

C meeting requirements of the IEC 651 and IEC 61672-1:2013 standard for the Class 1 “C” filter


Table C.1.3. Self-generated noise for different weighting filters

Weighting filter Range	Electrical *)			Acoustical compensated		
	A	C	Z	A	C	Z
Low	< 12 dB	< 12 dB	< 20 dB	< 17 dB	< 17 dB	< 23 dB
Normal	< 16 dB	< 16 dB	< 23 dB	< 20 dB	< 20 dB	< 27 dB

*) measured with the **ST 03** microphone equivalent impedance 18 pF ± 10%

Special filters

- **Diffuse Field** compensation filter that improves the complete instrument frequency response in the diffuse acoustic field (see below)
- **Windscreen** compensation filter that improves the instrument frequency response in the free acoustic field when windscreen SA 22 is mounted on the microphone (see Chapter C.1.2)

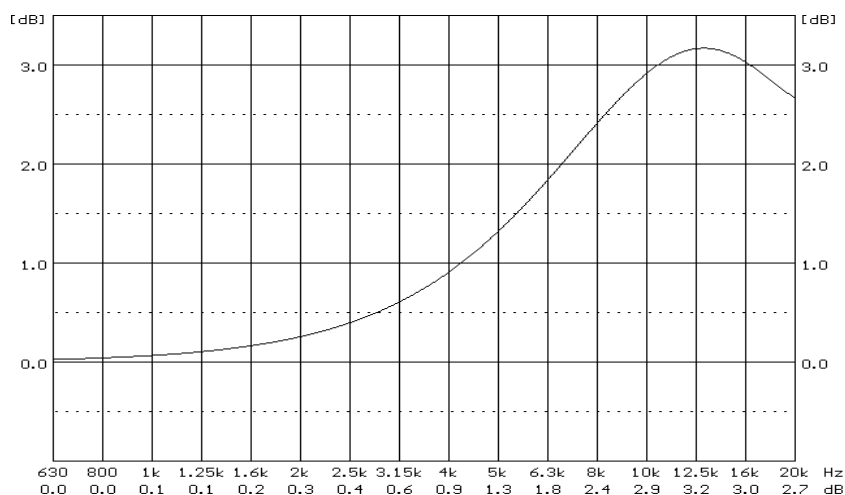

SV 971A Diffuse Field compensation filter



Note: Using special filters might change the frequency response and measuring ranges of SV 971A. Please check the below given specification.

Linear operating ranges for LEQ measurements with the Diffuse Field filter

The starting point at which tests of level linearity shall begin is 94.0 dB for the frequencies specifies below. For the **Low** measurement range and A weighting linearity test at 31.5 Hz, the starting point is 79 dB.

Table C.1.4. Linear operating ranges for the **Normal** measurement range for the **Diffuse Field** filter (for the sinusoidal signal and microphone sensitivity in the range 32 mV/Pa)

[dB]	$L_{AS/F}$		$L_{BS/F}$		$L_{CS/F}$		$L_{ZS/F}$		L_{AeqT}		L_{BeqT}		L_{CeqT}		L_{AE} ($t_{int} = 2\text{ s}$)		L_{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31.5 Hz	28	97	28	120	28	134	35	137	28	97	28	120	28	134	31	100	53	137
500 Hz	28	133	28	136	28	137	35	137	28	133	28	136	28	137	31	136	53	140
1 kHz	28	137	28	137	28	137	35	137	28	137	28	137	28	137	31	140	53	140
4 kHz	28	138	28	136	28	136	35	137	28	138	28	136	28	136	31	141	53	139
8 kHz	28	136	28	134	28	134	35	137	28	136	28	134	28	134	31	139	53	137
12.5 kHz	28	132	28	131	28	131	35	137	28	132	28	131	28	131	31	135	53	134

Table C.1.5. Linear operating ranges for the **Low** measurement range for the **Diffuse Field** filter (for the sinusoidal signal and microphone sensitivity in the range 32 mV/Pa)

[dB]	$L_{AS/F}$		$L_{BS/F}$		$L_{CS/F}$		$L_{ZS/F}$		L_{AeqT}		L_{BeqT}		L_{CeqT}		L_{AE} ($t_{int} = 2\text{ s}$)		L_{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31.5 Hz	25	83	25	106	25	120	33	123	25	83	25	106	25	120	28	86	50	123
500 Hz	25	119	25	122	25	123	33	123	25	119	25	122	25	123	28	122	50	126
1 kHz	25	123	25	123	25	123	33	123	25	123	25	123	25	123	28	126	50	126
4 kHz	25	124	25	122	25	122	33	123	25	124	25	122	25	122	28	127	50	126
8 kHz	25	122	25	120	25	120	33	123	25	122	25	120	25	120	28	125	50	123
12.5 kHz	25	118	25	117	25	117	33	123	25	118	25	117	25	117	28	121	50	120

RMS detector

- Digital "True RMS" with Peak detection,
- Resolution 0.1 dB
- Range 327.7 dB
- Crest Factor unlimited (for signals in 20 kHz band).

Overload detector

The instrument has the built-in overload detectors. Both A/D converter and input amplifier overload conditions are detected. The overload in the measurement channel (in its analogue part) and the overload of the analogue / digital converter are both detected. The "overload" indication appears when the input signal amplitude is 0.5 dB above the declared "Peak measurement range".

Underrange detector

The instrument has the built-in under-range detector. The "underrange" indication appears when the Leq value for the elapsed time or the last second L_{XY} value is below the lower linear operating range.

Time weighting characteristics (Exponential averaging)

- Slow** "S" according to IEC 61672 Class 1, Equivalent Time Constant 1000 ms
Fast "F" according to IEC 61672 Class 1, Equivalent Time Constant 125 ms
Impulse "I" according to IEC 60804 Class 1, Equivalent Time Constant 35 ms, Hold Time 1500 s

Reference conditions as per IEC 61672-1:2013

- Class of the acoustic field Free field
- Reference acoustic pressure 114.0 dB (related to 20 μ Pa)
- Reference frequency 1000 Hz
- Reference temperature +23°C
- Reference relative humidity 50 %
- Reference static pressure 1013.25 hPa
- Reference incidence direction perpendicular to the microphone diaphragm.

Maximum peak voltage 20 V Peak-Peak (Maximum peak voltage of input sinusoidal signal, which can be applied to the SLM without destruction the meter)

Warm-up time 1 min. (for 0.1 dB accuracy)

Typical stabilization time after change in environmental conditions by 20°C 1 hour

Nominal delay between operating of the **<Start>** (Reset) key and beginning of a new measurement ≥ 1 sec

Time shift after completion of a measurement, before a measurement is shown ≤ 1 sec



Note: When the instrument is moved from a warm environment with high humidity, to a colder environment, care should be taken not to produce condensation inside the instruments. In this case, much longer stabilization periods may be necessary.

Environmental, electrostatic and radio frequency criteria

Effect of humidity < 0.5 dB (for 30%<RH<90% at 40°C and 1000 Hz)

Effect of magnetic field below electrical noise level (for 80 A/m and 50 Hz)

Effect of radio frequency fields meets requirements of IEC 61672-1:2013

The greatest susceptibility (the least immunity) is achieved when the SLM is placed parallel to the radio frequency field and **Z** filter and time weighting **F** are selected and the SPL measurements are considered.

The instrument produces greatest radio-frequency emission when an extension cable is connected. The cable placed as a solenoid may produce unexpected emission depending on its physical dimensions. Any configuration w/o extension cable reduces emission below 30 dBuV/m.

Effect of electrostatic discharge meets requirements of IEC 61672-1:2013

During electrostatic discharge, the influence of the displayed results could be observed. No changes in instrument operation state, configuration or stored data corruption were found out.

Effect of ambient pressure < 0.01 dB/kPa

Effect of temperature < 0.5 dB (from -10°C to + 50°C)

Operating temperature from -10°C to + 50°C

Storage temperature from -20°C to + 60°C

Calibration

Acoustical - with the SV 36 sound calibrator (or equivalent):

- Calibration level for the pressure field 114.0 dB (equal to the calibrator pressure Level – see calibration chart of the used calibrator)
- Calibration level for the free field and 0 deg incidence angle 113.9 dB (equal to the calibration level for the pressure field minus free field correction of ACO 7152 at 1000 Hz – see [Table C.1.6](#))



Note: The above levels correspond to 114 dB of calibrator's sound pressure. If the calibrator has a sound pressure other than 114 dB, the calibration levels must be accordingly adjusted.

Microphone

ACO 7152 1/2" prepolarised free-field microphone
 Typical sensitivity 32 mV/Pa (corresponding to -30 dBV/Pa re 1 V/Pa)
 Capacitance 18 pF
 Reference point geometric centre of the microphone diaphragm



Note: Maximum level of sound pressure level, which can be affect the microphone without destruction the microphone: 155 dB.

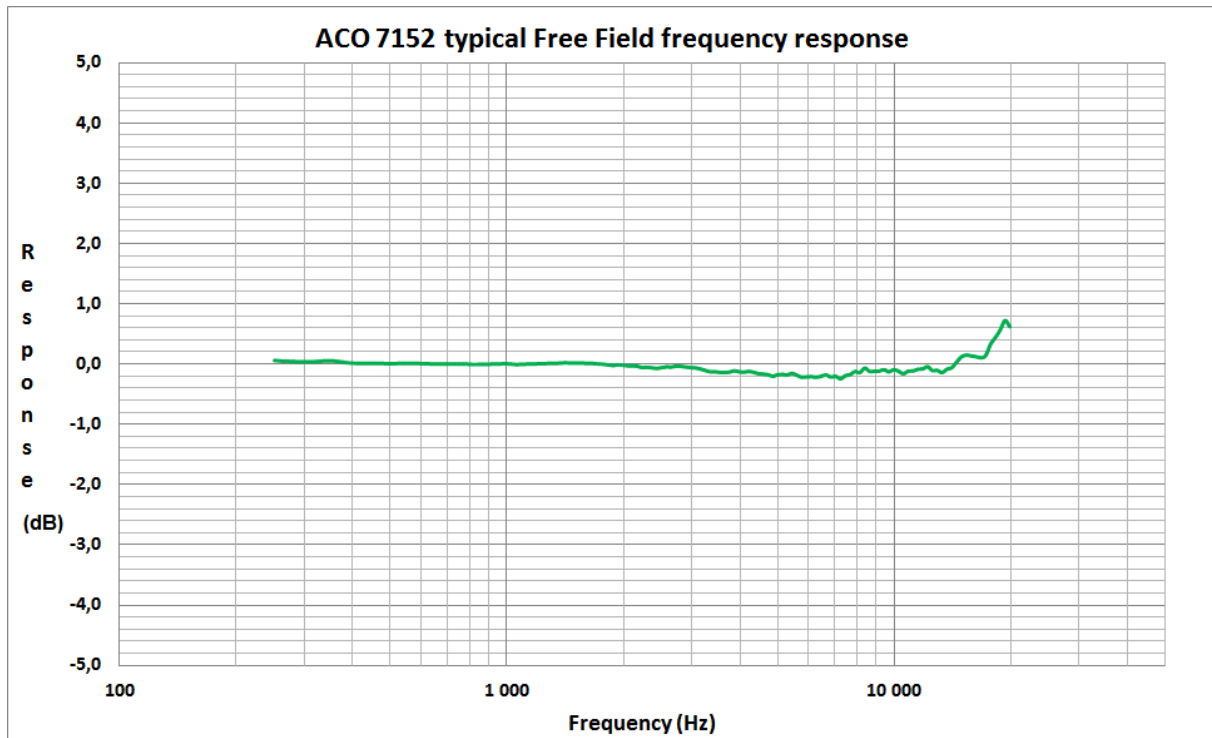


Table C.1.6. ACO 7152 Free Field correction for the electrostatic actuator and 0 deg incidence angle



[dB]	Frequency [Hz]																
	20	25	31.5	40	50	63	80	100	125	160	200	250	315	400	500	630	800
Correction factors	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.06	0.05	0.04	0.04	0.05	0.06
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25
[dB]	Frequency [Hz]																
	1000	1250	1600	2000	2500	3150	4000	5000	6300	8000	10000	12500	16000	20000			
Correction factors	0.10	0.15	0.21	0.27	0.40	0.59	0.86	1.27	1.86	2.83	4.11	5.77	8.31	11.58			
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.35	0.35	0.35	0.35	0.50	0.50	0.50			

Preamplifier

SV 18A

nominal preamplifier attenuation: 1.0 dB;

Power supply 2.5 mA@ 11 V \pm 7.5V

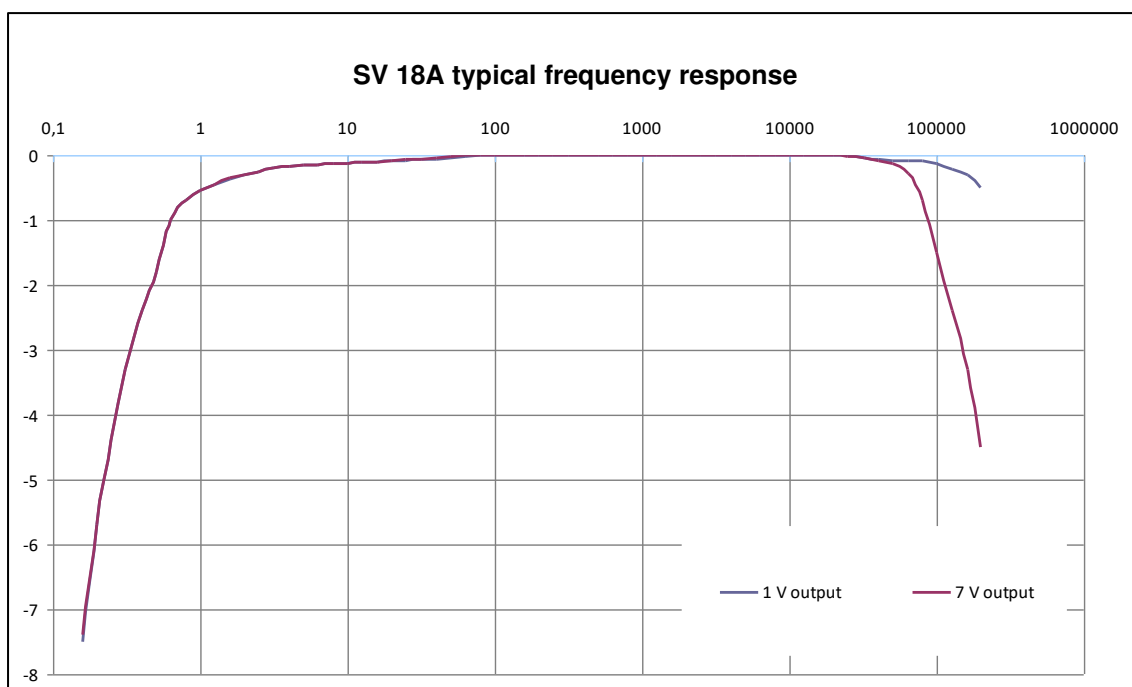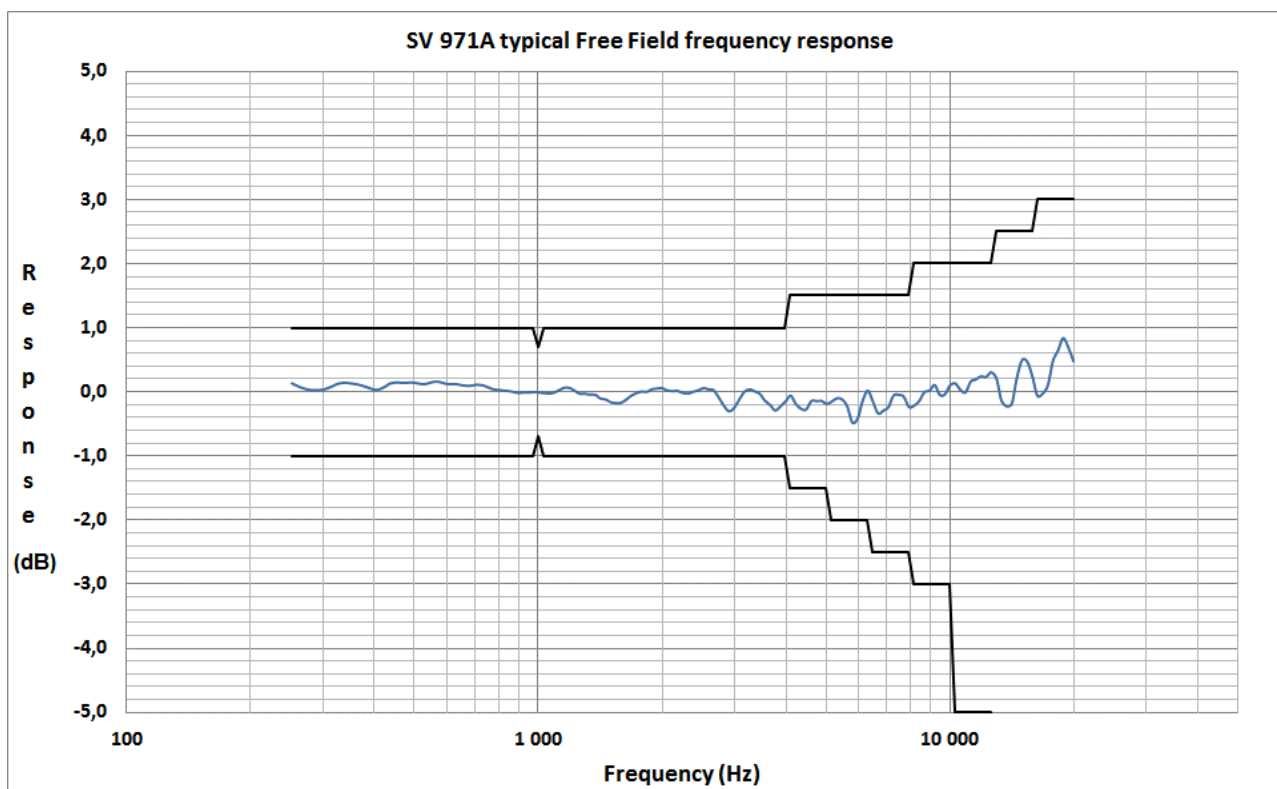**SV 971A frequency characteristics for 0 deg incidence angle**

Effect of reflections and diffraction of the acoustic plane wave from the case of SV 971A ("Case Effect")

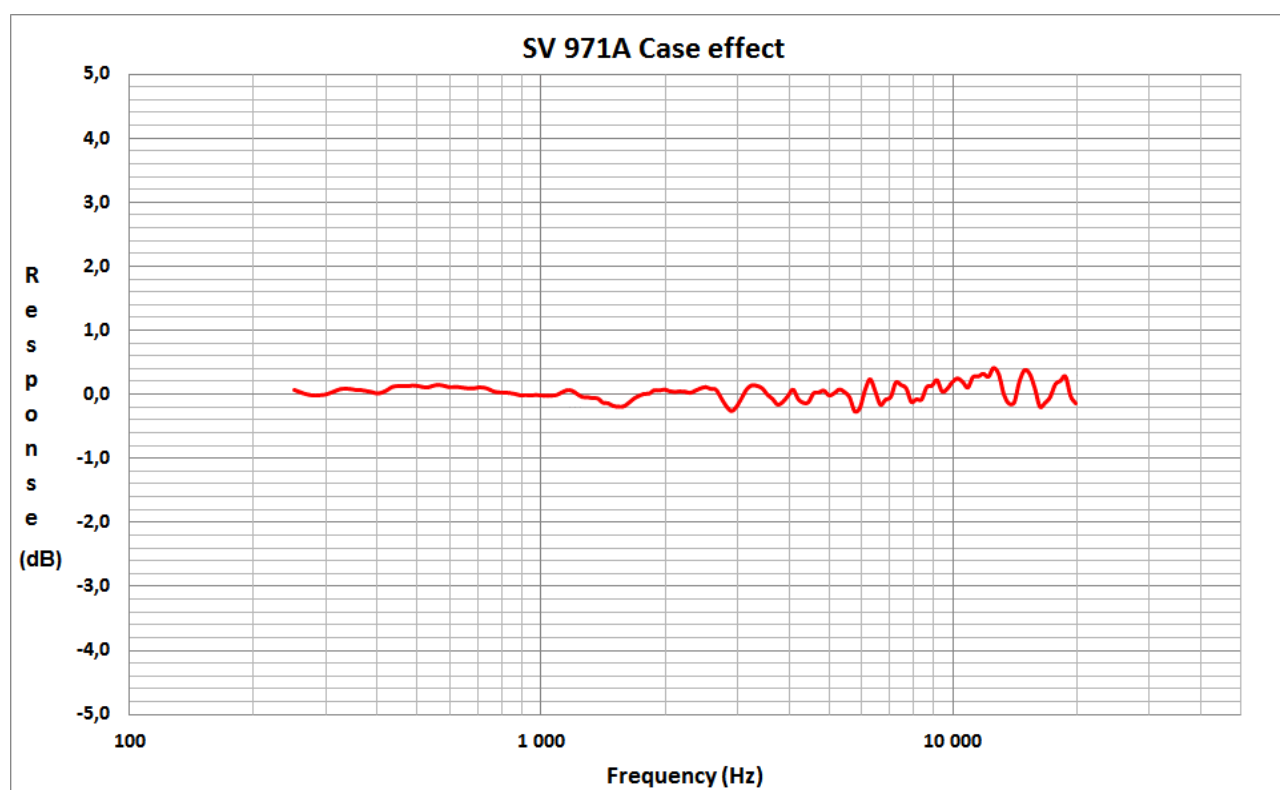


Table C.1.7. ACO 7152 and SV 971A typical frequency characteristics

Frequency [Hz]	ACO 7152 typical Free Field response [dB]	SV 971A typical Free Field response [dB]	SV 971A Case Effect [dB]	Uncertainty (IEC 62585:2012) [dB]
251	0.06	0.13	0.07	0.25
259	0.05	0.09	0.04	0.25
266	0.05	0.06	0.01	0.25
274	0.04	0.04	0.00	0.25
282	0.04	0.03	-0.01	0.25
290	0.04	0.03	-0.01	0.25
299	0.03	0.04	0.00	0.25
307	0.03	0.06	0.03	0.25
316	0.04	0.10	0.06	0.25
325	0.04	0.13	0.09	0.25
335	0.05	0.14	0.09	0.25
345	0.05	0.14	0.09	0.25
355	0.05	0.13	0.07	0.25
365	0.04	0.11	0.07	0.25
376	0.03	0.09	0.06	0.25
387	0.02	0.06	0.04	0.25
398	0.02	0.04	0.02	0.25
410	0.01	0.04	0.03	0.25
422	0.01	0.08	0.07	0.25
434	0.01	0.13	0.12	0.25
447	0.01	0.15	0.13	0.25
460	0.01	0.14	0.13	0.25
473	0.01	0.14	0.13	0.25

Frequency [Hz]	ACO 7152 typical Free Field response [dB]	SV 971A typical Free Field response [dB]	SV 971A Case Effect [dB]	Uncertainty (IEC 62585:2012) [dB]
487	0.01	0.15	0.14	0.25
501	0.00	0.14	0.14	0.25
516	0.01	0.12	0.12	0.25
531	0.01	0.12	0.11	0.25
546	0.01	0.15	0.14	0.25
562	0.01	0.16	0.15	0.25
579	0.01	0.15	0.14	0.25
596	0.01	0.13	0.12	0.25
613	0.00	0.12	0.12	0.25
631	0.00	0.12	0.12	0.25
649	0.00	0.11	0.11	0.25
668	0.00	0.09	0.10	0.25
688	0.00	0.10	0.10	0.25
708	0.00	0.11	0.11	0.25
729	0.00	0.11	0.11	0.25
750	0.00	0.08	0.08	0.25
772	0.00	0.04	0.04	0.25
794	0.00	0.03	0.04	0.25
818	-0.01	0.02	0.03	0.25
841	-0.01	0.02	0.02	0.25
866	-0.01	0.00	0.01	0.25
891	-0.01	-0.01	-0.01	0.25
917	0.00	-0.01	-0.01	0.25
944	0.00	-0.01	-0.01	0.25
972	0.00	0.00	0.00	0.25
1 000	0.00	-0.01	-0.01	0.25
1 029	0.00	-0.02	-0.02	0.25
1 059	-0.01	-0.02	-0.01	0.25
1 090	-0.01	-0.01	-0.01	0.25
1 122	0.00	0.03	0.03	0.25
1 155	0.00	0.07	0.07	0.25
1 189	0.00	0.06	0.06	0.25
1 223	0.01	0.02	0.01	0.25
1 259	0.01	-0.03	-0.04	0.25
1 296	0.01	-0.03	-0.04	0.25
1 334	0.01	-0.04	-0.05	0.25
1 372	0.01	-0.04	-0.06	0.25
1 413	0.02	-0.10	-0.12	0.25
1 454	0.02	-0.12	-0.13	0.25
1 496	0.01	-0.16	-0.17	0.25
1 540	0.01	-0.17	-0.18	0.25
1 585	0.01	-0.17	-0.18	0.25
1 631	0.01	-0.12	-0.13	0.25
1 679	0.01	-0.06	-0.06	0.25
1 728	0.00	-0.02	-0.02	0.25
1 778	0.00	0.01	0.01	0.25
1 830	-0.01	0.00	0.02	0.25
1 884	-0.02	0.04	0.07	0.25
1 939	-0.01	0.05	0.06	0.25
1 995	-0.02	0.06	0.08	0.25
2 054	-0.03	0.02	0.05	0.25
2 113	-0.03	0.01	0.04	0.25
2 175	-0.04	0.02	0.05	0.25

Frequency [Hz]	ACO 7152 typical Free Field response [dB]	SV 971A typical Free Field response [dB]	SV 971A Case Effect [dB]	Uncertainty (IEC 62585:2012) [dB]
2 239	-0.06	-0.01	0.05	0.25
2 304	-0.05	-0.03	0.03	0.25
2 371	-0.06	0.00	0.06	0.25
2 441	-0.07	0.02	0.10	0.25
2 512	-0.06	0.06	0.12	0.25
2 585	-0.05	0.04	0.09	0.25
2 661	-0.05	0.03	0.08	0.25
2 738	-0.04	-0.08	-0.05	0.25
2 818	-0.04	-0.21	-0.18	0.25
2 901	-0.05	-0.30	-0.25	0.25
2 985	-0.06	-0.25	-0.19	0.25
3 073	-0.06	-0.12	-0.05	0.25
3 162	-0.08	0.00	0.08	0.25
3 255	-0.10	0.04	0.15	0.25
3 350	-0.13	0.01	0.13	0.25
3 447	-0.13	-0.03	0.10	0.25
3 548	-0.14	-0.14	0.00	0.25
3 652	-0.14	-0.20	-0.06	0.25
3 758	-0.13	-0.29	-0.15	0.25
3 868	-0.11	-0.22	-0.11	0.25
3 981	-0.13	-0.15	-0.02	0.25
4 097	-0.14	-0.06	0.08	0.35
4 217	-0.12	-0.19	-0.07	0.35
4 340	-0.13	-0.26	-0.12	0.35
4 467	-0.16	-0.27	-0.12	0.35
4 597	-0.16	-0.14	0.02	0.35
4 732	-0.17	-0.14	0.03	0.35
4 870	-0.20	-0.14	0.06	0.35
5 012	-0.17	-0.18	-0.01	0.35
5 158	-0.17	-0.15	0.02	0.35
5 309	-0.18	-0.10	0.08	0.35
5 464	-0.15	-0.11	0.04	0.35
5 623	-0.18	-0.23	-0.04	0.35
5 788	-0.22	-0.48	-0.26	0.35
5 957	-0.21	-0.41	-0.20	0.35
6 131	-0.21	-0.14	0.07	0.35
6 310	-0.22	0.02	0.24	0.35
6 494	-0.20	-0.15	0.05	0.35
6 683	-0.18	-0.33	-0.15	0.35
6 879	-0.21	-0.29	-0.08	0.35
7 079	-0.20	-0.24	-0.03	0.35
7 286	-0.24	-0.06	0.19	0.35
7 499	-0.19	-0.04	0.15	0.35
7 718	-0.17	-0.07	0.10	0.35
7 943	-0.12	-0.23	-0.11	0.35
8 175	-0.14	-0.21	-0.07	0.35
8 414	-0.07	-0.14	-0.07	0.35
8 660	-0.12	0.00	0.12	0.35
8 913	-0.12	0.02	0.14	0.35
9 173	-0.12	0.11	0.22	0.35
9 441	-0.09	-0.04	0.05	0.35
9 716	-0.13	-0.04	0.09	0.35
10 000	-0.09	0.10	0.20	0.35

Frequency [Hz]	ACO 7152 typical Free Field response [dB]	SV 971A typical Free Field response [dB]	SV 971A Case Effect [dB]	Uncertainty (IEC 62585:2012) [dB]
10 292	-0.12	0.13	0.25	0.35
10 593	-0.16	0.04	0.20	0.35
10 902	-0.12	-0.01	0.11	0.35
11 220	-0.11	0.16	0.27	0.35
11 548	-0.09	0.19	0.28	0.35
11 885	-0.08	0.24	0.32	0.35
12 232	-0.04	0.23	0.28	0.35
12 589	-0.11	0.30	0.41	0.35
12 957	-0.10	0.21	0.32	0.35
13 335	-0.14	-0.13	0.01	0.35
13 725	-0.08	-0.22	-0.14	0.35
14 125	-0.06	-0.18	-0.12	0.35
14 538	0.03	0.22	0.19	0.35
14 962	0.12	0.50	0.38	0.35
15 399	0.15	0.47	0.33	0.35
15 849	0.13	0.24	0.11	0.35
16 312	0.12	-0.06	-0.18	0.35
16 788	0.10	-0.02	-0.13	0.35
17 278	0.14	0.10	-0.04	0.35
17 783	0.32	0.48	0.16	0.35
18 302	0.43	0.64	0.21	0.35
18 836	0.56	0.83	0.28	0.35
19 387	0.71	0.69	-0.02	0.35
19 953	0.61	0.48	-0.13	0.35


Table C.1.8. SV 971A Free Field corrections (combined: Microphone plus Case Effect) for electrostatic actuator and 0 deg incidence angle

[dB]	Frequency [Hz]																
	20	25	31.5	40	50	63	80	100	125	160	200	250	315	400	500	630	800
Correction factors	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.13	0.11	0.06	0.18	0.17	0.10
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25
[dB]	Frequency [Hz]																
	1000	1250	1600	2000	2500	3150	4000	5000	6300	8000	10000	12500	16000	20000			
Correction factors	0.09	0.11	0.03	0.35	0.52	0.67	0.84	1.26	2.10	2.72	4.31	6.18	8.42	11.45			
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.35	0.35	0.35	0.35	0.50	0.50	0.50			


SV 971A directional characteristics


Directional response of SV 971A with the ACO 7152 microphone and SV 18A preamplifier for specified frequencies.


Typical total directional characteristics

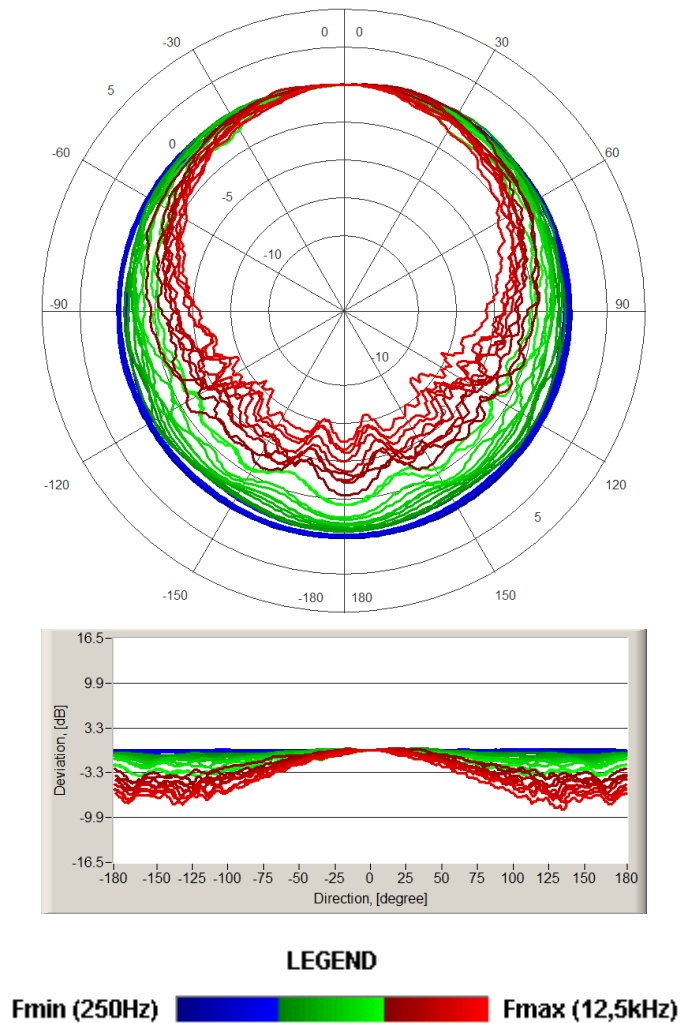


The round charts show the typical directional characteristic and the charts below shows the errors for angles.

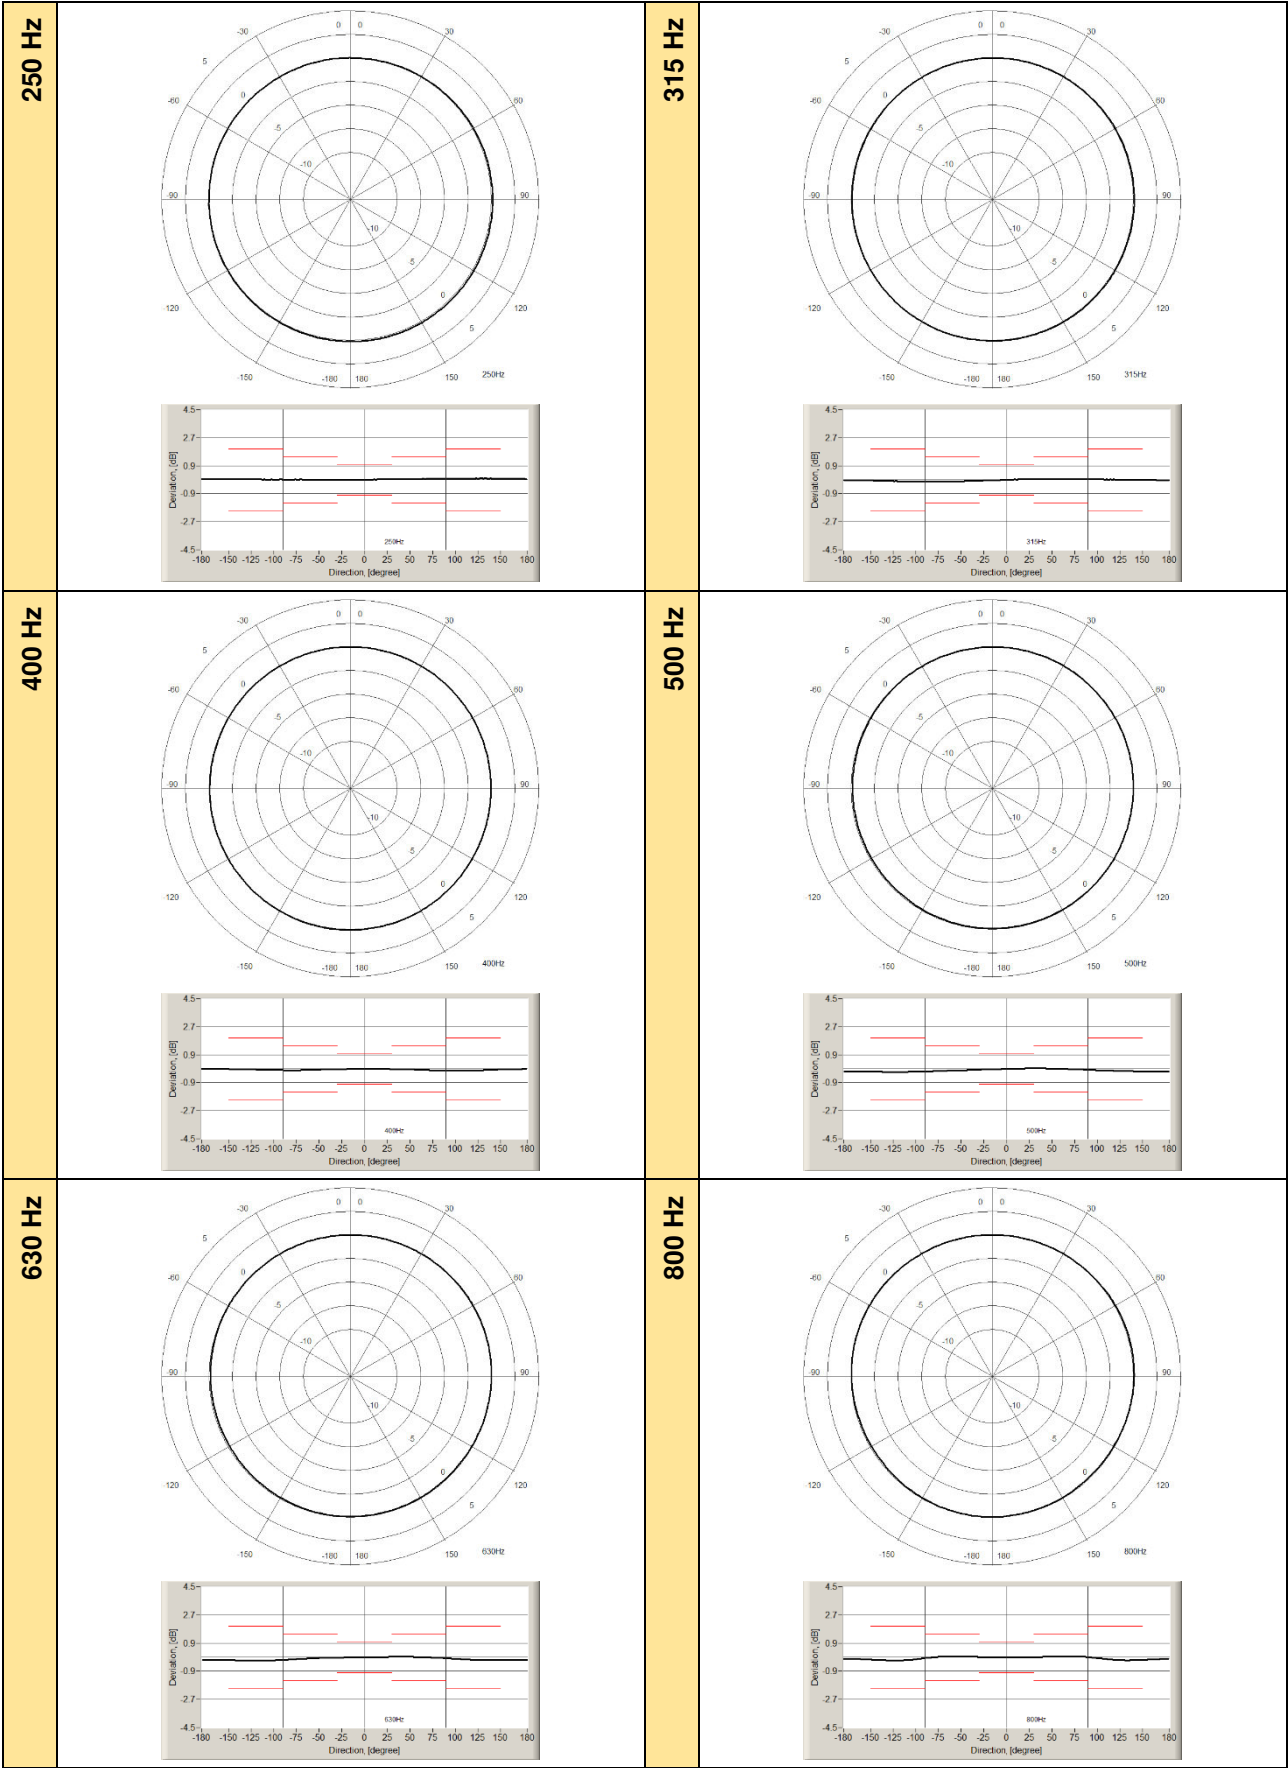

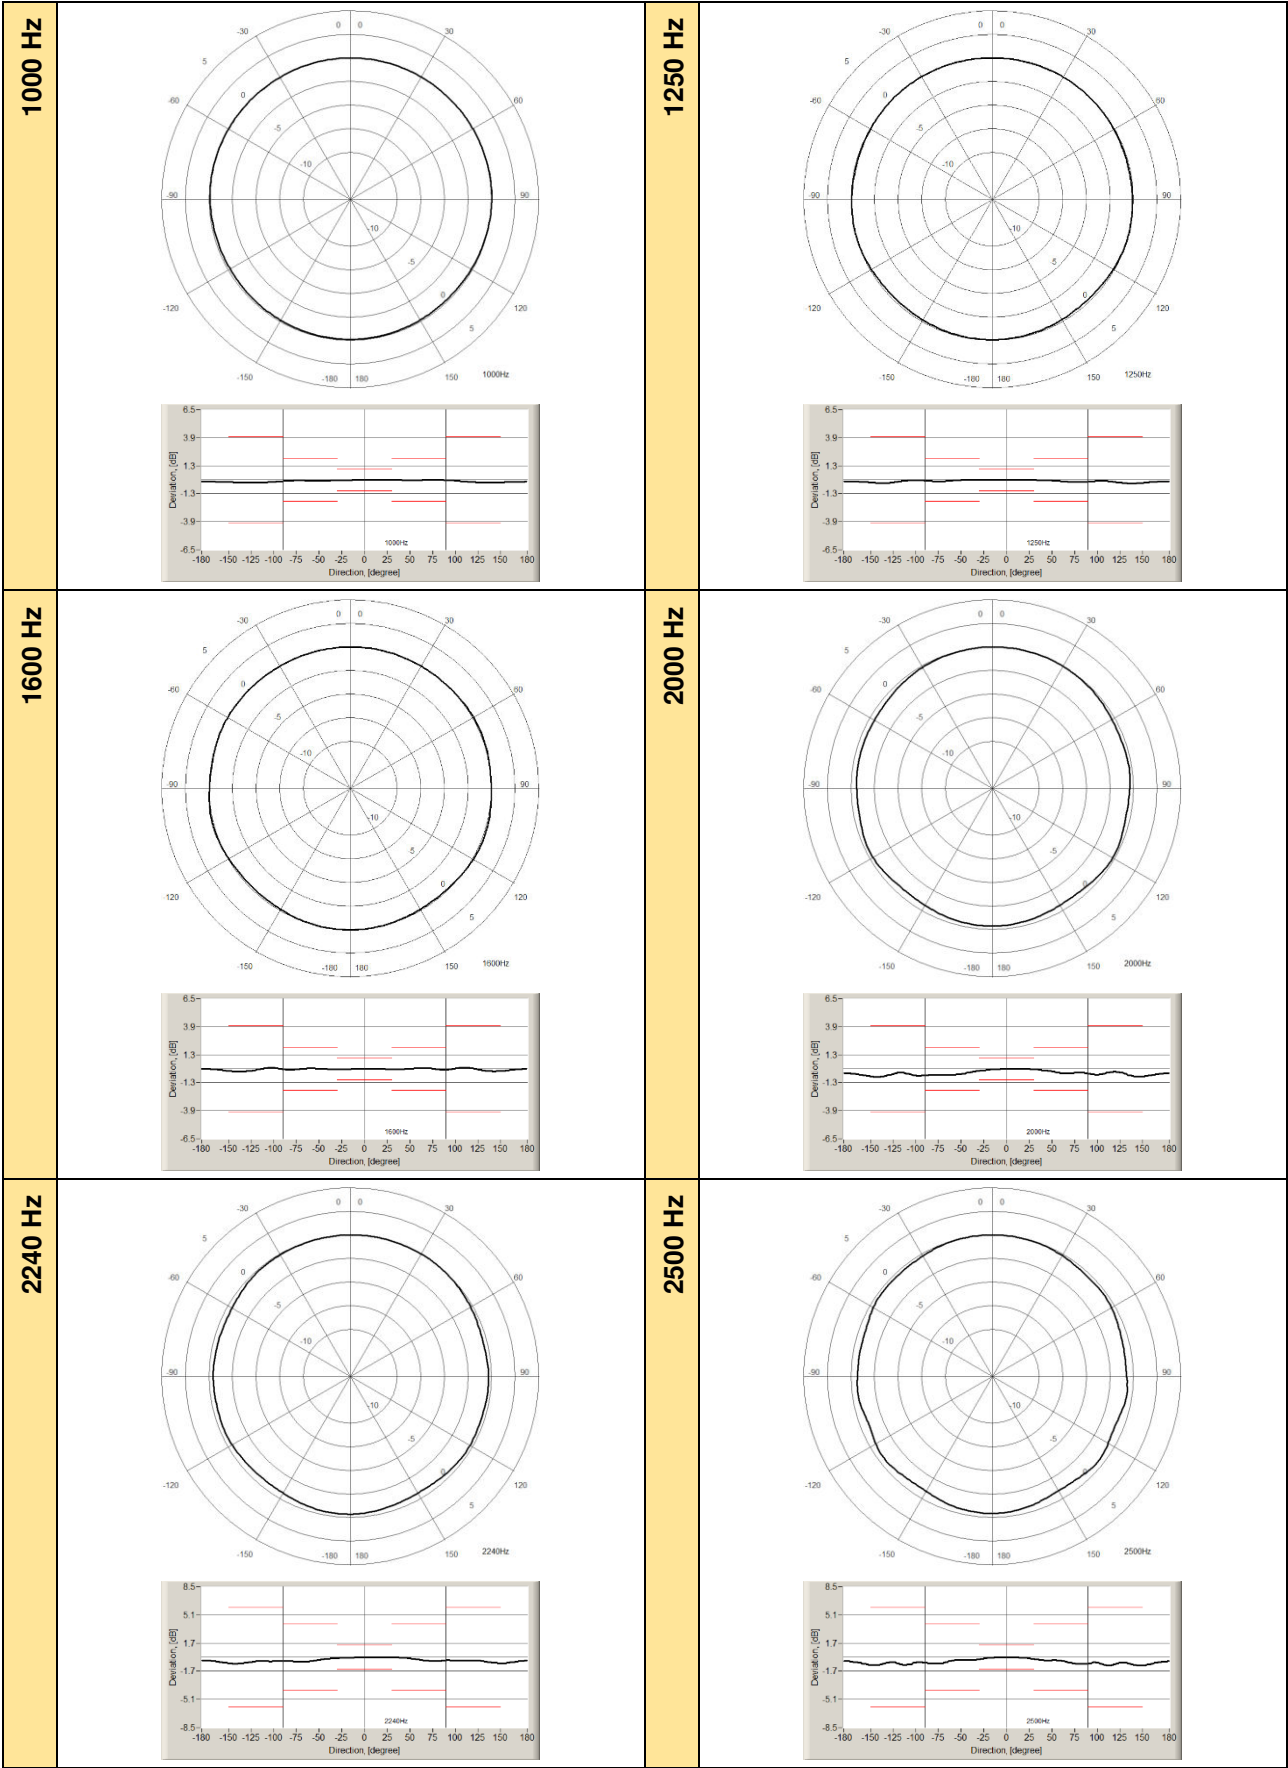

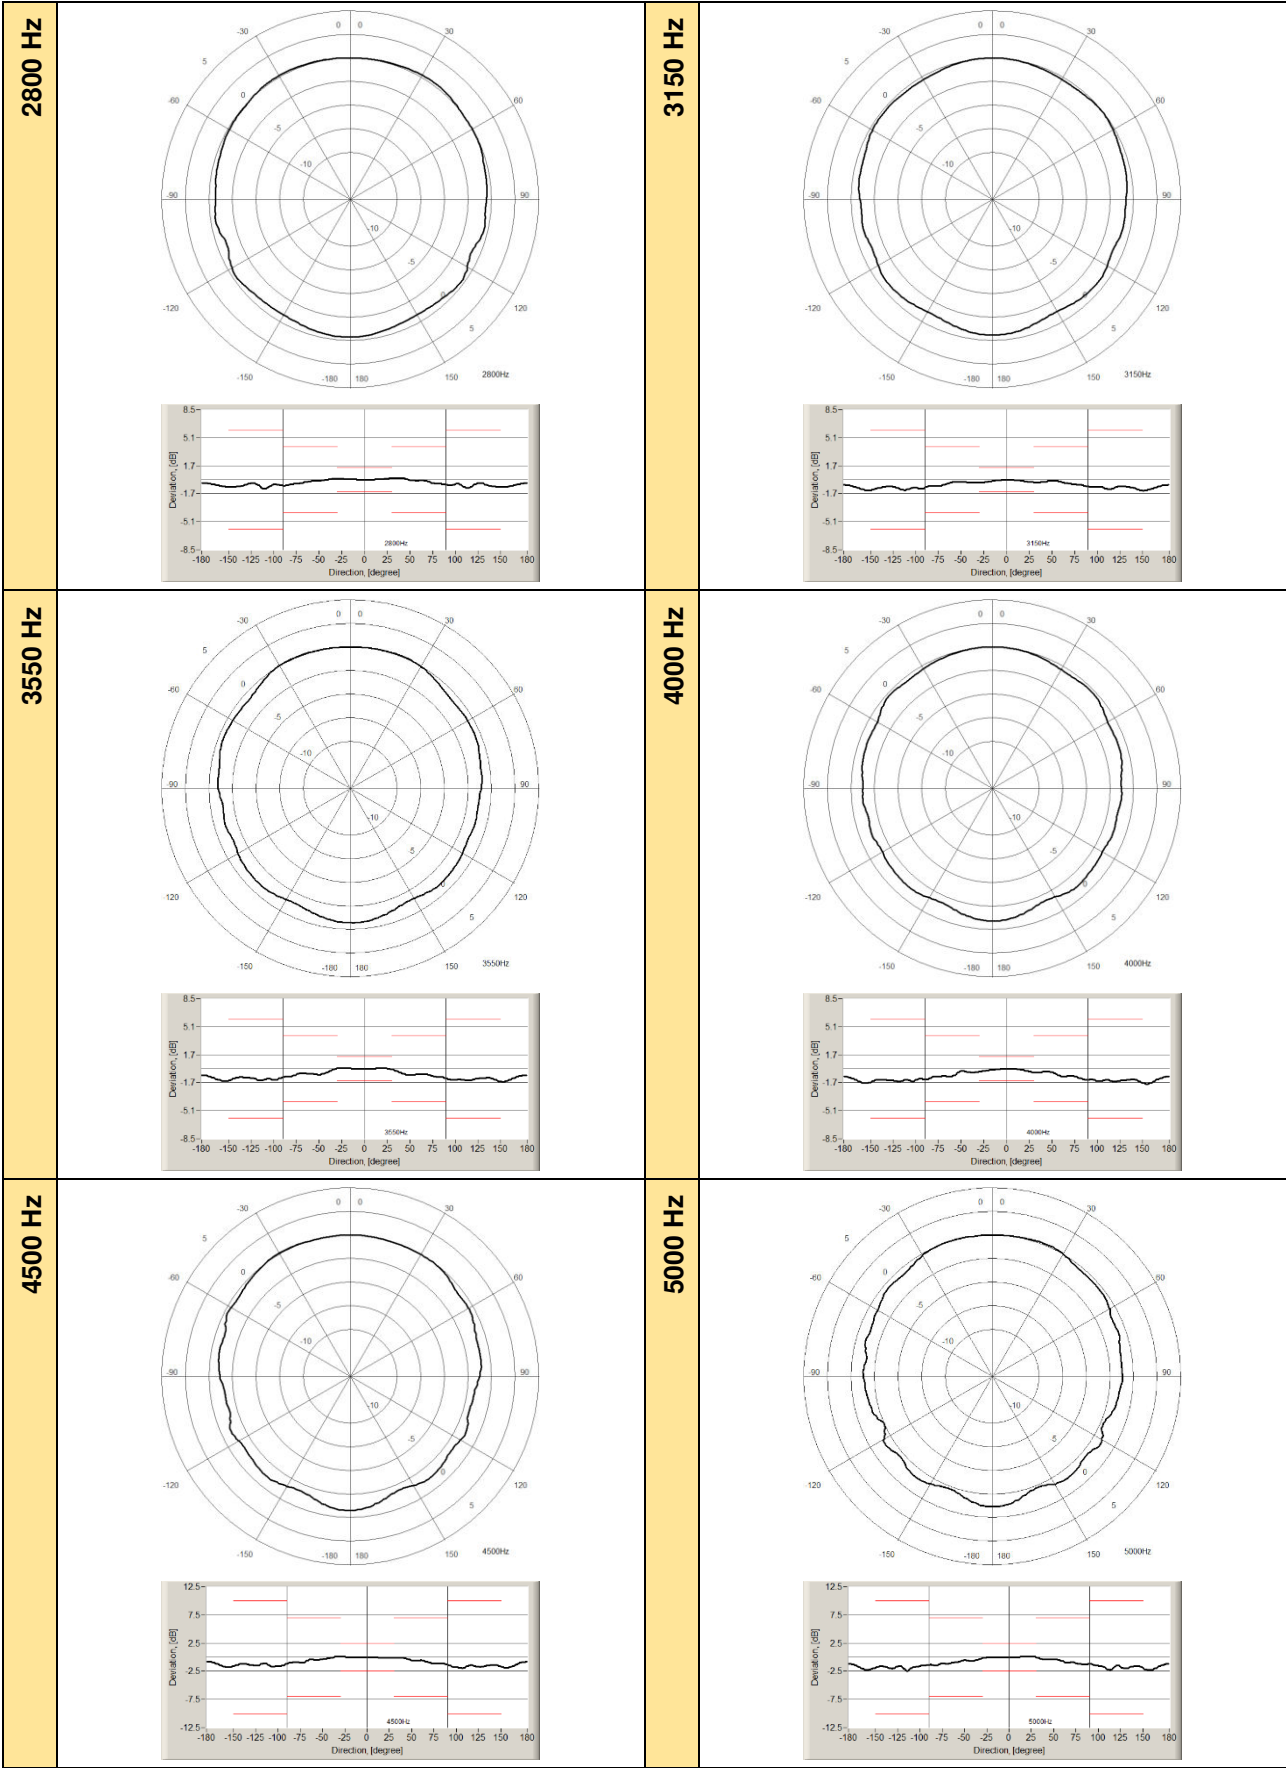

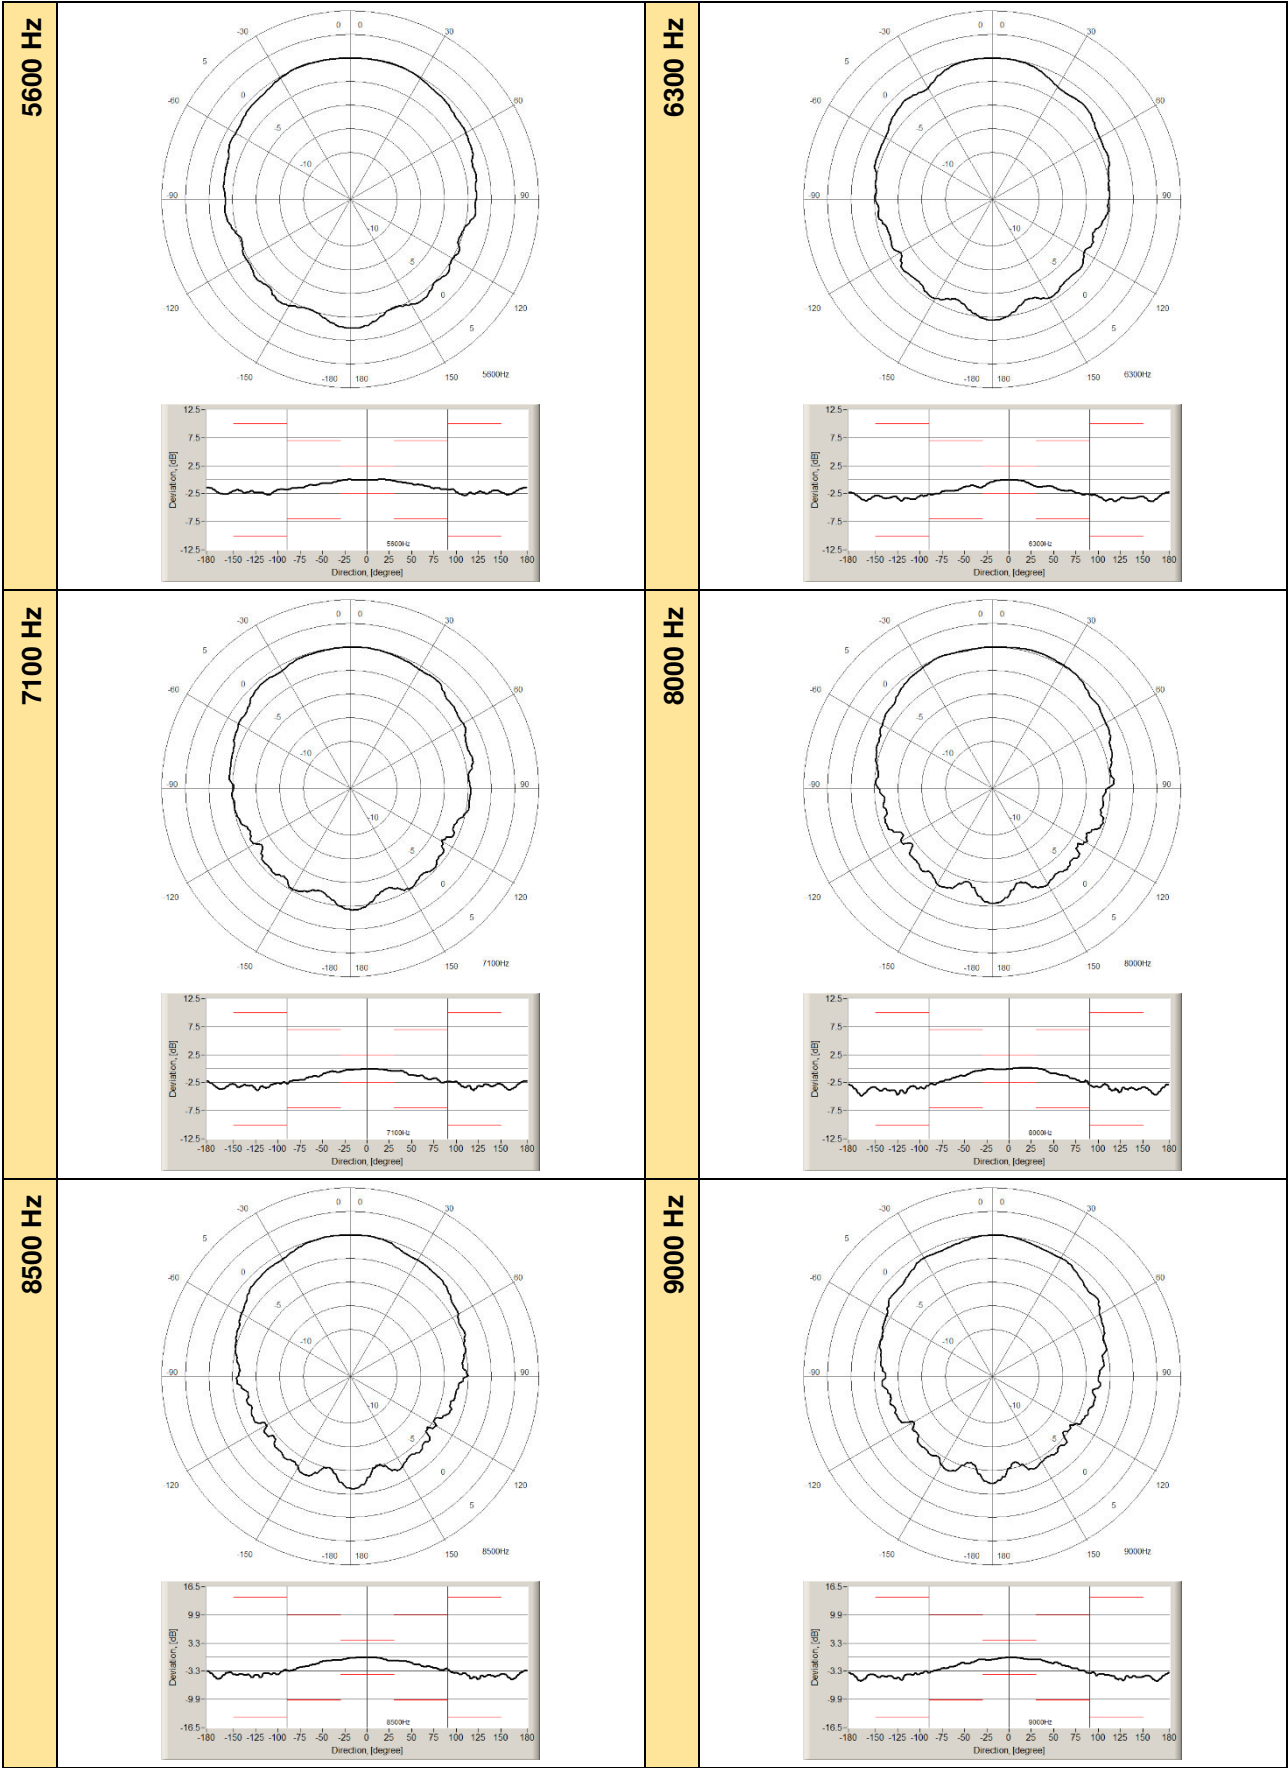

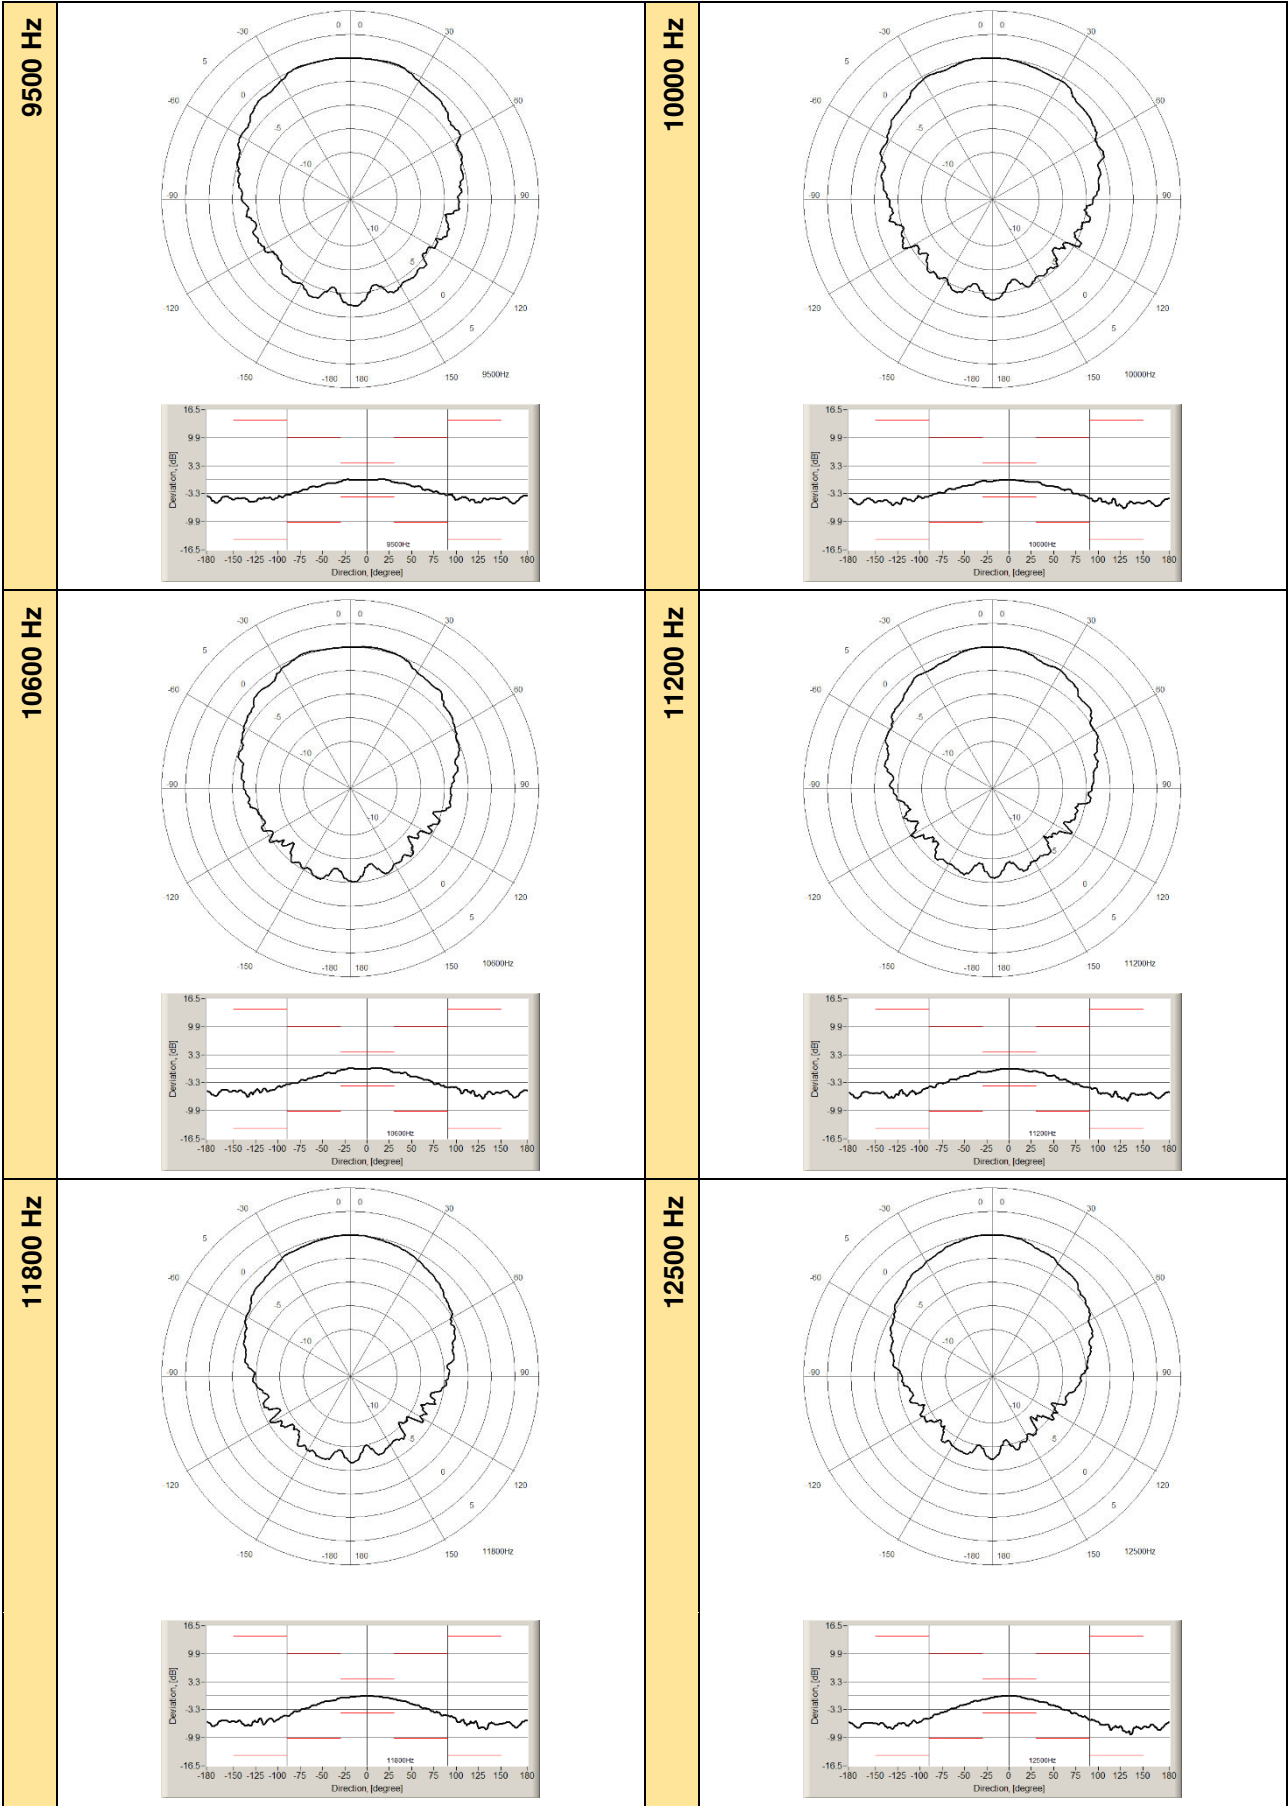


Table C.1.9. SV 971A typical directional response


f [Hz]	Angle [°]									
	0-10	10-20	20-30	30-40	40-50	50-60	60-70	70-80	80-90	90-100
250	0.03	0.03	0.03	0.04	0.04	0.05	0.06	0.06	0.07	0.08
315	0.02	0.03	0.03	0.04	0.04	0.04	0.04	0.04	0.03	0.03
400	-0.01	-0.01	-0.02	-0.04	-0.06	-0.08	-0.09	-0.11	-0.12	-0.12
500	0.01	0.02	0.03	0.03	0.03	0.02	-0.01	-0.03	-0.06	-0.09
630	0.01	0.01	0.02	0.02	0.02	0.02	0.00	-0.04	-0.07	-0.10
800	0.01	0.01	0.01	0.02	0.03	0.04	0.05	0.05	0.04	-0.06
1 000	-0.01	-0.02	-0.04	-0.05	-0.06	-0.06	-0.06	-0.07	-0.09	-0.16
1 250	0.00	-0.01	-0.02	-0.04	-0.08	-0.13	-0.19	-0.21	-0.21	-0.17
1 600	0.00	-0.02	-0.04	-0.04	-0.03	0.06	0.08	0.00	-0.08	-0.07
2 000	0.01	0.01	-0.05	-0.12	-0.25	-0.39	-0.42	-0.40	-0.45	-0.53
2 240	0.01	0.01	-0.01	-0.05	-0.16	-0.33	-0.43	-0.47	-0.44	-0.39
2 500	-0.02	-0.10	-0.25	-0.36	-0.38	-0.48	-0.68	-0.82	-0.83	-0.70
2 800	0.03	0.10	0.22	0.24	0.17	-0.10	-0.22	-0.45	-0.62	-0.66
3 150	-0.05	-0.18	-0.31	-0.32	-0.23	-0.26	-0.48	-0.60	-0.82	-0.87
3 550	0.03	0.06	-0.02	-0.48	-0.75	-0.76	-0.69	-0.99	-1.12	-1.35
4 000	-0.03	-0.24	-0.44	-0.47	-0.36	-0.86	-0.90	-1.05	-1.32	-1.44
4 500	-0.04	-0.08	-0.08	-0.13	-0.60	-0.62	-0.96	-1.09	-1.34	-1.81
5 000	0.05	0.15	0.15	-0.37	-0.38	-0.72	-0.94	-1.20	-1.24	-1.48
5 600	0.04	0.08	-0.13	-0.46	-0.73	-0.85	-1.20	-1.52	-1.65	-1.93
6 300	-0.06	-0.47	-1.23	-1.30	-1.31	-1.89	-1.95	-2.47	-2.68	-3.07
7 100	0.02	-0.15	-0.39	-0.41	-1.00	-1.26	-1.79	-1.90	-2.38	-2.28
8 000	0.15	0.24	0.19	-0.21	-0.70	-1.11	-1.71	-2.35	-2.91	-3.31
8 500	-0.01	-0.29	-0.59	-0.80	-1.07	-1.51	-1.94	-2.44	-2.67	-3.23
9 000	-0.17	-0.47	-0.53	-0.95	-1.32	-1.91	-2.51	-3.08	-3.72	-4.13
9 500	0.01	0.14	-0.59	-0.80	-1.54	-1.83	-2.42	-3.05	-3.55	-4.55
10 000	-0.14	-0.39	-0.50	-1.32	-1.51	-2.41	-2.98	-3.56	-4.34	-5.16
10 600	0.11	0.13	-0.68	-1.03	-1.74	-2.12	-2.65	-3.49	-4.16	-4.39
11 200	-0.05	-0.57	-0.71	-1.09	-1.68	-2.63	-3.16	-4.14	-4.40	-5.73
11 800	-0.12	-0.38	-0.69	-1.18	-1.83	-2.60	-3.13	-3.82	-4.63	-5.45
12 500	-0.15	-0.73	-1.28	-1.54	-2.37	-3.31	-4.12	-4.81	-5.65	-6.24
f [Hz]	100-110	110-120	120-130	130-140	140-150	150-160	160-170	170-180	180-190	190-200
250	0.08	0.08	0.09	0.09	0.08	0.08	0.08	0.07	0.05	0.04
315	0.02	0.02	0.01	0.01	-0.01	-0.02	-0.02	-0.03	-0.03	-0.04
400	-0.12	-0.11	-0.10	-0.08	-0.06	-0.04	-0.03	-0.02	-0.01	-0.02
500	-0.11	-0.13	-0.15	-0.16	-0.16	-0.17	-0.17	-0.17	-0.17	-0.18
630	-0.14	-0.16	-0.18	-0.18	-0.18	-0.18	-0.17	-0.16	-0.16	-0.17
800	-0.12	-0.17	-0.19	-0.20	-0.19	-0.16	-0.14	-0.12	-0.11	-0.13
1 000	-0.22	-0.25	-0.28	-0.28	-0.27	-0.25	-0.21	-0.17	-0.13	-0.13
1 250	-0.12	-0.21	-0.32	-0.34	-0.34	-0.29	-0.20	-0.15	-0.15	-0.19
1 600	0.11	0.11	-0.14	-0.23	-0.23	-0.20	-0.11	-0.03	-0.03	-0.10
2 000	-0.53	-0.37	-0.45	-0.68	-0.72	-0.69	-0.54	-0.45	-0.45	-0.57
2 240	-0.42	-0.40	-0.46	-0.66	-0.72	-0.71	-0.58	-0.46	-0.45	-0.60
2 500	-0.98	-0.99	-0.71	-0.94	-1.02	-0.96	-0.72	-0.54	-0.57	-0.76
2 800	-0.86	-1.01	-0.54	-0.78	-0.88	-0.88	-0.76	-0.51	-0.51	-0.72
3 150	-1.09	-1.15	-0.84	-1.03	-1.30	-1.30	-1.03	-0.68	-0.79	-1.15
3 550	-1.37	-1.42	-1.25	-1.16	-1.54	-1.58	-1.32	-0.87	-0.99	-1.41
4 000	-1.47	-1.51	-1.50	-1.37	-1.76	-1.84	-1.51	-1.10	-1.20	-1.71
4 500	-1.91	-1.58	-1.72	-1.56	-1.75	-1.91	-1.67	-0.98	-1.16	-1.72
5 000	-2.13	-2.24	-1.97	-1.92	-1.94	-2.28	-2.13	-1.39	-1.63	-2.27
5 600	-2.77	-2.71	-2.41	-2.41	-2.09	-2.66	-2.58	-1.58	-1.94	-2.59
6 300	-3.72	-3.76	-3.48	-3.34	-3.19	-3.80	-3.72	-2.47	-3.00	-3.74
7 100	-3.32	-3.75	-3.67	-3.09	-3.13	-3.64	-3.61	-2.57	-3.27	-3.71
8 000	-3.16	-3.92	-4.31	-3.73	-3.74	-4.56	-4.66	-3.34	-4.46	-4.79
8 500	-3.69	-4.38	-4.68	-4.32	-4.72	-5.06	-5.00	-4.03	-4.76	-5.04
9 000	-4.16	-5.05	-5.39	-4.69	-4.63	-5.08	-5.58	-4.50	-5.39	-5.62
9 500	-4.71	-5.17	-5.33	-4.66	-4.58	-4.85	-5.53	-4.43	-5.37	-5.58
10 000	-5.49	-6.05	-6.61	-6.26	-5.47	-5.46	-6.21	-5.12	-5.88	-5.90
10 600	-5.79	-5.91	-6.76	-6.67	-5.83	-5.74	-6.67	-5.89	-6.48	-6.46
11 200	-5.95	-6.49	-7.02	-7.53	-6.24	-6.14	-7.06	-6.53	-7.12	-6.84
11 800	-6.32	-6.83	-7.50	-7.76	-6.70	-6.47	-7.39	-6.90	-7.23	-7.07
12 500	-7.04	-8.04	-8.57	-8.89	-7.68	-7.22	-8.04	-7.41	-7.68	-7.50

f [Hz]	200-210	210-220	220-230	230-240	240-250	250-260	260-270	270-280	280-290	290-300
250	0.04	0.03	0.03	0.03	0.02	0.02	0.02	0.02	0.02	0.02
315	-0.05	-0.07	-0.08	-0.09	-0.10	-0.11	-0.11	-0.11	-0.11	-0.11
400	-0.03	-0.04	-0.05	-0.07	-0.08	-0.09	-0.09	-0.10	-0.09	-0.08
500	-0.18	-0.19	-0.20	-0.20	-0.20	-0.19	-0.18	-0.17	-0.15	-0.13
630	-0.18	-0.20	-0.21	-0.22	-0.22	-0.21	-0.19	-0.17	-0.13	-0.10
800	-0.15	-0.18	-0.21	-0.21	-0.21	-0.18	-0.12	-0.05	0.04	0.05
1 000	-0.15	-0.17	-0.18	-0.18	-0.17	-0.13	-0.09	-0.06	-0.03	-0.05
1 250	-0.26	-0.31	-0.32	-0.28	-0.19	-0.07	-0.09	-0.14	-0.15	-0.13
1 600	-0.20	-0.26	-0.27	-0.21	-0.09	0.09	0.01	-0.09	-0.08	0.03
2 000	-0.71	-0.76	-0.73	-0.56	-0.44	-0.63	-0.64	-0.60	-0.55	-0.55
2 240	-0.75	-0.77	-0.74	-0.61	-0.50	-0.51	-0.48	-0.51	-0.56	-0.56
2 500	-0.96	-0.98	-0.86	-0.76	-0.96	-0.88	-0.70	-0.74	-0.75	-0.64
2 800	-0.87	-0.87	-0.81	-0.54	-1.07	-1.03	-0.73	-0.72	-0.51	-0.37
3 150	-1.28	-1.21	-0.94	-1.02	-1.26	-1.14	-1.08	-0.92	-0.75	-0.62
3 550	-1.50	-1.36	-1.09	-1.31	-1.45	-1.37	-1.36	-0.98	-0.83	-0.63
4 000	-1.76	-1.50	-1.39	-1.56	-1.57	-1.52	-1.27	-1.27	-0.95	-0.97
4 500	-1.78	-1.49	-1.43	-1.49	-1.54	-1.72	-1.61	-1.10	-1.05	-0.73
5 000	-2.25	-1.74	-2.06	-1.89	-2.49	-1.84	-1.54	-1.55	-1.27	-1.22
5 600	-2.58	-2.11	-2.36	-2.35	-2.73	-2.66	-1.82	-1.75	-1.46	-1.17
6 300	-3.61	-3.32	-3.34	-3.81	-3.53	-3.52	-2.96	-2.69	-2.27	-2.01
7 100	-3.44	-3.39	-3.10	-3.89	-3.53	-3.04	-2.66	-2.64	-2.04	-1.75
8 000	-3.65	-3.96	-3.98	-4.69	-4.43	-3.58	-3.59	-2.83	-2.41	-1.96
8 500	-4.53	-4.15	-4.40	-4.17	-4.01	-3.46	-3.20	-2.69	-2.09	-1.53
9 000	-4.52	-4.78	-4.89	-5.42	-4.52	-4.18	-3.77	-3.60	-2.91	-2.42
9 500	-4.74	-4.65	-5.21	-5.37	-4.57	-4.67	-4.14	-3.52	-3.05	-2.37
10 000	-5.36	-5.18	-6.08	-5.84	-4.81	-5.11	-4.37	-3.82	-3.11	-2.24
10 600	-5.52	-5.49	-6.65	-6.10	-5.45	-5.20	-4.32	-3.78	-3.39	-2.75
11 200	-5.94	-5.95	-7.08	-6.60	-6.41	-6.08	-5.40	-4.57	-3.53	-3.17
11 800	-6.27	-6.65	-7.22	-6.79	-6.82	-6.10	-5.50	-4.84	-3.76	-2.97
12 500	-6.79	-7.29	-7.97	-7.24	-7.26	-6.35	-6.05	-5.11	-4.35	-3.42
f [Hz]	300-310	310-320	320-330	330-340	340-350	350-360				
250	0.01	0.01	0.00	0.00	-0.01	0.01				
315	-0.10	-0.09	-0.07	-0.06	-0.04	-0.02				
400	-0.07	-0.05	-0.04	-0.02	-0.01	0.00				
500	-0.11	-0.09	-0.08	-0.06	-0.04	-0.02				
630	-0.07	-0.05	-0.03	-0.02	-0.01	0.00				
800	0.05	0.04	0.03	0.01	0.01	0.00				
1 000	-0.06	-0.06	-0.05	-0.03	-0.02	0.00				
1 250	-0.07	-0.03	0.02	0.02	0.02	0.01				
1 600	0.03	-0.03	-0.04	-0.04	-0.03	-0.01				
2 000	-0.55	-0.46	-0.31	-0.16	-0.08	-0.03				
2 240	-0.47	-0.27	-0.15	-0.11	-0.06	-0.02				
2 500	-0.39	-0.36	-0.34	-0.21	-0.08	-0.01				
2 800	-0.16	-0.10	0.13	0.13	0.08	0.03				
3 150	-0.28	-0.35	-0.36	-0.34	-0.21	-0.06				
3 550	-0.73	-0.71	-0.25	0.07	0.05	0.01				
4 000	-0.78	-0.47	-0.48	-0.32	-0.16	-0.04				
4 500	-0.52	-0.28	0.10	0.08	-0.03	-0.02				
5 000	-0.88	-0.68	-0.61	-0.12	0.01	-0.01				
5 600	-0.97	-0.59	-0.52	-0.09	0.06	0.00				
6 300	-1.75	-1.23	-1.41	-0.93	-0.24	-0.03				
7 100	-1.37	-0.91	-0.61	-0.57	-0.18	-0.10				
8 000	-1.39	-1.11	-0.40	-0.16	-0.11	-0.10				
8 500	-1.25	-0.79	-0.58	-0.38	-0.08	0.01				
9 000	-1.84	-1.40	-0.88	-0.60	-0.52	-0.11				
9 500	-1.77	-1.22	-0.86	-0.31	-0.03	-0.02				
10 000	-1.96	-1.40	-0.89	-0.44	-0.40	0.03				
10 600	-1.88	-1.45	-1.06	-0.35	0.18	0.01				
11 200	-2.46	-1.76	-1.05	-0.82	-0.57	-0.07				
11 800	-2.26	-1.50	-1.12	-0.43	-0.34	-0.10				
12 500	-2.56	-2.06	-1.25	-0.90	-0.43	-0.04				

C.1.2 Effect of the SA 22 windscreen



Note: When using the SA22 windscreen the **Windscreen** compensation filter must be **On** to ensure good tolerances margin of the SV 971A frequency response.

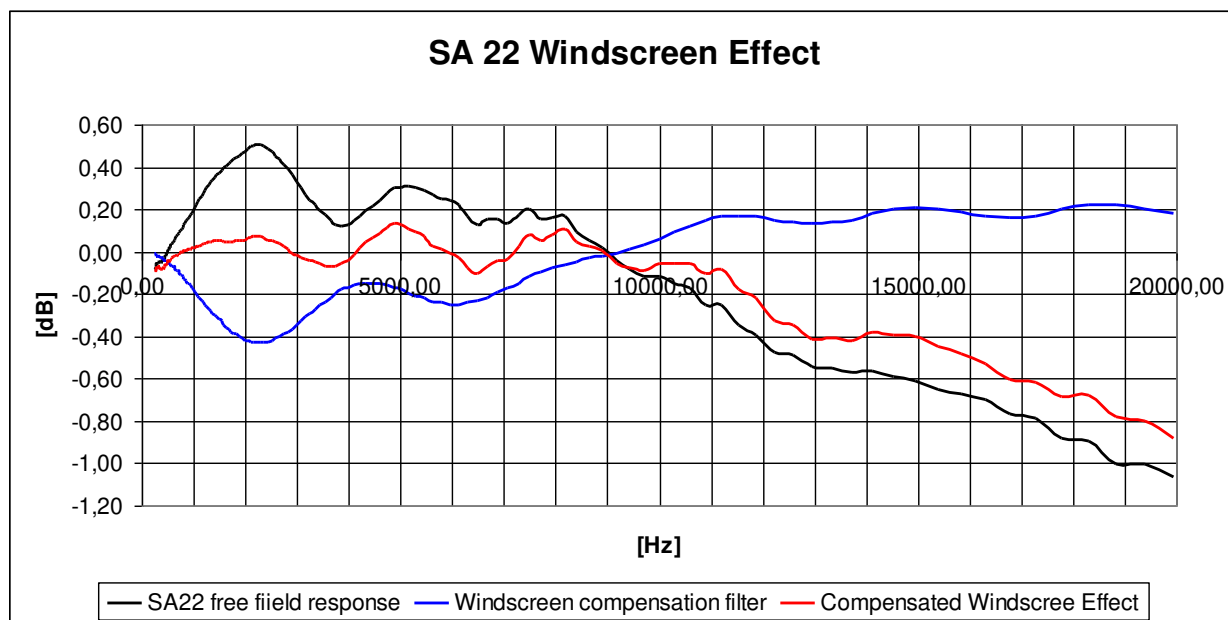

Windscreen SA22 Free Field typical response and compensated effect

Table C.1.10. Effect of the SA 22 windscreen

Frequency [Hz]	SA 22 typical Free Field effect [dB]	Compensation filter [dB]	Compensated SA 22 Free Field effect [dB]	Uncertainty (IEC 62585:2012) [dB]
251	-0.08	-0.01	-0.09	0.20
259	-0.08	-0.01	-0.09	0.20
266	-0.08	-0.01	-0.09	0.20
274	-0.07	-0.02	-0.09	0.20
282	-0.07	-0.02	-0.09	0.20
290	-0.06	-0.02	-0.08	0.20
299	-0.06	-0.02	-0.08	0.20
307	-0.05	-0.02	-0.07	0.20
316	-0.05	-0.02	-0.07	0.20
325	-0.05	-0.02	-0.07	0.20
335	-0.05	-0.02	-0.07	0.20
345	-0.05	-0.02	-0.07	0.20
355	-0.05	-0.03	-0.08	0.20
365	-0.05	-0.03	-0.08	0.20
376	-0.05	-0.03	-0.08	0.20
387	-0.05	-0.03	-0.08	0.20
398	-0.05	-0.03	-0.08	0.20
410	-0.05	-0.03	-0.08	0.20
422	-0.04	-0.04	-0.08	0.20

Frequency [Hz]	SA 22 typical Free Field effect [dB]	Compensation filter [dB]	Compensated SA 22 Free Field effect [dB]	Uncertainty (IEC 62585:2012) [dB]
434	-0.03	-0.04	-0.07	0.20
447	-0.03	-0.04	-0.07	0.20
460	-0.02	-0.04	-0.06	0.20
473	-0.01	-0.05	-0.06	0.20
487	-0.01	-0.05	-0.06	0.20
501	0.00	-0.05	-0.05	0.20
516	0.01	-0.05	-0.04	0.20
531	0.01	-0.06	-0.05	0.20
546	0.02	-0.06	-0.04	0.20
562	0.03	-0.06	-0.03	0.20
579	0.03	-0.07	-0.04	0.20
596	0.04	-0.07	-0.03	0.20
613	0.05	-0.07	-0.02	0.20
631	0.05	-0.08	-0.03	0.20
649	0.06	-0.08	-0.02	0.20
668	0.07	-0.09	-0.02	0.20
688	0.08	-0.09	-0.01	0.20
708	0.08	-0.1	-0.02	0.20
729	0.09	-0.1	-0.01	0.20
750	0.10	-0.11	-0.01	0.20
772	0.11	-0.11	0.00	0.20
794	0.12	-0.12	0.00	0.20
818	0.12	-0.13	-0.01	0.20
841	0.13	-0.13	0.00	0.20
866	0.14	-0.14	0.00	0.20
891	0.15	-0.15	0.00	0.20
917	0.16	-0.15	0.01	0.20
944	0.17	-0.16	0.01	0.20
972	0.18	-0.17	0.01	0.20
1 000	0.19	-0.18	0.01	0.20
1 029	0.21	-0.19	0.02	0.20
1 059	0.22	-0.2	0.02	0.20
1 090	0.23	-0.21	0.02	0.20
1 122	0.25	-0.22	0.03	0.20
1 155	0.26	-0.23	0.03	0.20
1 189	0.28	-0.24	0.04	0.20
1 223	0.29	-0.25	0.04	0.20
1 259	0.30	-0.26	0.04	0.20
1 296	0.31	-0.27	0.04	0.20
1 334	0.33	-0.28	0.05	0.20
1 372	0.34	-0.29	0.05	0.20
1 413	0.35	-0.3	0.05	0.20
1 454	0.36	-0.31	0.05	0.20
1 496	0.37	-0.32	0.05	0.20
1 540	0.38	-0.33	0.05	0.20
1 585	0.39	-0.35	0.04	0.20
1 631	0.40	-0.36	0.04	0.20
1 679	0.41	-0.37	0.04	0.20
1 728	0.42	-0.38	0.04	0.20
1 778	0.43	-0.38	0.05	0.20
1 830	0.44	-0.39	0.05	0.20
1 884	0.45	-0.40	0.05	0.20
1 939	0.46	-0.40	0.06	0.20


Frequency [Hz]	SA 22 typical Free Field effect [dB]	Compensation filter [dB]	Compensated SA 22 Free Field effect [dB]	Uncertainty (IEC 62585:2012) [dB]
1 995	0.47	-0.41	0.06	0.20
2 054	0.48	-0.42	0.06	0.20
2 113	0.50	-0.43	0.07	0.20
2 175	0.50	-0.43	0.07	0.20
2 239	0.50	-0.43	0.07	0.20
2 304	0.50	-0.43	0.07	0.20
2 371	0.50	-0.43	0.07	0.20
2 441	0.48	-0.43	0.05	0.20
2 512	0.47	-0.42	0.05	0.20
2 585	0.45	-0.41	0.04	0.20
2 661	0.44	-0.4	0.04	0.20
2 738	0.41	-0.39	0.02	0.20
2 818	0.39	-0.38	0.01	0.20
2 901	0.36	-0.37	-0.01	0.20
2 985	0.33	-0.35	-0.02	0.20
3 073	0.30	-0.33	-0.03	0.20
3 162	0.27	-0.31	-0.04	0.20
3 255	0.24	-0.29	-0.05	0.20
3 350	0.22	-0.27	-0.05	0.20
3 447	0.20	-0.25	-0.05	0.20
3 548	0.17	-0.24	-0.07	0.20
3 652	0.15	-0.22	-0.07	0.20
3 758	0.13	-0.2	-0.07	0.20
3 868	0.12	-0.18	-0.06	0.20
3 981	0.13	-0.17	-0.04	0.20
4 097	0.15	-0.16	-0.01	0.30
4 217	0.17	-0.15	0.02	0.30
4 340	0.19	-0.15	0.04	0.30
4 467	0.21	-0.15	0.06	0.30
4 597	0.24	-0.15	0.09	0.30
4 732	0.27	-0.16	0.11	0.30
4 870	0.30	-0.17	0.13	0.30
5 012	0.31	-0.18	0.13	0.30
5 158	0.31	-0.2	0.11	0.30
5 309	0.30	-0.21	0.09	0.30
5 464	0.29	-0.22	0.07	0.30
5 623	0.27	-0.24	0.03	0.30
5 788	0.25	-0.24	0.01	0.30
5 957	0.24	-0.25	-0.01	0.30
6 131	0.22	-0.25	-0.03	0.30
6 310	0.17	-0.24	-0.07	0.30
6 494	0.12	-0.23	-0.11	0.30
6 683	0.15	-0.22	-0.07	0.30
6 879	0.15	-0.19	-0.04	0.30
7 079	0.14	-0.17	-0.03	0.30
7 286	0.17	-0.15	0.02	0.30
7 499	0.20	-0.12	0.08	0.30
7 718	0.15	-0.1	0.05	0.30
7 943	0.16	-0.08	0.08	0.30
8 175	0.17	-0.06	0.11	0.30
8 414	0.09	-0.05	0.04	0.30
8 660	0.05	-0.03	0.02	0.30
8 913	0.02	-0.02	0.00	0.30

Frequency [Hz]	SA 22 typical Free Field effect [dB]	Compensation filter [dB]	Compensated SA 22 Free Field effect [dB]	Uncertainty (IEC 62585:2012) [dB]
9 173	-0.04	-0.01	-0.05	0.30
9 441	-0.09	0.01	-0.08	0.30
9 716	-0.12	0.03	-0.09	0.30
10 000	-0.12	0.06	-0.06	0.30
10 292	-0.15	0.09	-0.06	0.30
10 593	-0.17	0.12	-0.05	0.30
10 902	-0.25	0.15	-0.10	0.30
11 220	-0.25	0.17	-0.08	0.30
11 548	-0.35	0.17	-0.18	0.30
11 885	-0.39	0.17	-0.22	0.30
12 232	-0.47	0.15	-0.32	0.30
12 589	-0.49	0.14	-0.35	0.30
12 957	-0.54	0.13	-0.41	0.30
13 335	-0.55	0.14	-0.41	0.30
13 725	-0.57	0.15	-0.42	0.30
14 125	-0.56	0.18	-0.38	0.30
14 538	-0.59	0.2	-0.39	0.30
14 962	-0.61	0.21	-0.40	0.30
15 399	-0.65	0.2	-0.45	0.30
15 849	-0.67	0.19	-0.48	0.30
16 312	-0.70	0.17	-0.53	0.30
16 788	-0.77	0.16	-0.61	0.30
17 278	-0.79	0.17	-0.62	0.30
17 783	-0.88	0.2	-0.68	0.30
18 302	-0.90	0.22	-0.68	0.30
18 836	-1.00	0.22	-0.78	0.30
19 387	-1.00	0.2	-0.80	0.30
19 953	-1.06	0.18	-0.88	0.30


Directional characteristics of SV 971A with SA 22


Directional response of SV 971A with the ACO 7152 microphone, SV 18A preamplifier and SA 22 windscreen for specified frequencies.


Combined typical directional characteristics

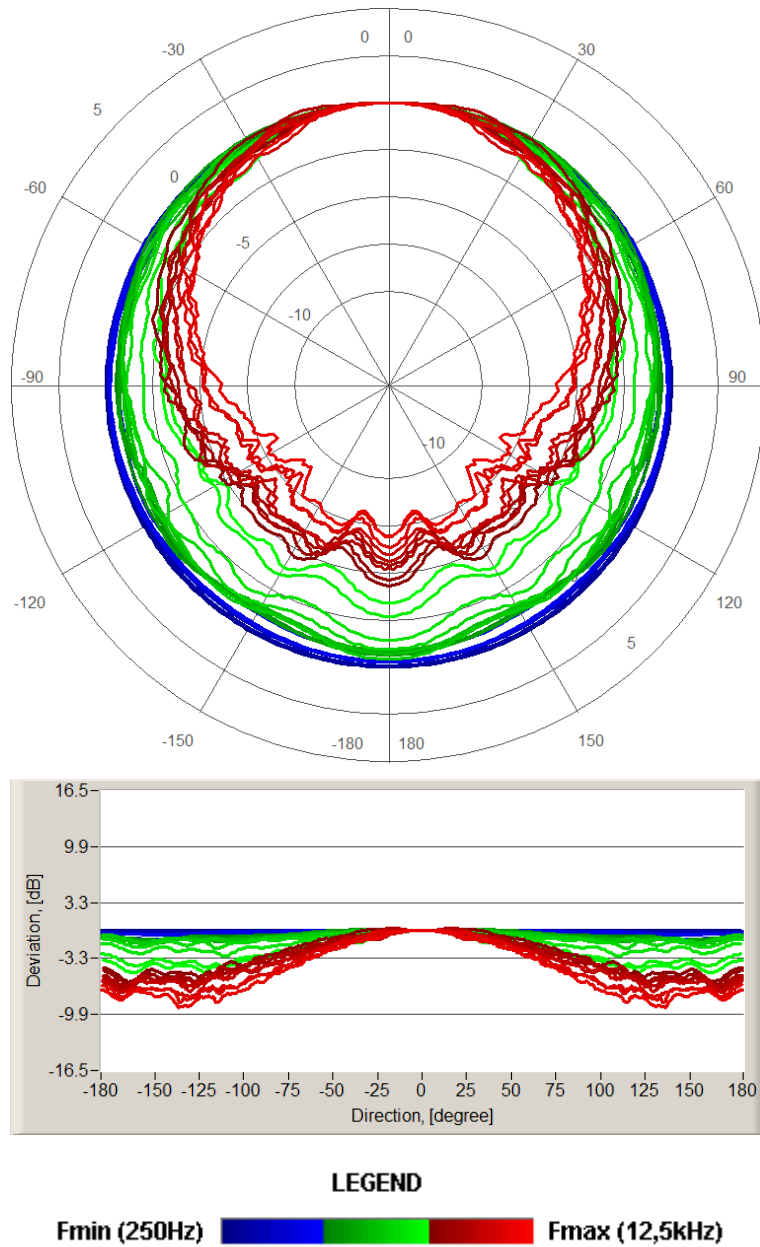


The round charts show the typical directional characteristic and the charts below shows the errors for angles.

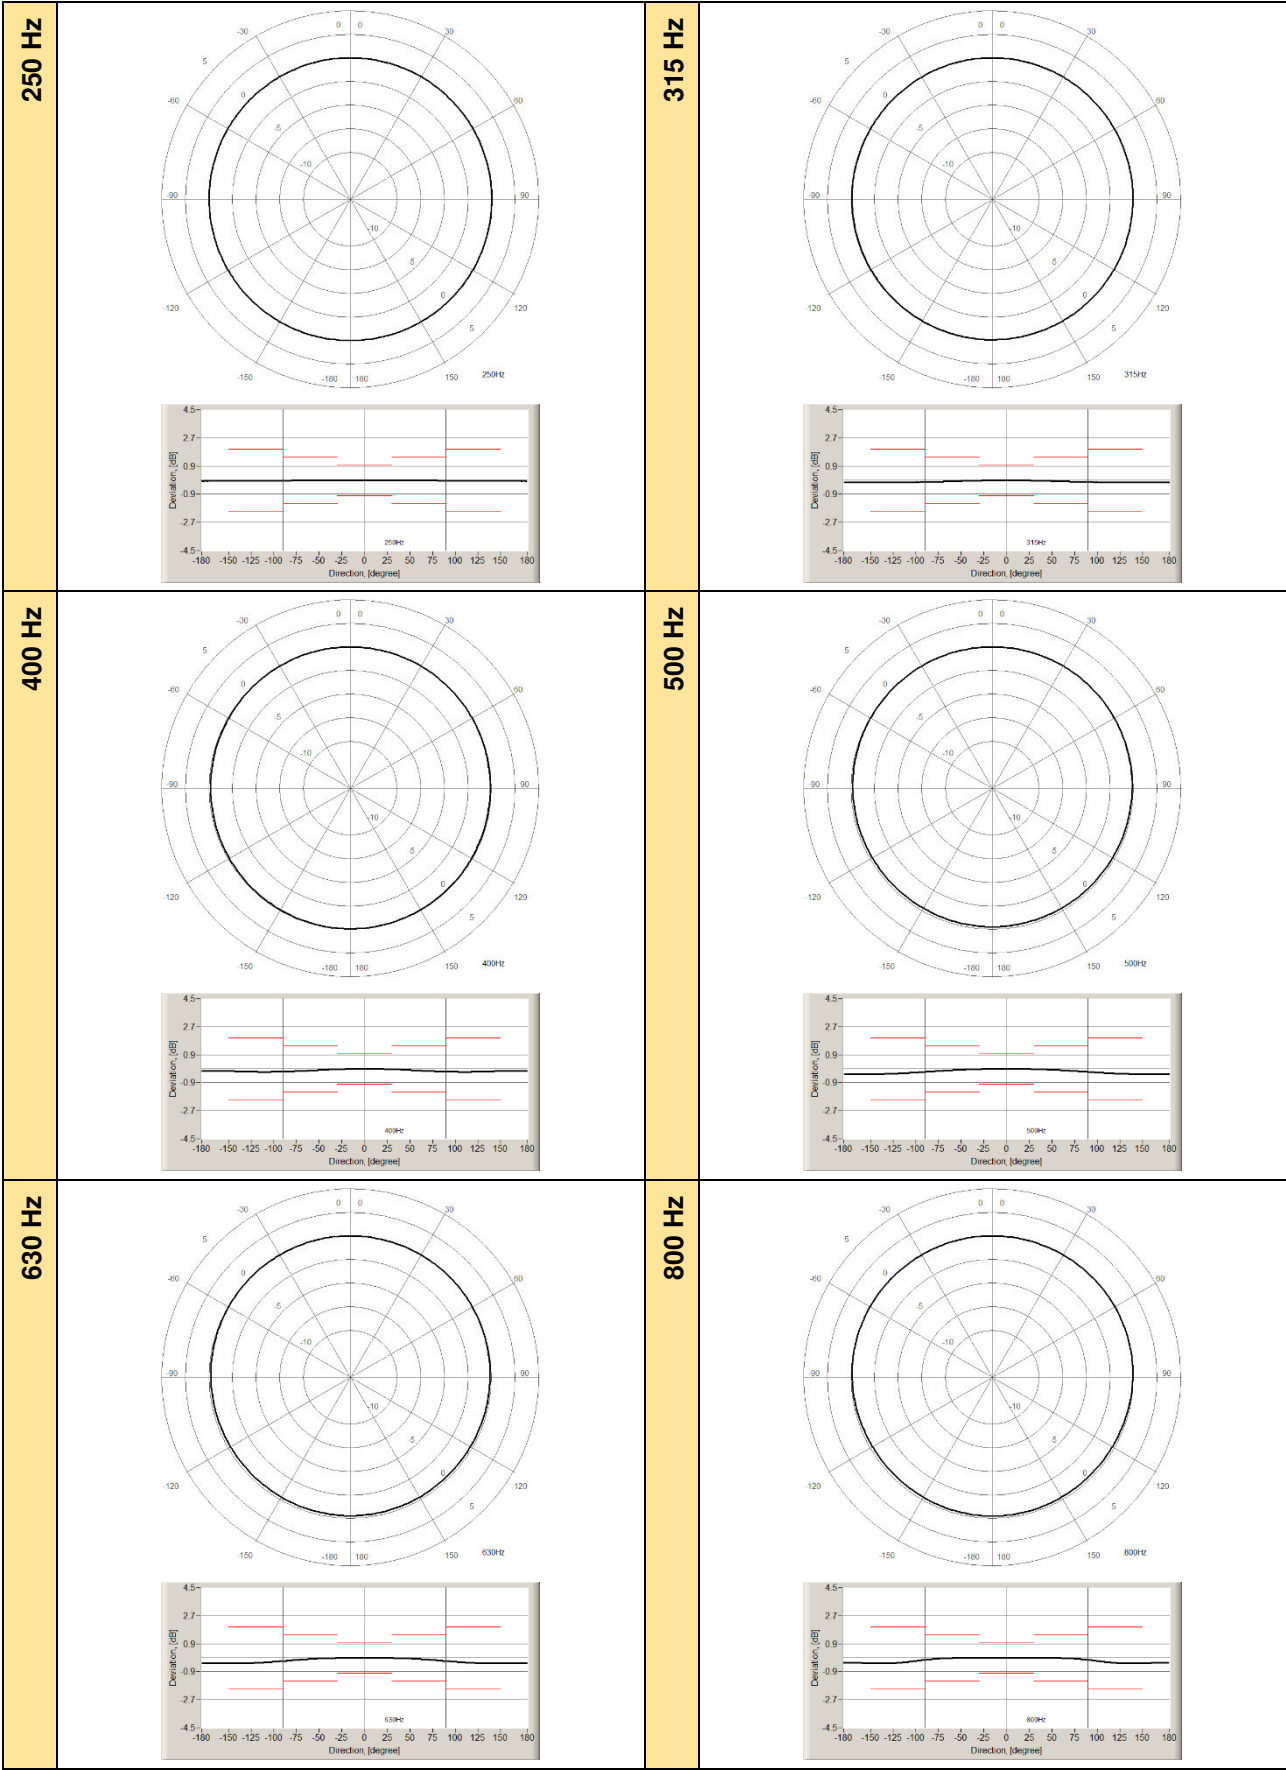

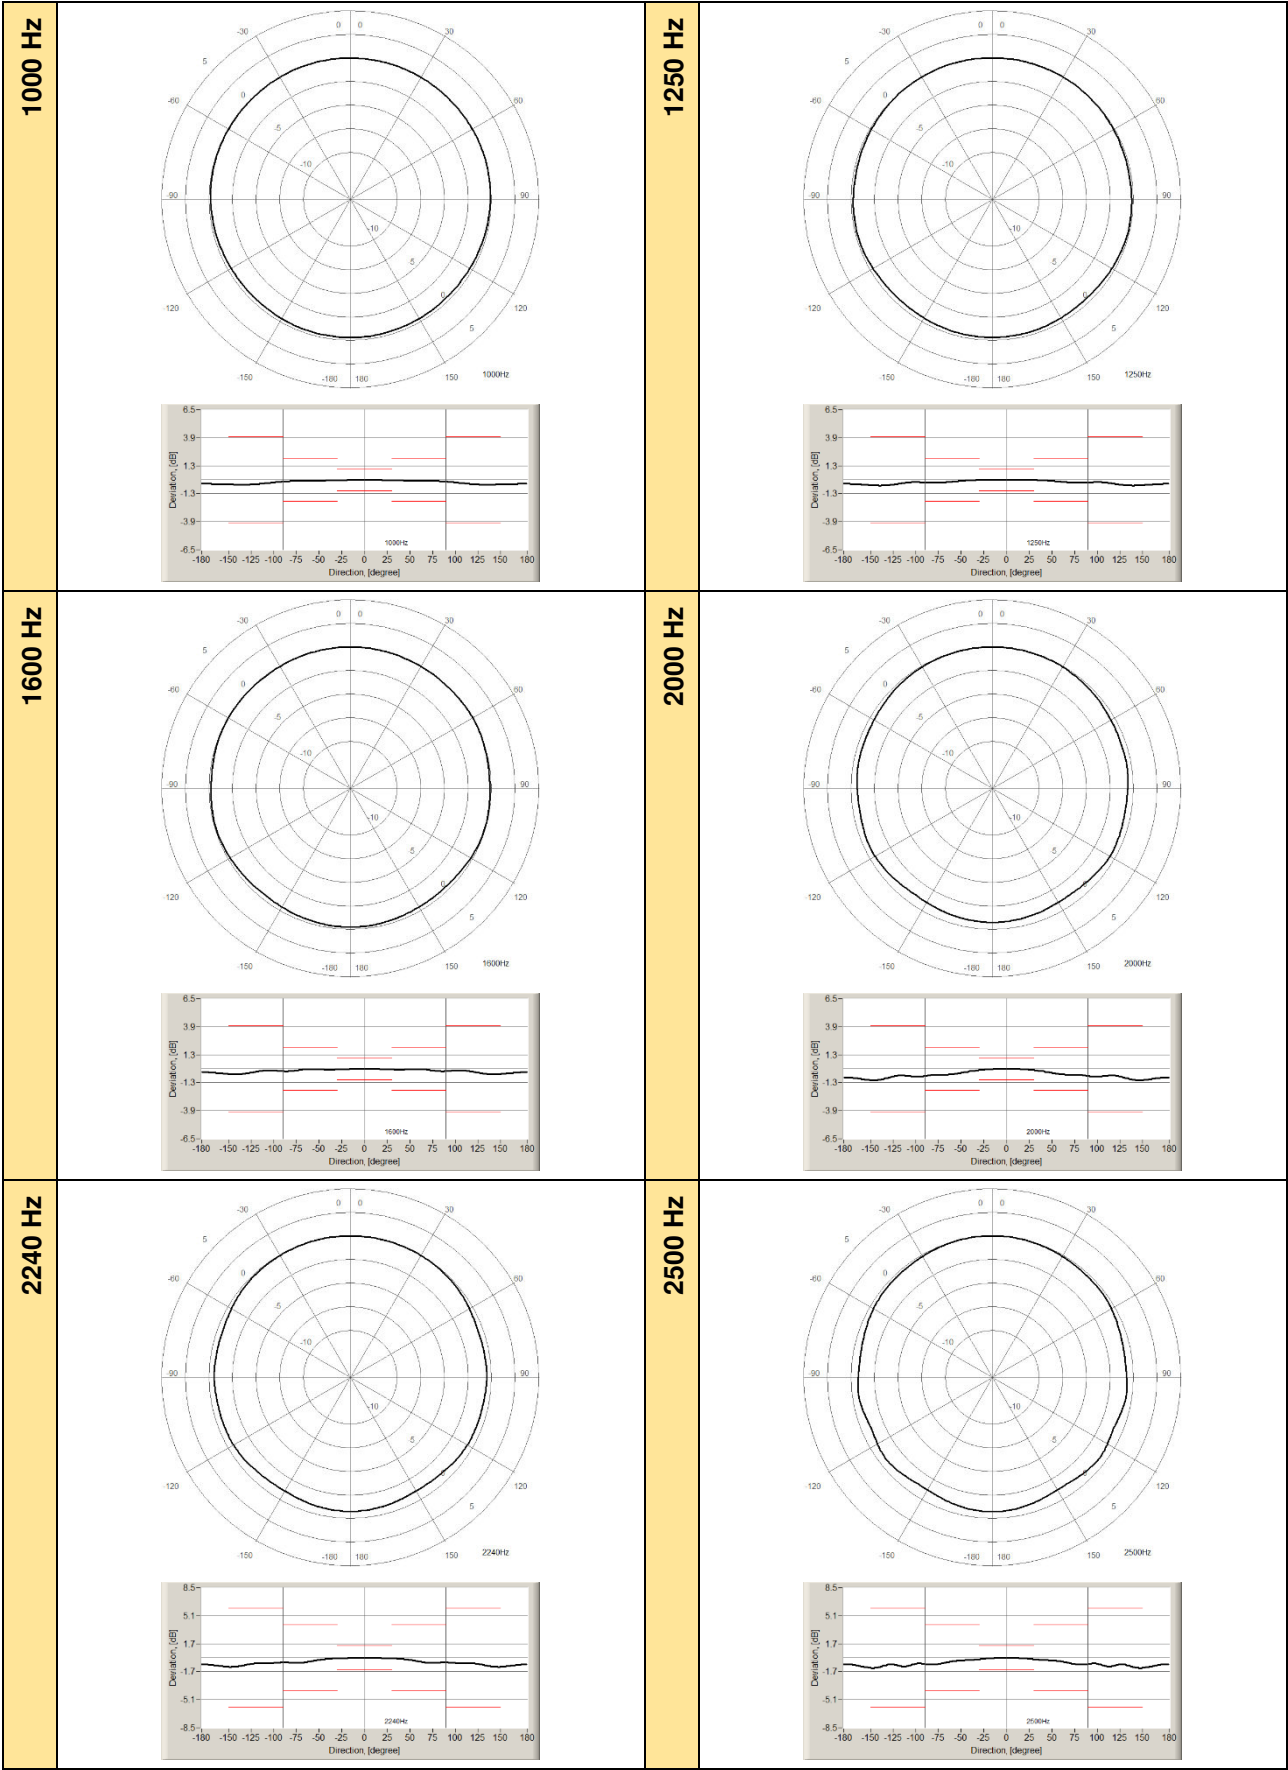

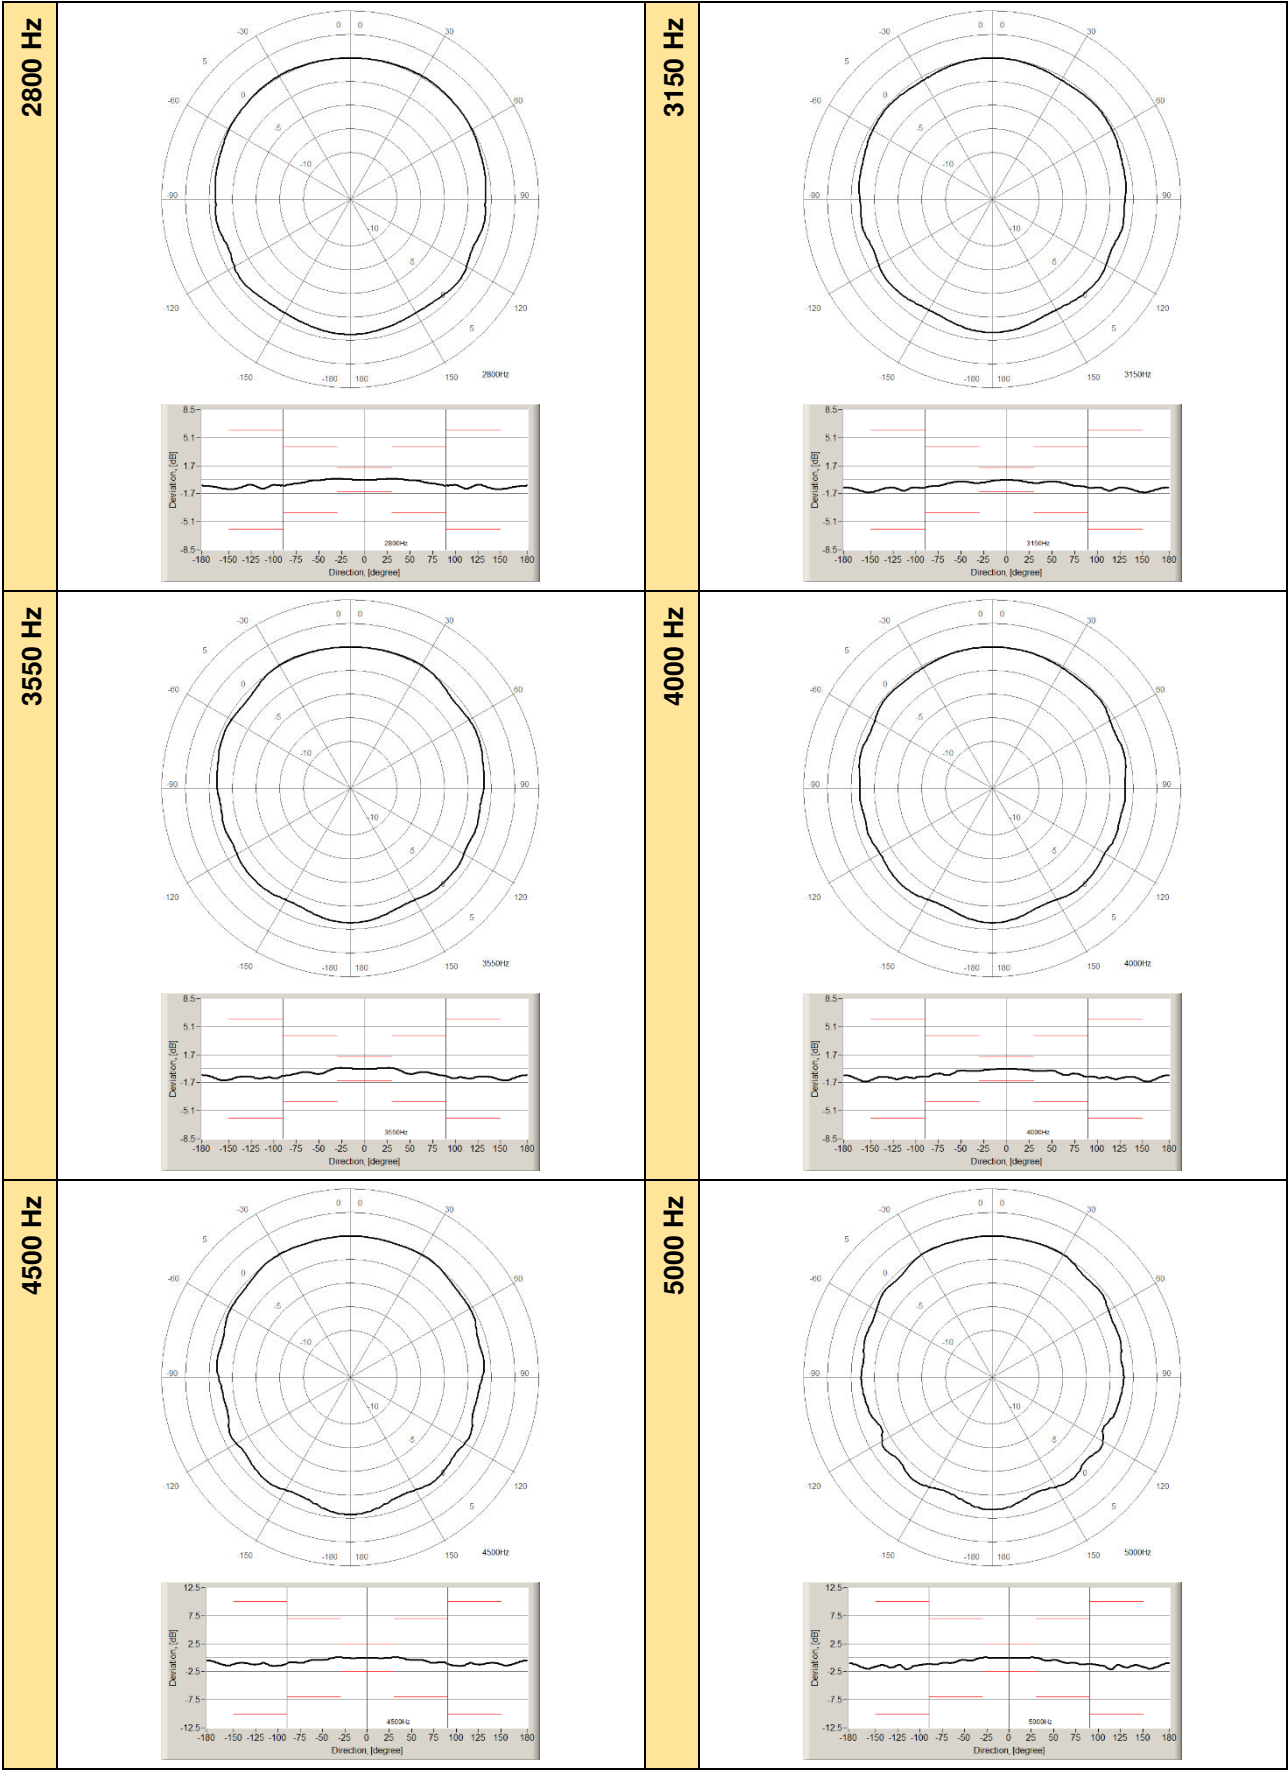

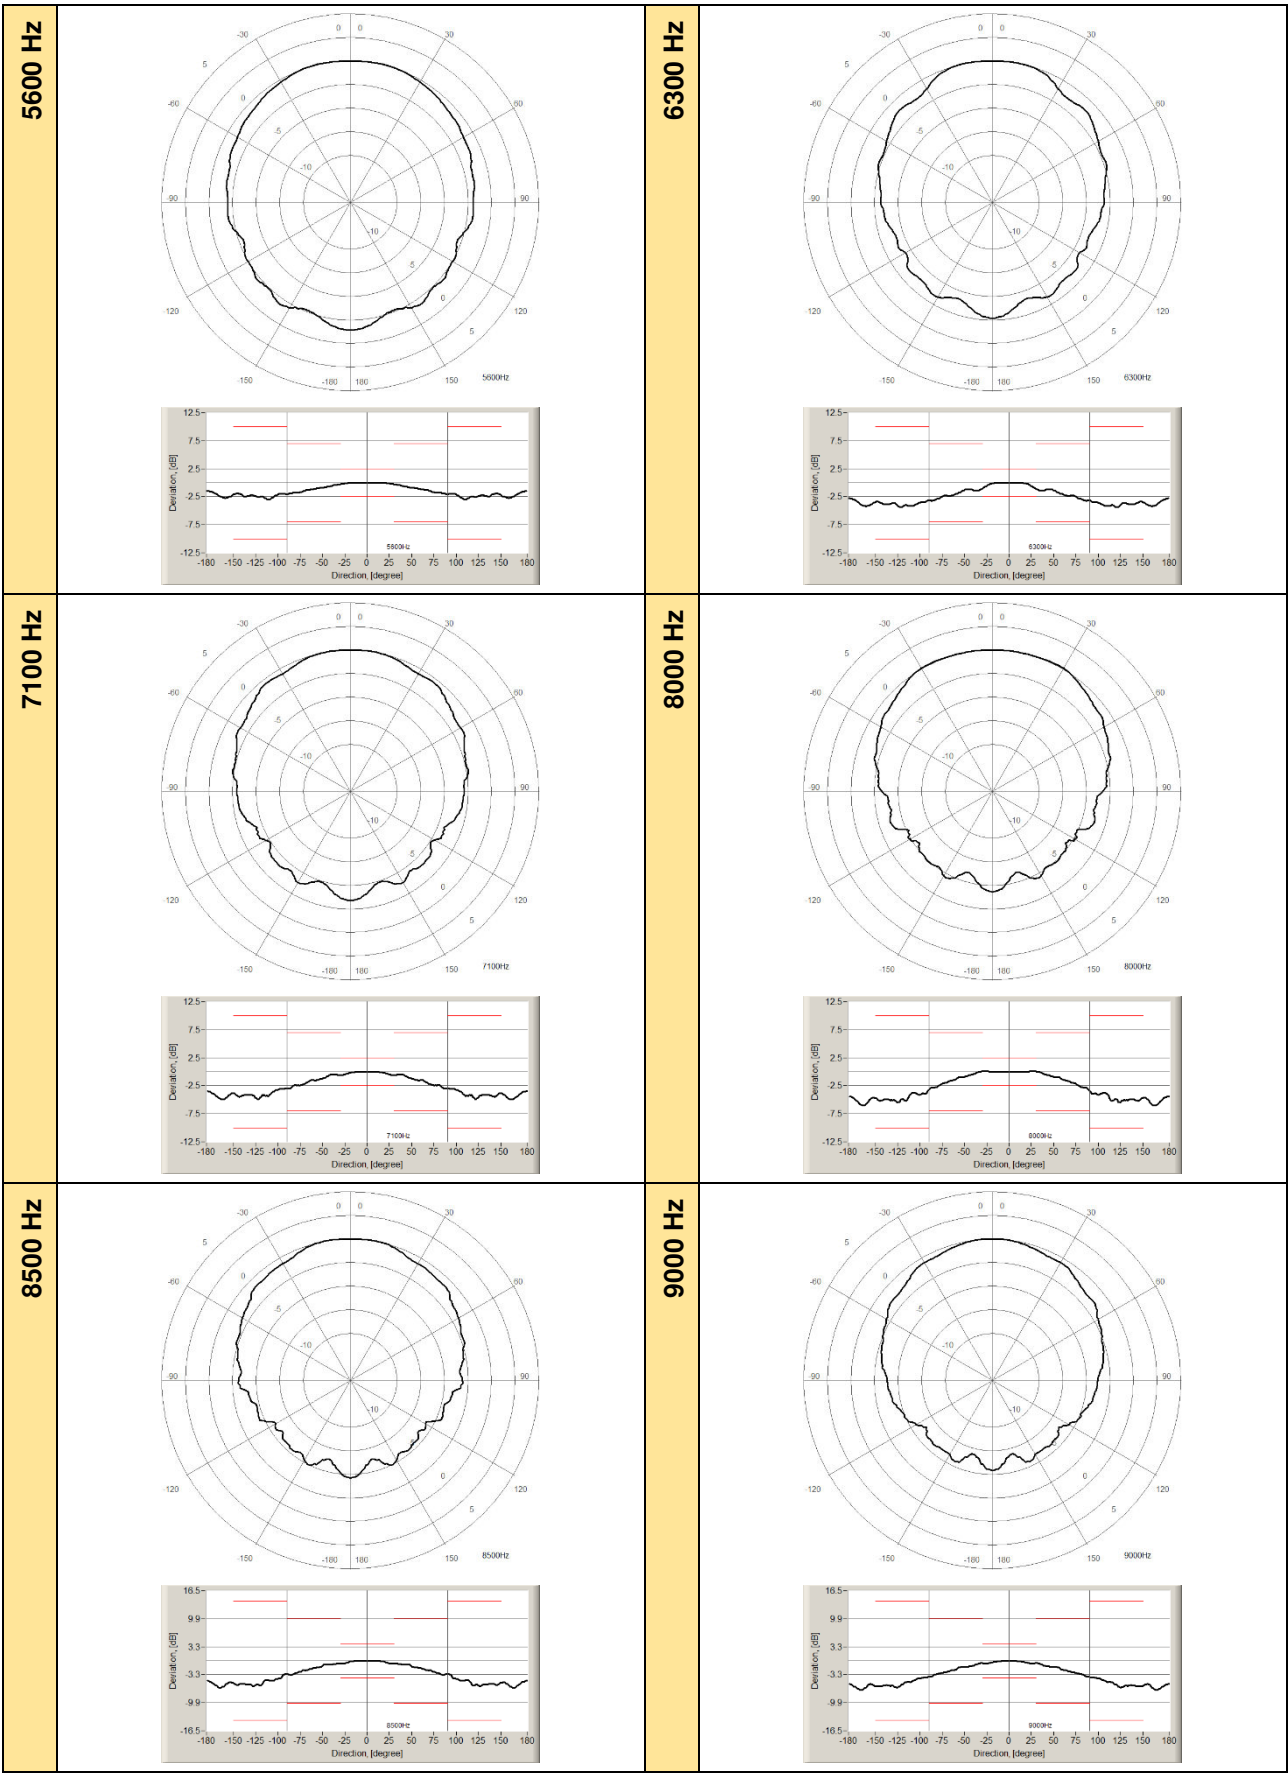

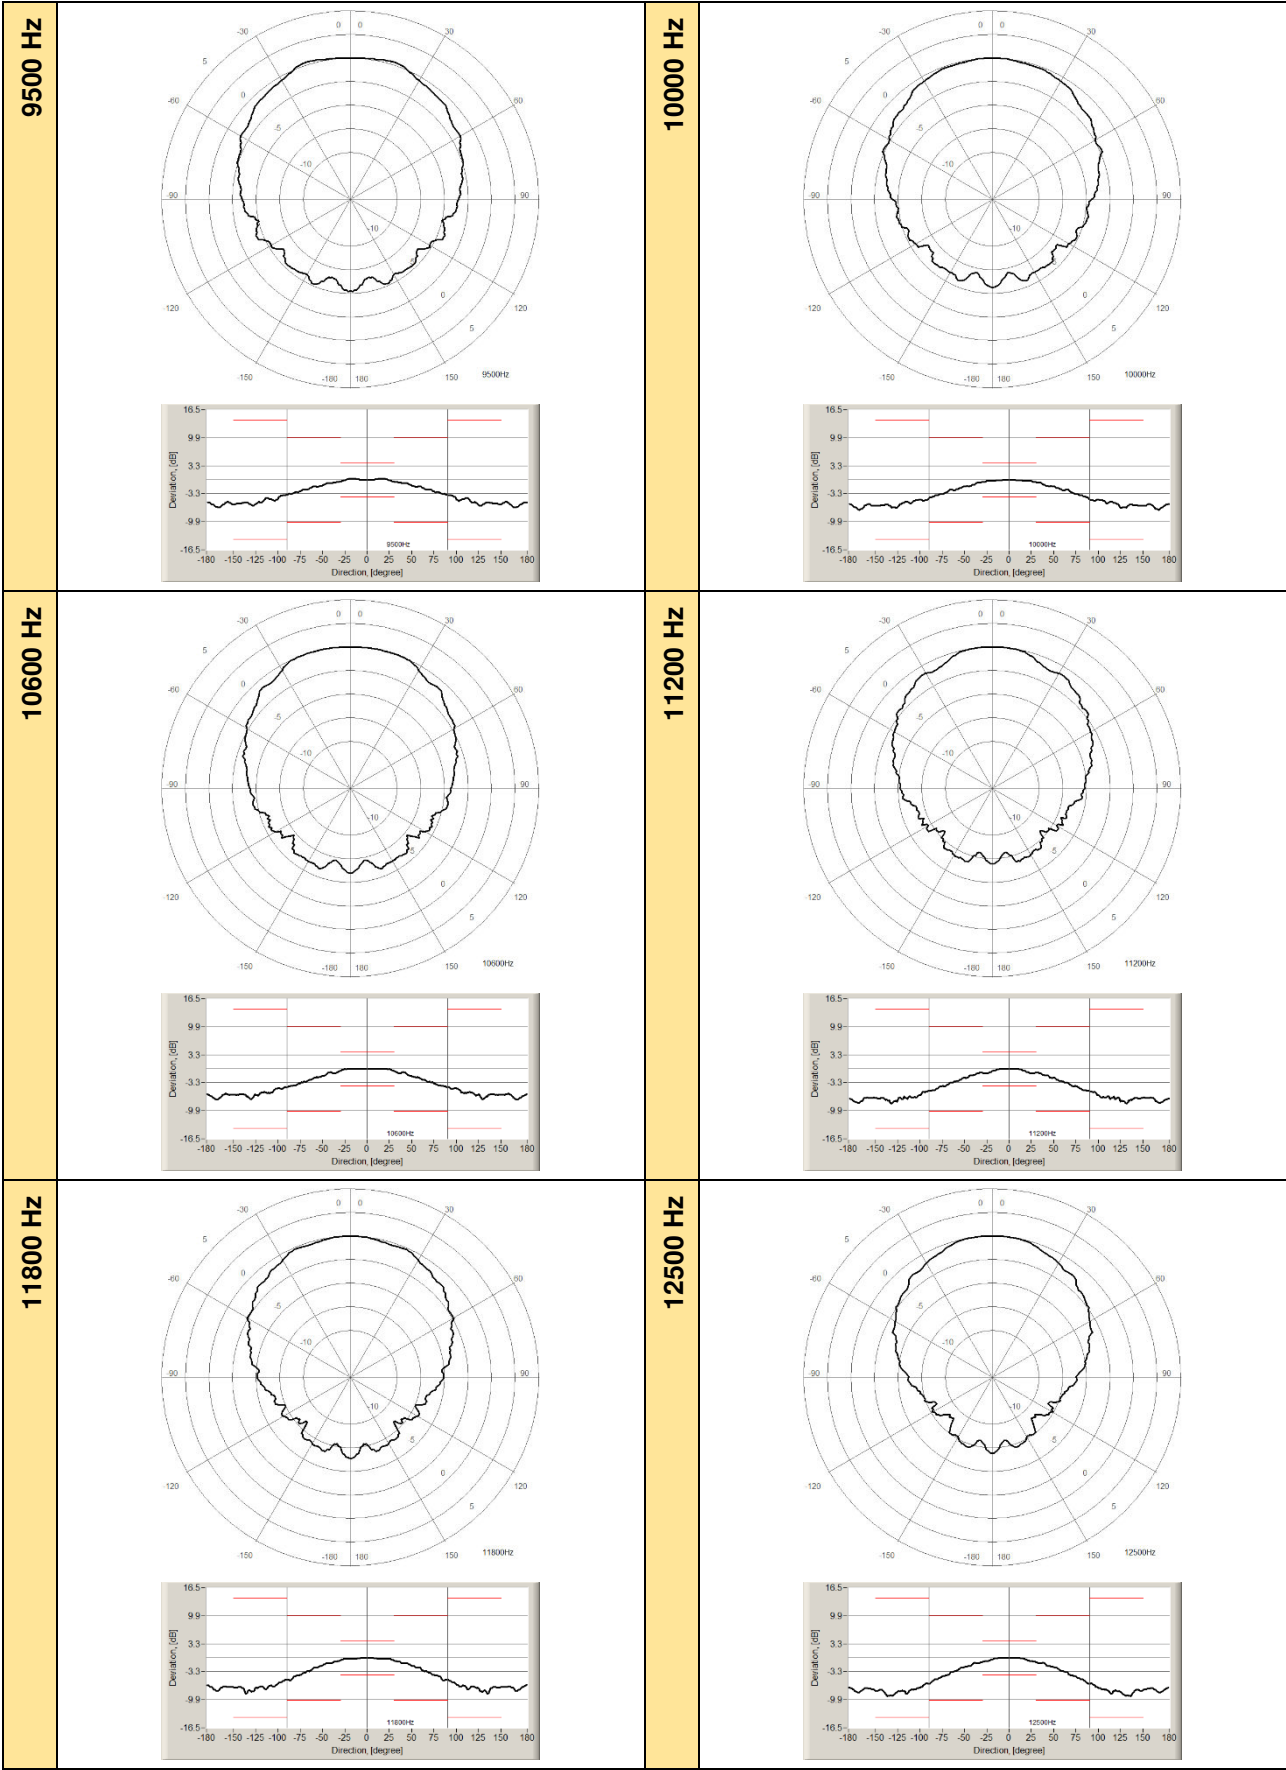


Table C.1.11. Typical directional response of SV 971A with the SA 22 windscreen

f [Hz]	Angle [°]									
	0-10	10-20	20-30	30-40	40-50	50-60	60-70	70-80	80-90	90-100
250	0.01	0.02	0.02	0.01	0.00	0.00	-0.01	-0.01	-0.01	-0.02
315	0.02	0.02	0.03	0.02	0.02	0.01	-0.03	-0.05	-0.06	-0.08
400	-0.01	-0.01	-0.03	-0.04	-0.07	-0.10	-0.13	-0.16	-0.18	-0.19
500	0.01	0.02	0.02	0.02	-0.01	-0.04	-0.07	-0.11	-0.15	-0.20
630	0.01	0.00	0.01	0.00	-0.01	-0.03	-0.06	-0.09	-0.15	-0.19
800	0.00	0.00	0.00	-0.01	-0.01	-0.01	-0.03	-0.05	-0.09	-0.17
1 000	-0.01	-0.02	-0.03	-0.06	-0.07	-0.07	-0.08	-0.10	-0.14	-0.23
1 250	0.00	-0.01	-0.04	-0.07	-0.14	-0.21	-0.28	-0.30	-0.30	-0.27
1 600	-0.01	-0.03	-0.06	-0.08	-0.08	-0.06	-0.07	-0.18	-0.23	-0.23
2 000	0.01	0.01	-0.04	-0.10	-0.26	-0.42	-0.49	-0.49	-0.58	-0.70
2 240	0.00	-0.01	-0.04	-0.09	-0.17	-0.34	-0.55	-0.56	-0.53	-0.61
2 500	-0.01	-0.07	-0.19	-0.26	-0.32	-0.46	-0.68	-0.83	-0.85	-0.78
2 800	0.03	0.10	0.17	0.17	0.13	0.04	-0.34	-0.39	-0.70	-0.73
3 150	-0.04	-0.20	-0.35	-0.35	-0.19	-0.23	-0.55	-0.66	-0.86	-0.97
3 550	0.02	0.09	0.14	-0.20	-0.62	-0.61	-0.42	-0.66	-0.84	-1.14
4 000	0.01	-0.06	-0.19	-0.26	-0.25	-0.65	-0.70	-0.62	-0.87	-0.99
4 500	-0.04	-0.05	0.08	-0.11	-0.35	-0.41	-0.72	-0.91	-1.01	-1.40
5 000	0.01	0.09	0.17	-0.32	-0.37	-0.67	-0.83	-1.10	-1.10	-1.17
5 600	0.03	-0.06	-0.22	-0.59	-0.80	-1.13	-1.51	-1.76	-1.94	-2.29
6 300	0.03	-0.30	-1.08	-1.33	-1.36	-2.08	-2.33	-2.86	-3.17	-3.66
7 100	-0.01	-0.28	-0.50	-0.47	-1.30	-1.49	-2.23	-2.37	-2.96	-3.13
8 000	0.10	0.23	0.24	-0.31	-0.65	-1.12	-1.84	-2.58	-3.31	-4.10
8 500	-0.01	-0.39	-0.75	-0.86	-1.42	-1.85	-2.22	-2.87	-3.28	-4.09
9 000	-0.11	-0.50	-0.55	-1.14	-1.44	-2.04	-2.69	-3.13	-3.87	-4.43
9 500	0.11	0.34	-0.45	-0.74	-1.36	-1.64	-2.39	-2.91	-3.50	-4.75
10 000	-0.14	-0.22	-0.66	-1.48	-1.61	-2.61	-3.34	-4.05	-5.11	-5.28
10 600	0.03	0.04	-0.71	-0.98	-1.89	-2.49	-2.99	-3.88	-4.76	-4.96
11 200	-0.04	-0.84	-0.99	-1.56	-2.09	-3.05	-3.97	-4.96	-5.35	-6.39
11 800	-0.08	-0.28	-0.57	-1.08	-1.93	-2.47	-3.46	-4.34	-5.08	-6.25
12 500	-0.07	-0.55	-1.03	-1.55	-2.35	-3.35	-4.27	-5.03	-6.18	-7.48
f [Hz]	100-110	110-120	120-130	130-140	140-150	150-160	160-170	170-180	180-190	190-200
250	-0.02	-0.02	-0.01	-0.01	-0.02	-0.03	-0.04	-0.05	-0.07	-0.06
315	-0.09	-0.10	-0.11	-0.12	-0.12	-0.12	-0.13	-0.13	-0.14	-0.15
400	-0.20	-0.20	-0.19	-0.18	-0.17	-0.15	-0.14	-0.13	-0.13	-0.13
500	-0.24	-0.28	-0.31	-0.33	-0.34	-0.35	-0.35	-0.35	-0.35	-0.35
630	-0.25	-0.29	-0.33	-0.35	-0.35	-0.35	-0.35	-0.35	-0.35	-0.36
800	-0.23	-0.31	-0.35	-0.37	-0.37	-0.36	-0.34	-0.32	-0.32	-0.33
1 000	-0.32	-0.40	-0.45	-0.46	-0.46	-0.43	-0.41	-0.38	-0.37	-0.39
1 250	-0.30	-0.42	-0.52	-0.55	-0.54	-0.49	-0.43	-0.38	-0.39	-0.44
1 600	-0.16	-0.23	-0.36	-0.50	-0.51	-0.50	-0.42	-0.34	-0.34	-0.40
2 000	-0.73	-0.67	-0.73	-1.01	-1.10	-1.09	-0.97	-0.87	-0.82	-0.91
2 240	-0.65	-0.64	-0.81	-1.02	-1.09	-1.09	-0.99	-0.86	-0.86	-1.00
2 500	-1.04	-1.08	-0.88	-1.17	-1.26	-1.24	-1.03	-0.82	-0.85	-1.05
2 800	-0.94	-1.12	-0.75	-0.99	-1.16	-1.15	-1.01	-0.79	-0.75	-0.94
3 150	-1.14	-1.25	-1.00	-1.23	-1.51	-1.55	-1.36	-0.98	-1.05	-1.38
3 550	-1.11	-1.17	-1.03	-1.01	-1.38	-1.47	-1.29	-0.89	-0.97	-1.27
4 000	-1.07	-1.19	-1.19	-1.01	-1.46	-1.58	-1.36	-0.96	-1.01	-1.45
4 500	-1.44	-1.16	-1.31	-1.16	-1.22	-1.46	-1.29	-0.68	-0.80	-1.26
5 000	-1.86	-1.99	-1.66	-1.70	-1.64	-1.99	-1.94	-1.17	-1.40	-1.93
5 600	-2.95	-2.85	-2.53	-2.45	-2.20	-2.71	-2.65	-1.68	-2.05	-2.73
6 300	-4.10	-4.38	-4.19	-3.81	-3.62	-4.22	-4.22	-3.07	-3.43	-4.16
7 100	-4.42	-4.93	-4.67	-4.28	-4.26	-4.80	-4.80	-3.72	-4.41	-5.02
8 000	-3.90	-5.23	-5.58	-5.18	-5.28	-5.80	-6.03	-4.92	-5.43	-6.05
8 500	-4.86	-5.94	-6.26	-5.72	-5.81	-6.13	-6.34	-5.52	-5.93	-6.33
9 000	-5.09	-6.09	-6.38	-6.05	-6.08	-6.84	-7.05	-5.82	-6.88	-6.96
9 500	-4.96	-5.40	-6.05	-5.57	-5.66	-5.85	-6.51	-5.77	-6.47	-6.57
10 000	-5.95	-6.39	-7.01	-6.17	-6.17	-6.23	-7.28	-6.50	-6.97	-6.97
10 600	-6.29	-5.87	-7.44	-6.65	-6.27	-6.59	-7.31	-6.76	-7.15	-7.15
11 200	-6.98	-7.34	-8.40	-8.40	-7.06	-7.10	-8.09	-7.47	-8.12	-8.12
11 800	-7.25	-7.62	-8.28	-8.34	-7.00	-6.91	-7.62	-7.37	-8.03	-7.92
12 500	-8.14	-8.74	-9.25	-9.31	-7.71	-7.29	-8.09	-7.73	-8.34	-8.24

f [Hz]	200-210	210-220	220-230	230-240	240-250	250-260	260-270	270-280	280-290	290-300
250	-0.07	-0.06	-0.06	-0.06	-0.06	-0.05	-0.05	-0.04	-0.02	-0.01
315	-0.15	-0.16	-0.16	-0.16	-0.17	-0.17	-0.16	-0.16	-0.15	-0.14
400	-0.14	-0.16	-0.17	-0.18	-0.19	-0.19	-0.19	-0.18	-0.17	-0.15
500	-0.35	-0.35	-0.35	-0.34	-0.33	-0.31	-0.28	-0.24	-0.21	-0.17
630	-0.37	-0.37	-0.38	-0.38	-0.37	-0.35	-0.30	-0.27	-0.21	-0.16
800	-0.35	-0.36	-0.37	-0.37	-0.36	-0.31	-0.24	-0.16	-0.08	-0.05
1 000	-0.41	-0.44	-0.44	-0.44	-0.41	-0.35	-0.25	-0.19	-0.13	-0.11
1 250	-0.50	-0.53	-0.52	-0.46	-0.34	-0.23	-0.22	-0.25	-0.25	-0.21
1 600	-0.49	-0.54	-0.54	-0.47	-0.34	-0.15	-0.23	-0.25	-0.24	-0.11
2 000	-1.03	-1.08	-1.06	-0.92	-0.64	-0.79	-0.81	-0.75	-0.64	-0.63
2 240	-1.12	-1.13	-1.09	-0.90	-0.72	-0.72	-0.68	-0.63	-0.65	-0.65
2 500	-1.22	-1.23	-1.04	-0.95	-1.06	-0.94	-0.77	-0.81	-0.79	-0.64
2 800	-1.11	-1.13	-1.08	-0.70	-1.22	-1.20	-0.77	-0.80	-0.61	-0.45
3 150	-1.49	-1.43	-1.19	-1.18	-1.37	-1.18	-1.08	-0.99	-0.83	-0.71
3 550	-1.39	-1.29	-0.98	-1.20	-1.25	-1.13	-1.16	-0.89	-0.79	-0.52
4 000	-1.50	-1.29	-1.08	-1.29	-1.24	-1.20	-1.07	-1.03	-0.78	-0.81
4 500	-1.37	-1.16	-1.09	-1.20	-1.40	-1.53	-1.39	-0.94	-0.92	-0.77
5 000	-1.94	-1.50	-1.86	-1.94	-2.19	-1.61	-1.40	-1.35	-1.24	-1.14
5 600	-2.72	-2.32	-2.44	-2.51	-3.01	-2.83	-2.10	-2.12	-1.84	-1.35
6 300	-4.10	-3.90	-3.93	-4.46	-4.27	-4.10	-3.56	-3.27	-2.76	-2.44
7 100	-4.69	-4.70	-4.25	-5.16	-4.50	-3.76	-3.20	-3.00	-2.65	-2.13
8 000	-5.31	-5.17	-5.13	-5.56	-5.30	-4.21	-4.00	-3.14	-2.55	-1.96
8 500	-5.29	-5.59	-5.81	-5.79	-5.31	-4.72	-4.33	-3.47	-2.98	-2.33
9 000	-6.08	-5.96	-6.06	-6.46	-5.13	-4.56	-3.93	-3.59	-2.87	-2.44
9 500	-5.99	-5.79	-6.01	-6.24	-5.18	-5.12	-4.09	-3.44	-3.07	-2.32
10 000	-6.18	-6.19	-7.03	-6.59	-5.68	-5.43	-4.82	-3.80	-3.24	-2.36
10 600	-6.30	-6.32	-7.34	-6.99	-6.40	-5.79	-4.57	-4.12	-3.82	-3.24
11 200	-7.14	-7.23	-8.27	-7.62	-7.08	-6.66	-5.74	-5.30	-4.34	-3.58
11 800	-7.14	-7.41	-8.50	-7.50	-7.64	-6.71	-5.86	-5.47	-4.28	-3.35
12 500	-7.79	-8.37	-9.09	-8.34	-8.26	-7.25	-6.71	-5.81	-4.67	-3.79
f [Hz]	300-310	310-320	320-330	330-340	340-350	350-360				
250	-0.01	0.01	0.01	0.00	0.01	0.01				
315	-0.12	-0.10	-0.08	-0.05	-0.02	-0.01				
400	-0.12	-0.09	-0.06	-0.04	-0.02	0.00				
500	-0.14	-0.11	-0.08	-0.06	-0.04	-0.01				
630	-0.12	-0.07	-0.05	-0.03	-0.02	0.00				
800	-0.02	-0.01	-0.01	-0.01	-0.01	0.00				
1 000	-0.11	-0.10	-0.08	-0.06	-0.03	-0.01				
1 250	-0.14	-0.07	-0.02	0.01	0.01	0.00				
1 600	-0.06	-0.09	-0.09	-0.08	-0.05	-0.01				
2 000	-0.61	-0.49	-0.33	-0.19	-0.10	-0.04				
2 240	-0.50	-0.30	-0.16	-0.09	-0.05	-0.01				
2 500	-0.41	-0.32	-0.28	-0.17	-0.07	-0.01				
2 800	-0.26	-0.12	0.08	0.09	0.04	-0.01				
3 150	-0.38	-0.43	-0.45	-0.40	-0.22	-0.05				
3 550	-0.68	-0.62	-0.18	0.07	0.04	-0.01				
4 000	-0.59	-0.34	-0.35	-0.29	-0.13	-0.03				
4 500	-0.44	-0.42	0.06	-0.06	-0.06	-0.03				
5 000	-0.83	-0.67	-0.47	-0.06	-0.06	-0.03				
5 600	-1.12	-0.90	-0.50	-0.27	0.05	0.02				
6 300	-1.90	-1.42	-1.50	-0.65	-0.10	-0.01				
7 100	-1.68	-1.04	-0.75	-0.72	-0.15	0.00				
8 000	-1.31	-1.03	-0.53	-0.16	-0.15	-0.06				
8 500	-1.67	-1.02	-0.86	-0.65	-0.14	0.02				
9 000	-1.75	-1.51	-0.87	-0.66	-0.37	-0.04				
9 500	-1.66	-1.25	-0.69	-0.34	0.21	0.04				
10 000	-1.98	-1.53	-0.67	-0.30	-0.23	-0.08				
10 600	-2.05	-1.50	-1.04	-0.05	-0.05	0.01				
11 200	-2.71	-2.32	-1.42	-1.25	-0.49	-0.06				
11 800	-2.51	-1.61	-1.10	-0.55	-0.32	-0.12				
12 500	-2.92	-1.98	-1.31	-0.79	-0.35	-0.01				

C.1.3 Effect of the SA 271A outdoor microphone kit

See Chapter C.5 for the details related to using of the SA 271A outdoor microphone kit.

C.1.4 Effect of Vibration

1. Mechanical vibration with an acceleration of 1 m/s^2 perpendicular to the membrane of the microphone for the frequencies 31.5 Hz, 63 Hz, 125 Hz, 250 Hz, 500 Hz, 630 Hz, 800 Hz and 1000 Hz increases the low level of the linear operation range according to the Table C.1.12.
2. Mechanical vibration with an acceleration of 1 m/s^2 parallel to the membrane of the microphone for the frequencies 31.5 Hz, 63 Hz, 125 Hz, 250 Hz, 500 Hz, 630 Hz, 800 Hz and 1000 Hz increases the low level of the linear operation range according to the Table C.1.13.

Test conditions:

SV 971A with microphone and preamplifier is mounted on the shaker.

Ref 1. Vibration is applied in a direction perpendicular to the plane of the microphone diaphragm.

Ref 2. Vibration is applied in a direction parallel to the plane of the microphone diaphragm.

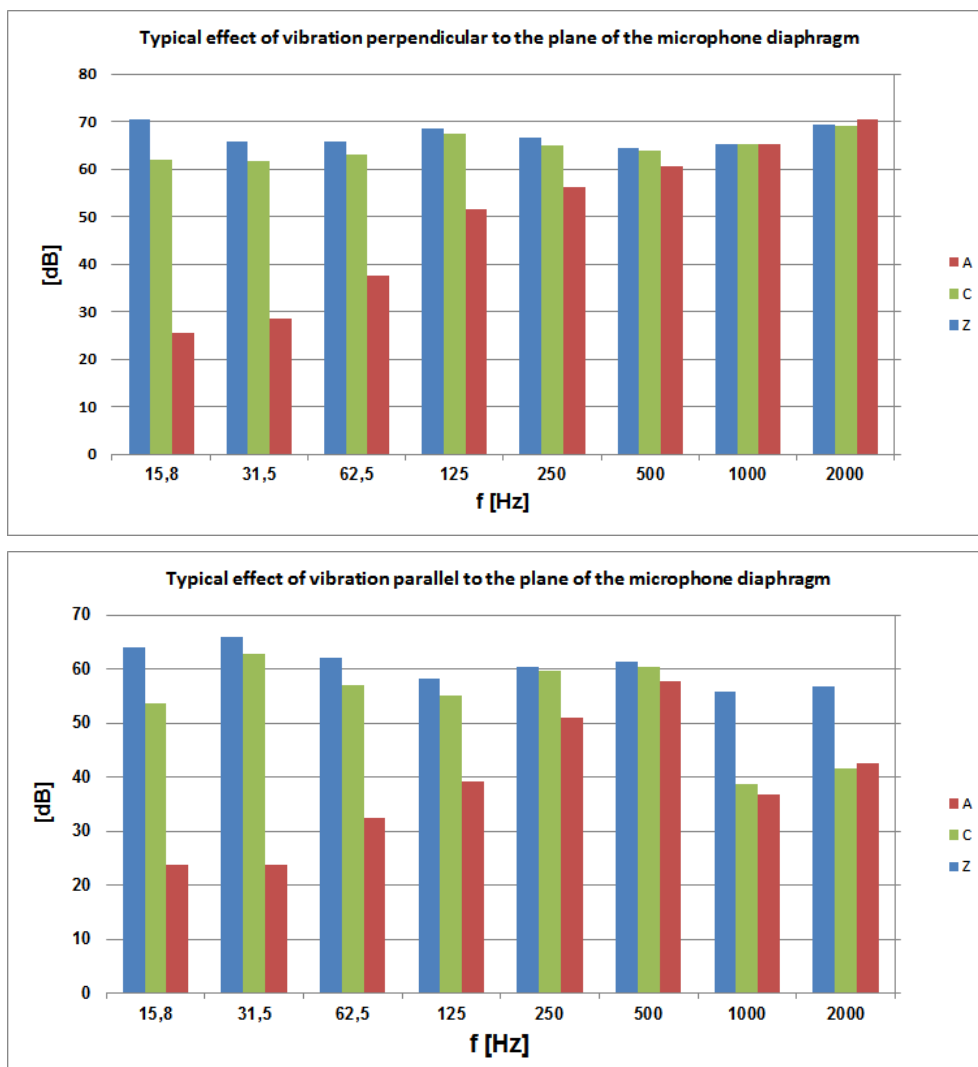


Table C.1.12. Typical effect of vibration perpendicular to the plane of the microphone diaphragm

f (Hz) [dB]	15.6	31.25	62.5	125	250	500	1000	2000
A filter	25.6	28.5	37.4	51.6	56.3	60.7	65.4	70.4
C filter	62.0	61.8	63.2	67.6	64.9	64.0	65.3	69.0
Z filter	70.5	65.7	65.8	68.5	66.6	61.3	65.3	69.3

Table C.1.13. Typical effect of vibration parallel to the plane of the microphone diaphragm

f (Hz) [dB]	15.6	31.25	62.5	125	250	500	1000	2000
A filter	23.8	23.7	32.4	39.3	50.9	57.8	36.9	42.6
C filter	53.6	62.7	57.1	55.0	59.6	60.4	38.7	41.7
Z filter	64.1	65.8	62.1	58.3	60.4	61.4	55.7	56.7

C.2 SPECIFICATION OF SV 971A AS 1/1 OCTAVE AND 1/3 OCTAVE ANALYSER

C.2.1 Specification of SV 971A as 1/1 and 1/3 octave analyser in the standard configuration

Statement of performance

SV 971A can operate as 1/1 octave or 1/3 octave analyser with all listed below accessories meeting requirements of the IEC 61260-1:2014 standard for the pass band filters for the Class 1 Group X instruments.



Note: Simultaneously to the frequency analysis SV 971A operates as a Sound Level Meter - see Chapters C.1 for specification.

Configuration of the complete analyser

SV 971A	sound level meter and analyser
SV 18A	microphone preamplifier
ST 03	adapter (input impedance 18 pF)

Normal operating mode

SV 971A in configuration with the **SV 18A** microphone preamplifier and **ST 03** adapter with following settings: **Normal** or **Low** measurement range (path: <Menu> / *Measurement* / *Range* – see Chapter 4.6), **Microphone** compensation – **Off**, **Field Compensation** – **Off**, **Windscreen** compensation – **Off** (path: <Menu> / *Measurement* / *Compensation Filter* – see Chapter 4.7).



Note: When the 1/1 or 1/3 octave analyser is used with the microphone installed (for acoustic signals), the **Microphone** compensation must be set to **On** (path: <Menu> / *Measurement* / *Compensation Filter*) – see Chapter 4.7.

Signal input

- SV 18A preamplifier throughout the ST 03 adapter
- Maximum input voltage: SV 971A meets the requirements of IEC 348 for the class 2 devices. The input voltage shall not exceed the limits between -10 V and +10 V.
- Impedance: 18 pF

Digital Filters

Weighting filters

- A** meeting requirements of IEC 61672-1:2013 for the Class 1 “A” filters
- C** meeting requirements of IEC 61672-1:2013 for the Class 1 “C” filters
- Z** meeting requirements of IEC 61672-1:2013 for the Class 1 “Z” filters
- B** meeting IEC651 for the Class 1 filters

See Chapter C.3 for the A, C, B and Z filters characteristics.

1/1 and 1/3 octave filters – see Chapter C.2.2 for filters characteristics.

Linear operating ranges

Two measurement ranges are available: **Normal** and **Low**

Table C.2.1. Linear operating range (with SV 18A preamplifier, ST 03 adapter)

Range	Linear operating range (with 10 dB margin from noise) (RMS for the sinusoidal signal at reference conditions @ 1 kHz, 0.0 dB calibration factor)	
Normal	from 14.1 μV_{RMS} "A"-weighting	to 4.467 V_{RMS} "A"-weighting
	from 14.1 μV_{RMS} "B"-weighting	to 4.467 V_{RMS} "B"-weighting
	from 14.1 μV_{RMS} "C"-weighting	to 4.467 V_{RMS} "C"-weighting
	from 31.6 μV_{RMS} "Z"-weighting	to 4.467 V_{RMS} "Z"-weighting
Low	from 10 μV_{RMS} "A"-weighting	to 0.891 V_{RMS} "A"-weighting
	from 10 μV_{RMS} "B"-weighting	to 0.891 V_{RMS} "B"-weighting
	from 10 μV_{RMS} "C"-weighting	to 0.891 V_{RMS} "C"-weighting
	from 20 μV_{RMS} "Z"-weighting	to 0.891 V_{RMS} "Z"-weighting

Table C.2.2. Peak for the sinusoidal signal 1 kHz, at reference conditions (with SV 1A8 preamplifier, ST 03 adapter)

Peak for the sinusoidal signal 1 kHz, at reference conditions @ 1 kHz (0.0 dB calibration factor)	
Range	Max Peak value
Normal	6.317 V "A"-weighting
	6.317 V "B"-weighting
	6.317 V "C"-weighting
	6.317 V "Z"-weighting
Low	1.260 V "A"-weighting
	1.260 V "B"-weighting
	1.260 V "C"-weighting
	1.260 V "Z"-weighting

Measuring frequency range

3 Hz ÷ 22.4 kHz with the **Z** filter (-3 dB)

Maximum peak voltage

20 V Peak-Peak (Maximum peak voltage of input sinusoidal signal, which can be lead to the SLM without destruction the meter)

RMS detector

- Digital "True RMS" with Peak detection
- Resolution 0.1 dB
- Range 327.7 dB
- Crest Factor unlimited (for signals in 20 kHz band)

Reference conditions as per IEC 61260-1:2014

- Reference temperature +23°C
- Reference relative humidity 50%
- Static pressure 101.325 kPa

Calibration (electrical)

Calibration level	0.32 V _{RMS} (114 dB re 0.64 µV)
Basic accuracy	< ± 0.2 dB (for the temperature T=+23°C ± 5°C for sinusoidal signal 1 V _{RMS} in the band 5 Hz ÷ 20 kHz with the Z filter)
Measurement deviation	< ± 0.1 dB (in the temperature range from -10°C to +50°C for the sinusoidal signal 1 V _{RMS} in the band 5 Hz ÷ 20 kHz with the Z filter)

Overload detector

The instrument has the built-in overload detectors. Both A/D converter and input amplifier overload conditions are detected. The overload in the measurement channel (in its analogue part) and the overload of the analogue / digital converter are both detected. The “overload” indication appears when the input signal amplitude is 0.5 dB above the declared “Peak measurement range”.

Warm-up time	1 min. (for 0.1 dB accuracy).
Effect of humidity	< 0.5 dB (for 30%<RH<90% at 40°C re Reference conditions).
Effect of temperature	< 0.5 dB (from -10°C to + 50°C)
Effect of magnetic field	< 15 dB (A) or < 25 dB (Z) (for 80 A/m and 50 Hz).
Effect of Vibration	< 0.1 dB (from 20 Hz to 1000 Hz at 1 m/s ²).

Electrostatic and radio frequency criteria – see Chapter C.1.1

Antialiasing filter


Built-in antialiasing filter. Second-order analogue filter, passive Class, combined with on-chip FIR digital filter of the analog-to-digital converter, ensuring correct sampling of the measured signal.

Pass band (-1 dB)	22.200 kHz
Pass band (-3 dB)	23.520 kHz
Stop band	26.256 kHz
Attenuation in the stop band	> 80 dB
Sampling frequency	48 kHz (internal only)
Analogue to digital converter	1 x 24 bit
Reference range	Normal
Input attenuator accuracy	± 0.1 dB (for f = 1 kHz and T = +23°C)
Internal oscillator accuracy	0.01 % (for f = 1 kHz and T = +23°C).


C.2.2 1/1 and 1/3 octave filters characteristics

1/1 octave filters


11 filters with centre frequencies from 16.0 Hz to 16 kHz (base 10), meeting IEC 61260-1:2014 standard for Class 1

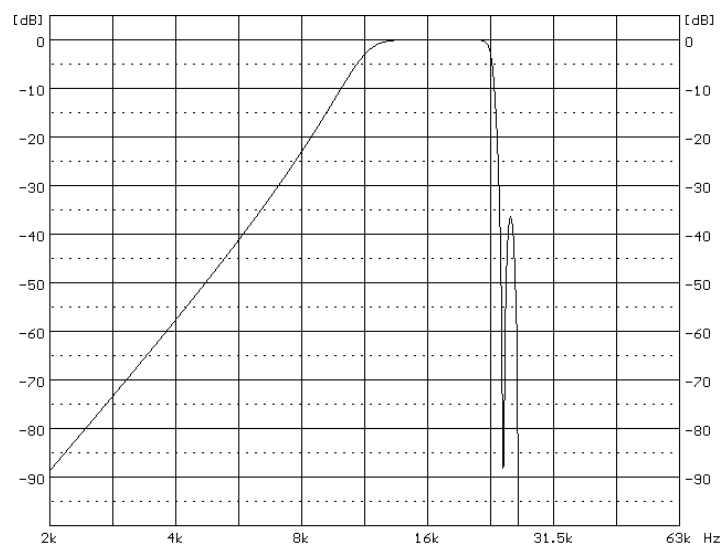


16.0 kHz 1/1 Octave filter (Audio/Full band)

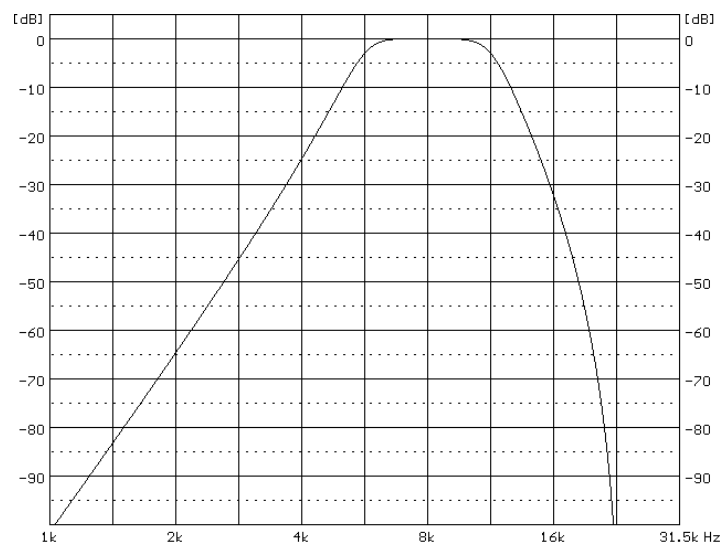


8.0 kHz 1/1 octave filter

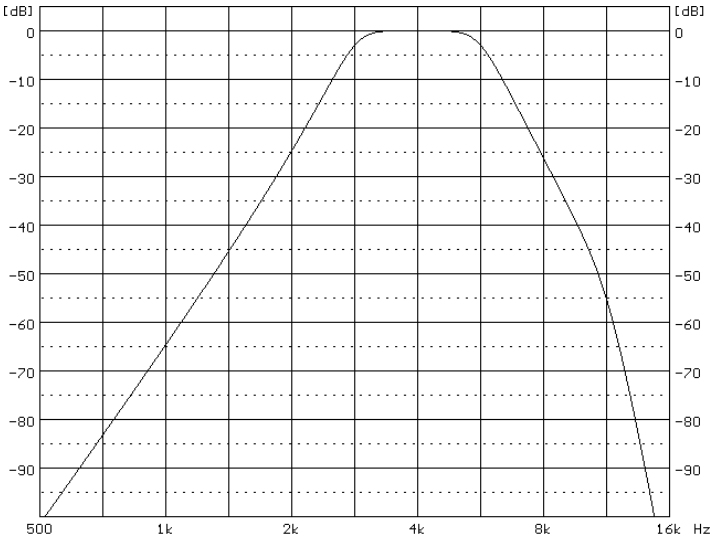


4.0 kHz 1/1 octave filter

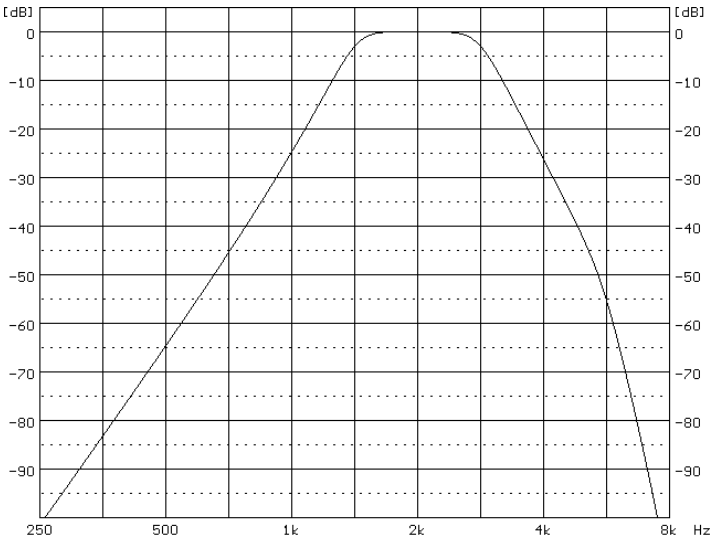


2.0 kHz 1/1 octave filter

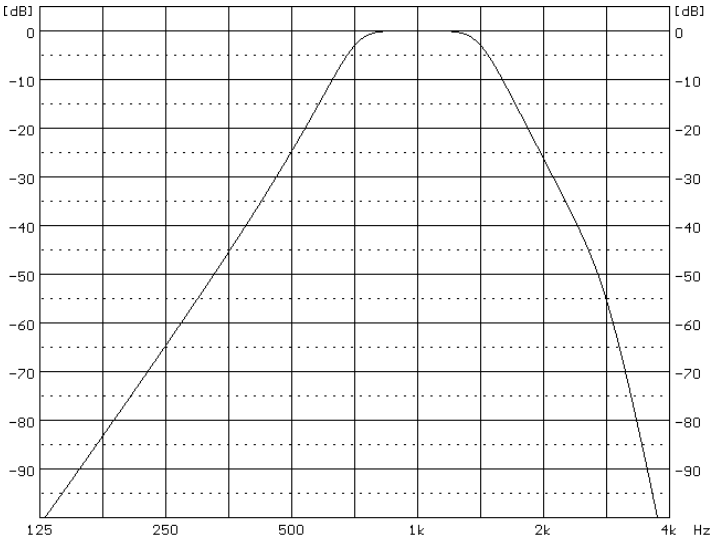


1.0 kHz 1/1 octave filter

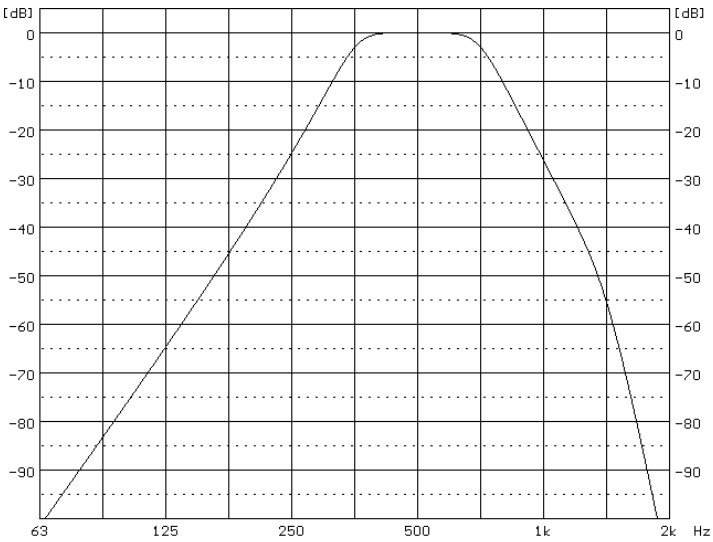


500 Hz 1/1 octave filter

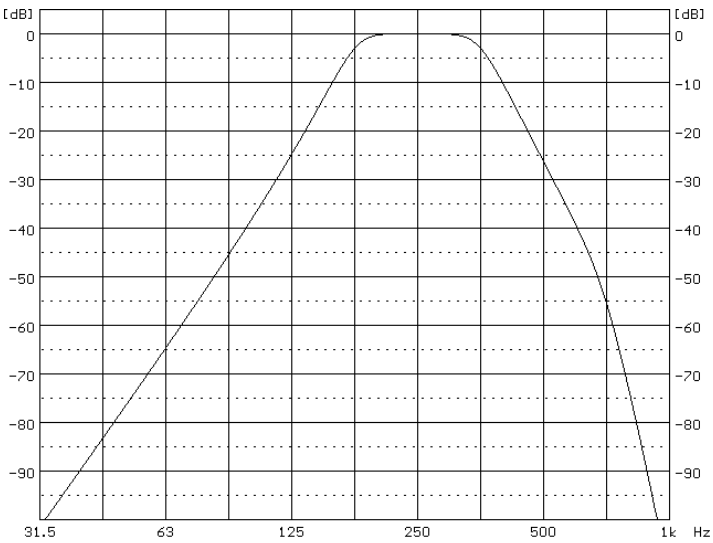


250 Hz 1/1 octave filter

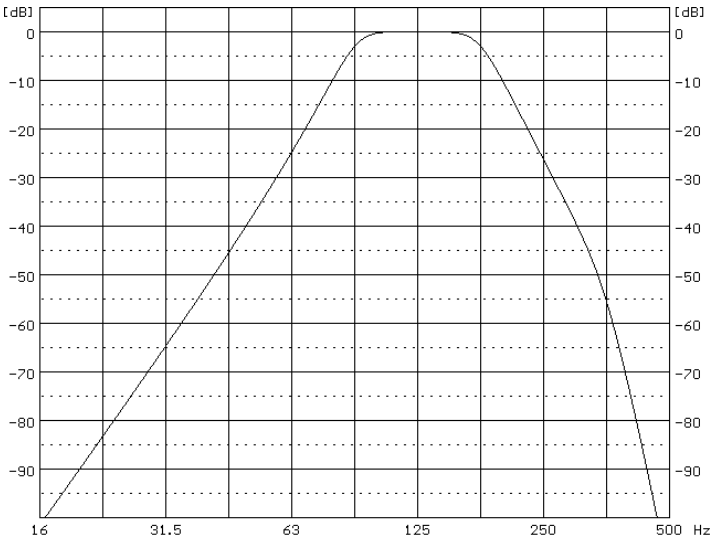


125 Hz 1/1 octave filter

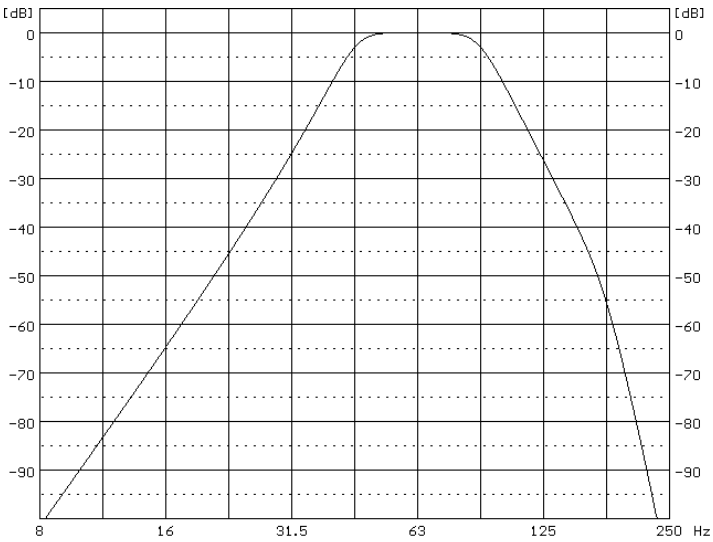

63.0 Hz 1/1 octave filter

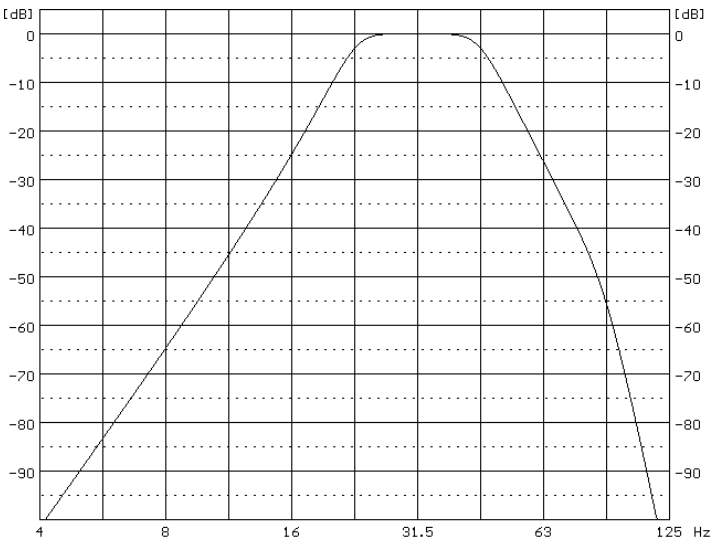


31.5 Hz 1/1 octave filter

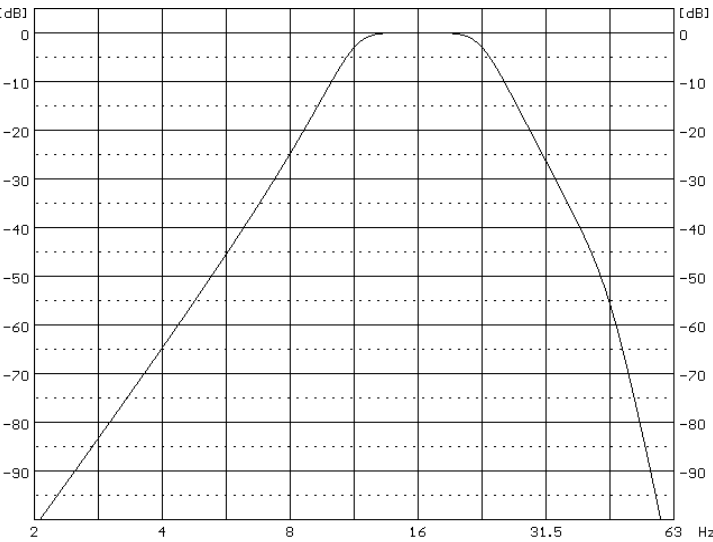


16.0 Hz 1/1 octave filter

1/3 octave filters


35 filters with centre frequencies from 8 Hz to 20 kHz (base 10), meeting IEC 61260-1:2014 standard for Class 1

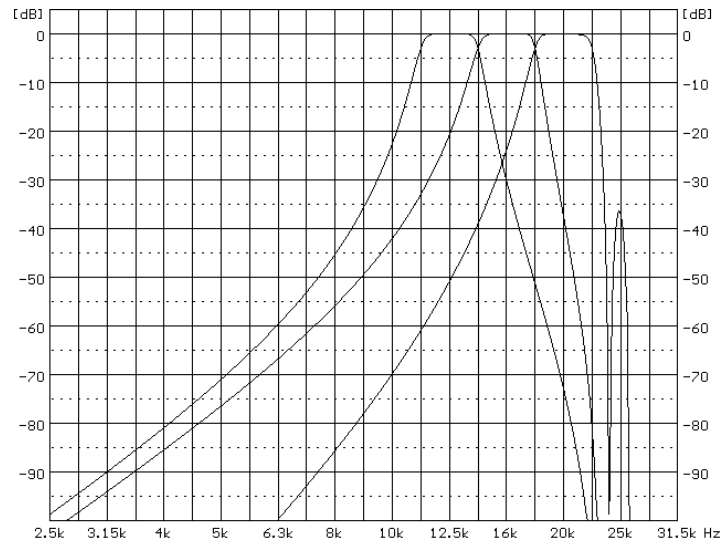


1/3 octave filters for 16.0 kHz 1/1 octave filter

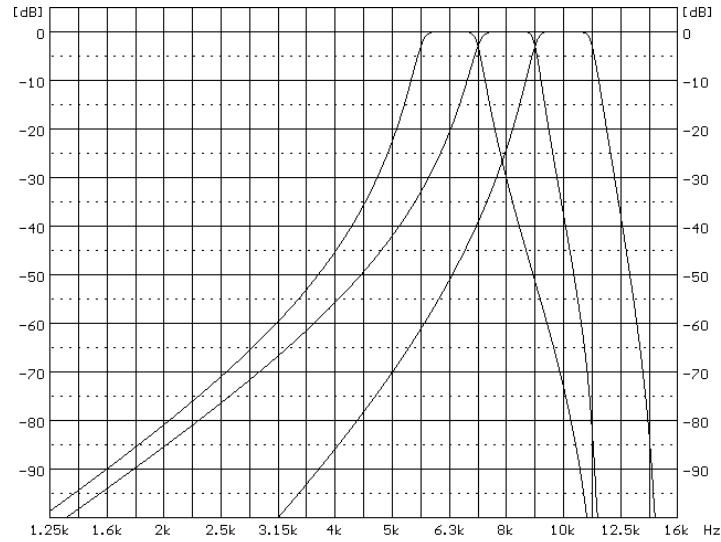


1/3 octave filters for 8.0 kHz 1/1 octave filter

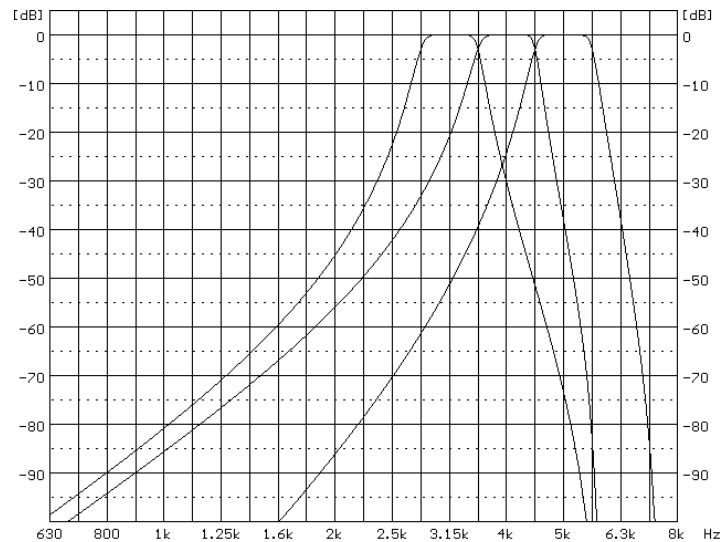


1/3 octave filters for 4.0 kHz 1/1 octave filter

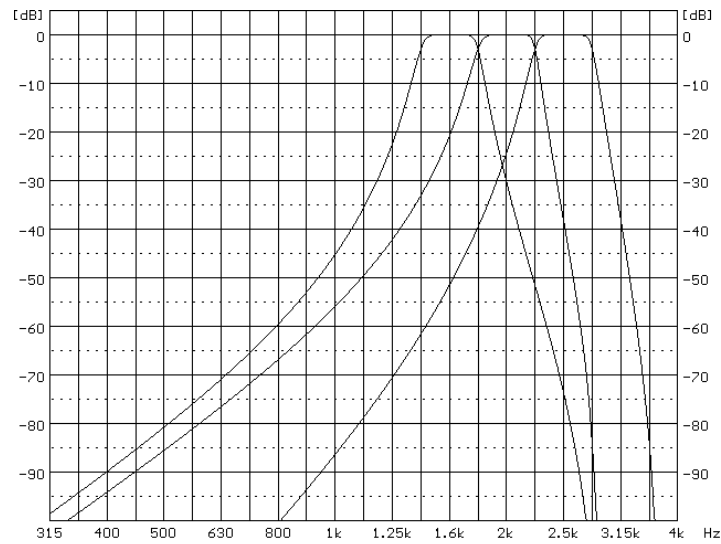


1/3 octave filters for 2.0 kHz 1/1 octave filter

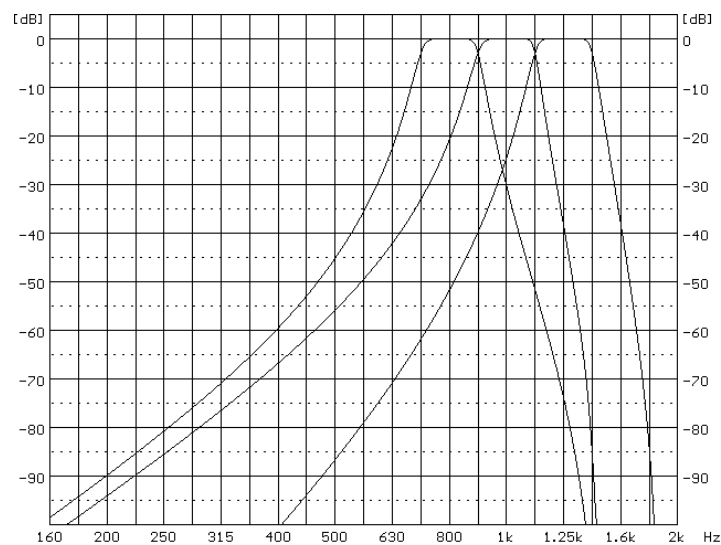


1/3 octave filters for 1.00 kHz 1/1 octave filter

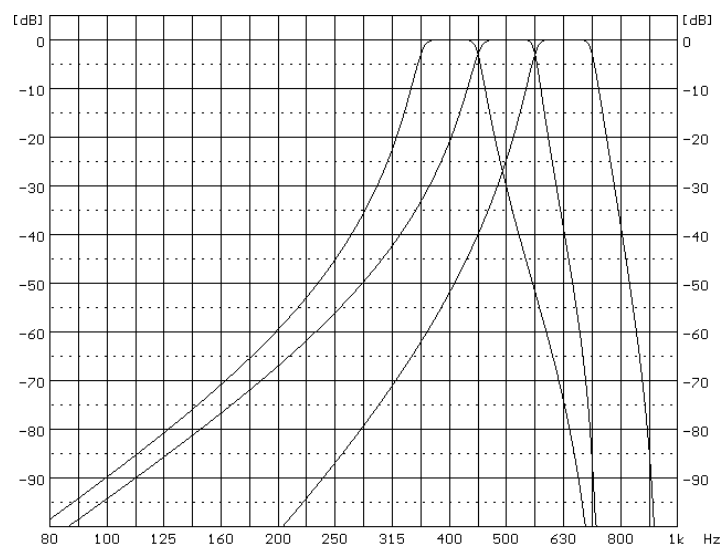


1/3 octave filters for 500 Hz 1/1 octave filter

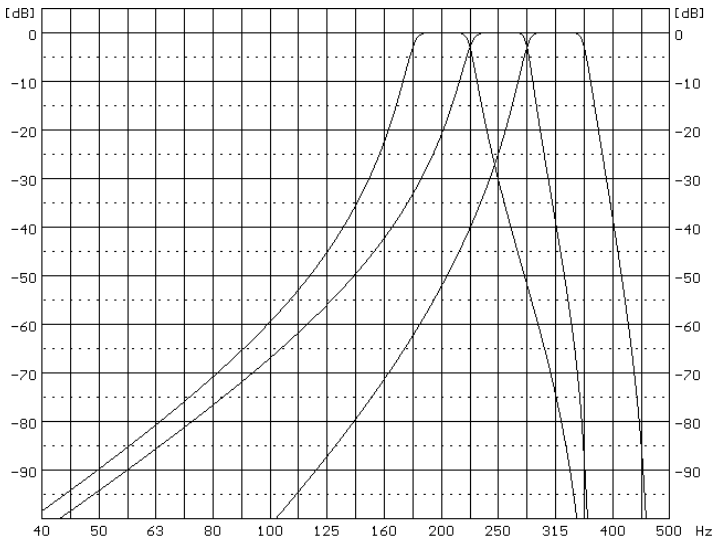


1/3 octave filters for 250 Hz 1/1 octave filter

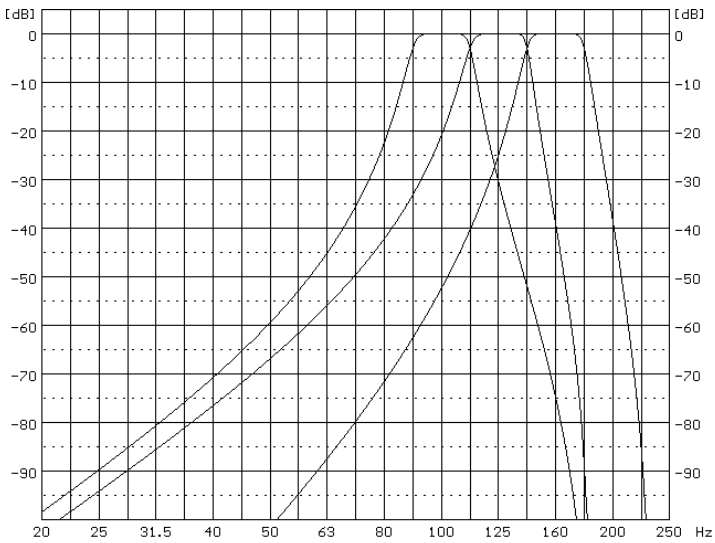


1/3 octave filters for 125 Hz 1/1 octave filter

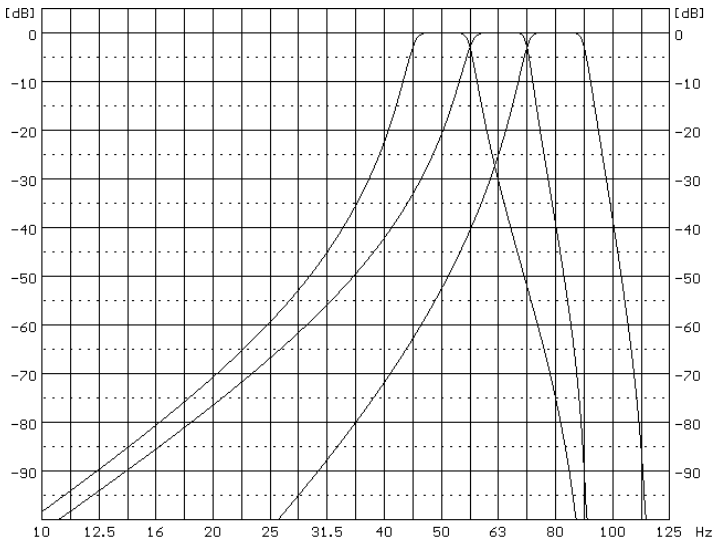


1/3 octave filters for 63.0 Hz 1/1 octave filter

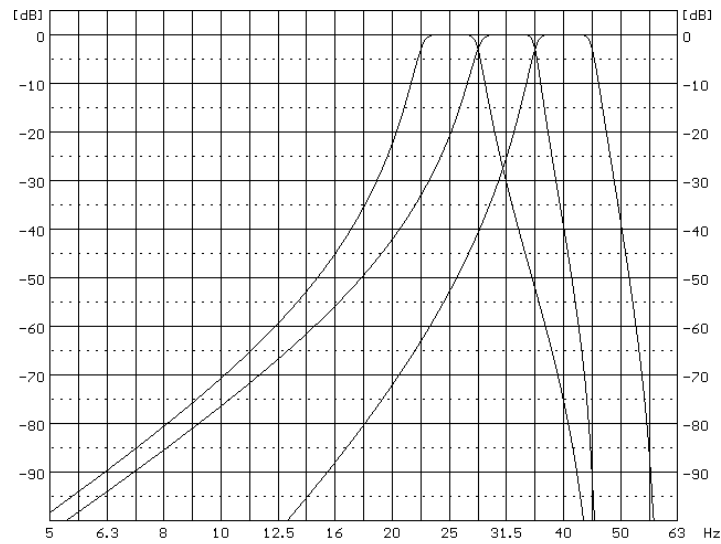

1/3 octave filters for 31.5 Hz 1/1 octave filter

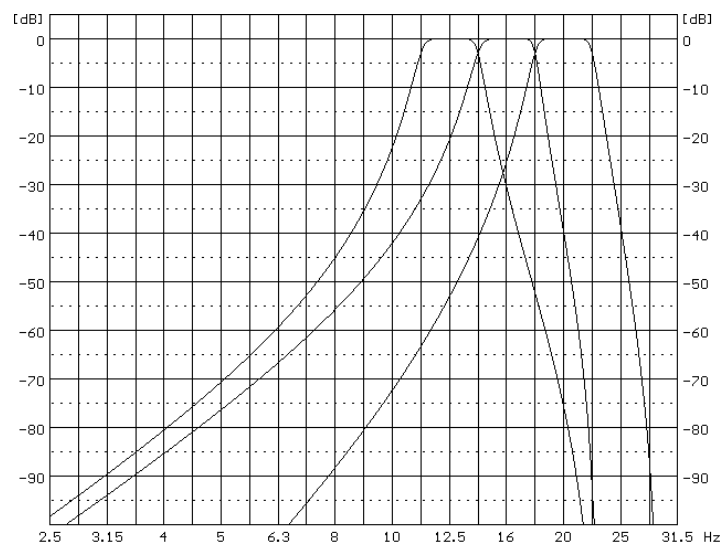



1/3 octave filters for 16.0 Hz 1/1 octave filter

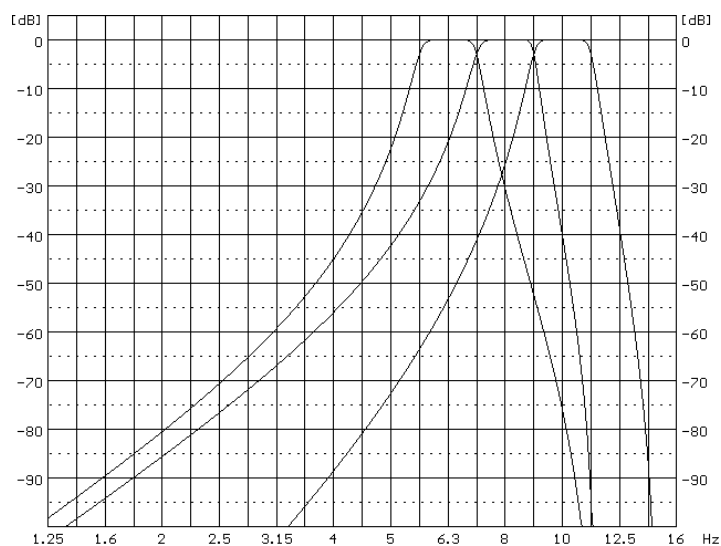

1/3 octave filters for 8.00 Hz 1/1 octave filter


1/1 and 1/3 octave filters noise levels

Typical electrical noise floor for SV 971A in configuration with the SV 18A microphone preamplifier, ST 03 adapter and 50 Ohm BNC terminal (Z weighted) for 1/1 and 1/3 octave filters.

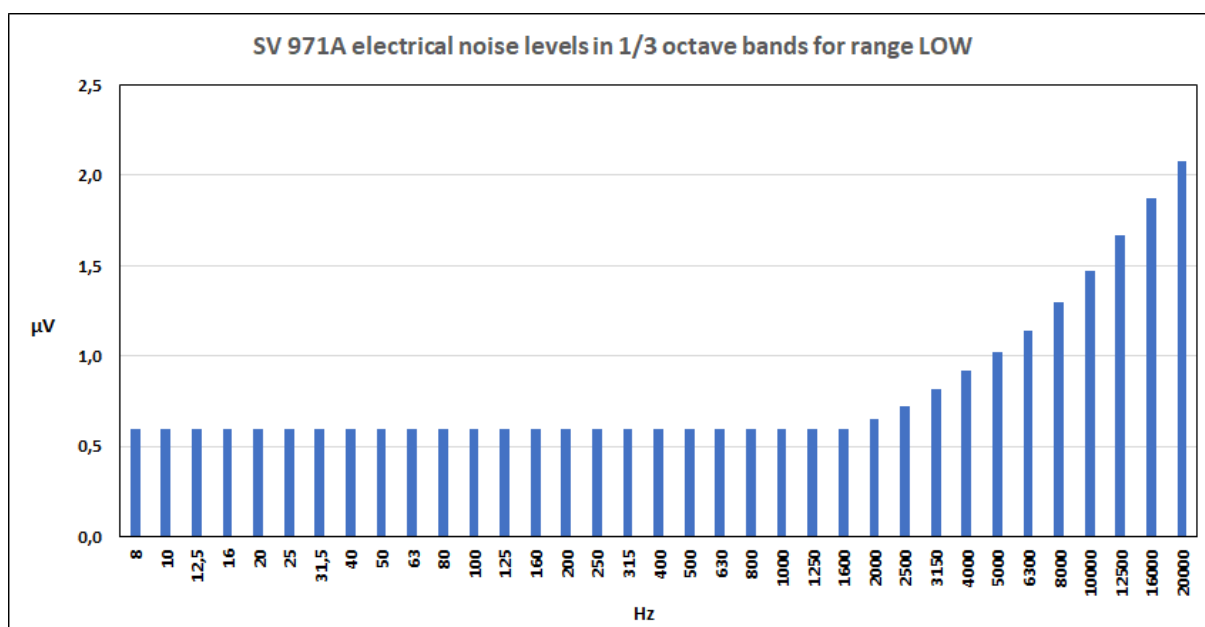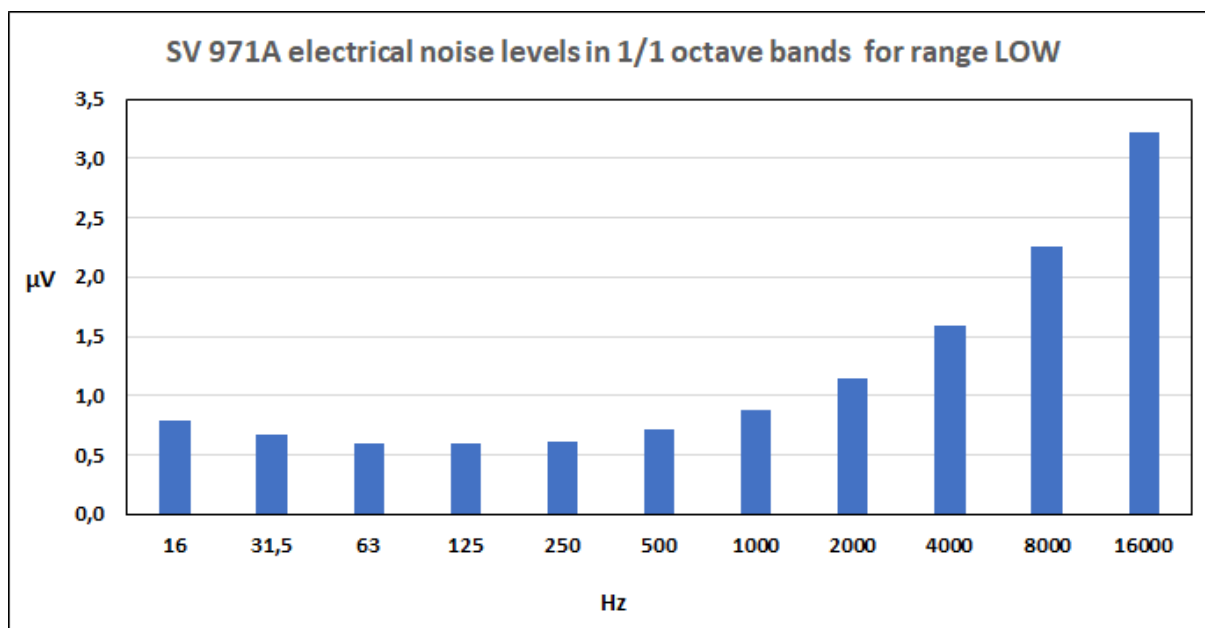


C.3 FREQUENCY CHARACTERISTICS OF THE IMPLEMENTED DIGITAL FILTERS


“A” filter Class 1 according to IEC 651& and IEC 61672-1:2013

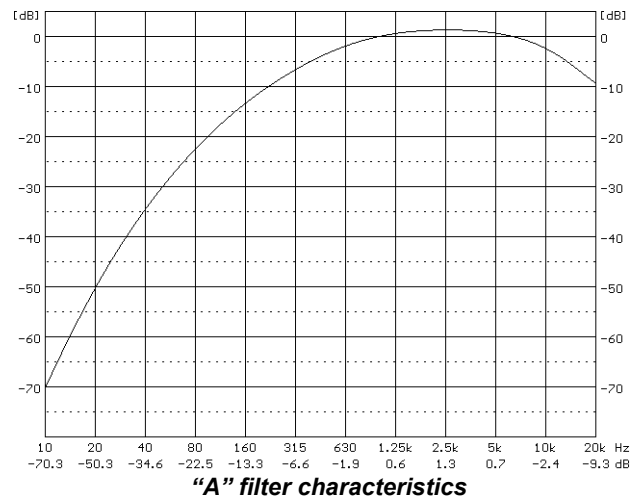

“C” filter Class 1 according to IEC 651 and IEC 61672-1:2013

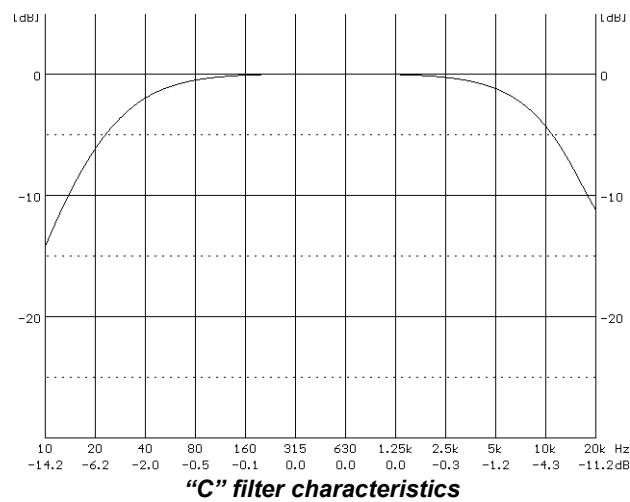


“B” filter Class 1 according to IEC 651

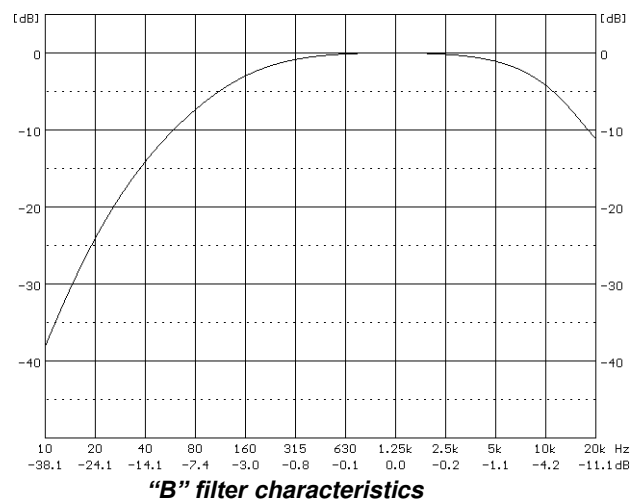

“Z” filter

Class 1 according to IEC 61672-1:2013

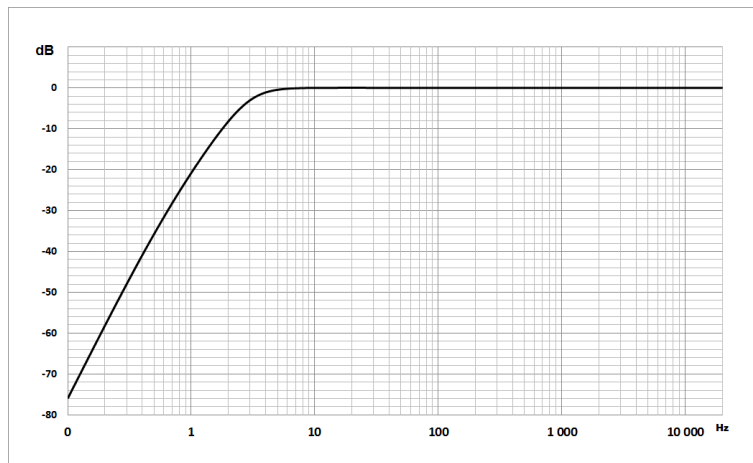***“Z” filter characteristics***

C.4 MISCELLANEOUS SPECIFICATION OF SV 971A

Display

Super contrast OLED colour display (96 x 96 pixels).

Memory


4 MB flash memory and 320 kB RAM memory.

Memory card

Can be used typical Micro-SD or Micro-SDHC cards. Supported for up to 128 GB (provided that card was formatted as FAT32).



Note: The originally supplied Kingston Industrial memory card has been tested by SVANTEK and cards of this type are strongly recommended for use when the original card is going to be replaced.

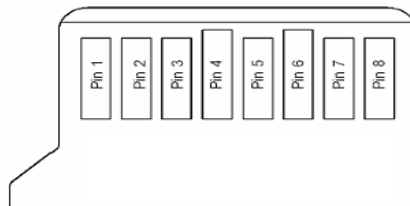


MicroSD contact pad assignment - outer view

Table C.4.1. Pin out of the MicroSD contact

Pin No.	Name	Description
1	DAT2	Data Line [Bit 2]
2	CD/DAT3	Card Detect / Data Line [Bit 3]
3	CMD	Command / Response
4	V _{DD}	Supply voltage
5	CLK	Clock
6	V _{SS}	Supply voltage ground
7	DAT0	Data Line [Bit 0]
8	DAT1	Data Line [Bit 1]

Input (Preamplifier) Connector

The input of the measured signal is taken from the microphone preamplifier:

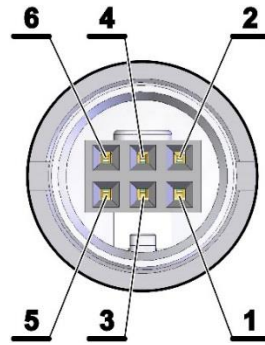

Connector view (external), contact assignment

Table C.4.2. Pin out of the TNC connector

Contact number	Signal name
1	+4V /+10 V power supply
2	-2.1V /-7.3 V power supply
3	GND
4	Pramp DC bias
5	Signal
6	Temperature sensor / TEDS
Preamplifier body	Shield / Cable Screen

Power Supply

Instrument is dedicated for the operation from the internal replaceable AAA batteries. Power consumption from the 6V source is approx. 60 mA (at + 20°C). So, typical operating time from 4 x AAA alkaline batteries will be about **16 hours**.

SV 971A can be also powered from the AAA Class rechargeable batteries.



Note: For the temperatures below 0°C operating time may be shortened (depending on the batteries)!

Interface USB Type C

The SV 971A USB-C 2.0 interface enables remote control of the instrument and data transfer with the speed up to that attainable with 480 MHz clock.



Note: For effective operation with the USB, the **High 480Mbps** speed mode should be used, however when the interference RF field strength may exceed the value of 3V/m, then it is recommended to switch to the **Full 12Mbps** speed mode.

The USB-C interface can work as external power source for the meter.

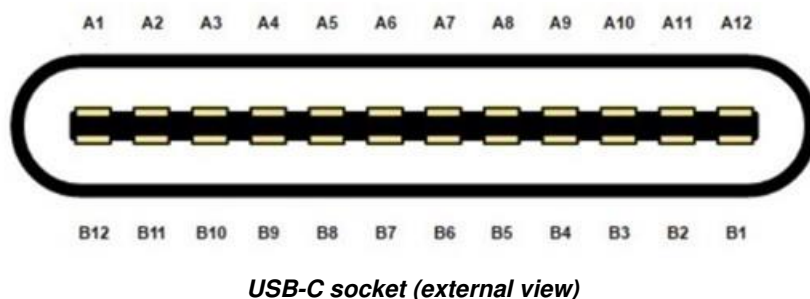


Table C.4.3. Pin-out of the USB-C device connector

Contact no.		Signal name	Description
A1	B1	GND	Ground return
A2	B2	SSTXp1	not used
A3	B3	SSTXn1	not used
A4	B4	V _{BUS}	Bus power (5VDC ±0.5V)
A5	B5	CC1	Configuration channel (5.1kΩ to ground as UFP receiver)
A6	B6	Dp1	USB 2.0 differential pair, position 1, positive
A7	B7	Dn1	USB 2.0 differential pair, position 1, negative
A8	B8	SBU1	not used
A9	B9	V _{BUS}	Bus power (5VDC ±0.5V)
A10	B10	SSRXn2	not used
A11	B11	SSRXp2	not used
A12	B12	GND	Ground return

RS 232 interface (optional)

The RS 232 interface option for SV 971A is provided by means of the **SP 75** interface. It conforms to the EIA Standard RS 232C. It enables the user to programme remotely all instrument functions and the transmissions to and from the meter with the speed from 300 bit/s to 115200 bit/s.



Note: The SP 75 interface must be connected to the SV 971A USB port and proper operation of this port has to be set-up in the instrument's **SETUP** Menu before!

The SP 75 - DB 09 F - pin female connector pin-out is given below.

Table C.4.4. SP 75 interface description

PC RS 232, 9 - pin connector Signal name	SP 75 connector (DB 09 F) Pin number
1 – LSD	1 (not connected)
2 – RXD	3
3 – TXD	2
4 – DTR	6 connected to pin 4
5 – GND	5
6 – DSR	4 connected to pin 6
7 – RTS	8
8 – CTS	7
9 – GND	9 (not connected)

Real Time Clock

Built-in real time. Accuracy better than 1 minute/month.

Wireless Bluetooth 5.2 Connectivity

This dosimeter supports wireless connection via Bluetooth® 5.2 (Low energy). This connectivity is compatible with mobile and PC devices that support Bluetooth® 5.2.

- TX power: up to 8 dBm
- Receiver sensitivity: -90 dBm
- Range: typically >50m line-of-sight and depending on local RF conditions.

The instrument contains a wireless transmission module, BGM121 from Silicon Laboratories technologies. Copies of the modules regional approvals certificates may be obtained from Svantek or Silicon Laboratories.

FCC and ISEDC

This product contains an FCC and Industry Canada certified Bluetooth® Low energy wireless transmission module:

- **FCC IDENTIFIER:** QOQBGM12LMA
- **Industry Canada IC:** 5123A-BGM12LMA
- Producer: Silicon Laboratories Inc.
- Model: BGM121A Bluetooth smart module
- Modular Type: Single Modular

FCC Statements:

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) this device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. End users must follow the specific operating instructions for satisfying RF exposure compliance.

This transmitter meets both portable and mobile limits as demonstrated in the RF Exposure Analysis and SAR test report. This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter except in accordance with FCC multi-transmitter product procedures.

ISED Statements:

This radio transmitter has been approved by Industry Canada to operate with its embedded antenna. Other antenna types are strictly prohibited for use with this device. This device complies with Industry Canada's license-exempt RSS standards. Operation is subject to the following two conditions:

- (1) this device may not cause interference, and
- (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Exception from routine SAR evaluation limits are given in RSS-102 Issue5. BGM121N meets the given requirements when the minimum separation distance to human body is less than equal to 15 mm. RF exposure or SAR evaluation is not required when the separation distance is 15 mm or more. BGM121A module has been tested for worst case RF exposure. As demonstrated in the SAR test report, BGM121A and BGM123A can be mounted in touch with human body without further SAR evaluation.

Environmental parameters

- | | |
|-----------------------------|---|
| • Working temperature range | -10°C ÷ +50°C |
| • Storing temperature range | -20°C ÷ +50°C (-30°C ÷ +60°C without batteries) |
| • Humidity | 90% RH in 40°C (uncondensed vapour) |
| • Ingress Protection Code | IP 54 |

Weight with batteries 225 g (including microphone and preamplifier).

Dimensions 20 x 56 x 232 mm .

Compliance with EU Directives (see Chapter C.6)

CE mark indicates compliance with RED Directive 2014/53/EU:

- Art 3.1a: Safety
- Art 3.1b: Electromagnetic Compatibility
- Art 3.2: Radio.



Note: *Electromagnetic compatibility is guaranteed only with the original accessories supplied by SVANTEK!*

C.5 USING THE SA 271A OUTDOOR MICROPHONE KIT

The **SA 271A** outdoor microphone kit protects the instrument's preamplifier and microphone from weather conditions. Using an outdoor microphone kit requires an extension cable between the instrument and its preamplifier (**SC 91A**).

SA 271A is made of lightweight materials and is easy to install on a tripod. This solution is recommended for short term outdoor noise measurements.

The outdoor microphone kit has $\frac{3}{4}$ " screw on its bottom which allows the use of standard tripods or other user specific mounts.

As an option the user may use desiccator – Silica gel. Desiccator absorbs moisture normally contained in the air.



Note: Desiccator should be regenerated after some period of use, when it changes colour to light grey, by drying it for 3 hours in a temperature of 150°C. Desiccator should be inspected at least every 2 weeks, and more often when used in conditions of high air humidity.



Note: See also Appendix F to learn how to assemble and disassemble the outdoor microphone kit.



Note: Using SA 271A changes the frequency response and measuring ranges of SV 971A. Please check the below given specification.

Depending on the measurement task SA 271A can be used in two operational modes:

1. With reference incidence angle 90 deg – so called “Environment” mode.
2. With reference incidence angle 0 deg – so called “Airport” mode.

The wave incidence angle is oriented to the microphone membrane surface. 0 deg means direction orthogonal to the membrane surface. 90 deg means direction parallel to the membrane surface.



Frequency response of SV 971A with the SA 271A outdoor microphone kit is compensated by means of two digital filters which can be set in the **Field Comp.** position (path: <Menu> / Measurement / Comp. Filter):



- **Environment**

compensation filter that improves the complete instrument frequency response in the free field for the reference acoustic wave incidence angle 90 deg

- **Airport**

compensation filter that improves the complete instrument frequency response in the free field for the reference acoustic wave incidence angle 0 deg



Note: For the conformance acoustical tests with SA 271A, the **Microphone** compensation must be switched **On** and the **Field Compensation** must be set to **Environment** or **Airport** (path: <Menu> / Measurement / Comp. Filter).

Statement of performance

SV 971A working as the SLM with SA 271A meets requirements of IEC 61672:2013 for the Class 1 Group X instruments.

Linear operating ranges with the **Environment** filter

The starting point at which tests of level linearity shall begin is 94.0 dB for the frequencies specifies below. For the **Low** measurement range and A weighting linearity test at 31.5 Hz, the starting point is 79 dB.

Table C.5.1. Linear operating ranges for the **Normal** measurement range and the **Environment** filter (for the sinusoidal signal and microphone sensitivity in the range 32 mV/Pa)

[dB]	L _{AS/F}		L _{BS/F}		L _{CS/F}		L _{ZS/F}		L _{AeqT}		L _{BeqT}		L _{CeqT}		L _{AE} (t _{int} = 2 s)		L _{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31.5 Hz	29	97	29	120	29	134	36	137	29	97	29	120	29	134	32	100	55	137
500 Hz	29	133	29	136	29	137	36	137	29	133	29	136	29	137	32	136	55	140
1 kHz	29	137	29	137	29	137	36	137	29	137	29	137	29	137	32	140	55	140
4 kHz	29	138	29	136	29	136	36	137	29	138	29	136	29	136	32	141	55	139
8 kHz	29	136	29	134	29	134	36	137	29	136	29	134	29	134	32	139	55	137
12.5 kHz	29	132	29	131	29	131	36	137	29	132	29	131	29	131	32	135	55	134

Table C.5.2. Linear operating ranges for the **Low** measurement range and the **Environment** filter (for the sinusoidal signal and microphone sensitivity in the range 32 mV/Pa)

[dB]	L _{AS/F}		L _{BS/F}		L _{CS/F}		L _{ZS/F}		L _{AeqT}		L _{BeqT}		L _{CeqT}		L _{AE} (t _{int} = 2 s)		L _{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31.5 Hz	26	80	26	103	26	117	31	120	26	80	26	103	26	117	29	83	51	120
500 Hz	26	116	26	119	26	120	31	120	26	116	26	119	26	120	29	119	50	123
1 kHz	26	120	26	120	26	120	31	120	26	120	26	120	26	120	29	123	50	123
4 kHz	26	121	26	119	26	119	31	120	26	121	26	119	26	119	29	124	50	123
8 kHz	26	119	26	117	26	117	31	120	26	119	26	117	26	117	29	122	50	120
12.5 kHz	26	115	26	114	26	114	31	120	26	115	26	114	26	114	29	118	50	117

Table C.5.3. Self-generated noise for different weighting filters

Weighting filter Range	Electrical *)			Acoustical compensated		
	A	C	Z	A	C	Z
Low	< 15 dB	< 15 dB	< 20 dB	< 16 dB	< 16 dB	< 21 dB
Normal	< 26 dB	< 26 dB	< 31 dB	< 27 dB	< 27 dB	< 31 dB

*) measured with the **ST 03** microphone equivalent impedance 18 pF ± 10%

Linear operating ranges with Airport filter

The starting point at which tests of level linearity shall begin is 94.0 dB for the frequencies specifies below. For the **Low** measurement range and A weighting linearity test at 31.5 Hz, the starting point is 79 dB.

Table C.5.4. Linear operating ranges for the **Normal** measurement range and the **Airport** filter (for the sinusoidal signal and microphone sensitivity 32 mV/Pa)

[dB]	L _{AS/F}		L _{BS/F}		L _{CS/F}		L _{ZS/F}		L _{AeqT}		L _{BeqT}		L _{CeqT}		L _{AE} (t _{int} = 2 s)		L _{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to	from	to
31,5 Hz	29	97	29	120	29	134	36	137	29	97	29	120	29	134	32	100	55	137
500 Hz	29	133	29	136	29	137	36	137	29	133	29	136	29	137	32	136	55	140
1 kHz	29	137	29	137	29	137	36	137	29	137	29	137	29	137	32	140	55	140
4 kHz	29	138	29	136	29	136	36	137	29	138	29	136	29	136	32	141	55	139
8 kHz	29	136	29	134	29	134	36	137	29	136	29	134	29	134	32	139	55	137
12.5 kHz	29	132	29	131	29	131	36	137	29	132	29	131	29	131	32	135	55	134


Table C.5.5. Linear operating ranges for the **Low** measurement range and the **Airport** filter (for the sinusoidal signal and microphone sensitivity in the range 32 mV/Pa)

[dB]	L _{AS/F}		L _{BS/F}		L _{CS/F}		L _{ZS/F}		L _{AeqT}		L _{BeqT}		L _{CeqT}		L _{AE} (t _{int} = 2 s)		L _{Cpeak}	
	from	to	from	to	from	to	from	to	from	to	from	to	From	to	from	to	from	to
31,5 Hz	26	80	26	103	26	117	32	120	26	80	26	103	26	117	29	83	50	120
500 Hz	26	116	26	119	26	120	32	120	26	116	26	119	26	120	29	119	50	123
1 kHz	26	120	26	120	26	120	32	120	26	120	26	120	26	120	29	123	50	123
4 kHz	26	121	26	119	26	119	32	120	26	121	26	119	26	119	29	124	50	123
8 kHz	26	119	26	117	26	117	32	120	26	119	26	117	26	117	29	123	50	120
12.5 kHz	26	115	26	114	26	114	32	120	26	115	26	114	26	114	29	118	50	117


Table C.5.6. Self-generated noise for different weighting filters

		Electrical *)			Acoustical compensated		
Weighting filter	Range	A	C	Z	A	C	Z
	Low	< 15 dB	< 14 dB	< 20 dB	< 16 dB	< 16 dB	< 22 dB
	Normal	< 26 dB	< 25 dB	< 32 dB	< 26 dB	< 26 dB	< 32 dB

*) measured with the **ST 03** microphone equivalent impedance 18 pF +/-10%

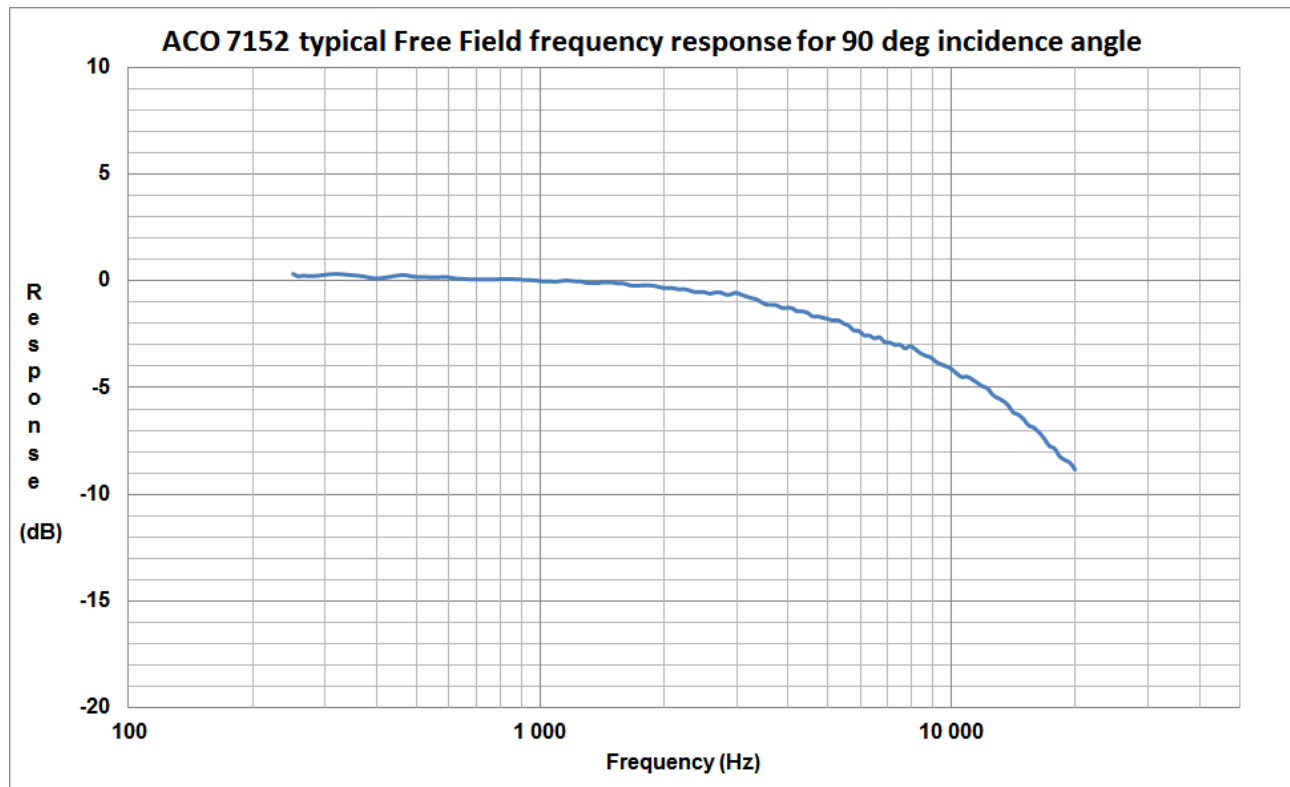ACO 7152 Free Field frequency response for 90 deg incidence angle**Table C.5.7.** ACO 7152 Free Field corrections for the electrostatic actuator for 90 deg incidence angle

[dB]	Frequency [Hz]																
	20	25	31.5	40	50	63	80	100	125	160	200	250	315	400	500	630	800
Correction factors	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.31	0.31	0.12	0.19	0.13	0.12
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25
[dB]	Frequency [Hz]																
	1000	1250	1600	2000	2500	3150	4000	5000	6300	8000	10000	12500	16000	20000			
Correction factors	0.08	0.10	0.07	-0.06	-0.09	-0.07	-0.28	-0.36	-0.49	-0.11	0.05	0.54	1.31	2.14			
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.35	0.35	0.35	0.35	0.50	0.50	0.50			

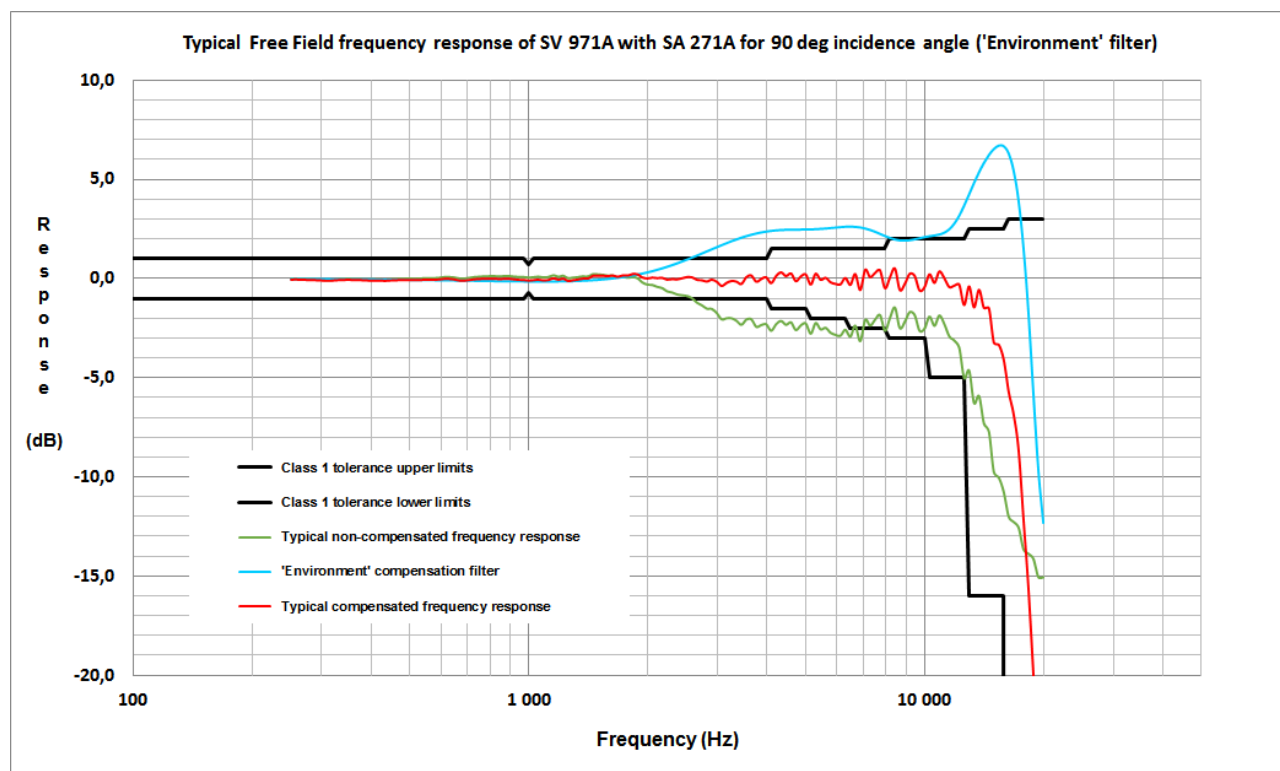
Free Field frequency characteristics of SV 971A with SA 271A for 90 deg incidence angle**Table C.5.8.** Typical Free Field frequency characteristics of SV 971A with SA 271A for 90 deg incidence angle

Frequency	Compensation filter for 90 deg incidence angle "Environment"	Typical compensated response of SV 971A with SA 271A for 90 deg incidence angle	Compensated Case Effect of SA 271A for 90 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
251	-0.01	-0.03	-0.34	0.25
259	-0.02	-0.03	-0.22	0.25
266	-0.02	-0.04	-0.27	0.25
274	-0.02	-0.05	-0.26	0.25
282	-0.02	-0.05	-0.26	0.25
290	-0.02	-0.06	-0.29	0.25
299	-0.02	-0.07	-0.34	0.25
307	-0.02	-0.09	-0.38	0.25
316	-0.02	-0.10	-0.40	0.25
325	-0.02	-0.07	-0.37	0.25
335	-0.03	-0.06	-0.34	0.25
345	-0.03	-0.05	-0.31	0.25
355	-0.03	-0.05	-0.29	0.25
365	-0.03	-0.06	-0.28	0.25
376	-0.03	-0.06	-0.24	0.25
387	-0.03	-0.08	-0.20	0.25
398	-0.04	-0.08	-0.18	0.25
410	-0.04	-0.09	-0.19	0.25
422	-0.04	-0.09	-0.23	0.25

Frequency	Compensation filter for 90 deg incidence angle "Environment"	Typical compensated response of SV 971A with SA 271A for 90 deg incidence angle	Compensated Case Effect of SA 271A for 90 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
434	-0.04	-0.10	-0.28	0.25
447	-0.04	-0.08	-0.30	0.25
460	-0.05	-0.07	-0.33	0.25
473	-0.05	-0.05	-0.30	0.25
487	-0.05	-0.05	-0.25	0.25
501	-0.05	-0.05	-0.22	0.25
516	-0.06	-0.06	-0.22	0.25
531	-0.06	-0.05	-0.21	0.25
546	-0.06	-0.05	-0.19	0.25
562	-0.07	-0.04	-0.19	0.25
579	-0.07	-0.04	-0.21	0.25
596	-0.07	-0.03	-0.18	0.25
613	-0.08	0.01	-0.11	0.25
631	-0.08	0.00	-0.08	0.25
649	-0.08	-0.03	-0.10	0.25
668	-0.09	-0.08	-0.14	0.25
688	-0.09	-0.08	-0.13	0.25
708	-0.09	-0.05	-0.10	0.25
729	-0.10	-0.02	-0.08	0.25
750	-0.10	-0.01	-0.05	0.25
772	-0.11	0.01	-0.04	0.25
794	-0.11	0.01	-0.05	0.25
818	-0.11	0.02	-0.04	0.25
841	-0.12	-0.01	-0.07	0.25
866	-0.12	0.00	-0.06	0.25
891	-0.12	0.01	-0.04	0.25
917	-0.13	-0.02	-0.05	0.25
944	-0.13	-0.04	-0.06	0.25
972	-0.13	-0.05	-0.06	0.25
1 000	-0.13	-0.08	-0.06	0.25
1 029	-0.14	-0.06	-0.01	0.25
1 059	-0.14	-0.04	0.01	0.25
1 090	-0.14	-0.07	-0.02	0.25
1 122	-0.14	-0.05	-0.03	0.25
1 155	-0.14	0.03	0.03	0.25
1 189	-0.13	-0.04	-0.02	0.25
1 223	-0.13	0.01	0.05	0.25
1 259	-0.12	-0.10	-0.06	0.25
1 296	-0.12	-0.06	0.05	0.25
1 334	-0.11	-0.03	0.08	0.25
1 372	-0.10	0.02	0.15	0.25
1 413	-0.09	0.02	0.11	0.25
1 454	-0.07	0.16	0.25	0.25
1 496	-0.05	0.16	0.24	0.25
1 540	-0.03	0.16	0.30	0.25
1 585	-0.01	0.14	0.27	0.25

Frequency	Compensation filter for 90 deg incidence angle "Environment"	Typical compensated response of SV 971A with SA 271A for 90 deg incidence angle	Compensated Case Effect of SA 271A for 90 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
1 631	0.02	0.17	0.36	0.25
1 679	0.05	0.11	0.35	0.25
1 728	0.09	0.18	0.42	0.25
1 778	0.13	0.17	0.40	0.25
1 830	0.17	0.25	0.47	0.25
1 884	0.22	0.23	0.47	0.25
1 939	0.27	0.07	0.36	0.25
1 995	0.33	0.02	0.37	0.25
2 054	0.39	0.07	0.42	0.25
2 113	0.46	0.04	0.40	0.25
2 175	0.53	0.05	0.46	0.25
2 239	0.61	-0.03	0.37	0.25
2 304	0.69	-0.01	0.45	0.25
2 371	0.78	-0.02	0.51	0.25
2 441	0.88	0.04	0.58	0.25
2 512	0.97	0.09	0.64	0.25
2 585	1.07	0.08	0.70	0.25
2 661	1.17	-0.04	0.52	0.25
2 738	1.28	-0.07	0.48	0.25
2 818	1.39	-0.13	0.52	0.25
2 901	1.49	-0.04	0.62	0.25
2 985	1.60	-0.14	0.43	0.25
3 073	1.70	-0.35	0.30	0.25
3 162	1.80	-0.20	0.54	0.25
3 255	1.90	-0.10	0.71	0.25
3 350	1.99	-0.14	0.73	0.25
3 447	2.08	-0.25	0.76	0.25
3 548	2.16	0.10	1.22	0.25
3 652	2.23	0.17	1.31	0.25
3 758	2.29	-0.14	1.01	0.25
3 868	2.34	0.00	1.27	0.25
3 981	2.39	0.08	1.36	0.25
4 097	2.42	-0.21	1.08	0.35
4 217	2.45	0.14	1.58	0.35
4 340	2.47	0.33	1.77	0.35
4 467	2.48	0.14	1.65	0.35
4 597	2.48	0.28	1.95	0.35
4 732	2.49	-0.11	1.57	0.35
4 870	2.49	0.13	1.87	0.35
5 012	2.49	0.22	2.02	0.35
5 158	2.50	-0.28	1.58	0.35
5 309	2.51	0.26	2.12	0.35
5 464	2.52	-0.04	1.96	0.35
5 623	2.54	0.06	2.17	0.35
5 788	2.56	-0.17	2.16	0.35
5 957	2.59	-0.25	2.11	0.35

Frequency	Compensation filter for 90 deg incidence angle "Environment"	Typical compensated response of SV 971A with SA 271A for 90 deg incidence angle	Compensated Case Effect of SA 271A for 90 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
6 131	2.61	-0.27	2.29	0.35
6 310	2.63	0.05	2.62	0.35
6 494	2.63	-0.30	2.40	0.35
6 683	2.62	0.25	2.90	0.35
6 879	2.59	-0.56	2.31	0.35
7 079	2.54	0.46	3.36	0.35
7 286	2.47	0.09	3.10	0.35
7 499	2.38	0.31	3.30	0.35
7 718	2.27	0.43	3.60	0.35
7 943	2.16	-0.47	2.59	0.35
8 175	2.07	0.07	3.29	0.35
8 414	1.99	0.53	3.93	0.35
8 660	1.94	-0.56	2.96	0.35
8 913	1.93	-0.26	3.35	0.35
9 173	1.95	0.26	4.06	0.35
9 441	1.99	0.15	4.07	0.35
9 716	2.05	-0.58	3.43	0.35
10 000	2.11	-0.41	3.73	0.35
10 292	2.15	0.23	4.58	0.35
10 593	2.19	-0.19	4.32	0.35
10 902	2.24	0.38	4.87	0.35
11 220	2.33	0.03	4.66	0.35
11 548	2.50	-0.41	4.37	0.35
11 885	2.79	-0.34	4.60	0.35
12 232	3.19	-0.29	4.75	0.35
12 589	3.70	-1.32	4.03	0.35
12 957	4.27	-0.38	5.12	0.35
13 335	4.84	-1.44	4.19	0.35
13 725	5.38	-0.55	5.29	0.35
14 125	5.85	-1.46	4.70	0.35
14 538	6.25	-1.48	4.80	0.35
14 962	6.55	-3.21	3.28	0.35
15 399	6.73	-3.32	3.46	0.35
15 849	6.69	-4.07	2.80	0.35
16 312	6.32	-5.70	1.40	0.35
16 788	5.46	-6.82	0.56	0.35
17 278	3.92	-8.64	-0.91	0.35
17 783	1.55	-12.12	-4.27	0.35
18 302	-1.76	-15.64	-7.43	0.35
18 836	-5.78	-19.92	-11.54	0.35
19 387	-9.68	-24.74	-16.23	0.35
19 953	-12.32	-27.39	-18.56	0.35

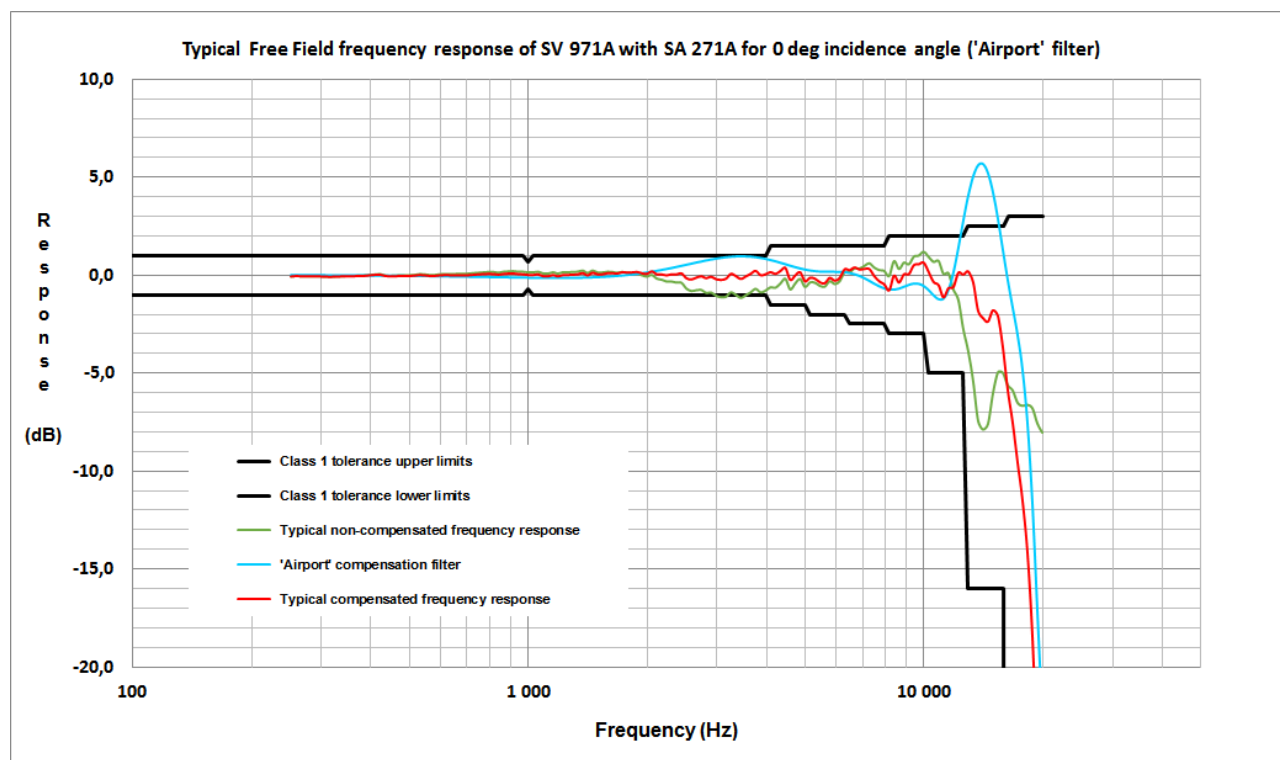Free Field frequency characteristics of SV 971A with SA 271A for 0 deg incidence angle**Table C.5.9.** Typical Free Field frequency characteristics of SV 971A with SA 271A for 0 deg incidence angle

Frequency	Compensation filter for 0 deg incidence angle "Airport"	SA 271A typical compensated response for 0 deg incidence angle	Compensated Case Effect for 0 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
251	-0.02	-0.08	-0.14	0.25
259	-0.02	-0.06	-0.11	0.25
266	-0.02	-0.07	-0.12	0.25
274	-0.02	-0.07	-0.11	0.25
282	-0.02	-0.07	-0.11	0.25
290	-0.02	-0.07	-0.11	0.25
299	-0.02	-0.08	-0.11	0.25
307	-0.02	-0.09	-0.13	0.25
316	-0.03	-0.10	-0.14	0.25
325	-0.03	-0.09	-0.13	0.25
335	-0.03	-0.08	-0.13	0.25
345	-0.03	-0.08	-0.13	0.25
355	-0.03	-0.07	-0.12	0.25
365	-0.03	-0.07	-0.11	0.25
376	-0.03	-0.06	-0.09	0.25
387	-0.04	-0.05	-0.07	0.25
398	-0.04	-0.02	-0.04	0.25
410	-0.04	0.00	-0.01	0.25
422	-0.04	0.01	0.00	0.25
434	-0.04	-0.05	-0.06	0.25
447	-0.05	-0.08	-0.10	0.25
460	-0.05	-0.07	-0.08	0.25

Frequency	Compensation filter for 0 deg incidence angle “Airport”	SA 271A typical compensated response for 0 deg incidence angle	Compensated Case Effect for 0 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
473	-0.05	-0.06	-0.07	0.25
487	-0.05	-0.06	-0.07	0.25
501	-0.06	-0.06	-0.06	0.25
516	-0.06	-0.04	-0.05	0.25
531	-0.06	-0.01	-0.02	0.25
546	-0.07	-0.03	-0.04	0.25
562	-0.07	-0.05	-0.06	0.25
579	-0.07	-0.06	-0.07	0.25
596	-0.08	-0.03	-0.04	0.25
613	-0.08	-0.01	-0.02	0.25
631	-0.08	-0.02	-0.02	0.25
649	-0.09	-0.03	-0.03	0.25
668	-0.09	-0.02	-0.02	0.25
688	-0.10	-0.03	-0.03	0.25
708	-0.10	-0.02	-0.02	0.25
729	-0.10	0.01	0.01	0.25
750	-0.11	0.02	0.02	0.25
772	-0.11	0.04	0.04	0.25
794	-0.12	0.05	0.05	0.25
818	-0.12	0.04	0.05	0.25
841	-0.13	0.01	0.02	0.25
866	-0.13	0.05	0.05	0.25
891	-0.13	0.06	0.07	0.25
917	-0.14	0.07	0.07	0.25
944	-0.14	0.04	0.04	0.25
972	-0.15	0.03	0.02	0.25
1 000	-0.15	-0.01	-0.01	0.25
1 029	-0.15	-0.01	-0.01	0.25
1 059	-0.16	0.02	0.03	0.25
1 090	-0.16	-0.07	-0.07	0.25
1 122	-0.16	-0.08	-0.08	0.25
1 155	-0.16	-0.01	-0.01	0.25
1 189	-0.16	-0.08	-0.08	0.25
1 223	-0.16	-0.01	-0.02	0.25
1 259	-0.16	-0.01	-0.01	0.25
1 296	-0.16	0.00	-0.01	0.25
1 334	-0.15	0.03	0.02	0.25
1 372	-0.15	0.09	0.07	0.25
1 413	-0.14	-0.02	-0.04	0.25
1 454	-0.13	0.10	0.09	0.25
1 496	-0.12	0.02	0.01	0.25
1 540	-0.11	0.03	0.02	0.25
1 585	-0.10	0.08	0.07	0.25
1 631	-0.08	0.09	0.08	0.25
1 679	-0.06	0.07	0.06	0.25
1 728	-0.04	0.13	0.13	0.25
1 778	-0.01	0.11	0.12	0.25
1 830	0.02	0.12	0.14	0.25
1 884	0.05	0.15	0.17	0.25
1 939	0.08	0.08	0.09	0.25
1 995	0.12	0.05	0.07	0.25

Frequency	Compensation filter for 0 deg incidence angle “Airport”	SA 271A typical compensated response for 0 deg incidence angle	Compensated Case Effect for 0 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
2 054	0.16	0.17	0.20	0.25
2 113	0.20	0.03	0.06	0.25
2 175	0.25	0.02	0.06	0.25
2 239	0.30	-0.02	0.04	0.25
2 304	0.35	0.03	0.08	0.25
2 371	0.40	0.02	0.09	0.25
2 441	0.46	0.07	0.15	0.25
2 512	0.51	-0.17	-0.11	0.25
2 585	0.57	-0.24	-0.19	0.25
2 661	0.63	-0.14	-0.09	0.25
2 738	0.68	-0.07	-0.04	0.25
2 818	0.73	-0.17	-0.13	0.25
2 901	0.78	-0.10	-0.05	0.25
2 985	0.83	-0.22	-0.16	0.25
3 073	0.87	-0.26	-0.20	0.25
3 162	0.90	-0.20	-0.12	0.25
3 255	0.92	0.05	0.15	0.25
3 350	0.94	-0.06	0.06	0.25
3 447	0.94	-0.21	-0.08	0.25
3 548	0.94	-0.08	0.05	0.25
3 652	0.93	0.05	0.19	0.25
3 758	0.90	0.21	0.34	0.25
3 868	0.86	-0.02	0.09	0.25
3 981	0.81	0.03	0.15	0.25
4 097	0.76	0.14	0.27	0.35
4 217	0.69	0.05	0.17	0.35
4 340	0.62	0.19	0.33	0.35
4 467	0.54	0.36	0.51	0.35
4 597	0.46	-0.26	-0.09	0.35
4 732	0.39	-0.03	0.14	0.35
4 870	0.32	0.13	0.33	0.35
5 012	0.27	-0.33	-0.16	0.35
5 158	0.22	-0.15	0.02	0.35
5 309	0.19	-0.20	-0.02	0.35
5 464	0.17	-0.38	-0.22	0.35
5 623	0.16	-0.42	-0.24	0.35
5 788	0.15	-0.15	0.07	0.35
5 957	0.15	-0.30	-0.09	0.35
6 131	0.15	-0.16	0.05	0.35
6 310	0.13	0.28	0.50	0.35
6 494	0.09	0.24	0.44	0.35
6 683	0.03	0.37	0.55	0.35
6 879	-0.06	0.28	0.49	0.35
7 079	-0.17	0.30	0.50	0.35
7 286	-0.31	0.30	0.54	0.35
7 499	-0.45	-0.07	0.13	0.35
7 718	-0.59	-0.33	-0.16	0.35
7 943	-0.70	-0.48	-0.36	0.35
8 175	-0.76	-0.79	-0.65	0.35
8 414	-0.76	-0.04	0.02	0.35
8 660	-0.71	-0.39	-0.27	0.35

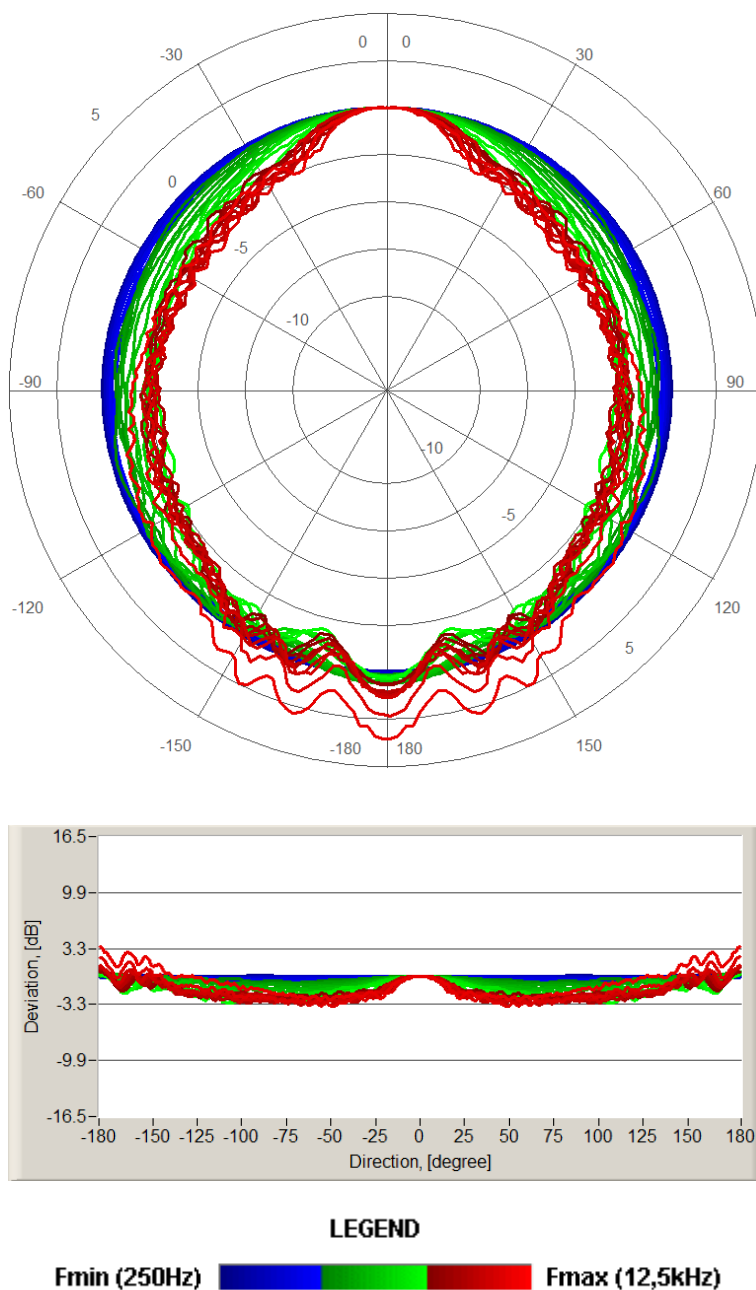
Frequency	Compensation filter for 0 deg incidence angle "Airport"	SA 271A typical compensated response for 0 deg incidence angle	Compensated Case Effect for 0 deg incidence angle	Uncertainty (IEC 62585:2012)
[Hz]	[dB]	[dB]	[dB]	[dB]
8 913	-0.61	0.03	0.15	0.35
9 173	-0.51	0.04	0.15	0.35
9 441	-0.45	0.49	0.59	0.35
9 716	-0.46	0.54	0.67	0.35
10 000	-0.57	0.62	0.71	0.35
10 292	-0.79	0.14	0.26	0.35
10 593	-1.05	-0.37	-0.21	0.35
10 902	-1.25	-0.52	-0.41	0.35
11 220	-1.21	-1.15	-1.03	0.35
11 548	-0.78	-0.68	-0.60	0.35
11 885	0.11	-0.62	-0.54	0.35
12 232	1.36	0.10	0.15	0.35
12 589	2.75	0.01	0.12	0.35
12 957	4.03	0.17	0.27	0.35
13 335	5.02	-0.39	-0.25	0.35
13 725	5.59	-1.84	-1.75	0.35
14 125	5.66	-2.21	-2.15	0.35
14 538	5.19	-2.39	-2.42	0.35
14 962	4.23	-1.81	-1.92	0.35
15 399	2.86	-2.10	-2.24	0.35
15 849	1.28	-3.70	-3.83	0.35
16 312	-0.28	-5.88	-6.00	0.35
16 788	-1.68	-7.55	-7.65	0.35
17 278	-3.09	-9.58	-9.72	0.35
17 783	-4.90	-11.56	-11.88	0.35
18 302	-7.64	-14.24	-14.67	0.35
18 836	-11.71	-18.49	-19.05	0.35
19 387	-17.18	-24.74	-25.45	0.35
19 953	-22.54	-30.56	-31.17	0.35

Table C.5.10. Free Field corrections for SV 971A with SA 271A (combined: Microphone plus Case Effect) for the electrostatic actuator


Correction factors [dB]	Frequency [Hz]																
	20	25	31.5	40	50	63	80	100	125	160	200	250	315	400	500	630	800
0 deg	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	-0.28	-0.35	-0.14	-0.18	-0.03	0.01
90 deg	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.0	0.17	0.20	0.08	0.13	0.11	0.17
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.25
Correction factors [dB]	Frequency [Hz]																
	1000	1250	1600	2000	2500	3150	4000	5000	6300	8000	10000	12500	16000	20000			
0 deg	0.04	0.09	0.48	0.64	1.04	1.13	2.22	3.29	4.48	5.42	7.84	9.80	11.11	-6.98			
90 deg	0.07	0.09	0.14	0.01	-0.20	-0.19	-0.13	-0.52	0.01	-0.47	0.76	0.66	-2.52	-29.03			
Uncertainty (IEC 62585)	0.25	0.25	0.25	0.25	0.25	0.25	0.25	0.35	0.35	0.35	0.35	0.50	0.50	0.50			


Free Field directional characteristics of SV 971A with SA 271A


Directional response of SV 971A with the ACO 7152 microphone, SV 18A preamplifier and SA 271A outdoor microphone kit for specified frequencies.

Combined typical directional characteristics


The round charts show the typical directional characteristics and the charts below shows the errors for 0 deg and 90 deg incidence angles.

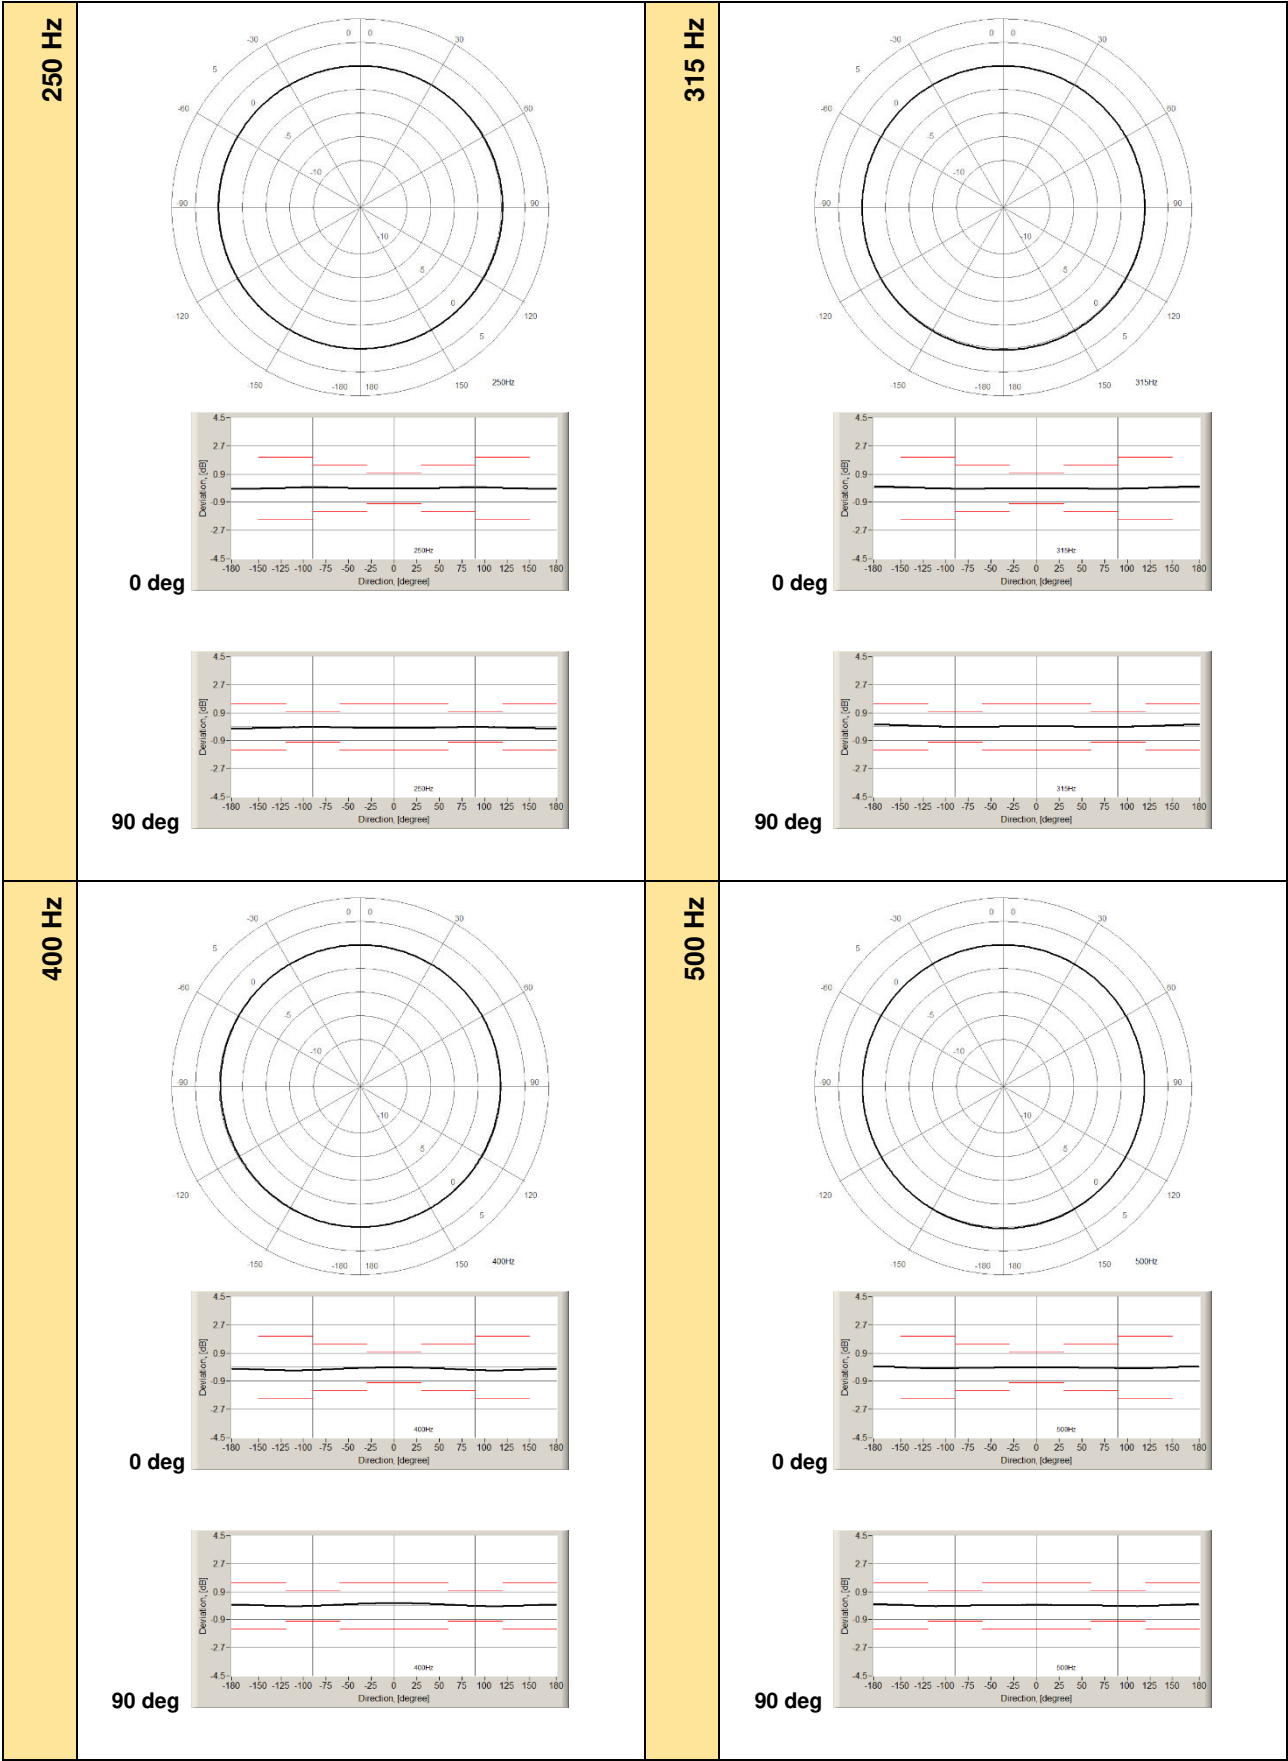

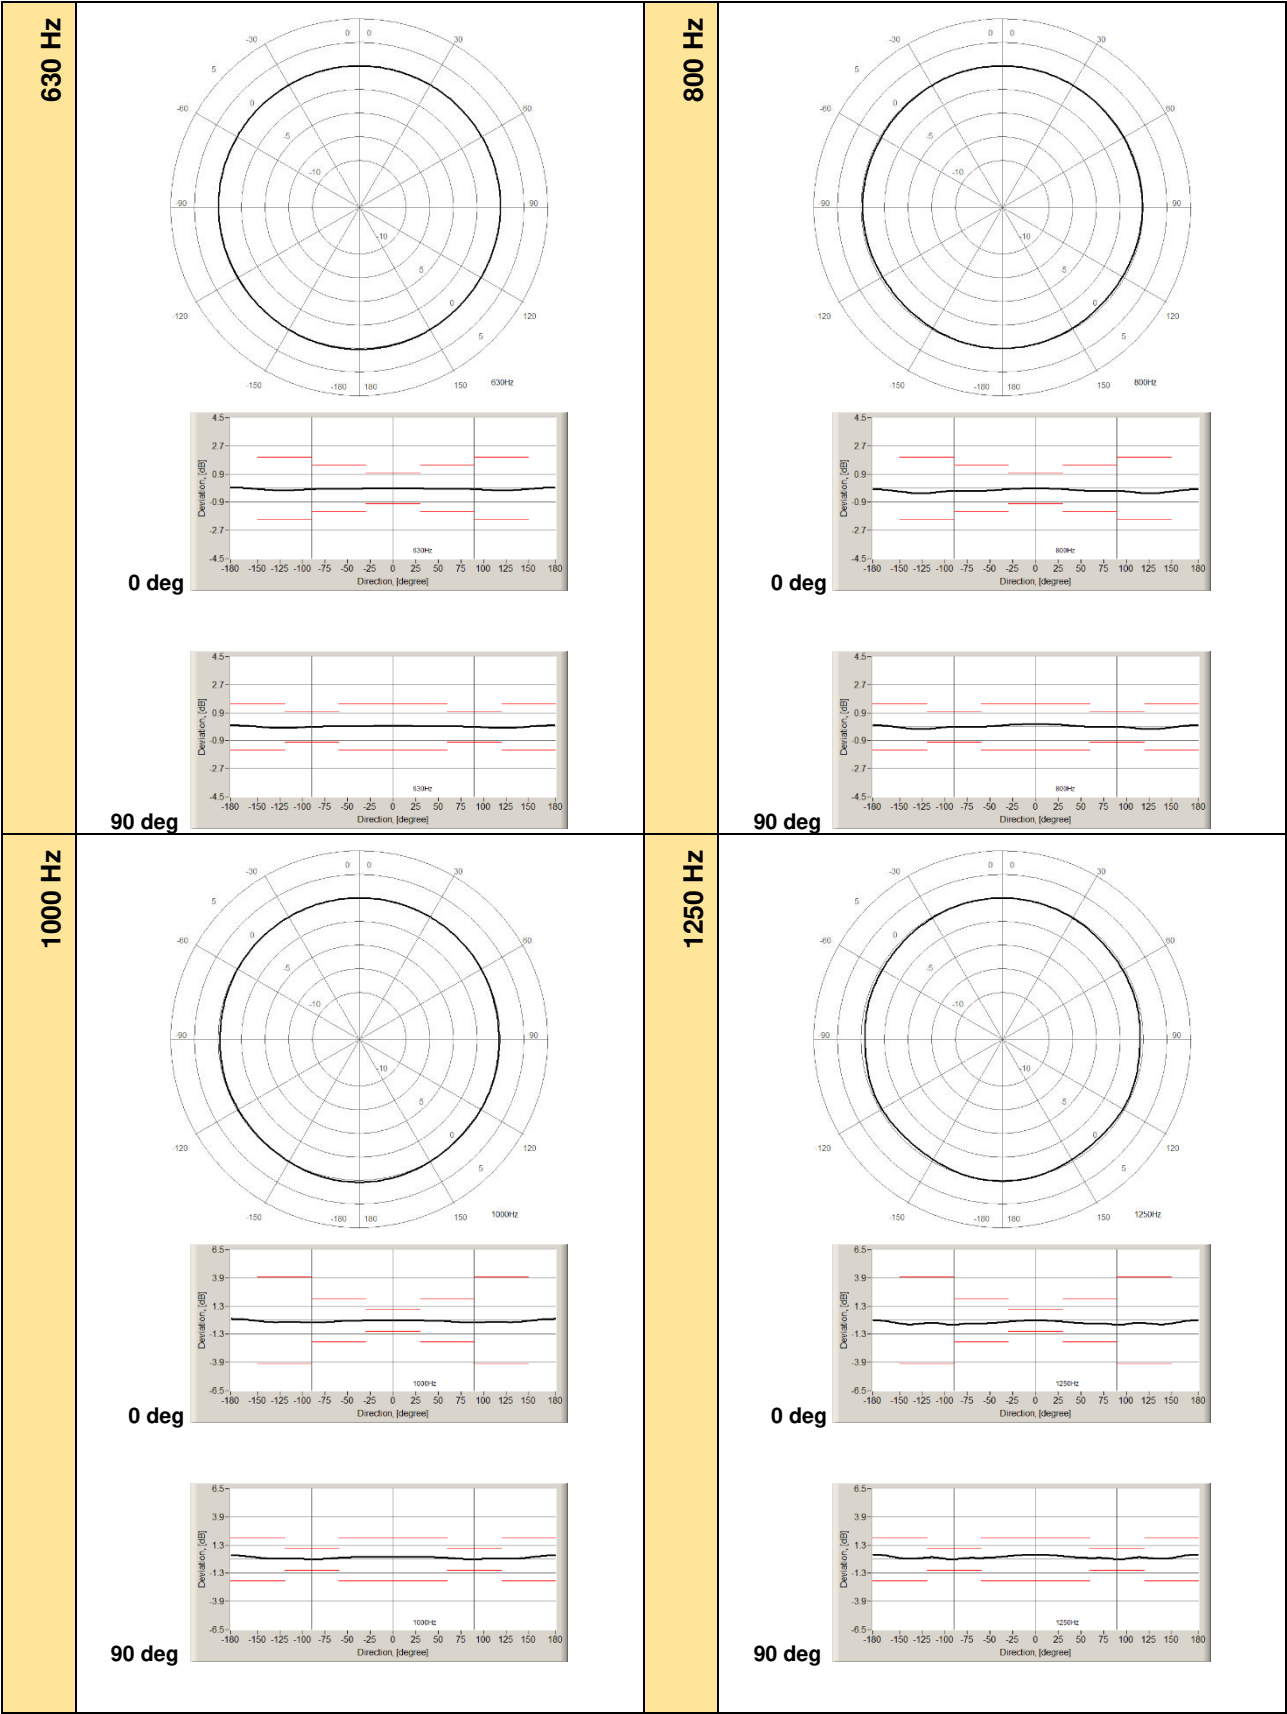


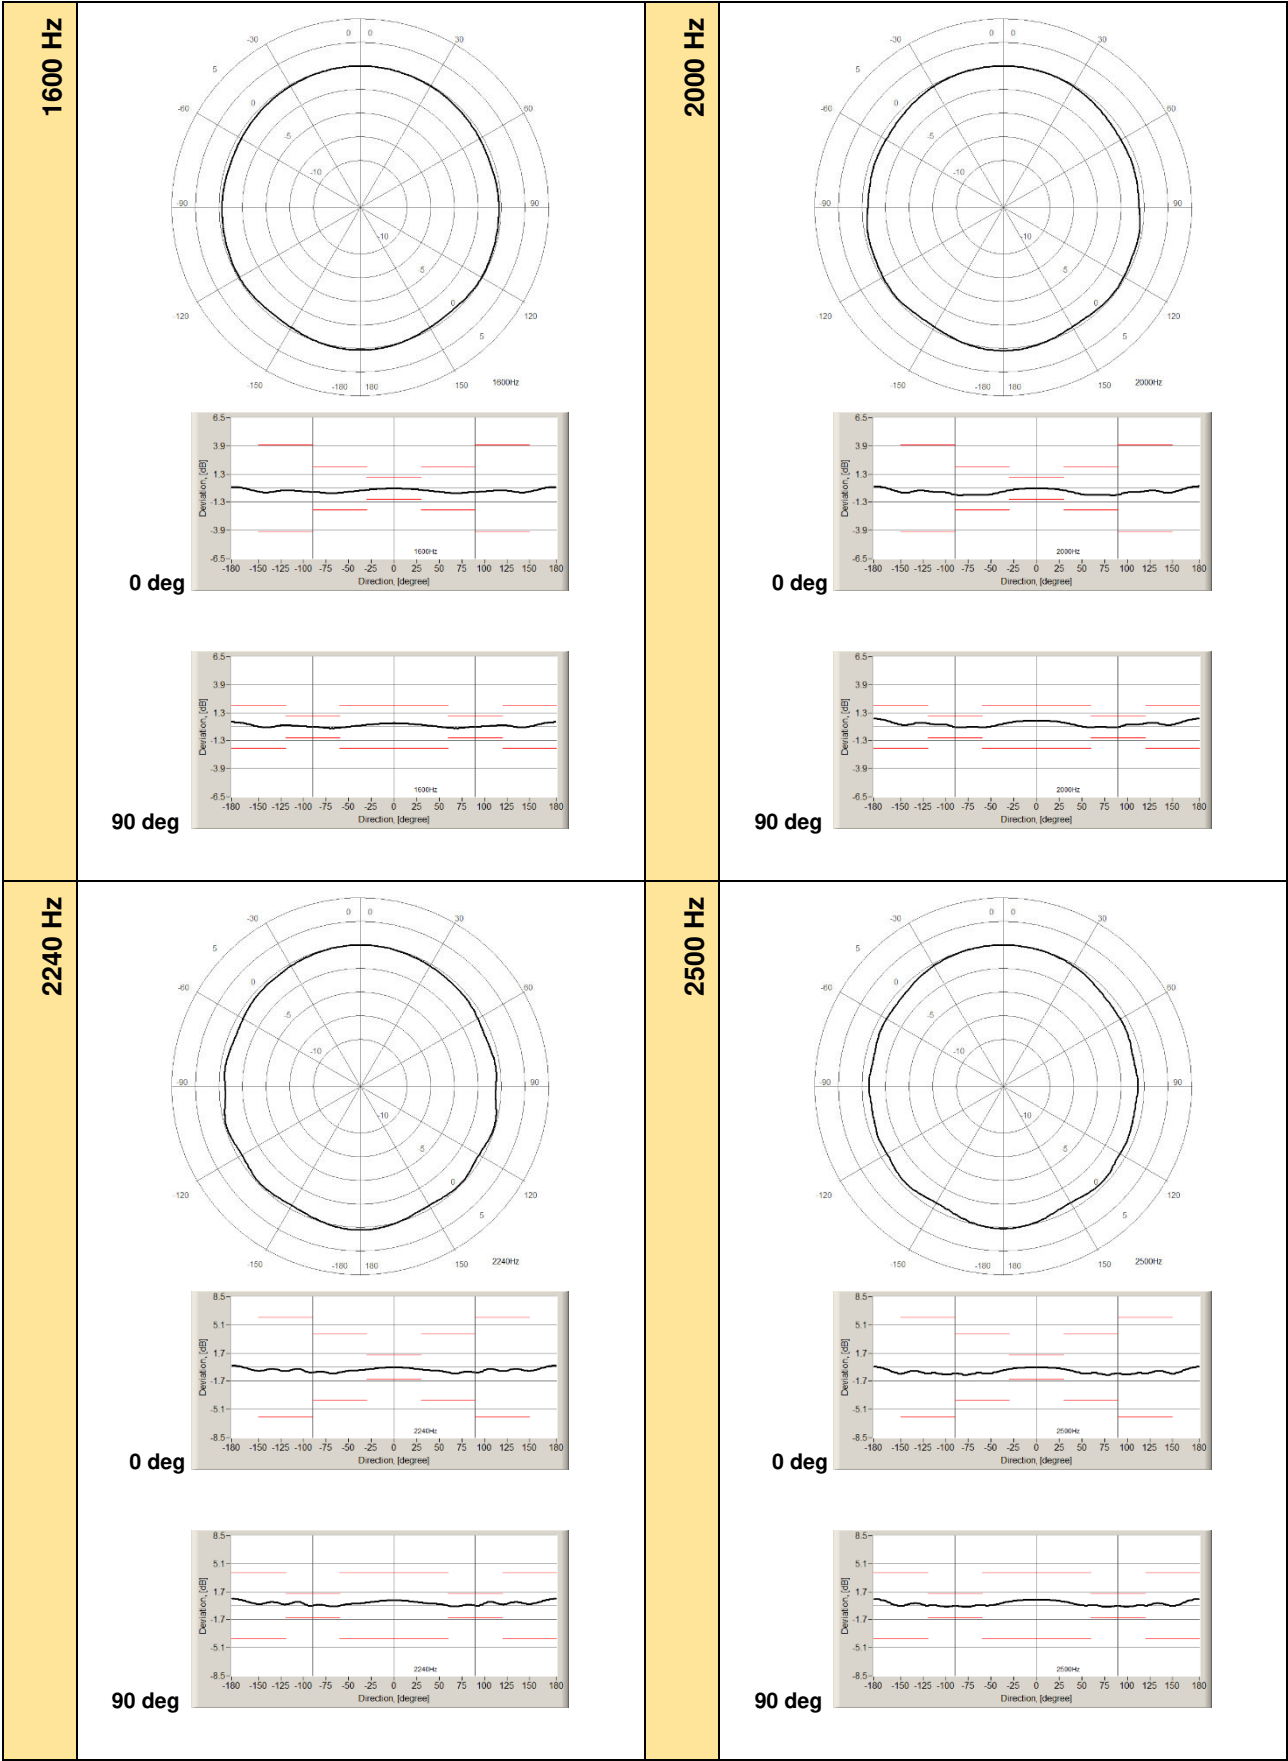


2800 Hz

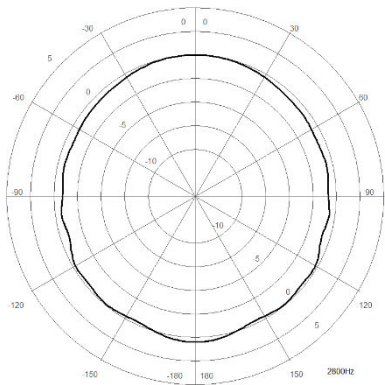


0 deg

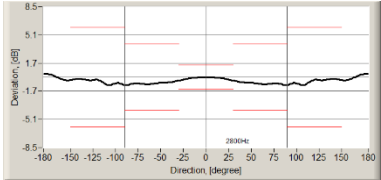


90 deg

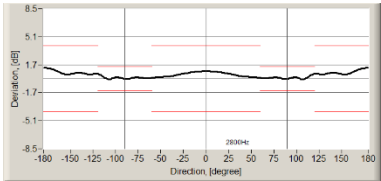


3150 Hz

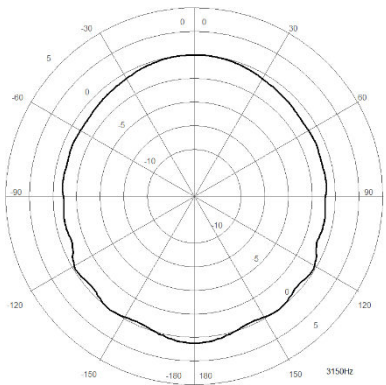


0 deg

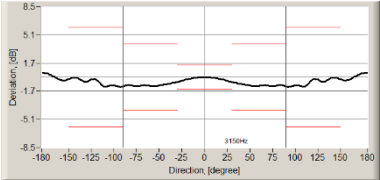


90 deg

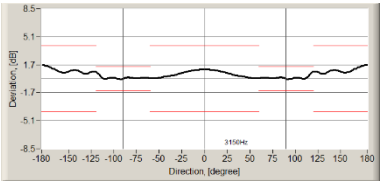


3550 Hz

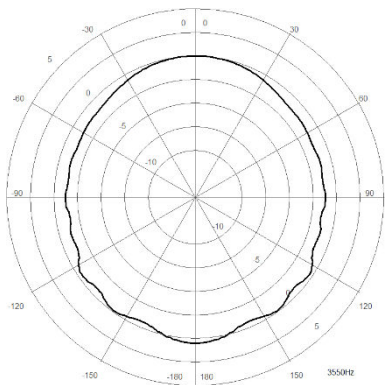


0 deg

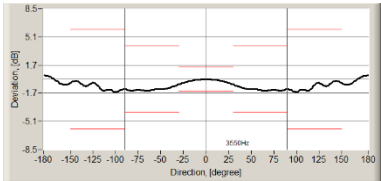


90 deg

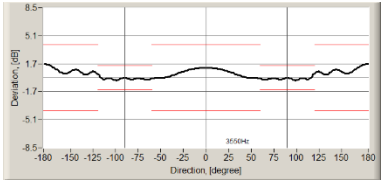


4000 Hz

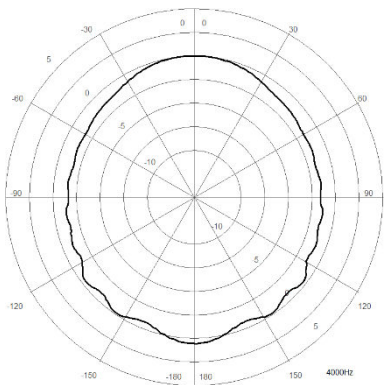



0 deg

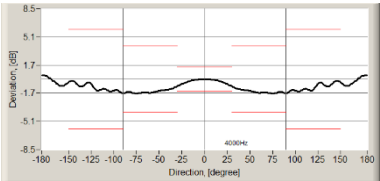


90 deg

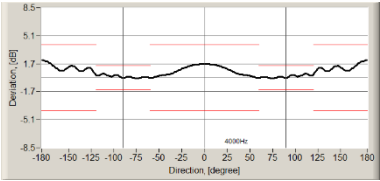

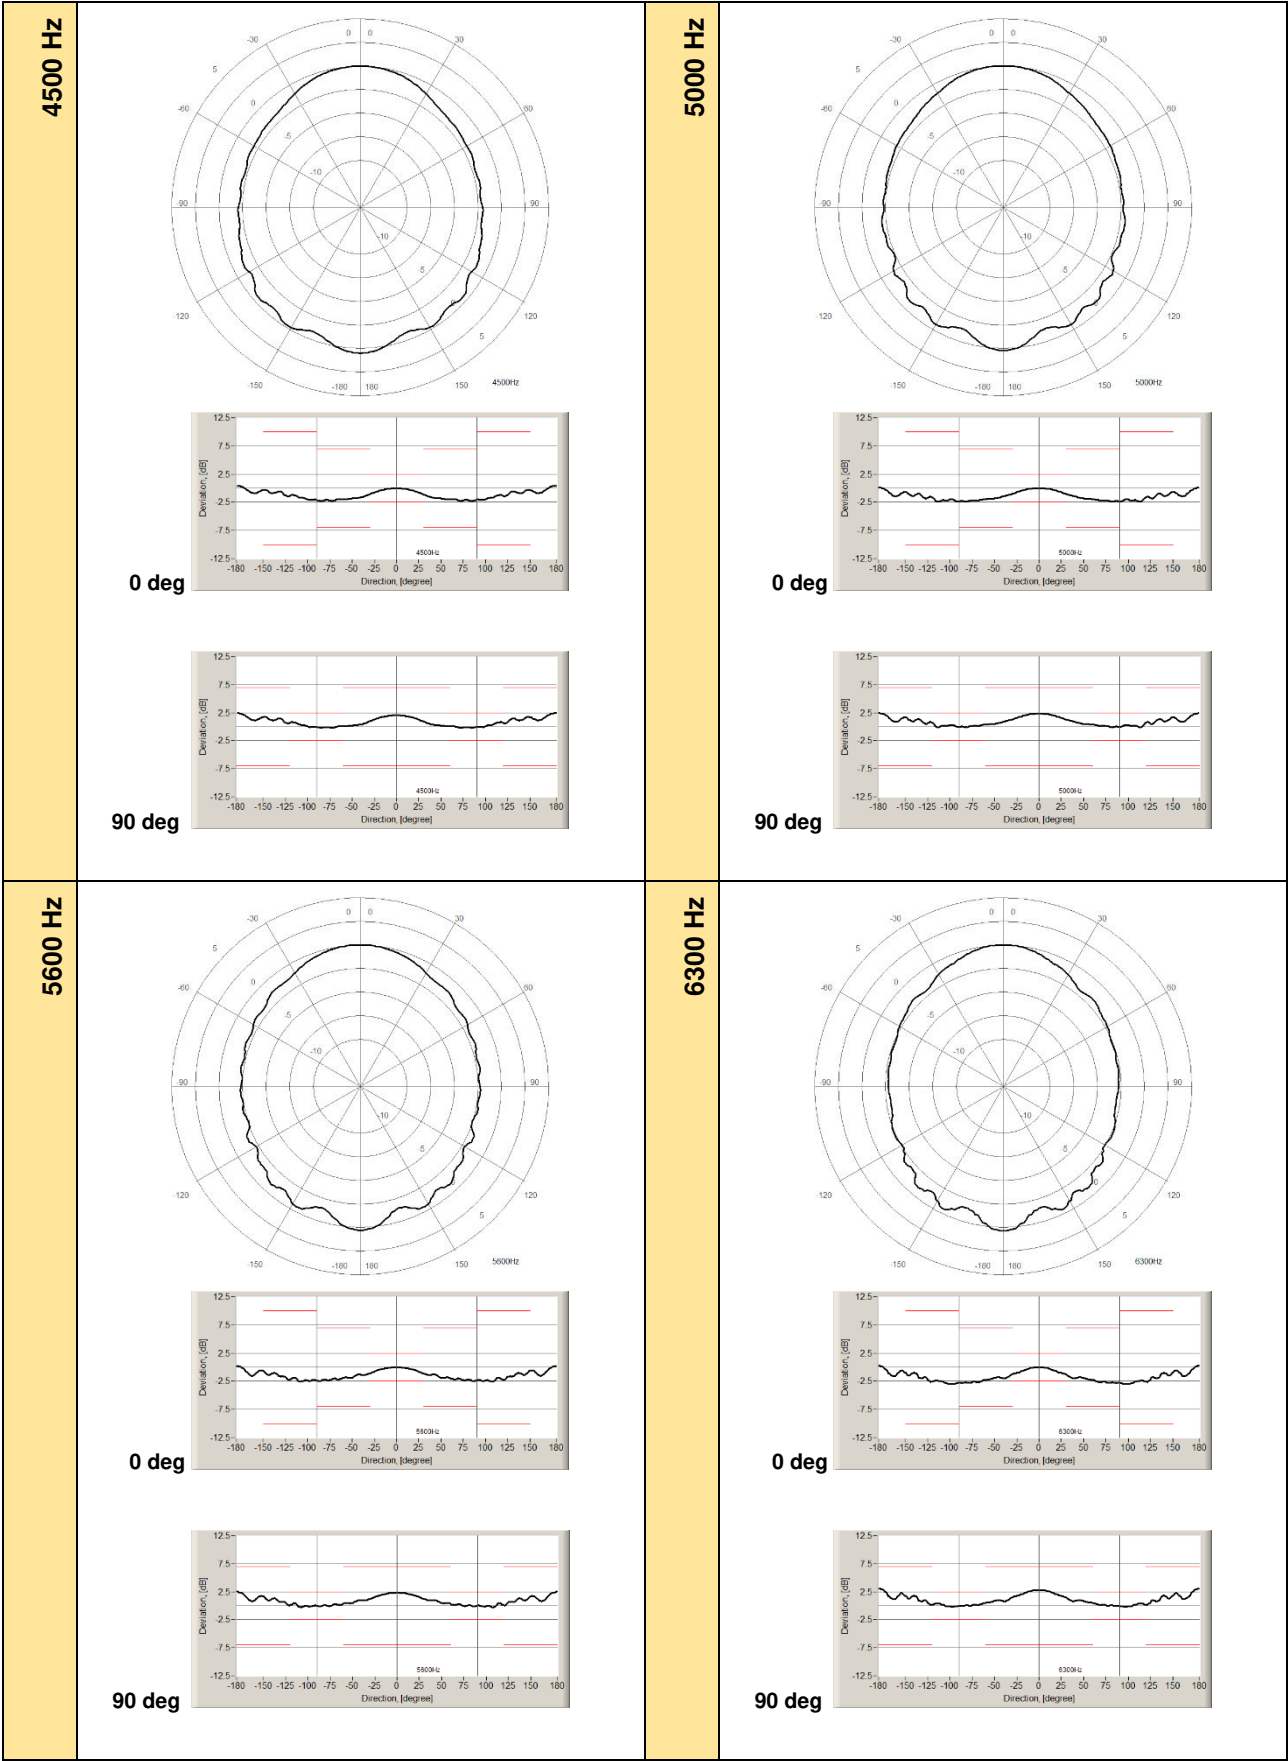

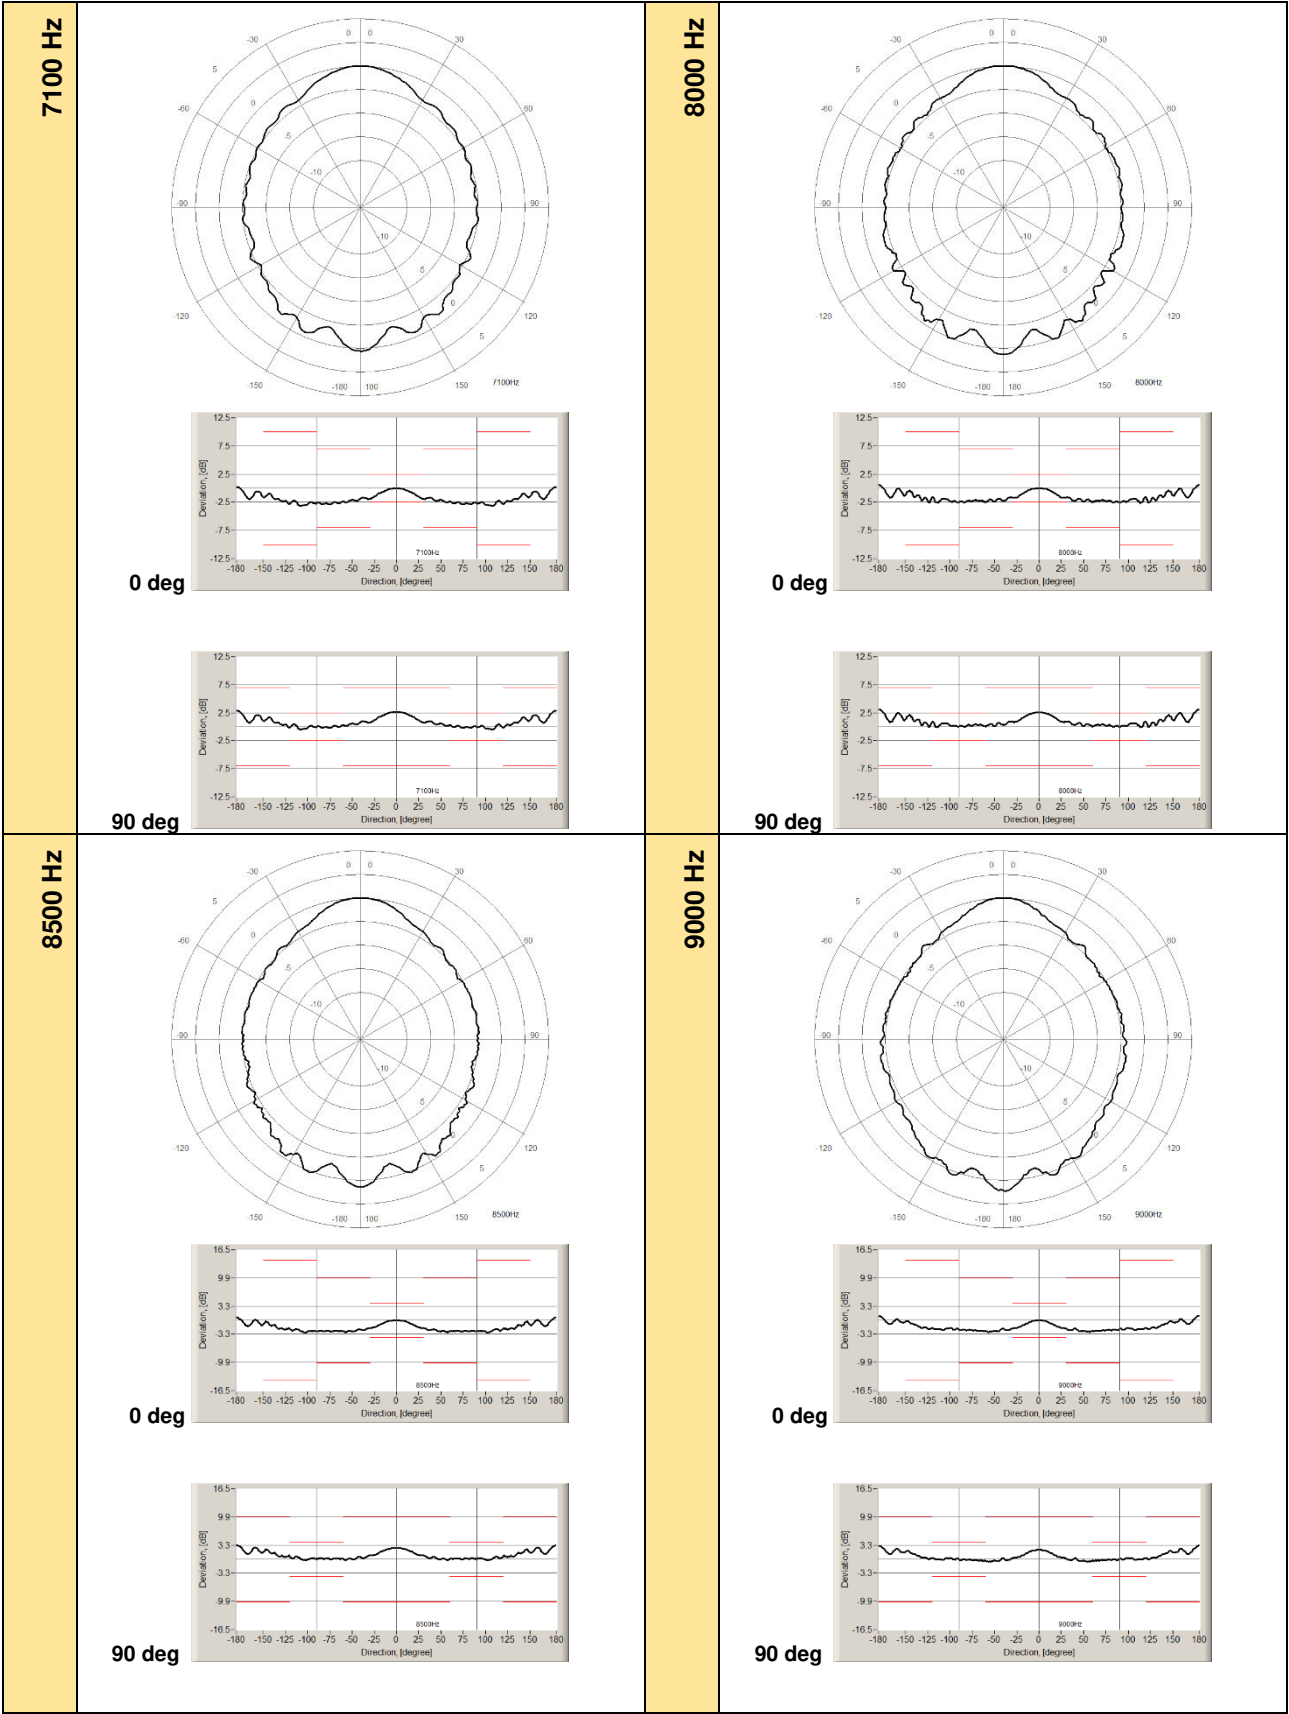

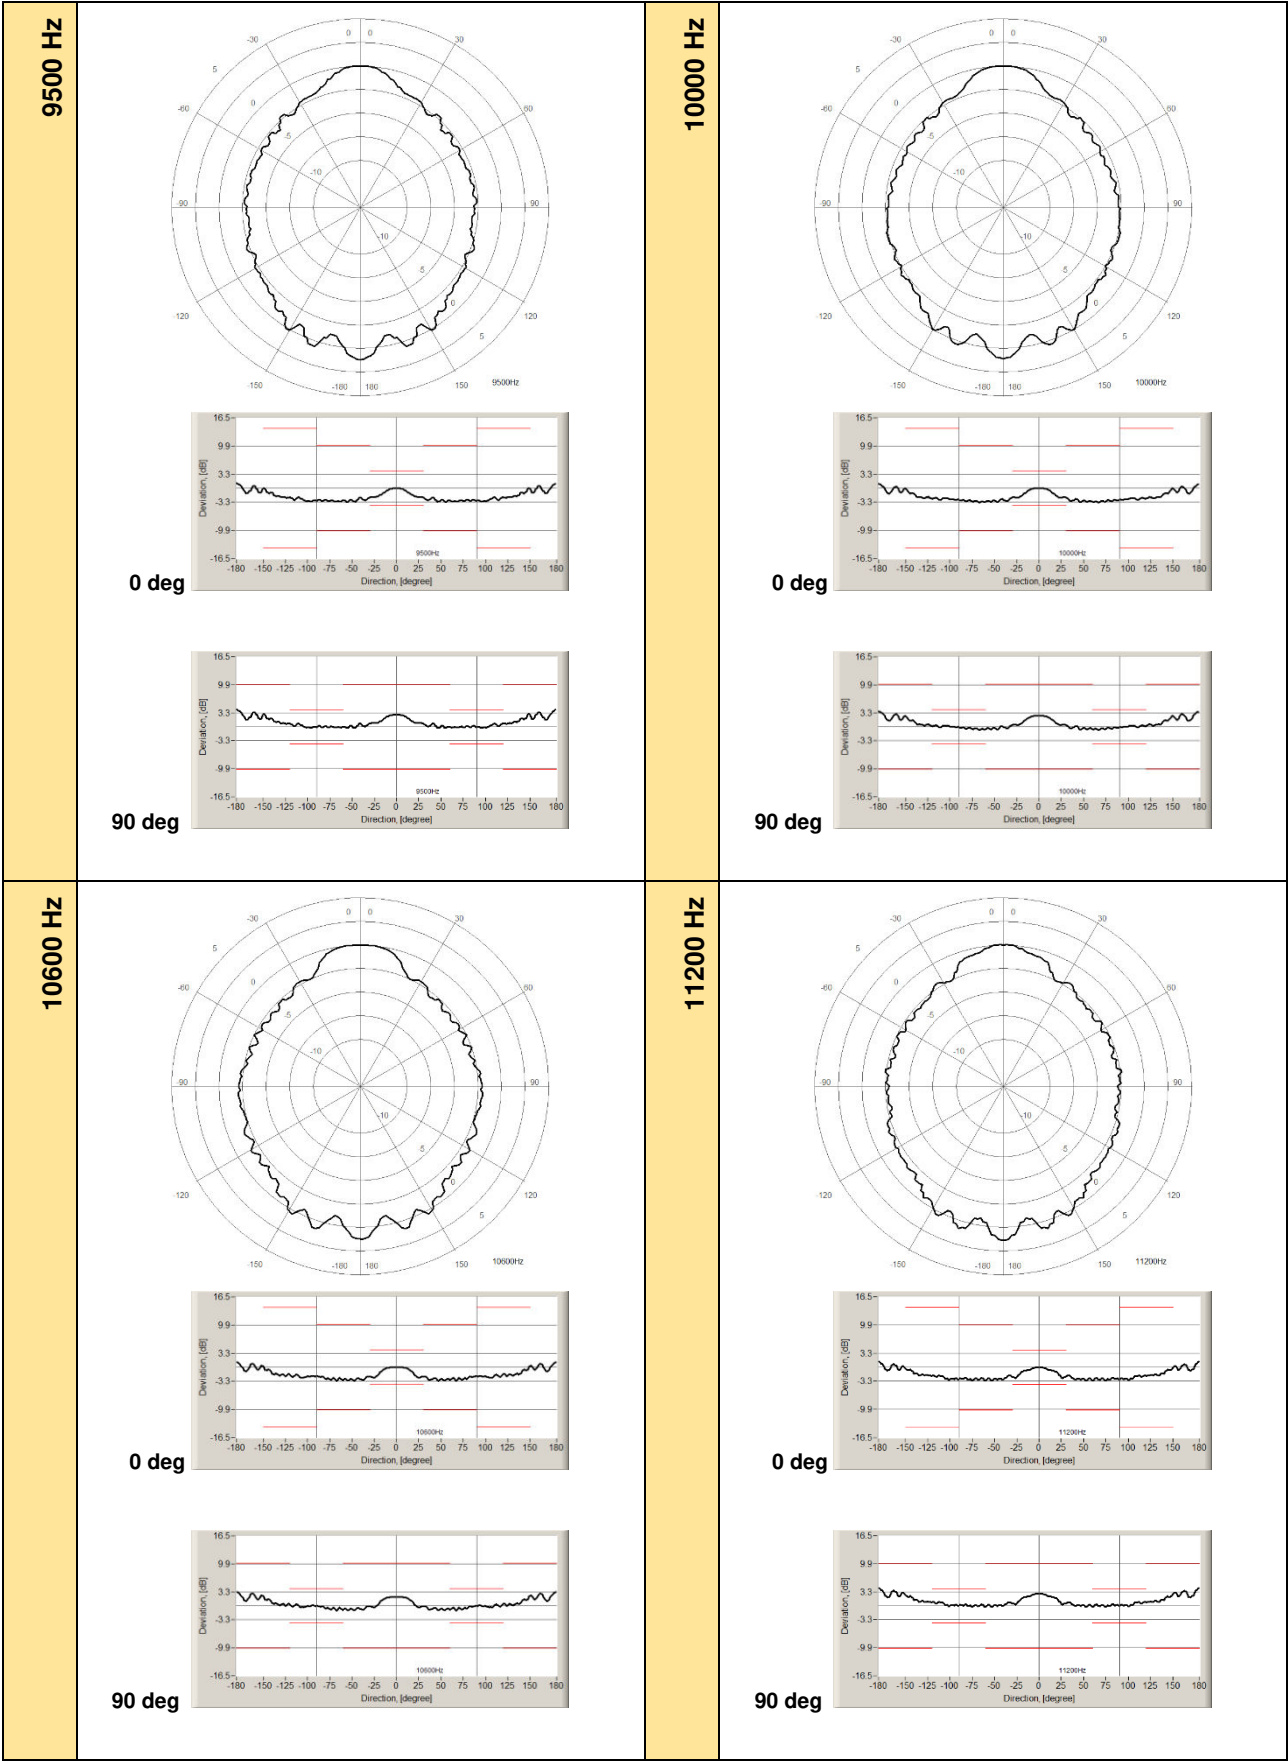

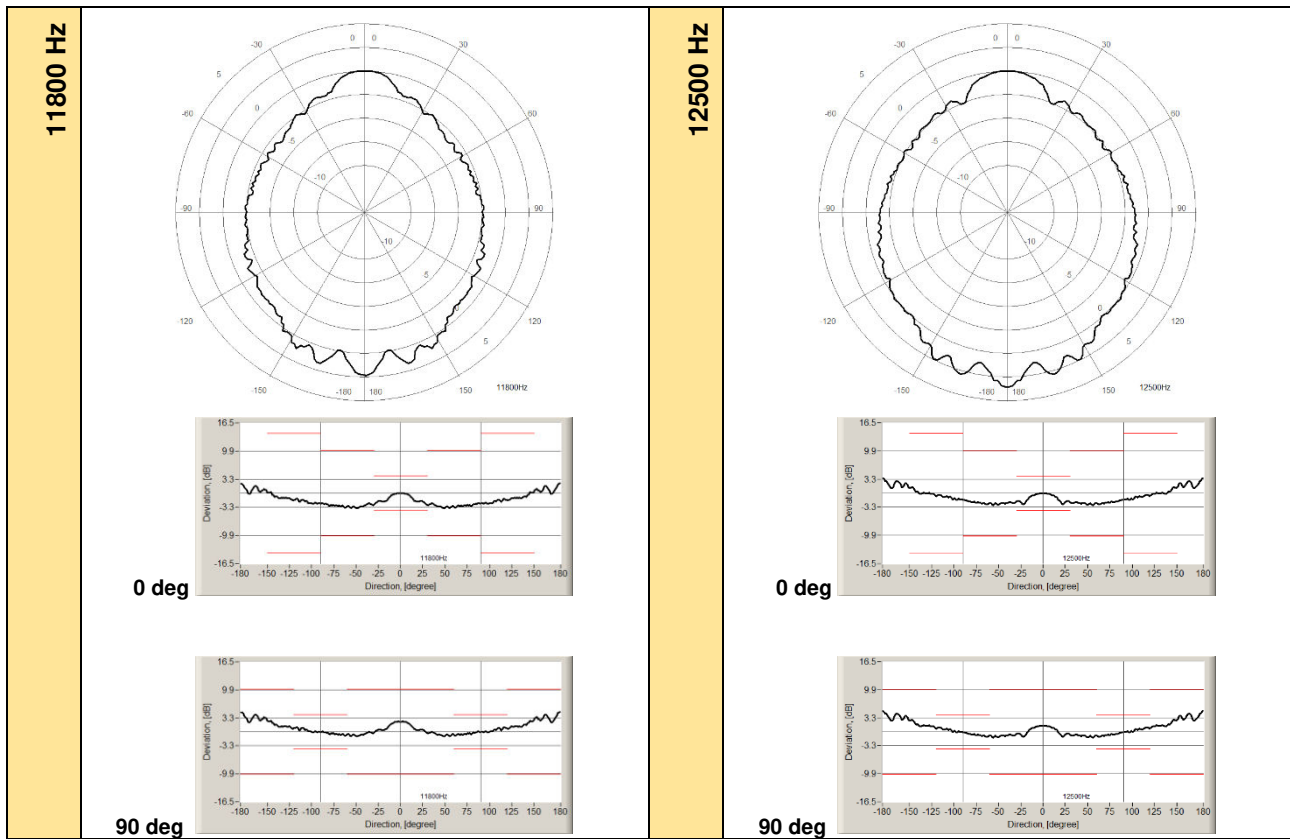


Table C.5.11. Typical directional response of SV 971A with SA 271A for 0 deg incidence angle

f [Hz]	0-10	10-20	20-30	30-40	40-50	50-60	60-70	70-80	80-90	90-100
250	-0.01	-0.01	-0.01	-0.01	0.00	0.02	0.03	0.05	0.08	0.07
315	-0.01	-0.02	-0.02	-0.03	-0.05	-0.06	-0.07	-0.07	-0.08	-0.07
400	-0.01	-0.02	-0.02	-0.04	-0.06	-0.09	-0.12	-0.15	-0.17	-0.19
500	0.00	-0.01	-0.02	-0.02	-0.04	-0.04	-0.06	-0.08	-0.09	-0.11
630	-0.01	-0.02	-0.03	-0.04	-0.05	-0.06	-0.07	-0.08	-0.10	-0.14
800	-0.02	-0.04	-0.08	-0.12	-0.18	-0.21	-0.22	-0.22	-0.21	-0.25
1 000	0.00	0.00	0.00	-0.01	-0.02	-0.07	-0.12	-0.19	-0.23	-0.23
1 250	-0.01	-0.06	-0.11	-0.19	-0.26	-0.28	-0.28	-0.34	-0.41	-0.42
1 600	-0.03	-0.09	-0.15	-0.23	-0.34	-0.41	-0.51	-0.51	-0.43	-0.38
2 000	-0.03	-0.11	-0.23	-0.37	-0.59	-0.65	-0.65	-0.65	-0.67	-0.59
2 240	-0.03	-0.13	-0.28	-0.41	-0.48	-0.67	-0.80	-0.77	-0.72	-0.74
2 500	-0.02	-0.09	-0.24	-0.42	-0.67	-0.72	-0.74	-0.89	-0.87	-0.84
2 800	-0.05	-0.19	-0.40	-0.63	-0.73	-0.81	-0.90	-0.84	-0.99	-0.92
3 150	-0.07	-0.30	-0.63	-0.81	-0.96	-1.07	-1.01	-1.04	-1.16	-1.19
3 550	-0.08	-0.32	-0.67	-1.01	-1.18	-1.22	-1.28	-1.29	-1.29	-1.45
4 000	-0.07	-0.33	-0.89	-1.22	-1.37	-1.63	-1.63	-1.66	-1.58	-1.58
4 500	-0.13	-0.57	-1.18	-1.72	-1.80	-1.94	-2.22	-2.24	-2.22	-2.07
5 000	-0.08	-0.49	-1.09	-1.49	-1.79	-2.03	-2.27	-2.34	-2.37	-2.32
5 600	-0.19	-0.51	-0.93	-1.31	-1.72	-1.83	-2.06	-2.21	-2.36	-2.41
6 300	-0.20	-0.93	-1.28	-1.90	-2.01	-2.34	-2.58	-2.62	-2.78	-2.97
7 100	-0.41	-0.94	-1.94	-1.97	-2.26	-2.55	-2.69	-2.91	-2.79	-2.83
8 000	-0.34	-1.31	-1.80	-2.41	-2.51	-2.63	-2.41	-2.36	-2.56	-2.22
8 500	-0.39	-1.52	-1.85	-2.51	-2.89	-3.00	-2.65	-2.73	-2.59	-2.93
9 000	-0.57	-1.65	-1.96	-2.46	-2.91	-3.24	-2.70	-2.54	-2.36	-2.01
9 500	-0.51	-2.09	-2.23	-2.94	-3.44	-3.48	-3.33	-3.01	-3.03	-3.15
10 000	-0.33	-2.03	-2.37	-2.97	-3.41	-3.45	-3.55	-3.28	-3.02	-2.74
10 600	-0.25	-1.85	-2.46	-2.98	-3.34	-3.35	-3.28	-3.13	-2.49	-2.44

11 200	-0.86	-1.47	-2.60	-2.80	-3.08	-3.16	-2.80	-2.72	-2.52	-2.77
11 800	-0.42	-2.06	-2.70	-2.96	-3.48	-3.53	-3.26	-3.24	-2.75	-2.79
12 500	-0.46	-2.51	-2.51	-2.25	-2.72	-2.77	-2.46	-2.37	-1.87	-1.67
f [Hz]	100-110	110-120	120-130	130-140	140-150	150-160	160-170	170-180	180-190	190-200
250	0.06	0.05	0.03	0.03	0.03	-0.01	-0.02	-0.03	-0.04	-0.04
315	-0.07	-0.05	-0.03	0.04	0.06	0.08	0.10	0.11	0.11	0.11
400	-0.21	-0.21	-0.21	-0.20	-0.18	-0.15	-0.13	-0.11	-0.10	-0.11
500	-0.12	-0.12	-0.10	-0.09	-0.05	-0.02	0.03	0.05	0.05	0.05
630	-0.18	-0.18	-0.18	-0.16	-0.11	-0.05	0.03	0.04	0.04	0.02
800	-0.32	-0.37	-0.38	-0.37	-0.30	-0.21	-0.14	-0.09	-0.09	-0.13
1 000	-0.19	-0.18	-0.21	-0.21	-0.18	-0.07	0.10	0.13	0.13	0.12
1 250	-0.35	-0.28	-0.38	-0.42	-0.41	-0.28	-0.12	-0.03	-0.03	-0.16
1 600	-0.33	-0.28	-0.28	-0.44	-0.45	-0.33	-0.16	0.11	0.11	-0.08
2 000	-0.40	-0.38	-0.28	-0.46	-0.47	-0.38	0.12	0.18	0.17	-0.19
2 240	-0.36	-0.55	-0.55	-0.31	-0.48	-0.47	-0.21	0.20	0.20	-0.18
2 500	-0.83	-0.68	-0.68	-0.52	-0.75	-0.75	-0.34	0.07	-0.12	-0.54
2 800	-1.01	-0.80	-0.39	-0.35	-0.35	-0.40	0.20	0.42	0.42	0.19
3 150	-1.18	-0.96	-0.58	-0.53	-0.33	-0.43	0.31	0.54	0.53	-0.30
3 550	-1.39	-1.27	-0.73	-0.74	-0.47	-0.65	-0.46	0.46	0.42	-0.69
4 000	-1.44	-1.35	-1.04	-0.82	-0.42	-0.78	-0.51	0.48	0.47	-0.82
4 500	-1.84	-1.46	-1.38	-0.92	-0.54	-0.89	-0.71	0.44	0.38	-0.96
5 000	-2.38	-2.45	-1.84	-1.35	-1.27	-1.39	-1.30	-0.16	-0.64	-1.52
5 600	-2.54	-2.29	-2.26	-1.58	-1.32	-1.33	-1.49	-0.35	-0.53	-1.57
6 300	-2.92	-2.73	-2.46	-2.03	-1.58	-1.64	-1.64	0.31	-1.29	-1.64
7 100	-3.08	-2.80	-2.55	-1.93	-1.54	-1.46	-1.88	-0.74	-1.53	-1.98
8 000	-2.31	-2.54	-2.45	-2.13	-1.24	-1.24	-1.68	-0.85	-1.35	-1.68
8 500	-2.76	-2.55	-2.30	-2.03	-1.22	-0.92	-1.46	0.64	-1.37	-1.52
9 000	-2.45	-2.28	-2.08	-1.73	-0.94	-0.94	-1.19	1.08	-1.15	-0.84
9 500	-2.58	-2.72	-2.22	-1.84	-1.13	-0.90	-1.14	1.11	-1.31	-1.31
10 000	-2.92	-2.68	-2.36	-2.26	-1.29	-1.06	-1.32	1.00	-1.30	-1.23
10 600	-2.64	-2.27	-1.99	-1.87	-0.69	0.88	-0.95	1.21	-1.13	0.68
11 200	-2.63	-2.16	-1.89	-1.82	-0.52	0.84	0.96	1.30	1.06	0.62
11 800	-2.53	-2.04	-1.45	-1.13	1.03	1.64	1.64	2.30	2.19	1.64
12 500	-1.55	-1.16	-0.47	0.50	1.86	2.50	3.06	3.49	3.19	2.81
f [Hz]	200-210	210-220	220-230	230-240	240-250	250-260	260-270	270-280	280-290	290-300
250	-0.04	-0.04	-0.03	-0.02	0.05	0.05	0.07	0.07	0.07	0.06
315	0.10	0.09	0.08	0.07	0.05	0.05	0.04	0.03	0.03	0.02
400	-0.12	-0.14	-0.16	-0.18	-0.19	-0.19	-0.18	-0.18	-0.16	-0.14
500	0.04	0.03	-0.01	-0.03	-0.03	-0.03	-0.03	-0.02	-0.02	-0.01
630	-0.05	-0.08	-0.10	-0.10	-0.10	-0.07	-0.04	-0.02	-0.01	-0.01
800	-0.20	-0.27	-0.29	-0.29	-0.27	-0.21	-0.16	-0.16	-0.17	-0.17
1 000	0.06	-0.11	-0.16	-0.16	-0.15	-0.18	-0.22	-0.23	-0.22	-0.17
1 250	-0.30	-0.36	-0.36	-0.30	-0.26	-0.38	-0.43	-0.42	-0.33	-0.31
1 600	-0.24	-0.35	-0.35	-0.21	-0.19	-0.24	-0.31	-0.36	-0.45	-0.46
2 000	-0.38	-0.38	-0.24	-0.26	-0.35	-0.37	-0.61	-0.64	-0.59	-0.62
2 240	-0.41	-0.41	-0.20	-0.45	-0.43	-0.26	-0.60	-0.57	-0.69	-0.71
2 500	-0.81	-0.78	-0.56	-0.81	-0.79	-0.90	-0.90	-0.92	-0.94	-0.74
2 800	-0.39	-0.33	-0.34	-0.36	-0.90	-0.93	-0.89	-0.90	-0.78	-0.84
3 150	-0.37	-0.13	-0.52	-0.49	-1.13	-1.07	-1.16	-1.00	-1.10	-1.07
3 550	-0.75	-0.58	-0.94	-1.03	-1.50	-1.66	-1.58	-1.53	-1.48	-1.54
4 000	-0.84	-0.81	-0.95	-1.45	-1.45	-1.56	-1.75	-1.75	-1.86	-1.73
4 500	-0.89	-1.02	-0.93	-1.55	-1.73	-2.08	-2.23	-2.30	-2.24	-2.09
5 000	-1.31	-1.50	-1.74	-1.90	-2.53	-2.15	-2.33	-2.41	-2.32	-2.17
5 600	-1.29	-1.48	-1.72	-2.32	-2.52	-2.73	-2.52	-2.54	-2.52	-2.33
6 300	-1.24	-1.55	-2.07	-2.77	-2.53	-3.08	-3.11	-2.93	-2.96	-2.76
7 100	-1.79	-1.65	-2.42	-2.87	-3.23	-3.23	-2.85	-2.99	-2.94	-2.71

8 000	-1.57	-1.67	-2.23	-2.57	-2.69	-2.57	-2.68	-2.66	-2.35	-2.43
8 500	-1.34	-1.44	-2.09	-2.57	-2.62	-3.02	-2.72	-2.69	-2.79	-2.76
9 000	-1.07	-1.16	-2.03	-2.32	-2.66	-2.17	-2.61	-2.58	-2.53	-2.80
9 500	-1.24	-1.37	-2.11	-2.48	-2.98	-3.30	-3.27	-3.12	-3.24	-3.11
10 000	-1.01	-1.41	-2.49	-2.53	-2.95	-2.64	-2.98	-3.21	-3.17	-3.47
10 600	-0.85	-1.61	-2.41	-2.37	-2.41	-2.51	-2.22	-2.69	-2.86	-3.12
11 200	-0.90	-1.94	-2.27	-2.43	-2.78	-3.35	-3.26	-3.38	-3.50	-3.28
11 800	1.07	-1.15	-1.36	-1.70	-2.14	-2.43	-2.46	-3.20	-3.27	-3.48
12 500	2.37	1.35	-0.21	-0.54	-0.61	-1.20	-1.60	-2.18	-2.98	-2.90
f [Hz]	300-310	310-320	320-330	330-340	340-350	350-360				
250	0.05	0.03	0.02	0.01	0.01	0.01				
315	0.02	0.02	0.03	0.02	0.02	0.01				
400	-0.11	-0.08	-0.06	-0.04	-0.01	0.00				
500	-0.01	-0.01	-0.01	0.00	0.00	0.00				
630	-0.01	-0.01	-0.01	0.01	0.01	0.01				
800	-0.15	-0.12	-0.08	-0.05	-0.02	-0.01				
1 000	-0.12	-0.08	-0.06	-0.04	-0.02	-0.01				
1 250	-0.31	-0.29	-0.23	-0.13	-0.07	-0.02				
1 600	-0.41	-0.34	-0.23	-0.15	-0.08	-0.02				
2 000	-0.62	-0.50	-0.31	-0.15	-0.05	0.00				
2 240	-0.60	-0.40	-0.33	-0.25	-0.11	-0.02				
2 500	-0.75	-0.72	-0.45	-0.21	-0.08	-0.02				
2 800	-0.79	-0.64	-0.56	-0.40	-0.14	-0.02				
3 150	-1.11	-1.03	-0.77	-0.51	-0.24	-0.05				
3 550	-1.34	-1.28	-1.01	-0.56	-0.24	-0.06				
4 000	-1.73	-1.38	-1.25	-0.77	-0.31	-0.06				
4 500	-2.00	-1.77	-1.53	-0.95	-0.43	-0.10				
5 000	-1.88	-1.80	-1.27	-0.97	-0.43	-0.05				
5 600	-2.04	-1.86	-1.43	-0.99	-0.46	-0.03				
6 300	-2.38	-2.06	-2.06	-1.03	-0.66	-0.18				
7 100	-2.46	-2.19	-1.87	-1.77	-0.92	-0.09				
8 000	-2.26	-2.09	-1.99	-1.54	-0.85	-0.07				
8 500	-2.72	-2.63	-2.23	-1.66	-0.94	-0.06				
9 000	-2.87	-2.66	-2.35	-1.78	-1.08	-0.11				
9 500	-3.12	-3.22	-2.83	-1.98	-1.49	-0.28				
10 000	-3.10	-3.29	-3.10	-2.20	-1.61	-0.35				
10 600	-2.98	-3.03	-3.04	-2.45	-1.11	0.04				
11 200	-3.21	-3.00	-2.63	-2.63	-0.97	-0.09				
11 800	-3.51	-3.44	-2.92	-2.27	-1.93	-0.45				
12 500	-2.91	-2.74	-2.56	-2.59	-2.00	-0.10				

C.6 DECLARATION OF CONFORMITY

Manufacturer:	SVANTEK Sp. z o. o
Address:	Strzyglowska 81 04-872 Warszawa Poland
Kind of product:	SOUND LEVEL METER – ANALYZER, Class 1
Type:	SV 971A
Directive:	Directive 2014/53/EU of The European Parliament and of The Council of 16 April 2014 on the harmonization of the laws of the Member States relating to the making available on the market of radio equipment and repealing Directive 1999/5/EC (OJ L 153/62 of 22.5.2014).
Standards:	EN 61010-1:2010 Safety requirements for electrical equipment for measurement, control, and laboratory use - Part 1: General requirements
Art 3.1a: Safety	
Art 3.1b: EMC	ETSI EN 301 489-1 V2.2.3. Electromagnetic compatibility (EMC) standard for radio equipment and services; Part 1: Common technical requirements; Harmonised standard for Electromagnetic Compatibility. ETSI EN 301 489-17 V3.2.4. Electromagnetic Compatibility (EMC) standard for radio equipment and services; Part 17: Specific conditions for Broadband Data Transmission Systems; Harmonised standard for Electromagnetic Compatibility. EN 61000-4-2:2009. Electromagnetic compatibility (EMC). Testing and measurement techniques. Part 4-2; Electrostatic discharge immunity test. EN 61000-4-3:2006 + A1:2008 + A2:2010 + ISI:2009. Electromagnetic compatibility (EMC). Testing and measurement techniques. Part 4-3; Radiated, radio-frequency, electromagnetic field immunity test. EN 61000-4-8:2010. Electromagnetic compatibility (EMC). Part 4-8: Testing and measurement techniques - Power frequency magnetic field immunity test. EN 61000-4-20:2010. Electromagnetic compatibility (EMC). Testing and measurement techniques. Part 4-20: Emission and immunity testing in traverse electromagnetic (TEM) waveguides.
Art 3.2: Radio	ETSI EN 300 328 V2.2.2. Wideband transmission systems; Data transmission equipment operating in the 2,4 GHz band; Harmonised standard for access to radio spectrum.
Directive:	Restriction of Hazardous Substances (ROHS II) 2011/65/EU
Standards:	EN 50581:2012 <i>Assessment of electronic products with respect to RoHS</i> Auxiliary industry standards: EN 61672-1:2013. Electroacoustics - Sound level meters – Part 1: Specifications. EN 61260-1:2014. Octave-band filters

APPENDIX D. DEFINITIONS AND FORMULAE OF MEASURED VALUES

D.1 BASIC TERMS AND DEFINITIONS

T	Current time period of the measurement in seconds.
T_l	Last second of the measurement.
T_e	Exposure time in seconds (time period during which a person is exposed to the action of noise). This parameter can be set in the Exposure Time setup (Measurement menu). The available values are from 1 minute to 12 hours with 1-minute step.
T_{8h}	Time period equal to 8 hours (28 800 seconds).
τ	Exponential time constant in seconds for the giving time-weighting. Three time constants are available: Slow (1000 ms), Fast (125 ms), Impulse (35 ms, but on falling values a longer time constant of 1500 ms is applied).
W	Frequency-weighting filter: A , C , B or Z .
p_w(t)	Instantaneous frequency-weighted sound pressure with the weighting filter W . Sound pressure is expressed in pascals (Pa).
p_{wτ}(t)	<p>Instantaneous frequency and time-weighted sound pressure with the weighting filter W and time constant τ calculated from the equation:</p> $p_{w\tau}(t) = \sqrt{\frac{1}{\tau} \int_{-\infty}^t p_w^2(\xi) e^{-(t-\xi)/\tau} d\xi}$ <p>where: ξ – variable of integration.</p>
r(t)	<p>Instantaneous sound pressure depends on the <RMS Integration> parameter:</p> $r(t) = \begin{cases} p_w(t) & \text{RMS Integration = Lin} \\ p_{w\tau}(t) & \text{RMS Integration = Exp} \end{cases}$
p₀	Reference value (20 μPa).
log(x)	Logarithm of x to the base 10.
Q	Exchange rate in decibels is equal to 2, 3, 4, 5 or 6. The value of Q influences the calculations of dose meter results, namely DOSE , D_{8h} and LAV . The exposure rate equal to 3 complies with ISO R 1999 “Assessment of Occupational Noise Exposure for Hearing Conservation Purposes”, while Q equal to 5 complies with the American “Occupational Safety and Health Act” – OSHA.
q	<p>Value of q is used in the calculations of DOSE, D_{8h} and LAV is taken from the formula</p> $q = \begin{cases} \frac{Q}{\log 2} & \text{for } Q \neq 3 \\ 10 & \text{for } Q = 3 \end{cases}$

L_T Threshold sound level set in the **Threshold Level** parameter. The available values are as follows: **None**, **60dB** up to **90dB** in 5 dB steps.

L_C Criterion sound level set in the **Criterion Level** parameter. The available values are from **60dB** up to **90dB** in 5 dB steps.

L(t) Sound level (a function of time) measured with the selected time constant (**Impulse**, **Fast** or **Slow**) and the weighting filter (equal to **A**, **C** or **Z**)

$$L(t) = 20 \log \frac{p_w(t)}{p_0}$$

L_d(t) Sound level (a function of time) depends on the selected threshold level.

In the case **None** option is selected


$$L_d(t) = L(t)$$

In other cases (when **Threshold Level** is not set to none and equal to **60 dB** ... or up to **90 dB**)

$$L_d(t) = \begin{cases} L(t) & \text{for } L(t) \geq L_T \\ -\infty & \text{for } L(t) < L_T \end{cases}$$

D.2 DEFINITIONS AND FORMULAS OF THE SLM RESULT

The instrument calculates the sound measurement results for three profiles. The calculation flow diagram for one profile is presented below:

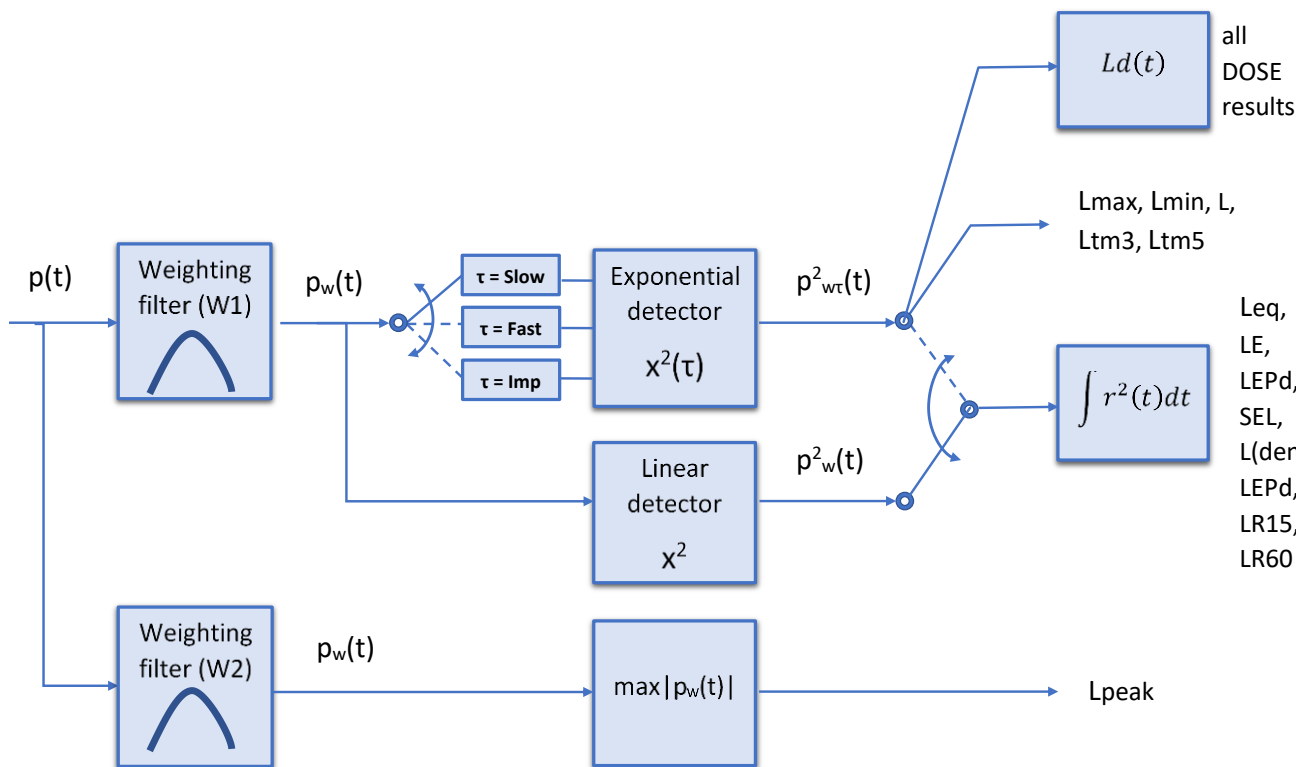

OVL Percentage of the overloaded input signal, which occurred during the current time period of the measurement (**T**)

L(A/C/Z)peak

Peak sound level expressed in dB, for frequency weightings A, C, Z, symbols are **LApeak**, **LCpeak** and **LZpeak**. Peak sound level is calculated for the given **T**.

$$\text{Peak} = 10 \log \left(\max_T \frac{p_w^2(t)}{p_0^2} \right)$$

L(A/C/Z)(S/F/I)max

The highest time weighted sound level (**Max**) expressed in dB, within a stated time interval, for frequency weightings A, C, Z and time weightings F, S, I symbols are **LAFmax**, **LASmax**, **LCFmax**, **LCSmax** etc.

$$\text{Max} = 10 \log \left(\max_T \frac{p_{wT}^2(t)}{p_0^2} \right)$$

L(A/C/Z)(S/F/I)min

The lowest time weighted sound level (**Min**) expressed in dB, within a stated time interval, for frequency weightings A, C, Z and time weightings F, S, I symbols are **LAFmin**, **LASmin**, **LCFmin**, **LCSmin** etc.

$$\text{Min} = 10 \log \left(\min_T \frac{p_{wT}^2(t)}{p_0^2} \right)$$

L(A/C/Z)(S/F/I)

Time weighted sound level expressed at observation time, expressed in dB, for frequency weightings A, C, Z and time weightings F, S, I symbols are **LAF**, **LAS**, **LCF**, **LCS** etc.

$$L = 10 \log \left(\frac{p_{wT}^2(t)}{p_0^2} \right)$$

L(A/C/Z)eq

Time averaged equivalent continuous sound level (**Leq**) expressed in dB, for frequency weightings A, C, Z symbols are **LAeq**, **LCeq** and **LZeq**. In principle time weighting is not involved in a determination of time averaged sound level. Time-averaged sound level is calculated for current time period of the measurement (**T**).

$$\text{Leq} = 10 \log \left(\frac{1}{T} \int_0^T (r(t)/p_0)^2 dt \right)$$

L(A/C/Z)E

Sound Exposure Level (**SEL**) expressed in dB, for frequency weightings A, C, Z, symbols are **LAE**, **LCE** and **LZE**. **SEL** is essentially the subset of the **Leq** result. Its value is equal to the **Leq** result referred to the integration time equal to one second (so, for the Integration time equal to 1 s, **SEL** is always equal to **Leq**).

$$\text{SEL} = 10 \log \left(\int_0^T (r(t)/p_0)^2 dt \right) = \text{Leq} + 10 \log \frac{T}{1s}$$

L(den)

Only one result from: **Lday**, **Leve**, **Lnight**, **Lde**, **Len**, **Lnd**, and **Lden** is available in the instrument. It depends on the day and night time in which the measurement was performed. Day and night time depend on the **<Day Time Limits>** option (**6h-18h** or **7h-19h**).

If **<6h-18h>** option is selected for the **<Day Time Limits>** in the instrument then:

T_d (day-time) starts from 6 am and ends at 6 pm,

T_e (evening-time) starts from 6 pm and ends at 10 pm,

T_n (night-time) starts at 10 pm and ends at 6 am.

If **<7h-19h>** option is selected for the **<Day Time Limits>** in the instrument then:

T_d (day-time) starts from 7 am and ends at 7 pm,

T_e (evening-time) starts from 7 pm and ends at 11 pm,

T_n (night-time) starts at 11 pm and ends at 7 am.

Lday

Lday is calculated for: $T_d \neq 0$, $T_e = 0$,
 $T_n = 0$.

$$L_d = 10 \log \left(\frac{1}{T_d} \int_{T_d} (r_w(t)/p_0)^2 dt \right)$$

Leve

Leve is calculated for: $T_d = 0$, $T_e \neq 0$,
 $T_n = 0$.

$$L_e = 5 \text{ dB} + 10 \log \left(\frac{1}{T_e} \int_{T_e} (r_w(t)/p_0)^2 dt \right)$$

Lnight

Lnight is calculated for: $T_d = 0$, $T_e = 0$,
 $T_n \neq 0$.

$$L_n = 10 \text{ dB} + 10 \log \left(\frac{1}{T_n} \int_{T_n} (r_w(t)/p_0)^2 dt \right)$$

Lde

Lde is calculated for: $T_d \neq 0$, $T_e \neq 0$,
 $T_n = 0$.

$$L_{de} = 10 \log \left[\frac{1}{12+4} (12 \cdot 10^{L_d/10} + 4 \cdot 10^{L_e/10}) \right]$$

Len

Len is calculated for: $T_d = 0$, $T_e \neq 0$,
 $T_n \neq 0$.

$$L_{en} = 10 \log \left[\frac{1}{4+8} (4 \cdot 10^{L_e/10} + 8 \cdot 10^{L_n/10}) \right]$$

Lnd

Lnd is calculated for: $T_d \neq 0$, $T_e = 0$,
 $T_n \neq 0$.

$$L_{nd} = 10 \log \left[\frac{1}{8+12} (8 \cdot 10^{L_n/10} + 12 \cdot 10^{L_d/10}) \right]$$

Lden

Lden is calculated for: $T_d \neq 0$, $T_e \neq 0$,
 $T_n \neq 0$.

$$L_{den} = 10 \log \left[\frac{1}{12+8+4} (12 \cdot 10^{L_d/10} + 4 \cdot 10^{L_e/10} + 8 \cdot 10^{L_n/10}) \right]$$

LEPd

Daily Personal Noise Exposure is the noise exposure level for a nominal 8-hour working day. The **LEPd** result is calculated on the base of the **LEQ**

$$LEPd = Leq + 10 \log \frac{T_e}{T_{8h}}$$

Ltm3 and Ltm5

The **Ltm3** and **Ltm5** results (Takt-Maximal Levels) are calculated according to the German standard TA Lärm.

Ln Statistical level is the certain boundary level surpassed by the temporary noise level values in not more than **n**% of the observation period see Chapter D.4

EX Expected value. Calculated on the basis of 100ms Leq results.

SD Standard deviation. Calculated on the basis of 100ms Leq results.

LR Rolling Leq measured in the time window for the last **Tw** seconds of the measurement. LR window is moving with 1 second step.

$$LR(Tw) = 10 \log \left(\frac{1}{Tw} \int_{T-Tw}^T (r(t)/p_0)^2 dt \right)$$



Note: If the current measurement time **T** is less than the time window **Tw** the **LR** result is undefined.

D.3 DEFINITIONS AND FORMULAS OF THE ADDITIONAL DOSIMETER FUNCTION RESULTS

DOSE Quantity of noise received by the worker, expressed as the percentage of the whole day acceptable value.

$$DOSE = \frac{100\%}{T_{8h}} \int_0^T 10^{\frac{L_d(t)-L_c}{q}} dt$$

D_8h Quantity of noise received by the worker during 8 hours.

$$D_{8h} = \frac{100\%}{T} \int_0^T 10^{\frac{L_d(t)-L_c}{q}} dt = \frac{T_{8h}}{T} \cdot DOSE$$

PrDOSE Quantity of noise received by the worker during exposure time.

$$Pr DOSE = \frac{100\%}{T} \int_0^T 10^{\frac{L_d(t)-L_c}{q}} dt = \frac{T_e}{T} \cdot DOSE$$

LAV Average level of the acoustic pressure for the given time period of the measurement.

$$LAV = q \cdot \log \left(\frac{1}{T} \int_0^T 10^{\frac{L_d(t)}{q}} dt \right)$$

SEL8 **SEL** result corresponding to the integration time equal to 8 hours. The **SEL8** result is calculated on the base of the **LEQ**.

$$SEL8 = LEQ + 10 \cdot \log \frac{T_{8h}[s]}{1[s]}$$

PSEL Individual Sound Exposure Level to the noise is equal to the standing sound level in a measurement period. The **PSEL** result is calculated on the base of the **LEQ**.

$$PSEL = LEQ + 10 \cdot \log \frac{T}{T_{8h}}$$

E	Amount of the acoustical energy received by the worker.	$E = \frac{T[s]}{3600} p_o^2 \cdot 10^{\frac{LEQ}{10}}$
E_8h	The E_8h result (Exposition in 8 hours) represents the amount of the acoustical energy received by the worker during 8 hours. The E_8h result is expressed in the linear units [Pa ² h].	$E_{8h} = 8[h] \cdot p_o^2 \cdot 10^{\frac{LEQ}{10}}$
PTC	Peak Threshold Counter – the number of the overpasses of the Threshold Level by Lpeak result. This result is incremented in 100 ms intervals.	
PTP	PTC result expressed in percent.	$PTP = \frac{100 \cdot PTC}{10T_c}$
ULT	Upper Limit Time - time that SPL exceeded the “ULT Threshold Level” set during configuration.	
TWA	Time Weighted Average is the average A-weighted sound level for a nominal 8-hour workday with Time Weighting S and Exchange Rate 5. TWA is usually measured with A-weighting and Slow response detector type. TWA is calculated from the measured LAV (taking Threshold Level into account) and a Reference time of 8 h. Mainly used in the USA for assessing the noise exposure for a worker during a workday.	<ul style="list-style-type: none"> • Sound levels at or above the THRESHOLD LEVEL are averaged into the calculations relating to noise exposure. TWA is calculated with no threshold level, or with threshold level (typically 80dB or 90dB) • In the case the time period is below 8 hours, the TWA is less than the LAV. In the case the time period is more than 8 hours, the TWA is greater than the LAV
PrTWA	Projected Time Weighted Average is calculated from the measured LAV (taking THRESHOLD LEVEL into account) and the exposure time.	
Lc-a	The C-A measurement is an Leq that enhances the low-frequency components of the sound signal. It is the result of subtracting an A-weighted LAeq from a simultaneously collected C-weighted Leq	$Lc-a = LCeq - LAeq$

D.4 STATISTICAL LEVELS – LN DEFINITION

The noise level **L(t)** is the continuous random variable. The probability that the temporary noise level **L(t)** belongs to the interval $\langle L_k, L_k + \Delta L \rangle$ is called the class density and it can be expressed by the equation:

$$P_k [L_k \leq L(t) \leq L_k + \Delta L] = \sum_{i=1}^n \Delta t_i / P$$

where: Δt_i - time intervals, in which the noise level $L(t) \in \langle L_k, L_k + \Delta L \rangle$ occurs,

ΔL - so-called class interval or distribution class of the series,

P - total observation period.

In the case when the class interval approaches infinity, the probability of **L(t)** tends to the probability of **L_k**. In practice, **ΔL** value is strictly determined for the measuring instrument. For SV 971A, there are 240 classes and the width of each class is 0.5 dB. The histogram is the set of the class density values calculated for all classes.

The statistical distribution function, which determines the probability (expressed in %) of the noise occurrence on the level equal or less than **L_k + ΔL** is given by the formulae:

$$P[L(t) \leq L_j] = \sum_{k=1}^j P_k(L)$$

The cumulative density function expressed by the equation:

$$P[L(t) > L_j] = 1 - P[L(t) \leq L_j]$$

is directly used to determine so-called statistical levels **Ln** or position parameters of the distribution.

The **Ln** is the certain boundary level surpassed by the temporary noise level values in not more than **n%** of the observation period.


Example:

Let us assume that **L35** is equal to 76.8 dB. It means that during the measurements the noise level 76.8 dB was exceeded in not more than 35% of the observation period.

The cumulative density function for the exemplary data is presented in Figure on the right side. In order to determine the **Ln** level, one must draw the horizontal cursor and find out the crossing point between the cumulative density function and the cursor. In the instrument the user can determine 10 statistical levels - from **L01** to **L99** (1% step of observation period).

The statistical level **Ln** value, the profile's number the statistics are taken from, the RMS detector (**Lin.**, or **Exp.: Fast, Slow or Imp.**), the filter's name (**A, C or Z**) and real time are displayed in the top-right side of the display in one-result view mode.

Exemplary cumulative density

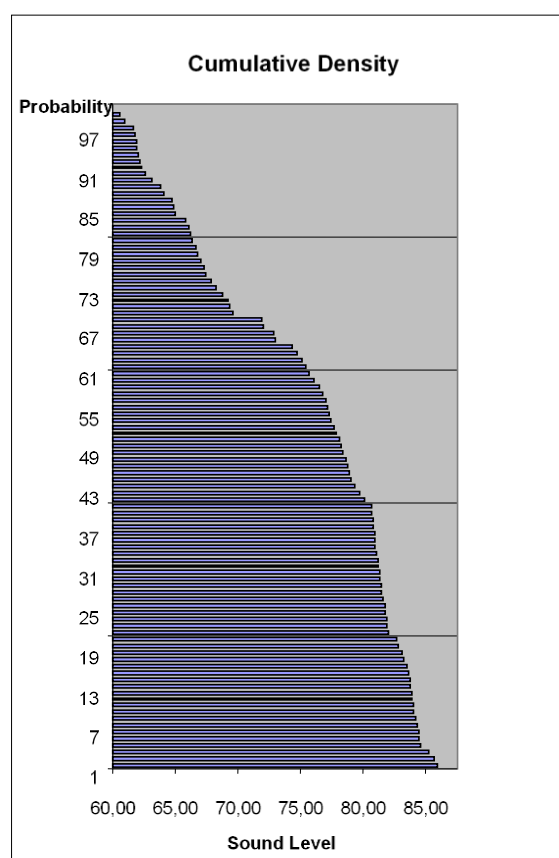

APPENDIX E. REVERBERATION TIME CALCULATIONS

E.1 INTRODUCTION

If an impulsive sound is generated in a room with reflecting boundaries, repeated reflections at the boundaries result in the rapid establishment of a more or less uniform sound field. This field then decays as the sound energy is absorbed by the bounding materials. The rate at which the sound energy decays is determined by the absorptive properties of the reflecting surfaces and the distances between them. The time taken for the sound intensity or the sound pressure level to decay by 60 dB is called the **reverberation time** (RT). The values of RT may range from fractions of a second to a few seconds and depend upon the size of the room and the nature of the materials used in its construction.

The graphs below present the reverberation time nature (in the case when only one frequency is emitted):

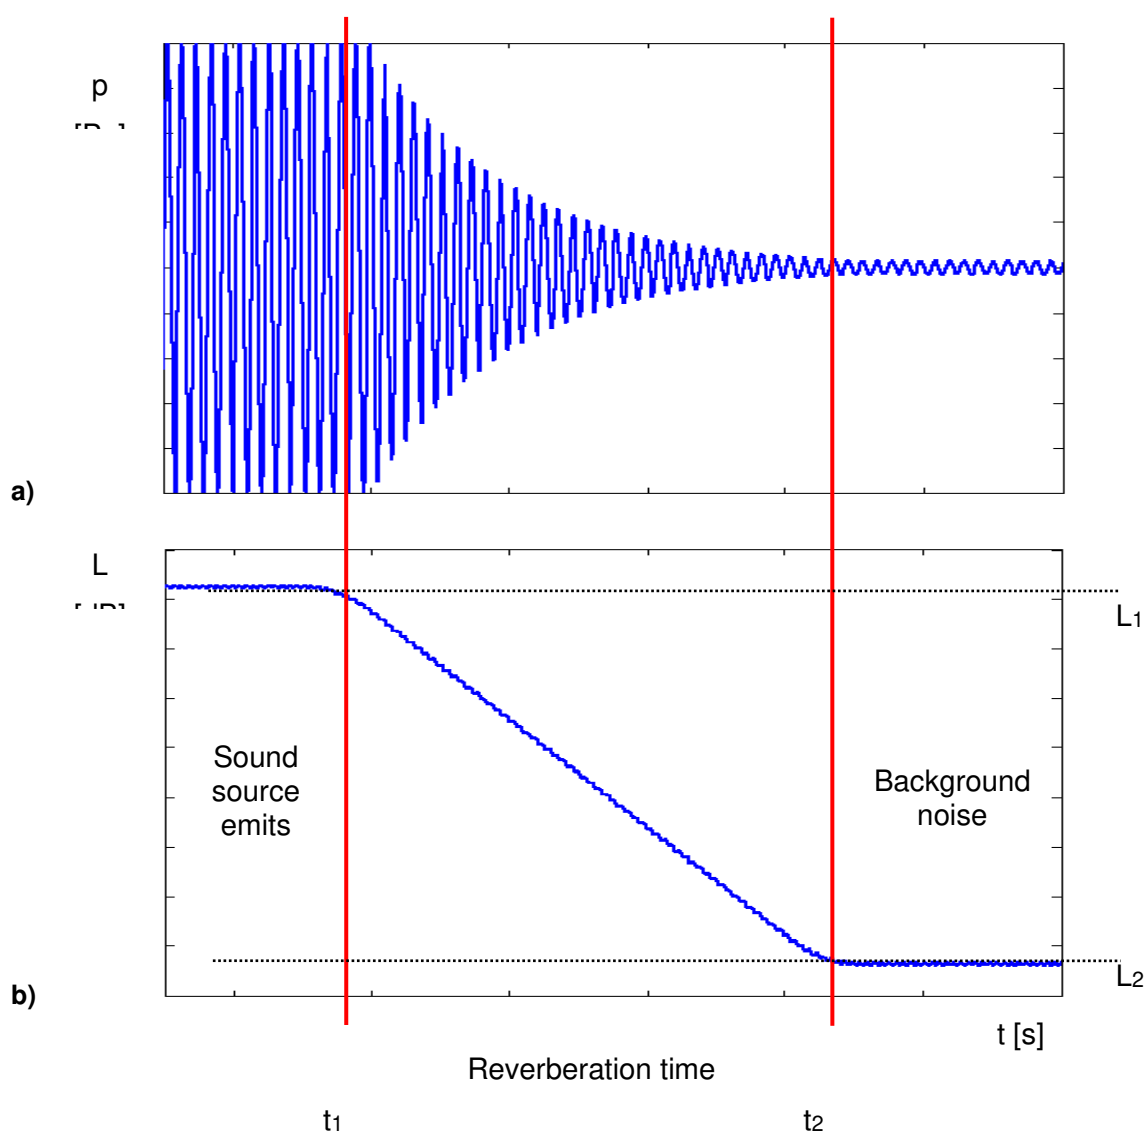


Fig 1. The acoustic pressure versus time (a) and the value of the sound pressure level versus time, so-called decay curve (b)

The marker t_1 indicates the moment when the sound source was switched off. From this moment the acoustic sound pressure / acoustic power (reflected waves propagate in the room) decreases till the moment indicated by the marker t_2 . The lower graph presents so-called the **decay curve**. The reverberation time value is equal to $t_2 - t_1$ when the difference between sound pressure levels L_1 and L_2 is 60 dB. The 60 dB dynamic condition is impractical in real measurements (very difficult to fulfil) hence the reverberation time

(RT 60) is obtained using the slope coefficient of the decay curve. The type of the definition from which slope coefficient is calculated (EDT, RT 20, RT 30 or user defined) depends on the difference between levels L_1 and L_2 (the difference between background noise level and sound source level) of the decay curve and it depends significantly from the acoustic source ability. If the level difference is larger than 45 dB, the RT 60 parameter can be calculated using three definitions: EDT, RT 20 and RT 30.

The real measurement results are not as smooth as the curves presented on graphs in Figure 1. In order to point out the interesting decay curve region (the position of the markers t_1 and t_2) some measurement data processing (in general signal smoothing by averaging) need to be applied.

E.2 DEFINITIONS AND CALCULATION OF THE RT 60 REVERBERATION TIME

➤ EDT (early decay time):

The EDT decay curve region is pointed out by markers t_1 and t_3 (cf. Fig. 2). It is checked whether the selected decay curve region has proper dynamics for the EDT calculation:

$$L_1 - L_2 \geq 10 \text{ dB}$$

$$L_2 - L_3 \geq \text{noise margin}$$

It is recommended by the ISO-3382 standard to set 10 dB value for noise margin.

In the case of the **impulse method**, the sound pressure level values between points t_1 (with L_1 level) and t_2 (with L_2) are approximated with the straight line ($y = a \cdot x + b$) by the linear regression. Before approximation the EDT value is calculated using the slope coefficient 'a' according to the formula:

$$\text{EDT} = -60.0 / a$$

In the case of the **decay method**, the EDT value is calculated according to the formula:

$$\text{EDT} = 6 \cdot (t_2 - t_1)$$

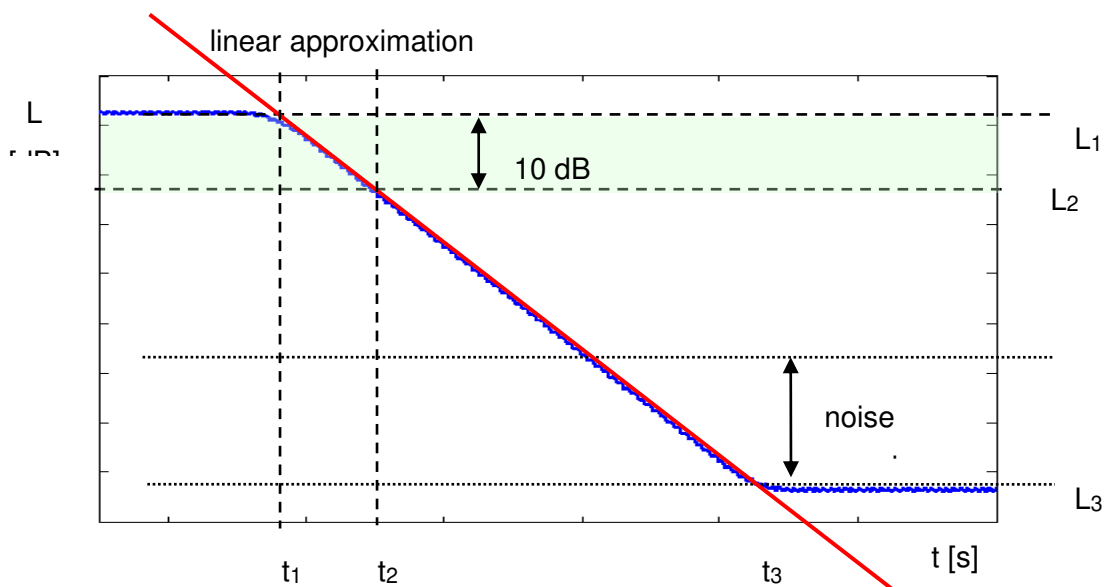


Fig 2. The EDT evaluation

➤ RT 20 (reverberation time calculated with 20 dB dynamics):

The RT 20 decay curve region is pointed out by markers t_1 and t_4 (cf. Fig. 3). It is checked whether the selected decay curve region has proper dynamics for the RT 20 calculation:

$$L_1 - L_4 > 5 \text{ dB} + 20 \text{ dB} + \text{noise margin}$$

It is recommended by the ISO-3382 standard to set 10 dB value for noise margin.

In the case of the **impulse method**, the sound pressure level values between points t_2 and t_3 are approximated with the straight line ($y = a \cdot x + b$) by the linear regression. The RT 20 value is calculated using the slope coefficient 'a' according to the formula:

$$\text{RT 20} = -60.0 / a$$

In the case of the **decay method**, the RT 20 value is calculated according to the formula:

$$\text{RT 20} = 3 \cdot (t_3 - t_2)$$

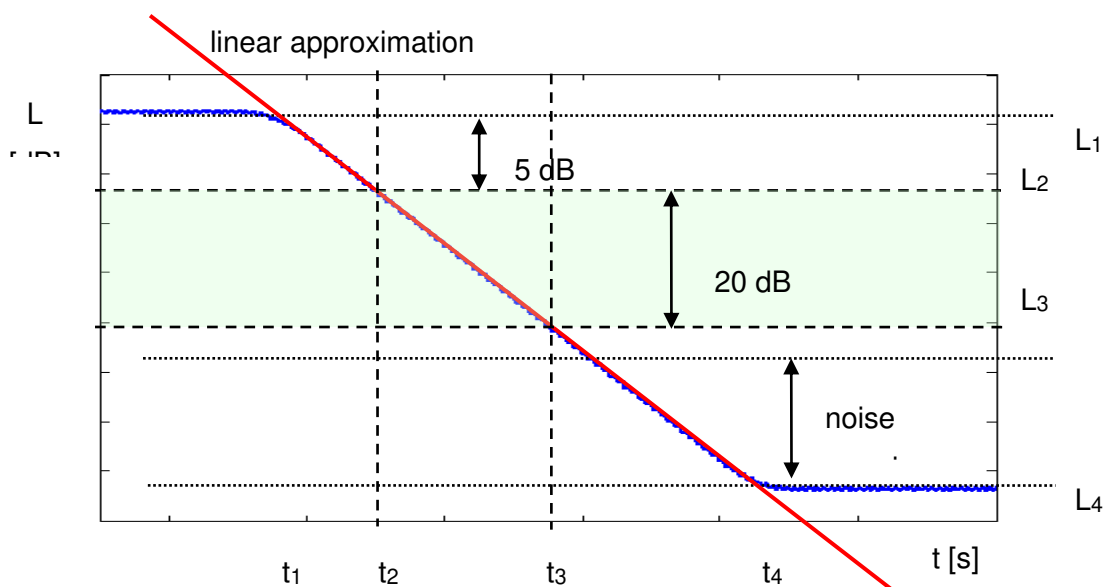


Fig 3. The RT 20 evaluation

➤ **RT 30 (reverberation time calculated with 30 dB dynamics):**

The RT 30 decay curve region is pointed out by markers t_1 and t_4 (cf. Fig. 4). It is checked whether the selected decay curve region has proper dynamics to the RT 30 calculation:

$$L_1 - L_4 > 5 + 30 \text{ dB} + \text{noise margin}$$

It is recommended by the ISO-3382 standard to set 10 dB value for noise margin.

In the case of the **impulse method**, the sound pressure level values between points t_2 and t_3 are approximated with the straight line ($y = a \cdot x + b$) by the linear regression. The RT 30 value is calculated using the slope coefficient 'a' according to the formula:

$$\text{RT 30} = -60.0 / a$$

In the case of the **decay method**, the RT 30 value is calculated according the formula

$$\text{RT 30} = 2 \cdot (t_3 - t_2)$$

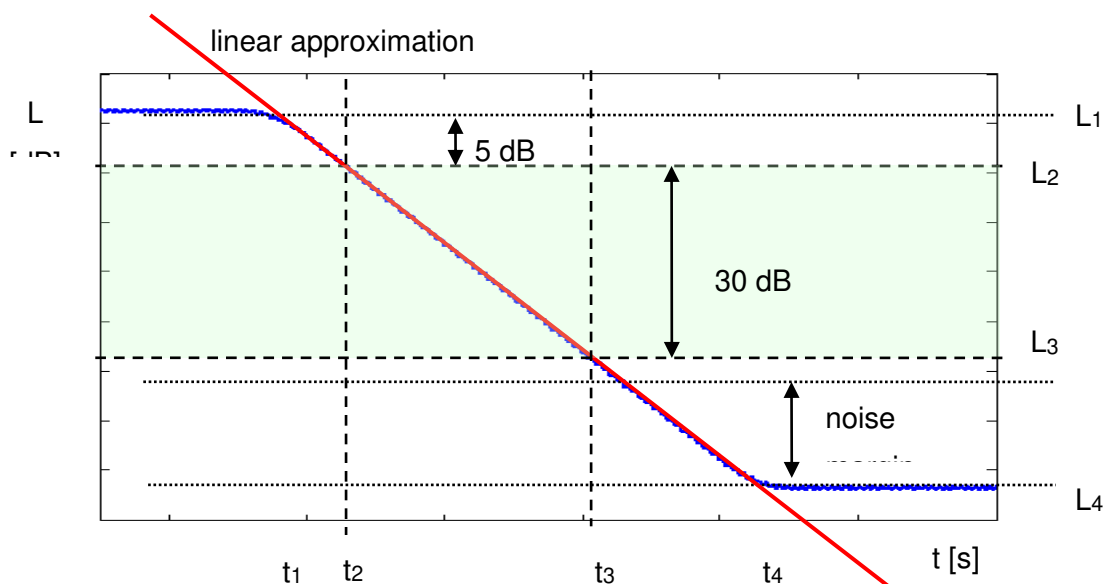


Fig 4. The RT 30 evaluation

E.3 DESCRIPTION OF THE DECAY CURVE RECORDING IN DIFFERENT MEASUREMENT METHODS

➤ DECAY method

This RT 60 measurement method requires omnidirectional sound source which emits pink noise in appropriate frequency band. The most critical parameter of the omnidirectional sound source is emitted sound pressure level as it was mentioned in the beginning of the appendix.

The graphical illustration of the data recording in this method is presented in Figure 5.

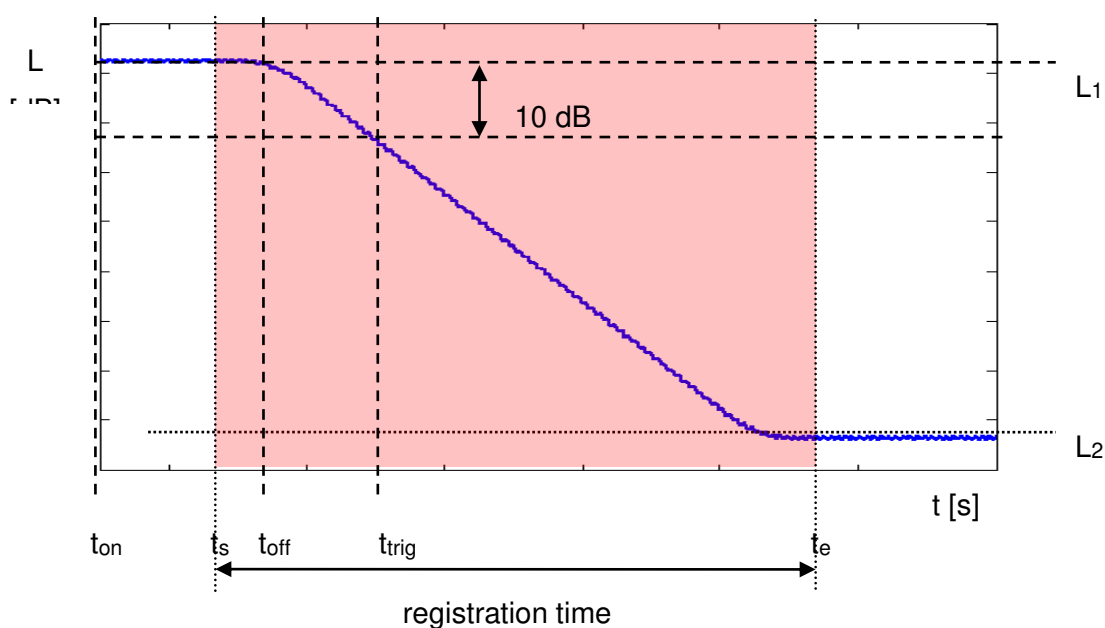


Fig 5. Data recording in the decay method of the reverberation time evaluation

The measurement time in this method consists of:

- The time between markers t_{on} and t_{off} in which the omnidirectional sound source emits acoustic power and the SVAN xxx analyser measures the actual sound pressure level.
- The time between markers t_{off} and t_{trig} in which the omnidirectional sound source is switched off and the SVAN xxx instrument waits for trigger condition fulfilment.
- The time between markers t_s and t_{trig} registered since the trigger condition fulfilment back till point t_s to allow recognising the beginning of the decay region. In the SVAN xxx instruments this time is equal to the **Time Step** (path: <Menu> / Measurement / RT60 Settings) parameter value multiplied by 50.
- The time between markers t_{trig} and t_e registered since t_{trig} forward to record whole decay curve together with significantly long period of the noise level. This time in SVAN xxx instruments is adjusted by **Recording Time** (path: <Menu> / Measurement / RT60 Settings) parameter.

The above graph shows that the proper setting of the **Recording Time** value is very important. The registration time has to be long enough to acquire sufficient number of background noise level values. In other case the decay curve region could not be properly analysed or decay region could not fulfil the dynamic condition mentioned above. It is recommended to set the **Recording Time** parameter two times longer than expected reverberation time.

➤ Impulse method

In the Impulse method, Reverberation Time is computed by using the reverse-time integrated impulse response. This way of measuring sound decay was introduced firstly by M. R. Schroeder in two historical articles:

- New Method of Measuring Reverberation Time, *Journal of Acoust. Soc. Am.* 1965
- Integrated-Impulse Method Measuring Sound Decay without Using Impulses, *Journal of Acoust. Soc. Am.* Vol. 66(2) 1979

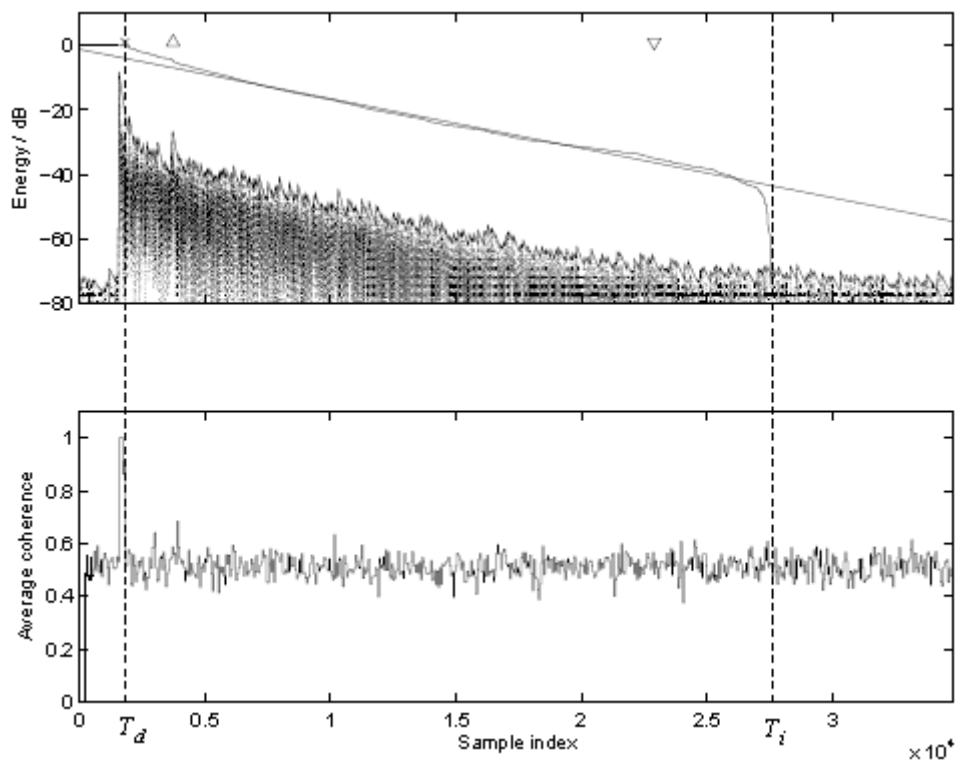


Fig. 6 An example of Schroeder integration with the limits T_i and T_d

This RT 60 measurement method requires impulse sound source like pistol, petard or other sound source which emits impulse signal with very high sound pressure level.

The graphical illustration of data registering in this method is presented in Figure 7.

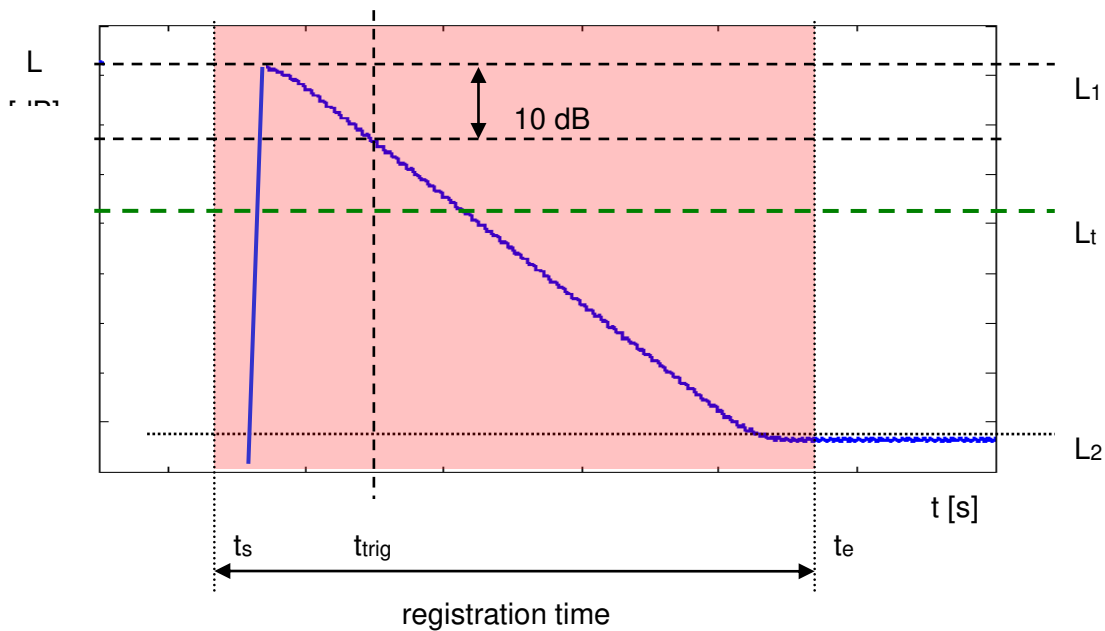


Fig 7. Data recording in the impulse method of the reverberation time evaluation


The measurement time in this method consists of:

- The time before marker t_{trig} in which the SVAN xxx analyser measures the actual sound pressure level and waits for the very high impulse sound pressure level which will fulfil the trigger condition. The trigger conditions will be fulfilled only when emitted impulse has maximal sound pressure level higher than L_t level (cf. Fig. 6). The L_t level in the SVAN xxx analyser is adjusted by parameter **Level** (path: <Menu> / Measurement / RT60 Settings).
- The time between markers t_s and t_{trig} registered since the trigger condition fulfilment back till point t_s to allow recognising the beginning of the decay region. In the SVAN xxx instruments this time is equal to the **Time Step** (path: <Menu> / Measurement / RT60 Settings) parameter value multiplied by 50.
- The time between markers t_{trig} and t_e registered since t_{trig} forward to record whole decay curve together with significantly long period of the noise level. This time in SVAN xxx instruments is adjusted by **Recording Time** (path: <Menu> / Measurement / RT60 Settings) parameter.

The above graph shows that the proper setting of the **Recording Time** value is very important. The registration time has to be long enough to acquire sufficient number of background noise level values. In other case the decay curve region could not be properly analysed or decay region could not fulfil the dynamic condition mentioned above. It is recommended to set the **Recording Time** parameter two times longer than expected reverberation time.

APPENDIX F. SA 271A OUTDOOR MICROPHONE KIT ASDosimeterBLY GUIDE

F.1 PART SET

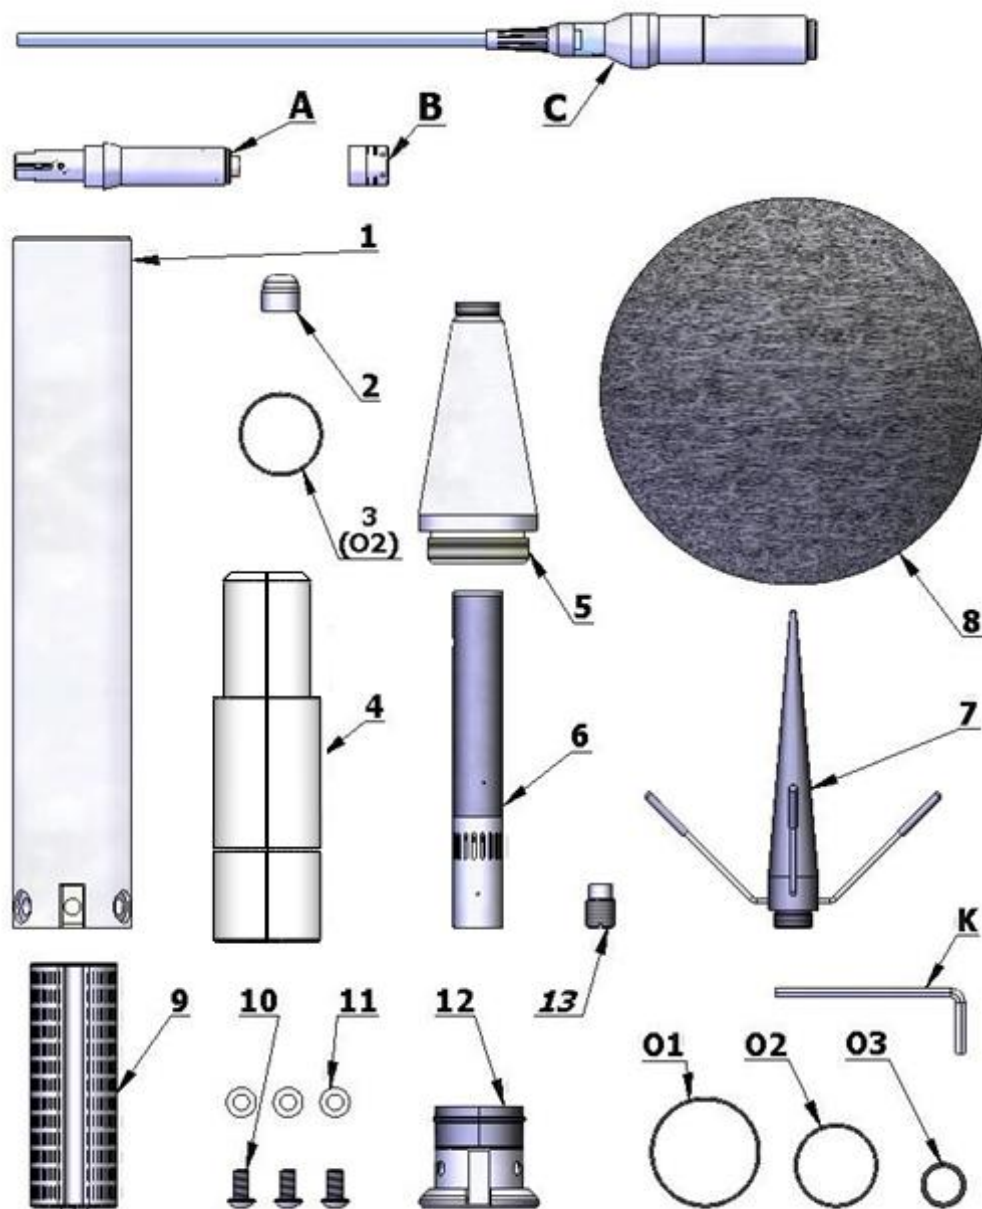

SA 271A kit:

- 1 - tube
- 2 - dummy microphone
- 3 - O-ring type gasket
- 4 - clamp (2 halves)
- 5 - upper cone
- 6 - microphone protecting tube
- 7 - anti-bird spikes
- 8 - windscreen (SA 209)
- 9 - desiccator (not included)
- 10 - M5x10 hex socket raised screw
- 11 - washer
- 12 - bottom
- 13 - 1/4" thread adapter (not included)

Tools:


- K - 3mm Allen key

Spare parts:

- 01 - O-ring type gasket Ø35x1
- 02 - O-ring type gasket Ø26x1
- 03 - O-ring type gasket Ø12x1.5

Parts not included:


- A – SV 18A preamplifier
- B – ACO 7152 microphone
- C – SC 91A cable

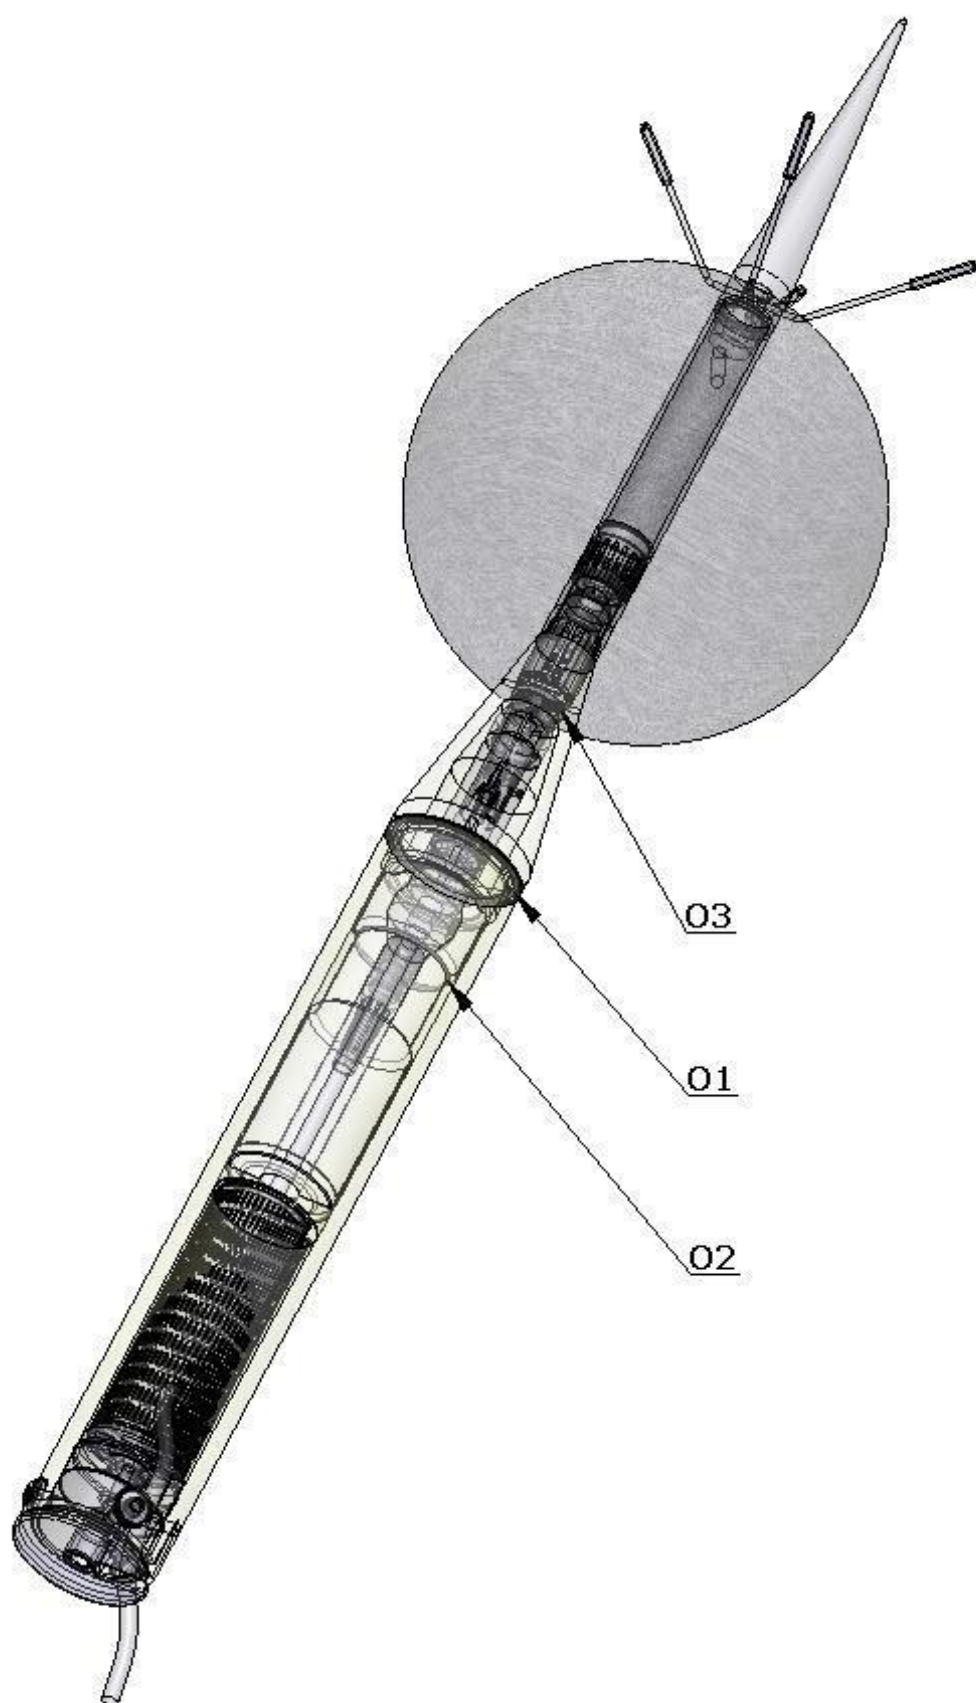


O-ring gasket locations inside

F.2 ASSEMBLY OF SA 271A


1. Secure preamplifier (A) with the dummy microphone (2) and connect the cable (C).

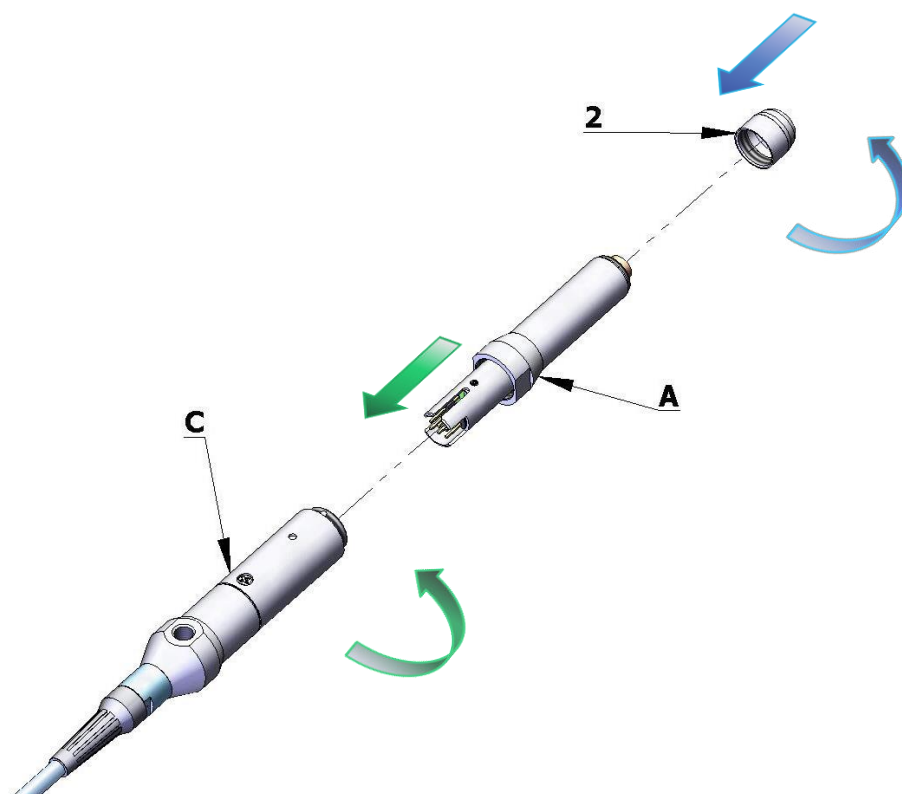


2. Pull tube (1) over the cable.

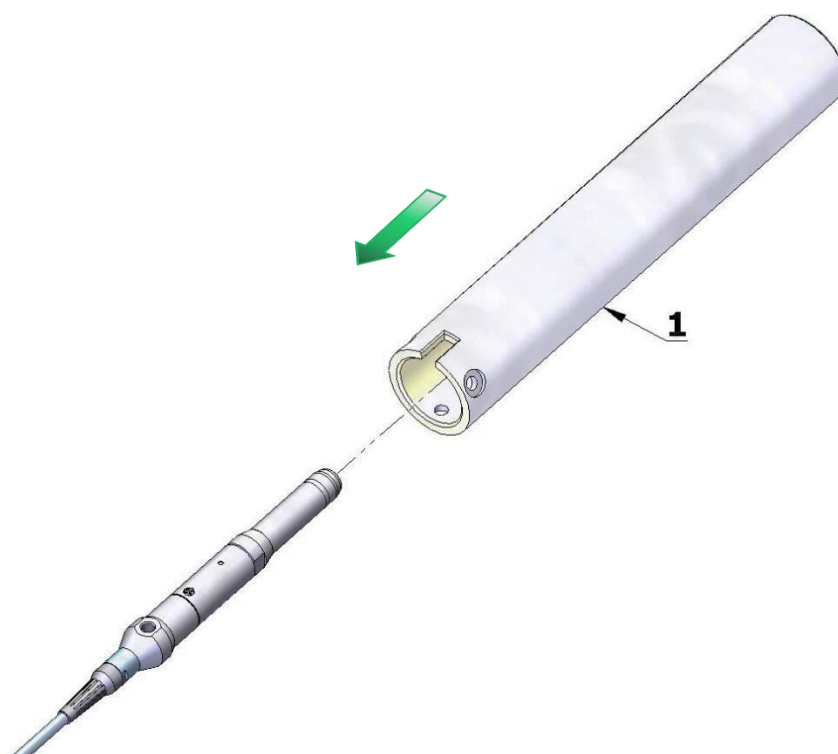

3. Connect the clamp halves (4) to the connector and insert O-ring gasket (3) on the lightning signed place.

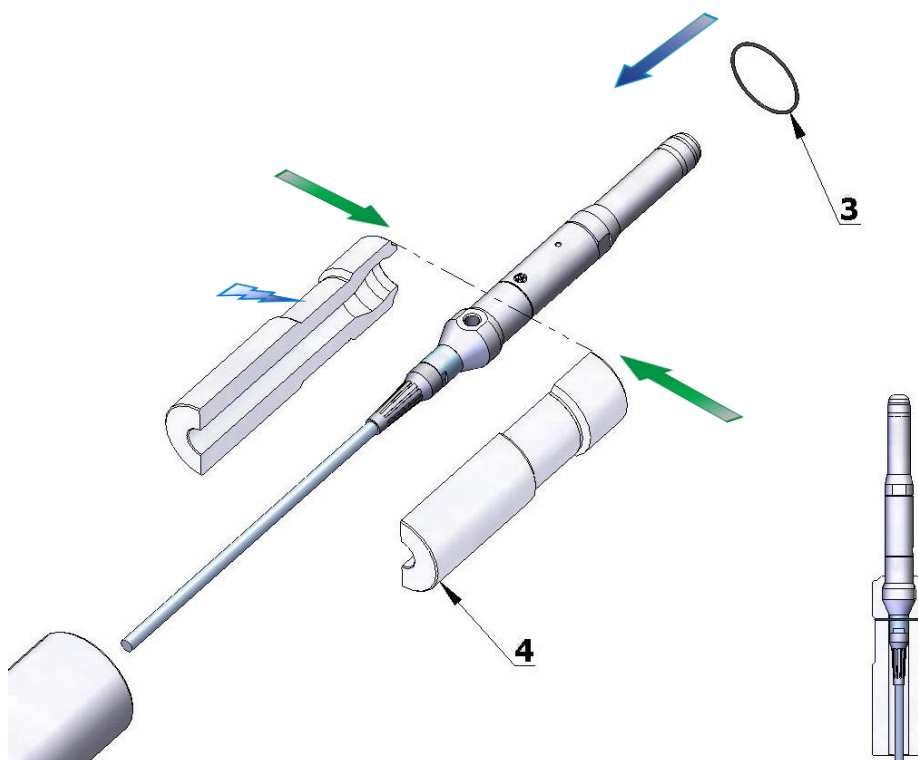


4. Apply the upper, conical part (5) on the preamplifier.

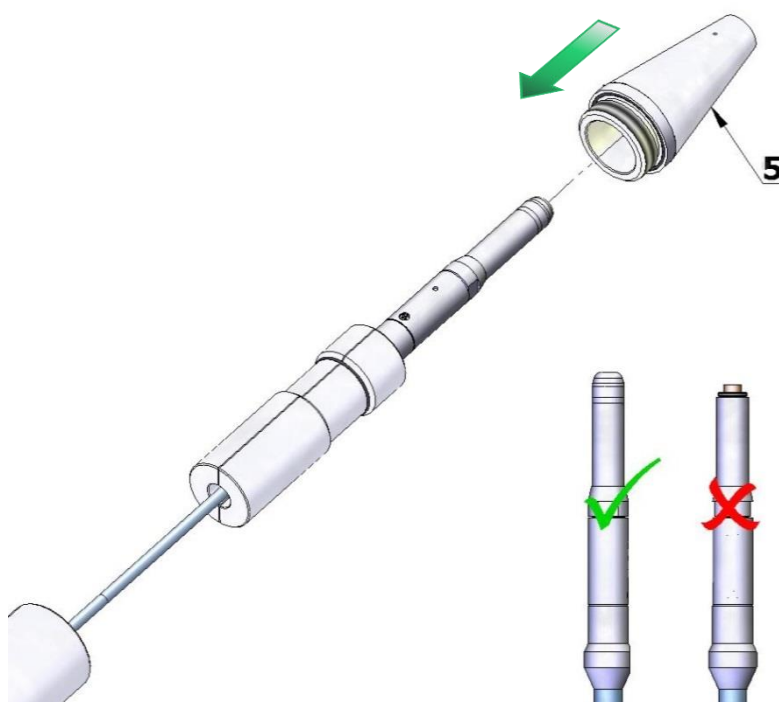


Note: Do not use preamplifier without the dummy microphone. It can cause damage of the O-ring gasket inside the cone.

5. Screw the tube on the cone by rotating the tube – so as to not twist the cable.

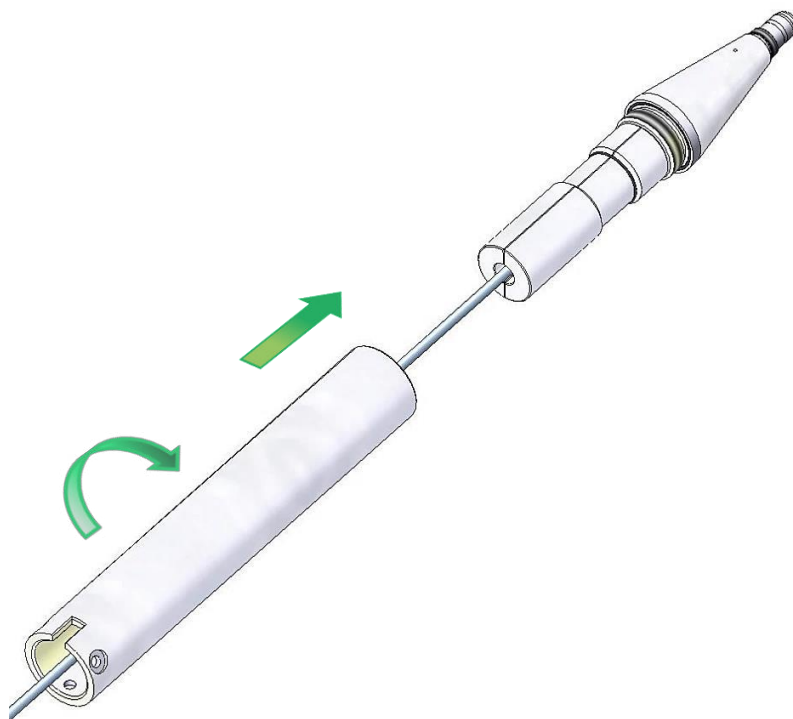


6. Replace the dummy microphone (2) with the 1/2" microphone cartridge (B).

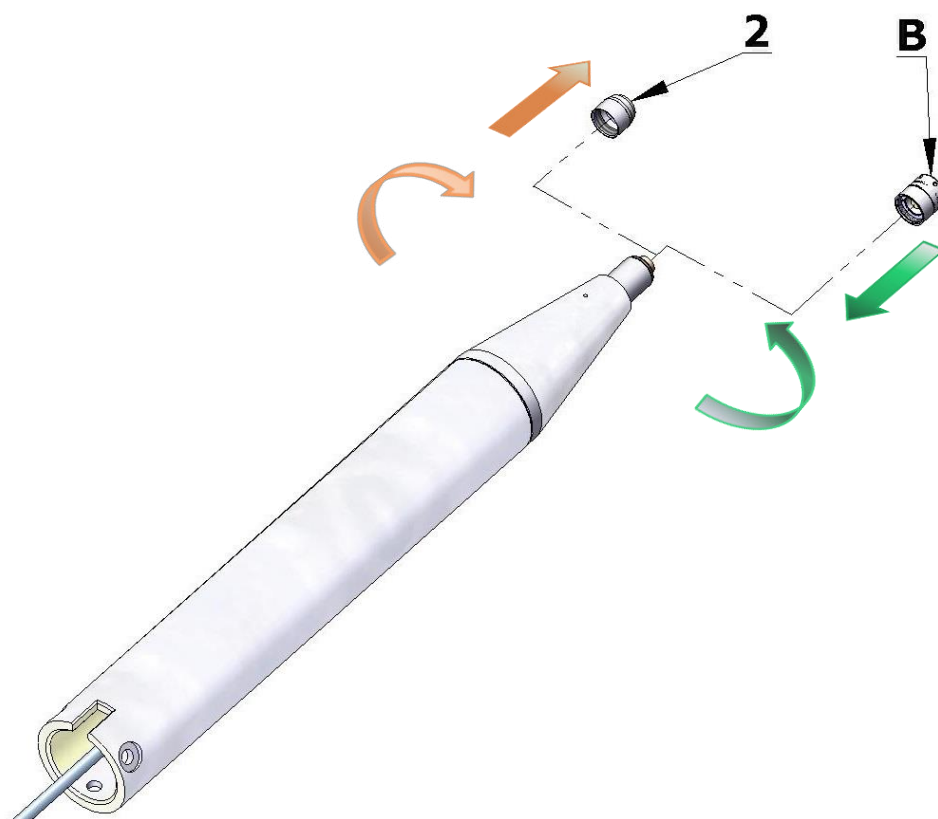


7. Calibrate the complete system using SVANTEK acoustic calibrator.




8. Install the microphone protection tube (6). Use the Allen key (K) as a pin at protecting tube orifice.

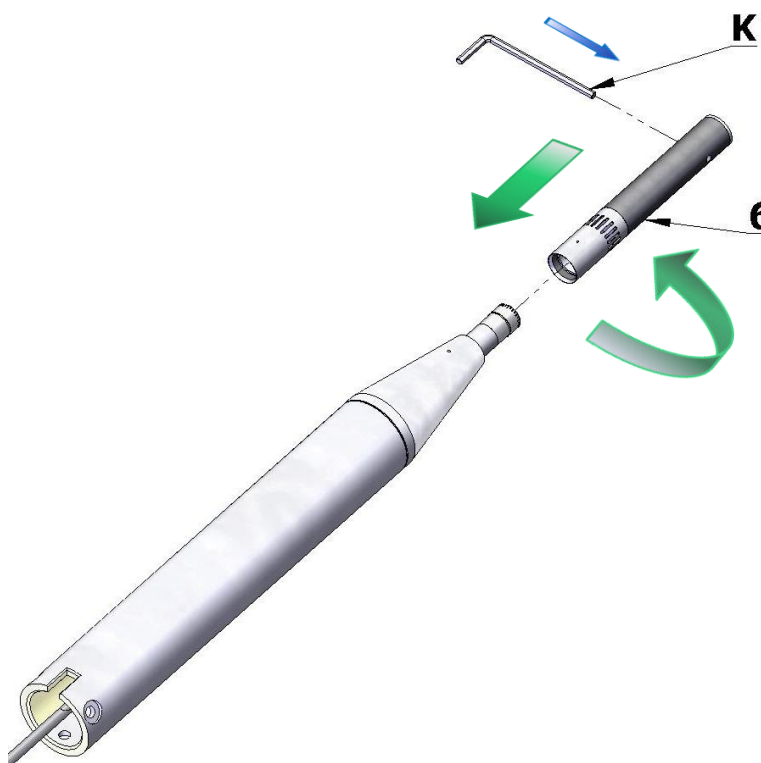


9. Mount windscreen (8) and the anti-bird spikes (7).

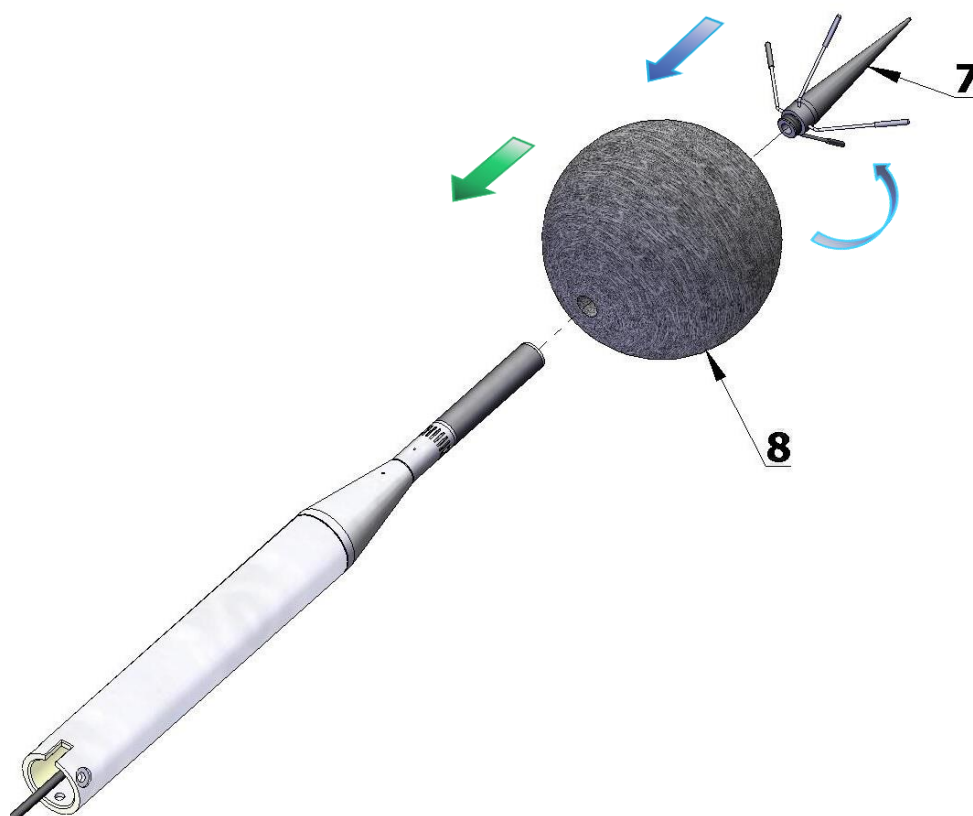


10. Slide the desiccator (9) inside the tube.

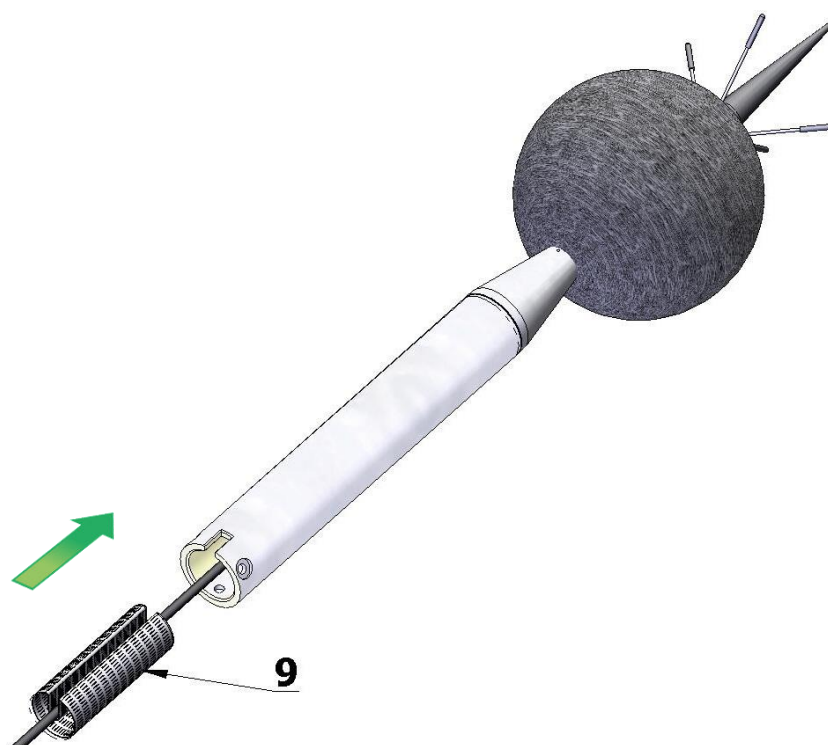

11. Place the cable in the slot and connect the bottom part (**12**) by three screws (**10**) with washers (**11**). Use the Allen key (**K**).

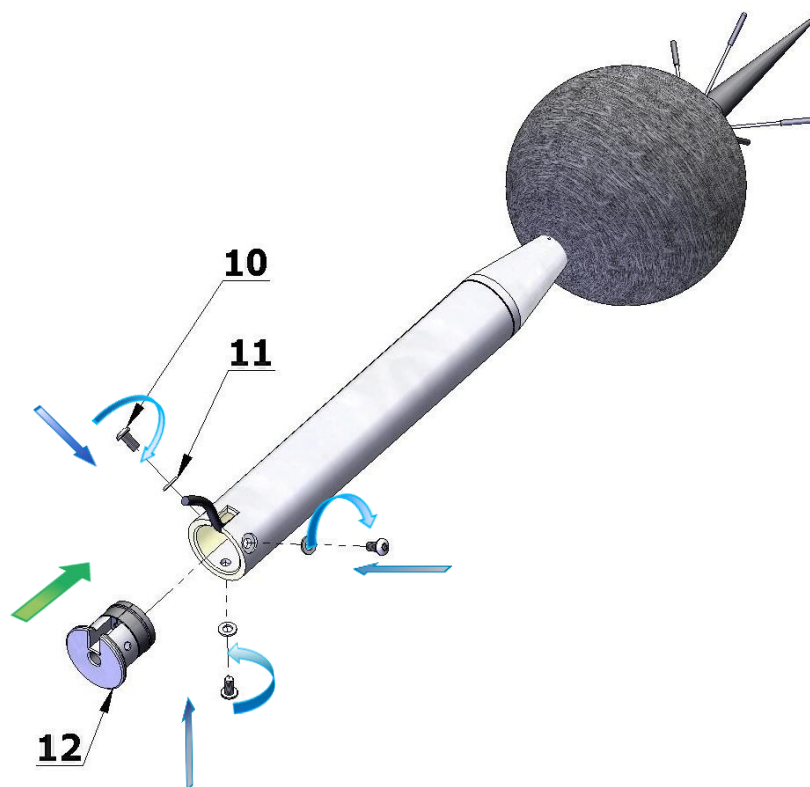

12. Mount the completed system on the dedicated tripod or pole. Use $\frac{1}{4}$ " thread adapter (**13**) (if necessary) (see last note on next page).

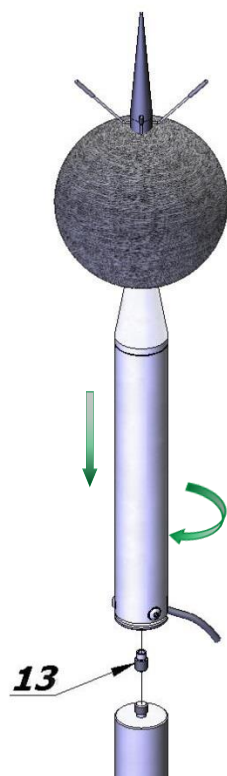

F.3 IMPORTANT NOTES




Note: The SA 209 (8) at the part set picture) foam windscreen protects microphone from wind and rain. If the SA 209 windscreen is used continuously for a long period of time it is recommended to replace it at least once a year.



Note: During continuous usage the SA 209 windscreen is exposed to different weather conditions with possibility of causing physical damage to the foam's structure. Therefore, it is recommended, at least once a quarter (3 months), to check the condition of the windscreen by examining the surface for cracks by squeezing the foam. If cracks or holes are observed, the SA 209 windscreen must be replaced. Take care when examining the foam, as squeezing it too aggressively can damage the surface.

Colour of the silica gel used in the desiccator (part 9) when it is dry is amber. If colour of the silica gel turns light grey it means that the gel is soaked (wetted) and the desiccator is not able to absorb more moisture. Colour of the silica gel is visible through the window of the desiccator. If colour of the gel becomes light grey, the desiccator should be regenerated by drying it for 3 hours in temperature of 150°C.

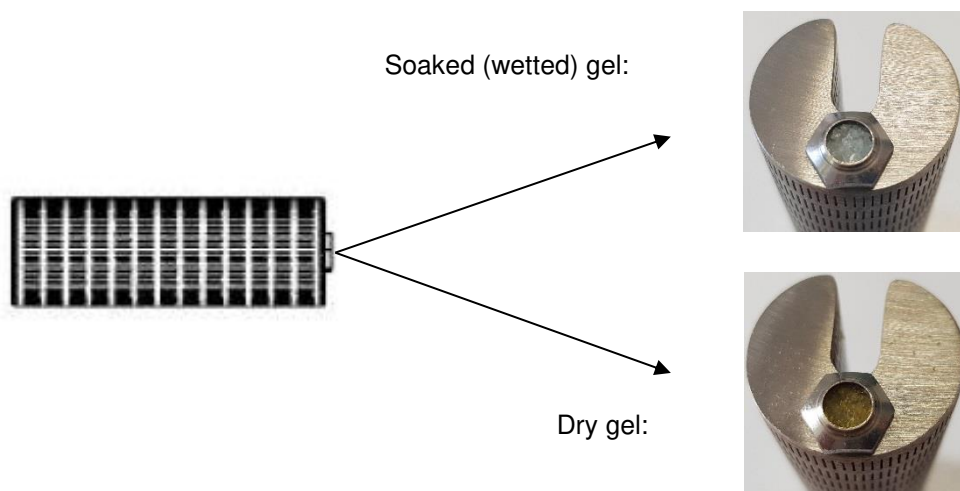

Note: Desiccator should be inspected at least every 2 weeks, and more often when used in conditions of high air humidity.



Note: Desiccator must be stored in a hermetic container when is not installed in SA 271A to prevent absorbing moisture unnecessarily.



Note: Tripod or pole with 1/4" thread is not recommended for stormy weather.